

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110118\
 Data File : PL041619.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2018 14:52
 Operator : AJ\SJ
 Sample : J5734-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 01:08:13 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.472	4.104	53167088	28675662	8.346	9.310
28)	SA Decachlor...	8.217	9.235	74893661	30455510	11.306	11.887
Target Compounds							
10)	B gamma-Chl...	5.429	0.000	3532100	0	0.434	N.D. #
11)	B alpha-Chl...	5.429f	0.000	3532100	0	0.436	N.D. #
12)	B 4,4'-DDE	5.633	6.463	3785764	2956602	0.529	0.903 #
13)	MA Dieldrin	5.758	0.000	3068560	0	0.386	N.D. #
16)	A 4,4'-DDD	6.214f	0.000	3851692	0	0.663	N.D. #
17)	MA 4,4'-DDT	6.384	7.229	5394529	1751117	0.887	0.697
18)	B Endrin al...	6.426f	7.229f	290207	1751117	0.053	0.800 #
19)	B Endosulfa...	6.670	0.000	1182017	0	0.185	N.D. #
20)	A Methoxychlor	6.914	0.000	2298102	0	0.684	N.D. #
23)	Chlordane-1	4.393	0.000	5138792	0	18.124	N.D. #
25)	Chlordane-3	5.429	0.000	3532100	0	3.963	N.D. #
26)	Chlordane-4	5.429	0.000	3532100	0	4.511	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110118\
Data File : PL041619.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2018 14:52
Operator : AJ\SJ
Sample : J5734-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 01:08:13 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

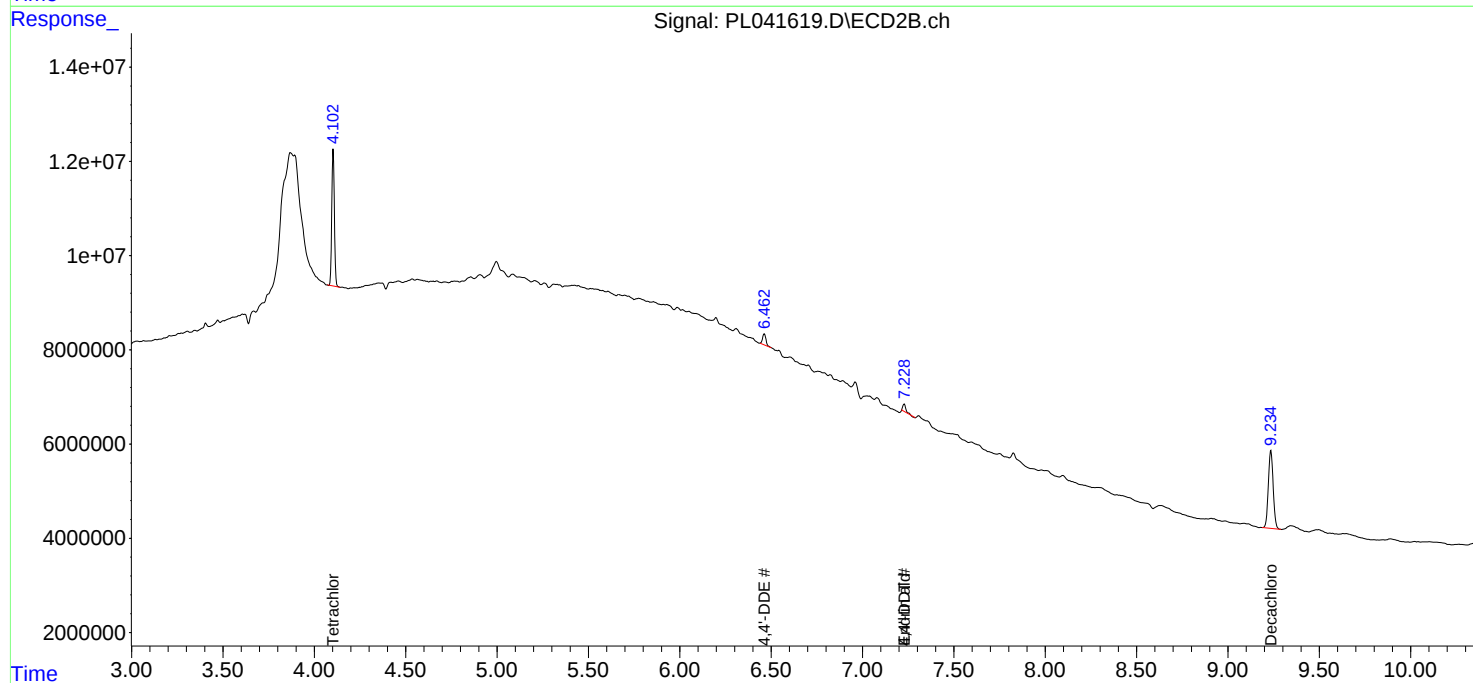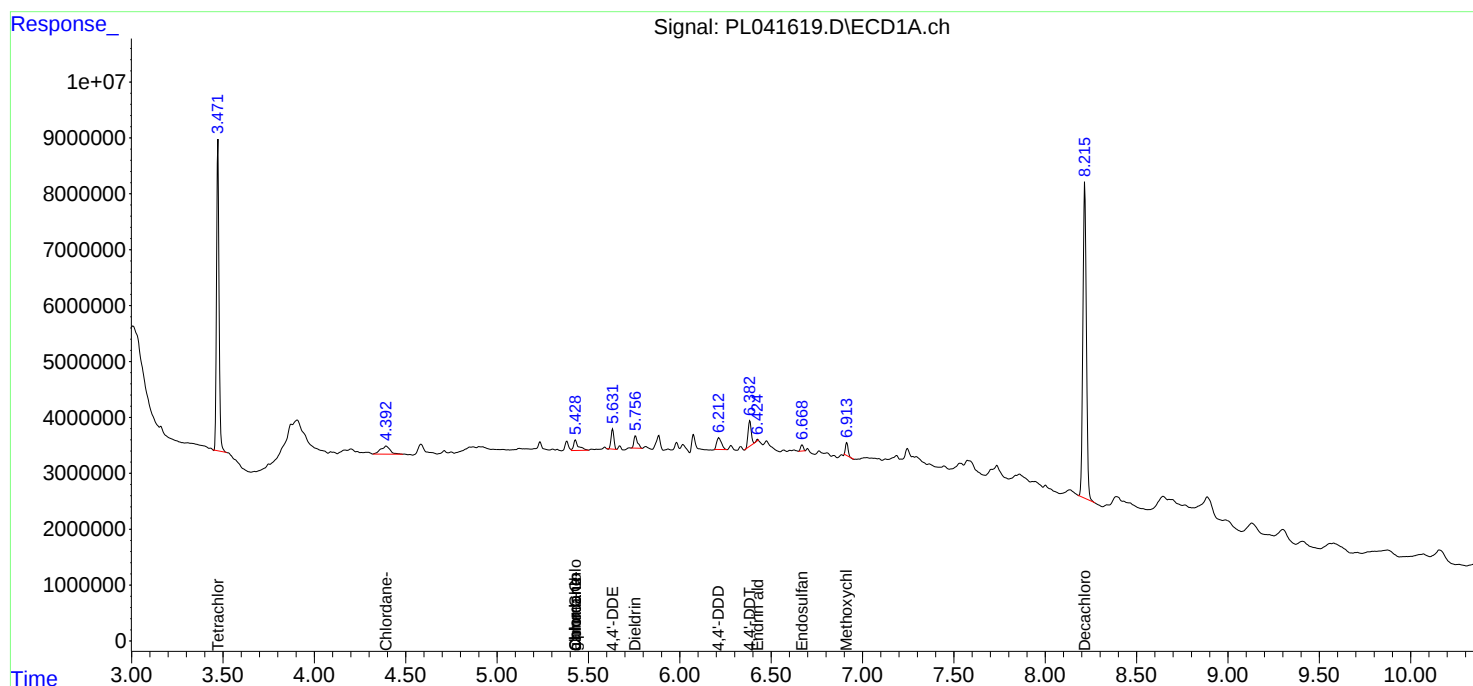


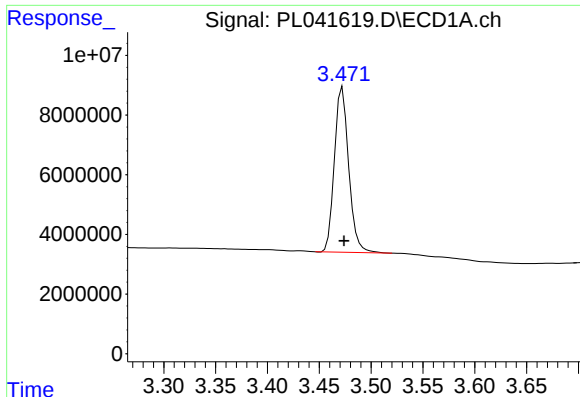

#1 Tetrachloro-m-xylene


R.T.: 3.472 min
Delta R.T.: -0.002 min
Response: 53167088
Conc: 8.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

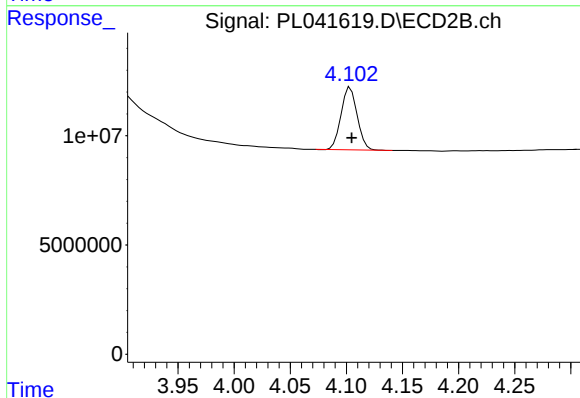


#1 Tetrachloro-m-xylene

R.T.: 4.104 min
Delta R.T.: -0.001 min
Response: 28675662
Conc: 9.31 ng/ml

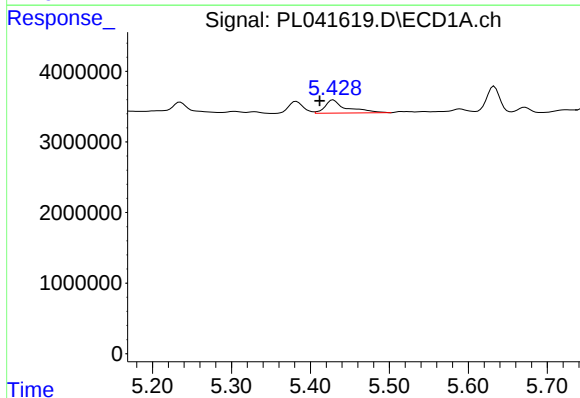


#10 gamma-Chlordane

R.T.: 5.429 min
Delta R.T.: 0.017 min
Response: 3532100
Conc: 0.43 ng/ml

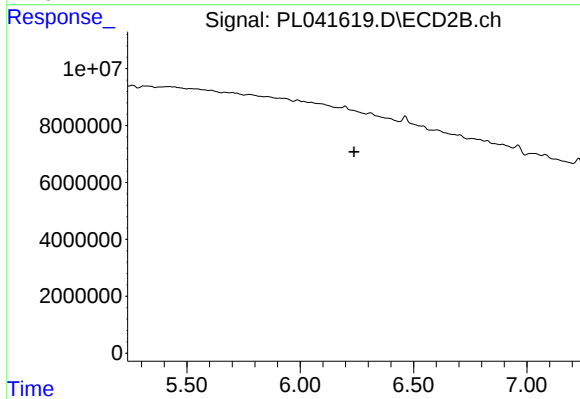

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.237 min
Response: 0
Conc: N.D.

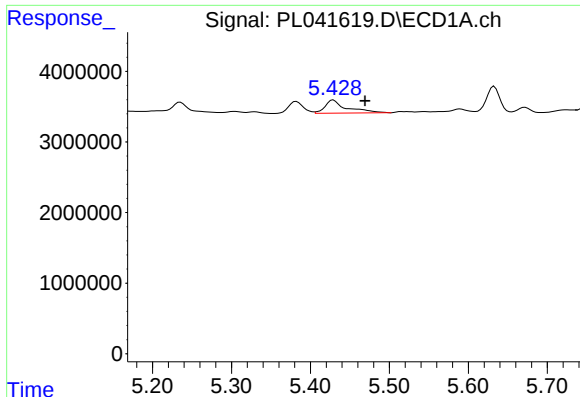

#11 alpha-Chlordane


R.T.: 5.429 min
Delta R.T.: -0.040 min
Response: 3532100
Conc: 0.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

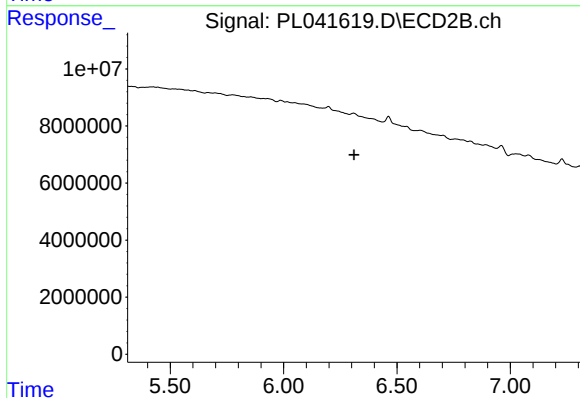


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.311 min
Response: 0
Conc: N.D.

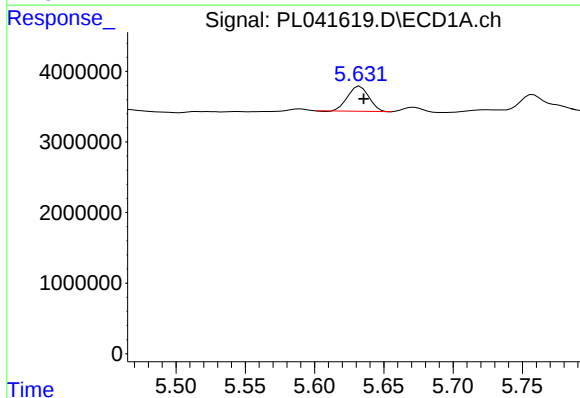


#12 4,4'-DDE

R.T.: 5.633 min
Delta R.T.: -0.003 min
Response: 3785764
Conc: 0.53 ng/ml

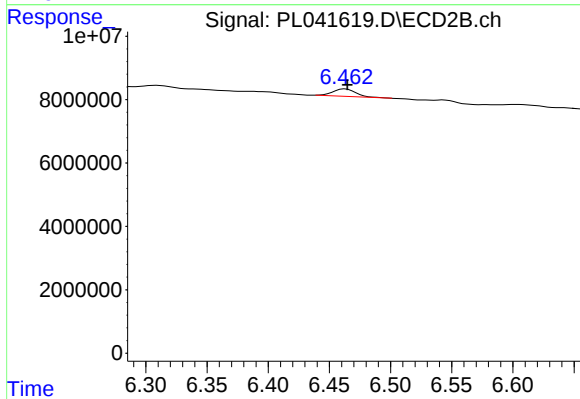

#12 4,4'-DDE


R.T.: 6.463 min
Delta R.T.: -0.002 min
Response: 2956602
Conc: 0.90 ng/ml

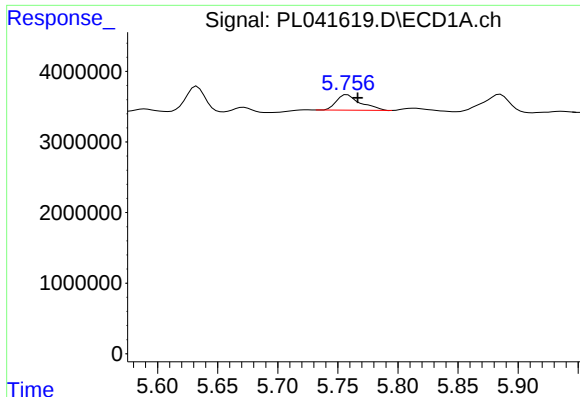

#13 Dieldrin


R.T.: 5.758 min
Delta R.T.: -0.009 min
Response: 3068560
Conc: 0.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

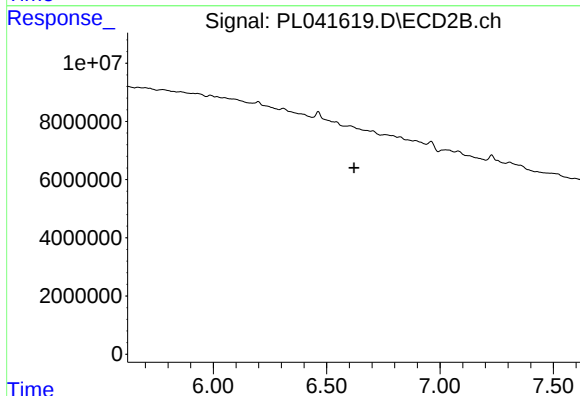


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.621 min
Response: 0
Conc: N.D.

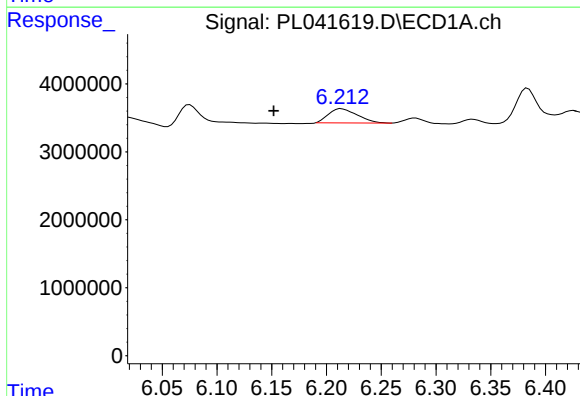


#16 4,4'-DDD

R.T.: 6.214 min
Delta R.T.: 0.062 min
Response: 3851692
Conc: 0.66 ng/ml

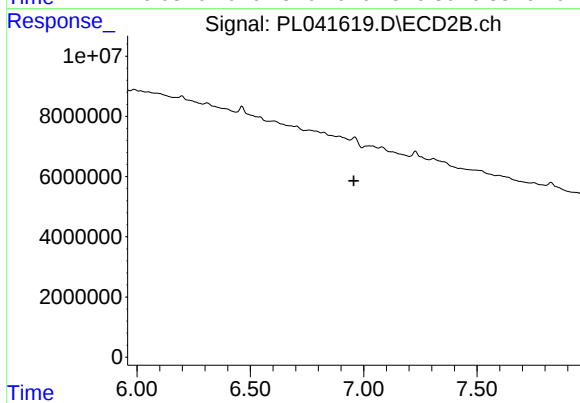

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.957 min
Response: 0
Conc: N.D.

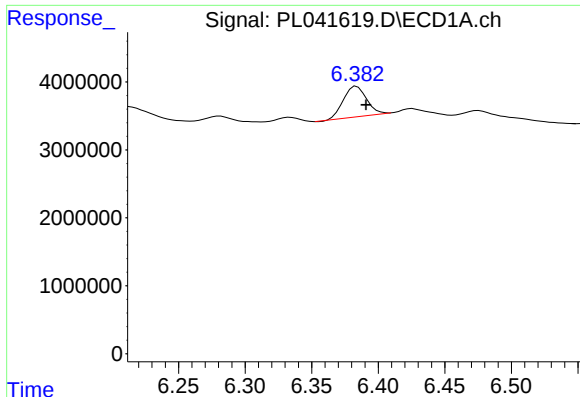

#17 4,4'-DDT


R.T.: 6.384 min
Delta R.T.: -0.007 min
Response: 5394529
Conc: 0.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

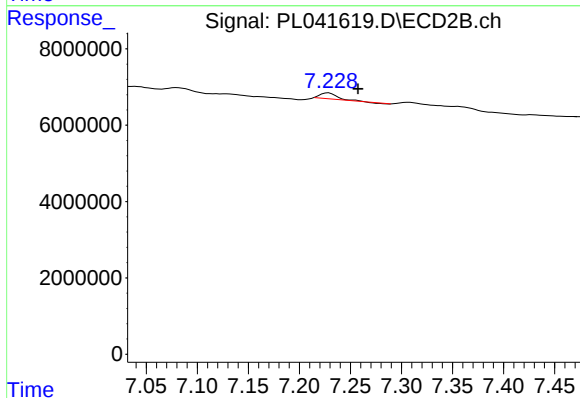


#17 4,4'-DDT

R.T.: 7.229 min
Delta R.T.: -0.029 min
Response: 1751117
Conc: 0.70 ng/ml

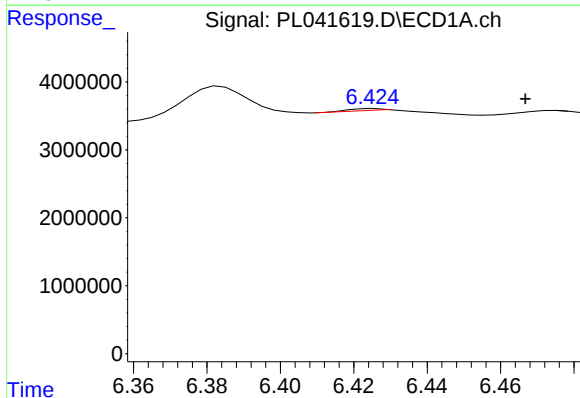


#18 Endrin aldehyde

R.T.: 6.426 min
Delta R.T.: -0.041 min
Response: 290207
Conc: 0.05 ng/ml

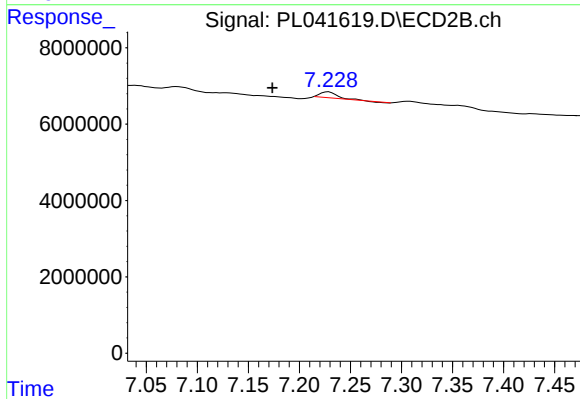

#18 Endrin aldehyde


R.T.: 7.229 min
Delta R.T.: 0.055 min
Response: 1751117
Conc: 0.80 ng/ml

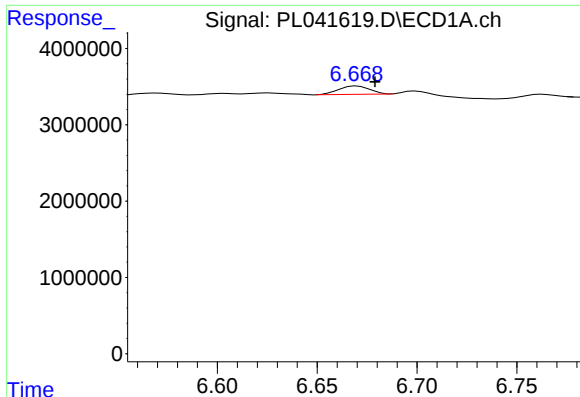

#19 Endosulfan Sulfate


R.T.: 6.670 min
Delta R.T.: -0.009 min
Response: 1182017
Conc: 0.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

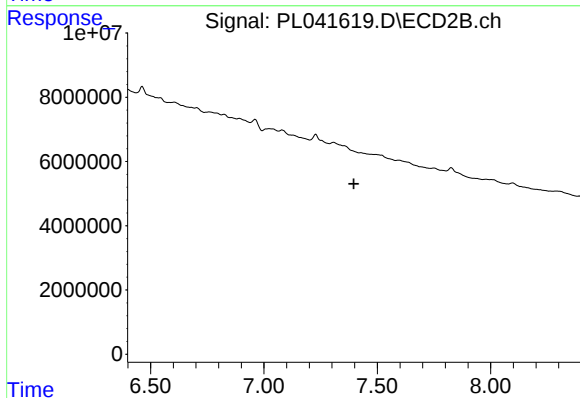


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.396 min
Response: 0
Conc: N.D.

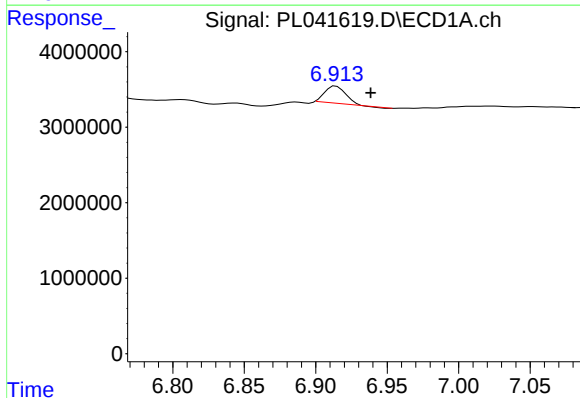


#20 Methoxychlor

R.T.: 6.914 min
Delta R.T.: -0.024 min
Response: 2298102
Conc: 0.68 ng/ml

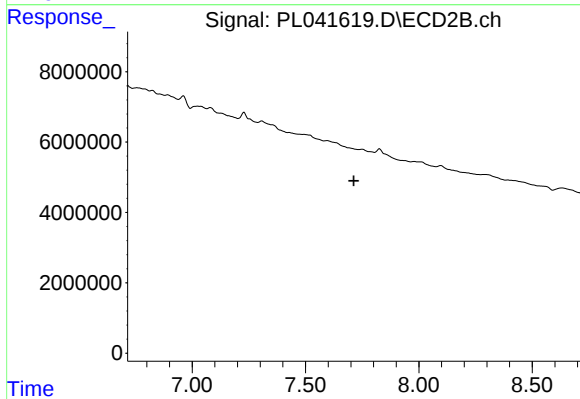

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.713 min
Response: 0
Conc: N.D.

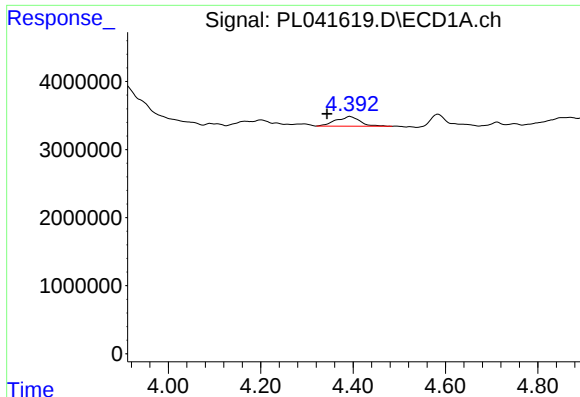

#23 Chlordane-1


R.T.: 4.393 min
Delta R.T.: 0.050 min
Response: 5138792
Conc: 18.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

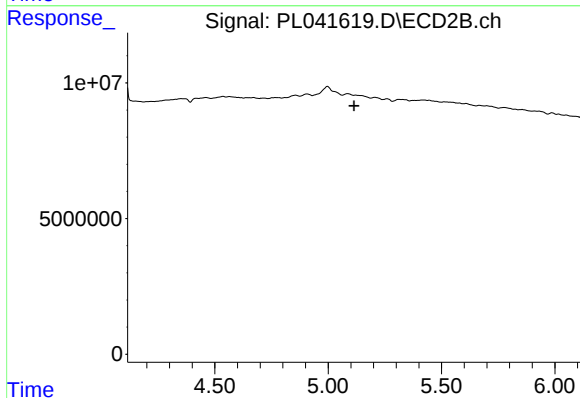


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.115 min
Response: 0
Conc: N.D.

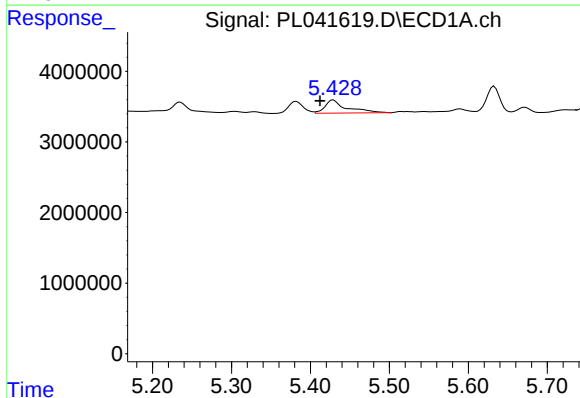


#25 Chlordane-3

R.T.: 5.429 min
Delta R.T.: 0.017 min
Response: 3532100
Conc: 3.96 ng/ml

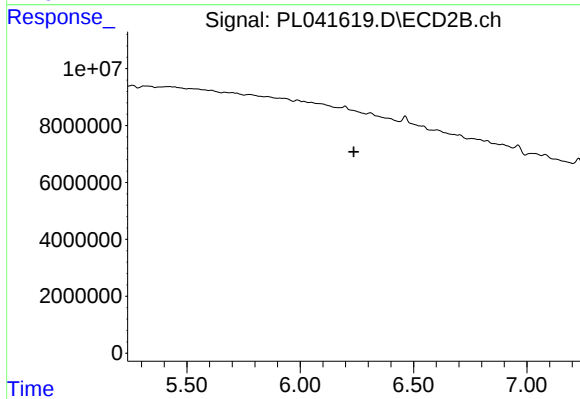

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.237 min
Response: 0
Conc: N.D.

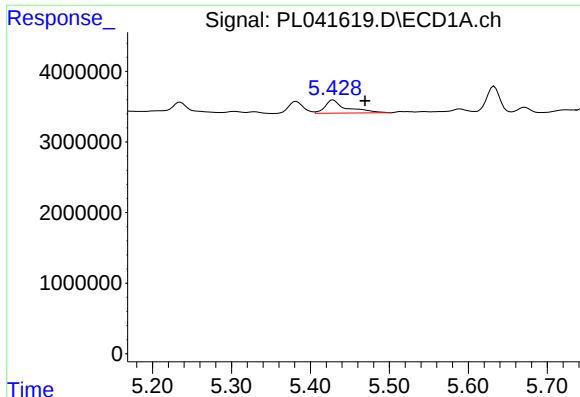

#26 Chlordane-4


R.T.: 5.429 min
Delta R.T.: -0.040 min
Response: 3532100
Conc: 4.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

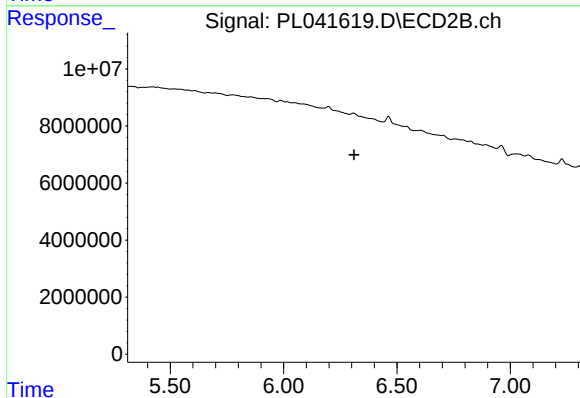


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.311 min
Response: 0
Conc: N.D.

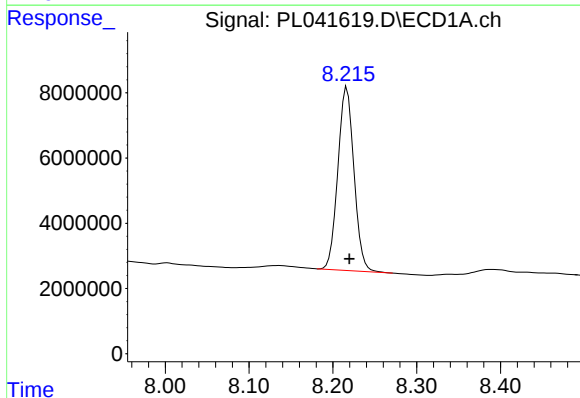

#28 Decachlorobiphenyl

R.T.: 8.217 min
Delta R.T.: -0.003 min
Response: 74893661
Conc: 11.31 ng/ml

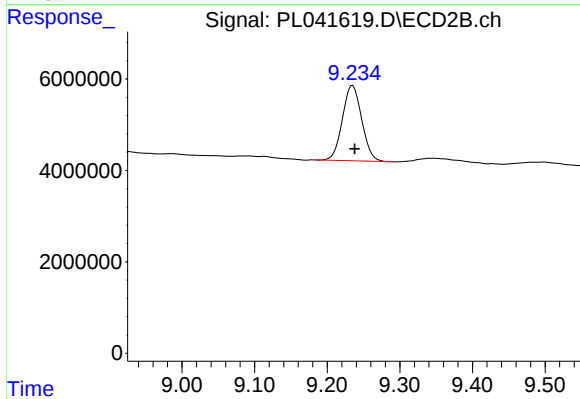

#28 Decachlorobiphenyl

R.T.: 9.235 min
Delta R.T.: -0.003 min
Response: 30455510
Conc: 11.89 ng/ml