

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110118\
 Data File : PL041628.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2018 16:59
 Operator : AJ\SJ
 Sample : J5741-31
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 01:10:12 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.472	4.105	113.9E6	56966063	17.884	18.494
28)	SA Decachlor...	8.216	9.237	108.0E6	43293253	16.297	16.897
Target Compounds							
15)	B Endosulfa...	6.229f	0.000	2685153	0	0.388	N.D. #
23)	Chlordane-1	4.366	0.000	1283000	0	4.525	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110118\
Data File : PL041628.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2018 16:59
Operator : AJ\SJ
Sample : J5741-31
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 01:10:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

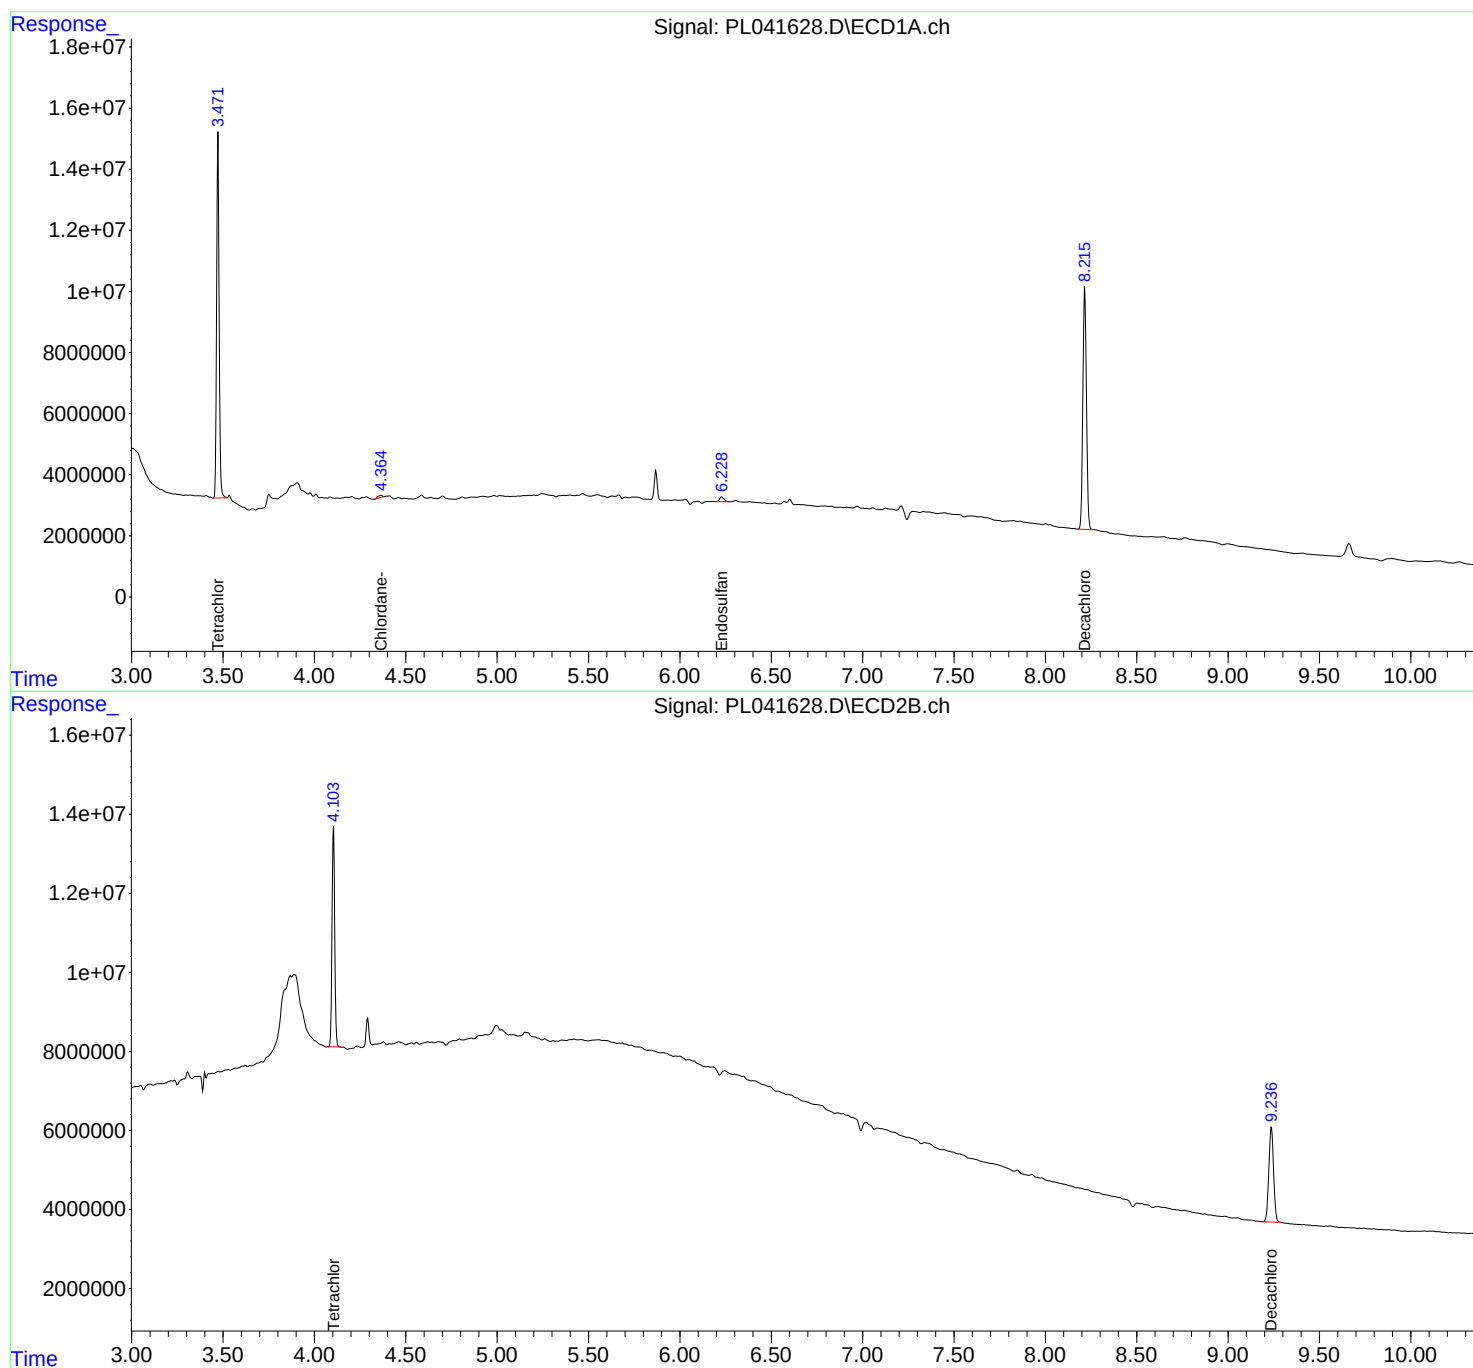


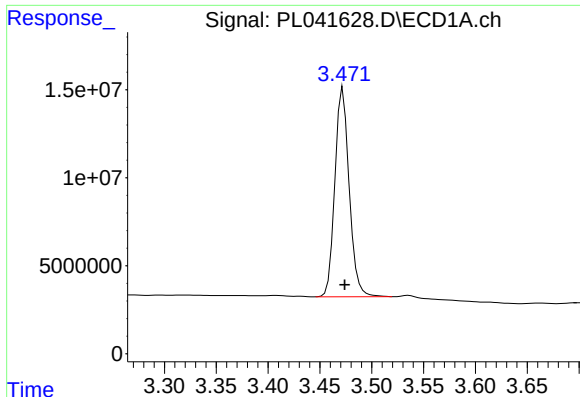

#1 Tetrachloro-m-xylene


R.T.: 3.472 min
Delta R.T.: -0.002 min
Response: 113924290
Conc: 17.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

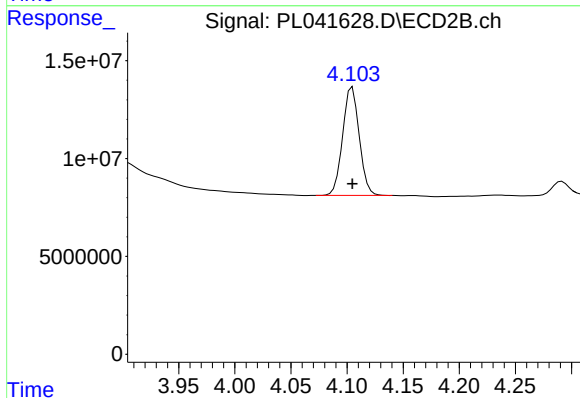


#1 Tetrachloro-m-xylene

R.T.: 4.105 min
Delta R.T.: 0.000 min
Response: 56966063
Conc: 18.49 ng/ml

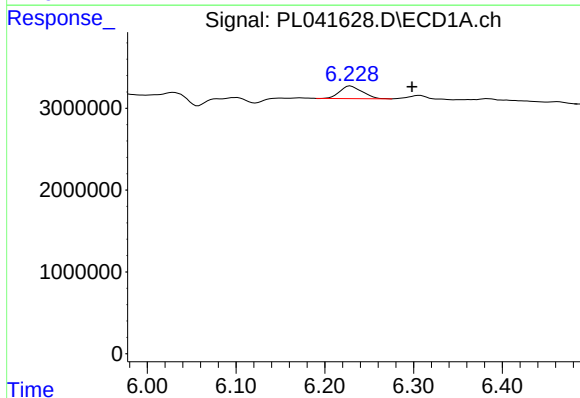


#15 Endosulfan II

R.T.: 6.229 min
Delta R.T.: -0.069 min
Response: 2685153
Conc: 0.39 ng/ml

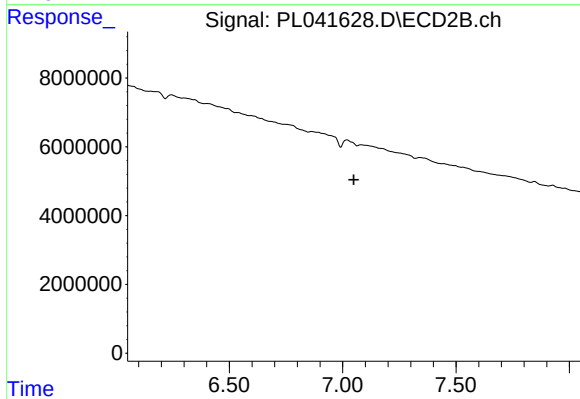

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 7.048 min
Response: 0
Conc: N.D.

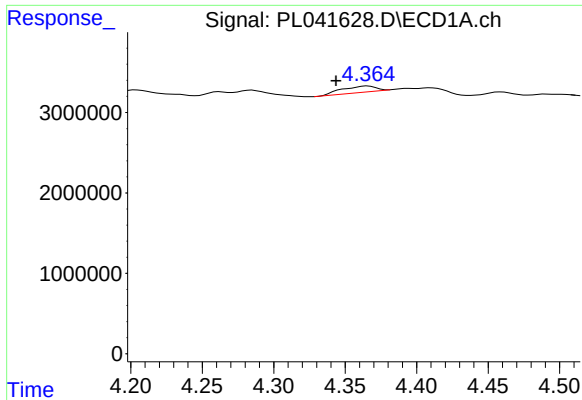

#23 Chlordane-1


R.T.: 4.366 min
Delta R.T.: 0.022 min
Response: 1283000
Conc: 4.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

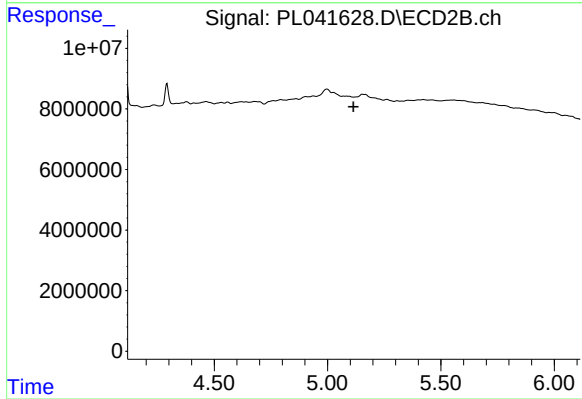


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.115 min
Response: 0
Conc: N.D.

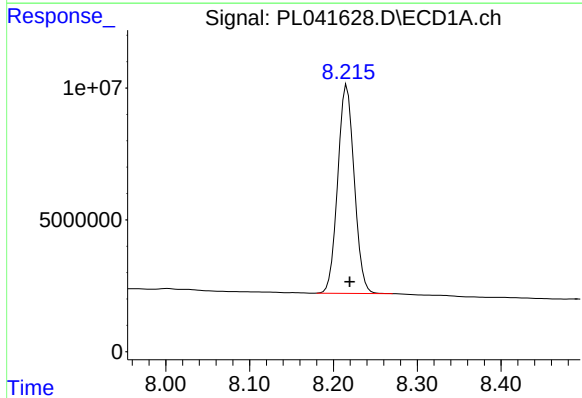

#28 Decachlorobiphenyl

R.T.: 8.216 min
Delta R.T.: -0.003 min
Response: 107952492
Conc: 16.30 ng/ml

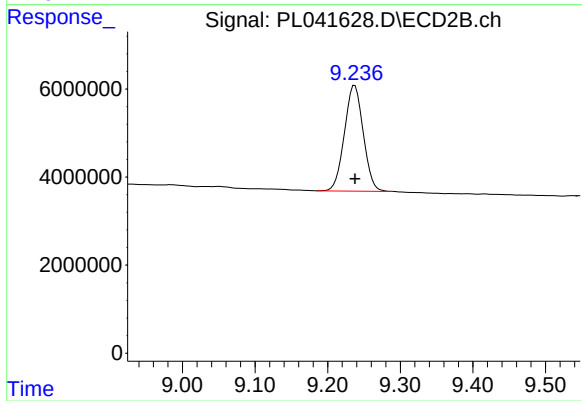

#28 Decachlorobiphenyl

R.T.: 9.237 min
Delta R.T.: 0.000 min
Response: 43293253
Conc: 16.90 ng/ml