Quantitation Report (Not Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110118\
Data File : PL041631.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2018 17:41
Operator : AJ\SJ
Sample : J5741-23
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 01:10:35 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	
	System Monitoring Compounds							
1)	SA Tetrachlo...	3.472	4.105	108.7E6	54120791	17.062	17.570	
28)	SA Decachlor...	8.216	9.237	107.2E6	41492970	16.188	16.195	
	Target Compounds							
15)	B Endosulfa...	6.229f	0.000	2799553	0	0.405	N.D.	#
23)	Chlordane-1	4.364	0.000	831621	0	2.933	N.D.	#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110118\
Data File : PL041631.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2018 17:41
Operator : AJ\SJ
Sample : J5741-23
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 01:10:35 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

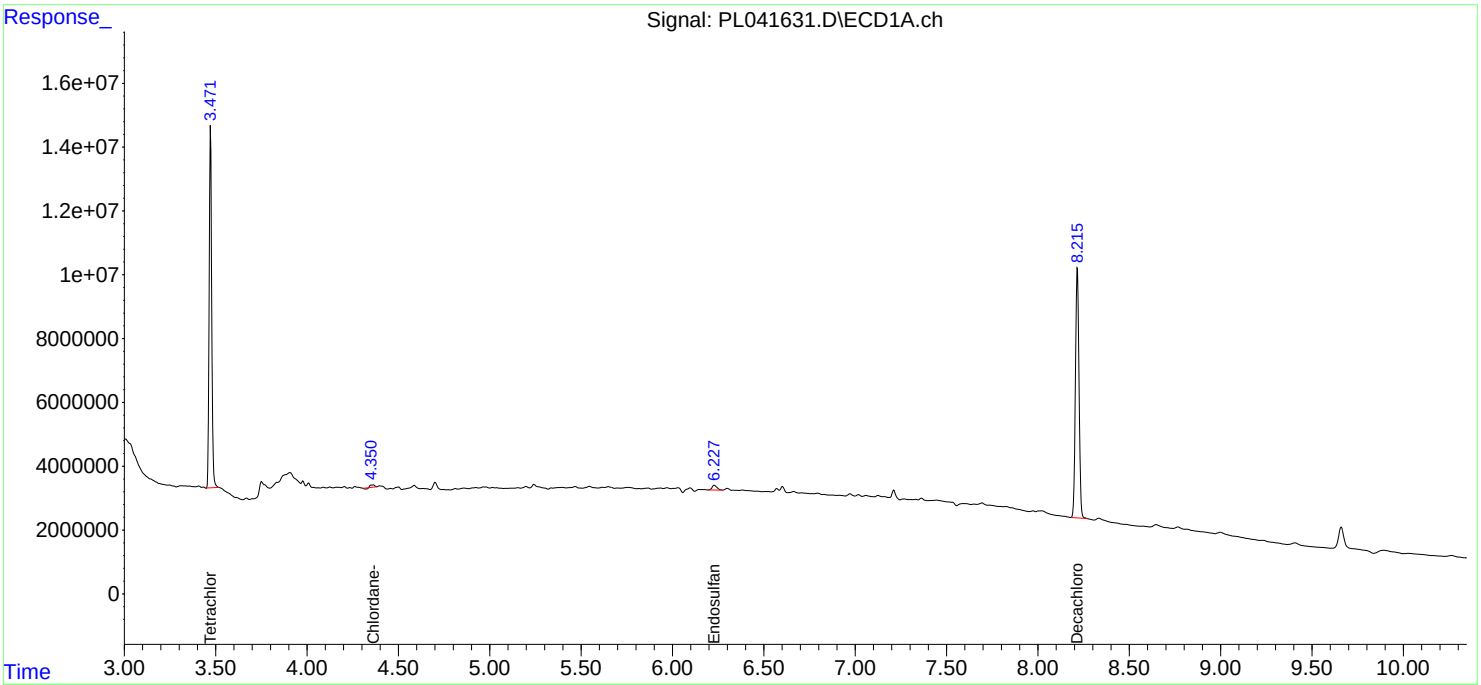

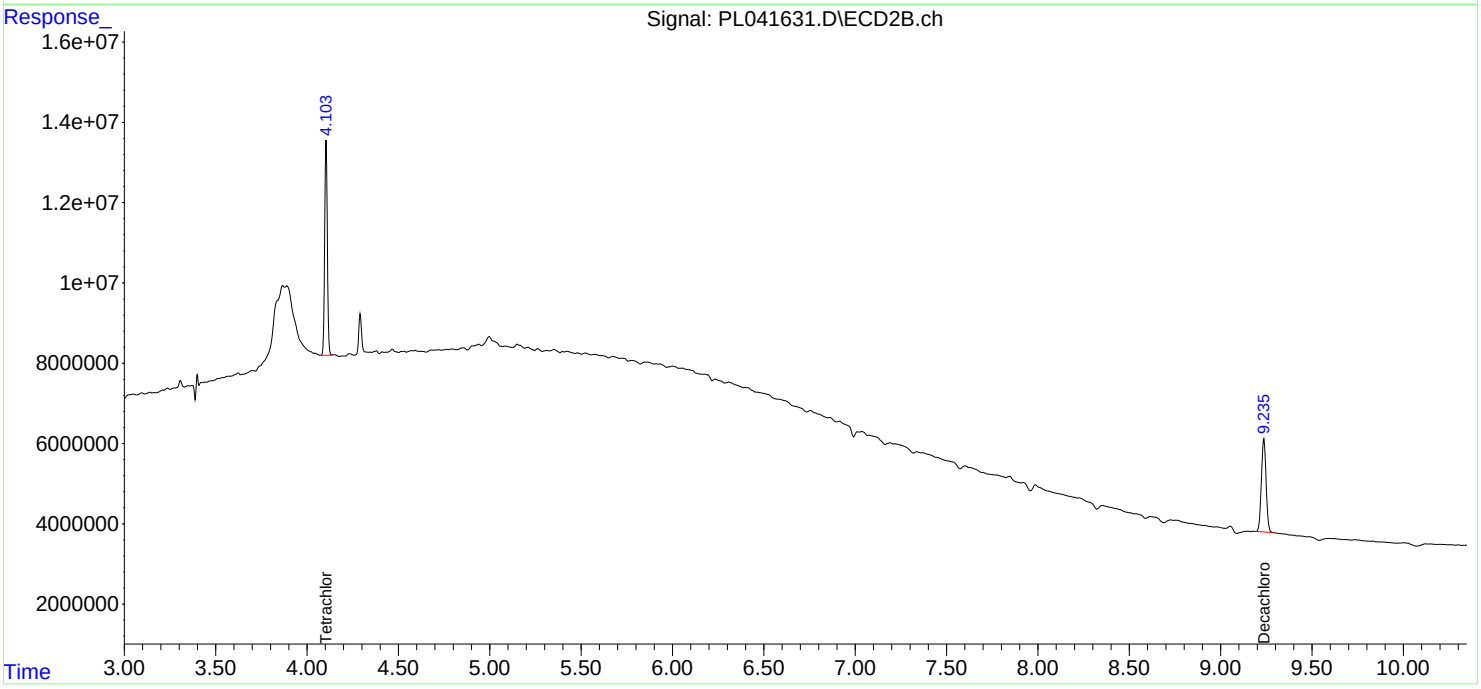

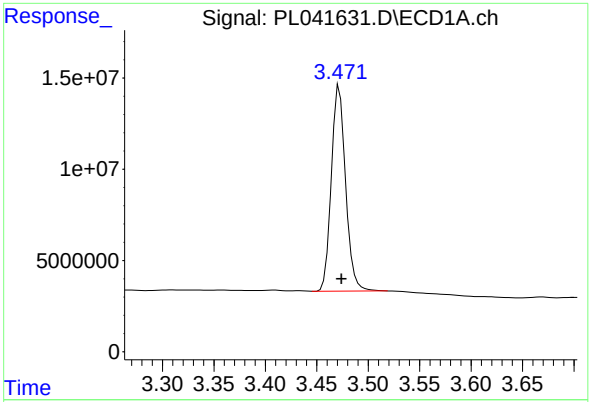

#1 Tetrachloro-m-xylene

R.T.: 3.472 min
Delta R.T.: -0.002 min
Response: 108688393
Conc: 17.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

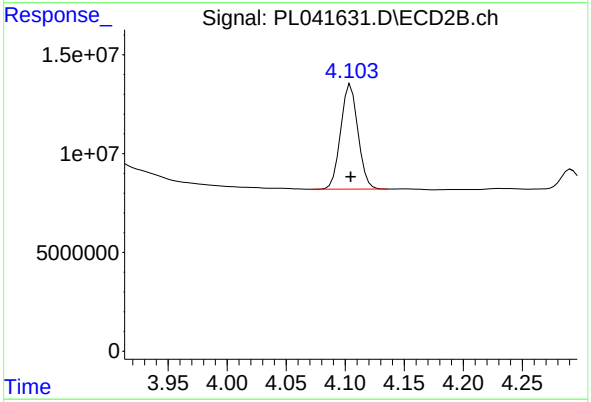

#1 Tetrachloro-m-xylene

R.T.: 4.105 min
Delta R.T.: 0.000 min
Response: 54120791
Conc: 17.57 ng/ml

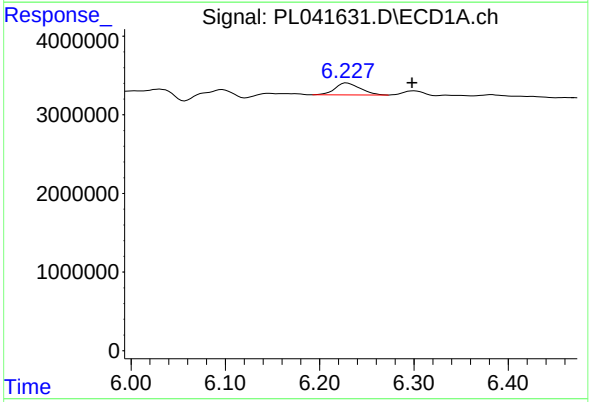

#15 Endosulfan II

R.T.: 6.229 min
Delta R.T.: -0.069 min
Response: 2799553
Conc: 0.41 ng/ml

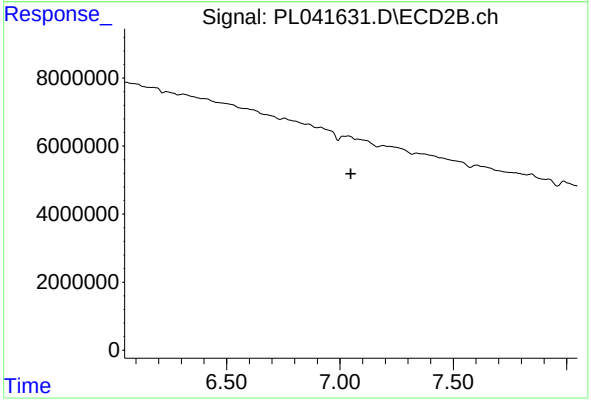

#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 7.048 min
Response: 0
Conc: N.D.

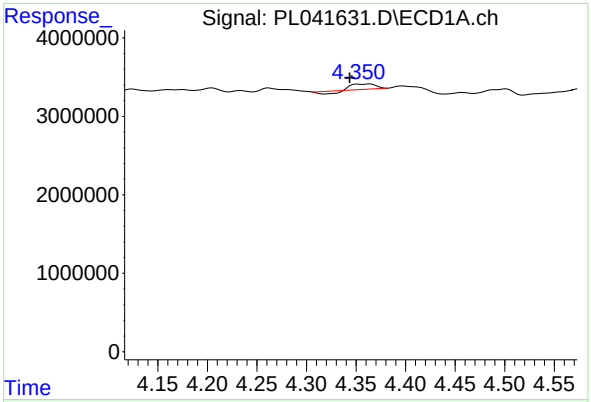

#23 Chlordane-1

R.T.: 4.364 min
Delta R.T.: 0.020 min
Response: 831621
Conc: 2.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

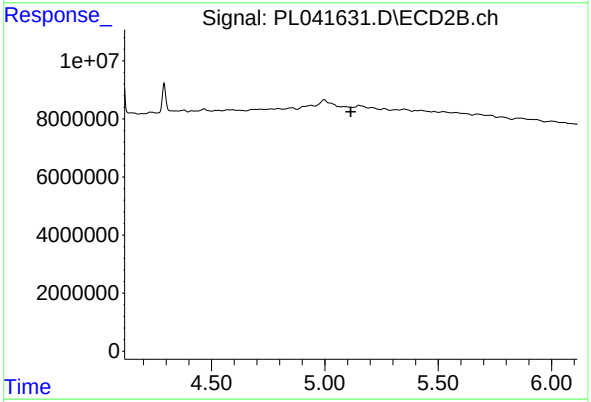

#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.115 min
Response: 0
Conc: N.D.

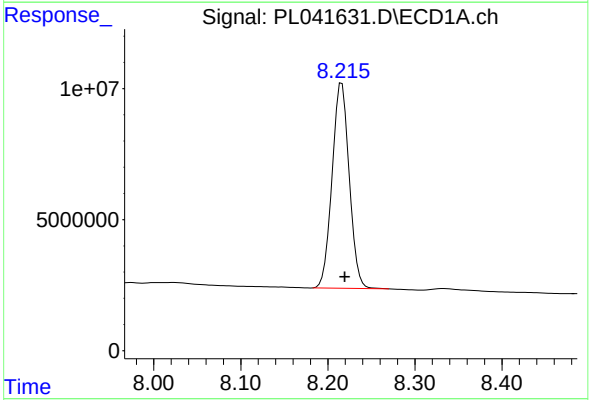

#28 Decachlorobiphenyl

R.T.: 8.216 min
Delta R.T.: -0.003 min
Response: 107227946
Conc: 16.19 ng/ml

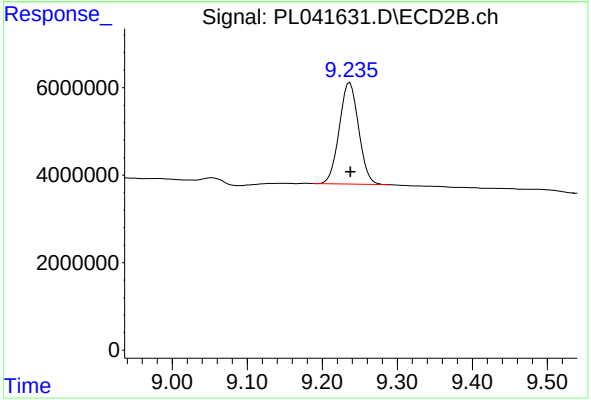

#28 Decachlorobiphenyl

R.T.: 9.237 min
Delta R.T.: 0.000 min
Response: 41492970
Conc: 16.19 ng/ml