

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110118\
 Data File : PL041668.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2018 02:37
 Operator : AJ\SJ
 Sample : J5200-20
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 03:02:37 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.473	4.105	122.4E6	63044589	19.208	20.468
28)	SA Decachlor...	8.217	9.239	117.4E6	49253452	17.728	19.223
Target Compounds							
2)	A alpha-BHC	3.868f	0.000	1318903	0	0.136	N.D. #
3)	MA gamma-BHC...	4.205	0.000	4151139	0	0.465	N.D. #
6)	B beta-BHC	4.409f	0.000	3802161	0	1.009	N.D. #
7)	B delta-BHC	0.000	5.152f	0	1880408	N.D.	0.466 #
8)	B Heptachlo...	5.251f	0.000	942138	0	0.117	N.D. #
9)	A Endosulfan I	5.549	0.000	1830762	0	0.246	N.D. #
13)	MA Dieldrin	5.747	0.000	4668644	0	0.587	N.D. #
16)	A 4,4'-DDD	6.107f	0.000	103996	0	0.018	N.D. #
23)	Chlordane-1	4.348	5.152	1507199	1880408	5.316	13.539 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110118\
Data File : PL041668.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2018 02:37
Operator : AJ\SJ
Sample : J5200-20
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 03:02:37 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

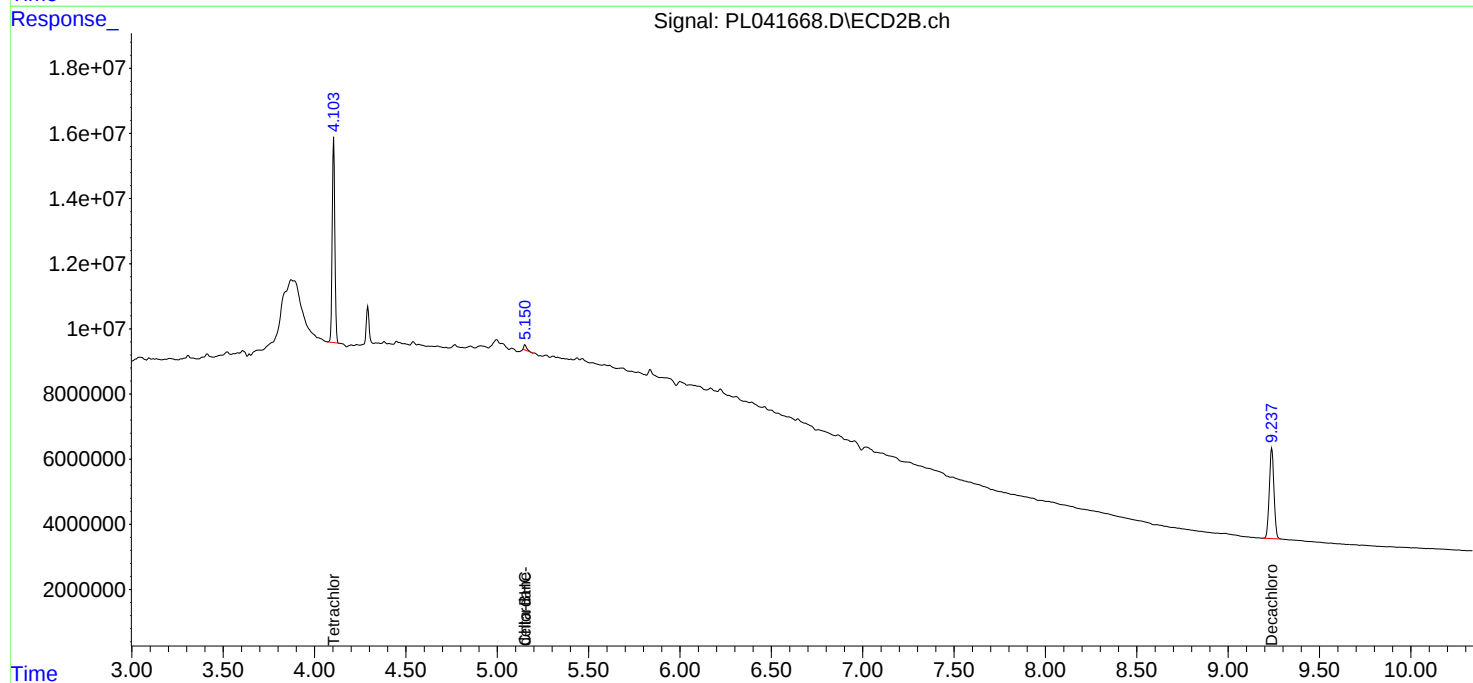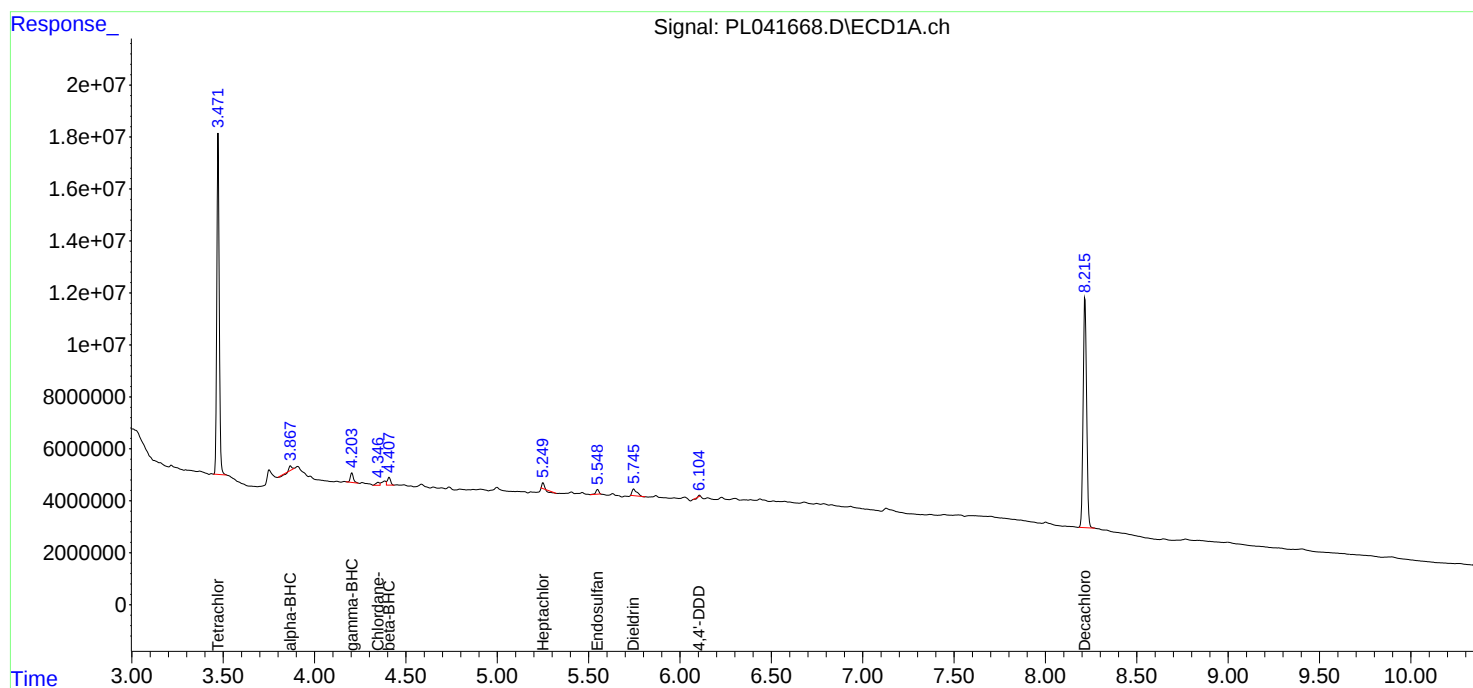


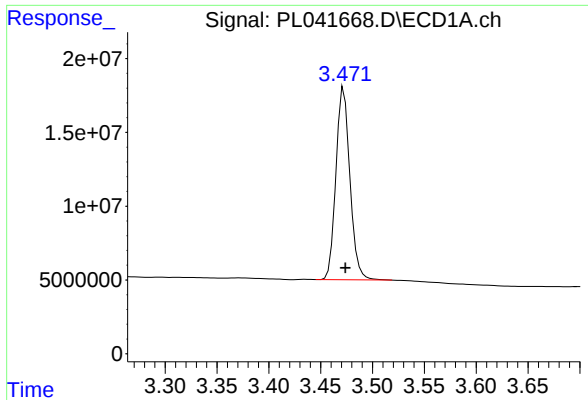

#1 Tetrachloro-m-xylene


R.T.: 3.473 min
Delta R.T.: -0.001 min
Response: 122359863
Conc: 19.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

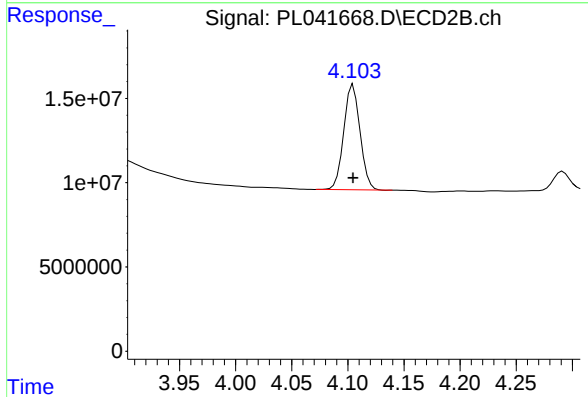


#1 Tetrachloro-m-xylene

R.T.: 4.105 min
Delta R.T.: 0.000 min
Response: 63044589
Conc: 20.47 ng/ml

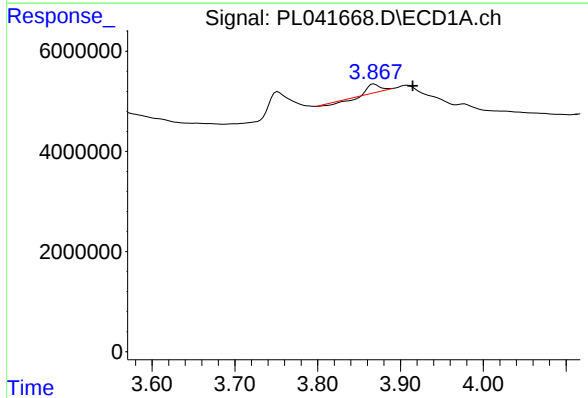


#2 alpha-BHC

R.T.: 3.868 min
Delta R.T.: -0.047 min
Response: 1318903
Conc: 0.14 ng/ml

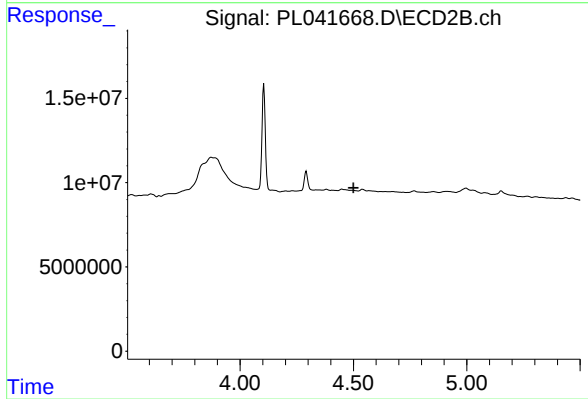

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.501 min
Response: 0
Conc: N.D.

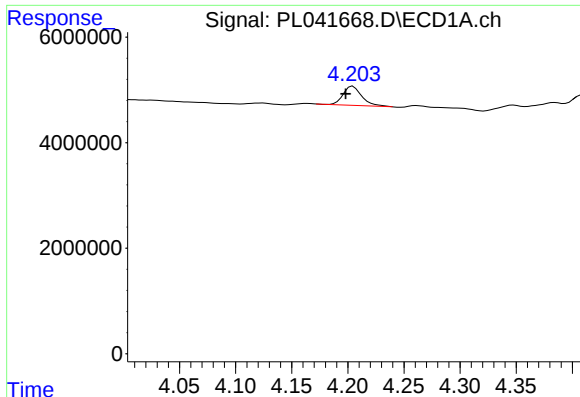

#3 gamma-BHC (Lindane)


R.T.: 4.205 min
Delta R.T.: 0.006 min
Response: 4151139
Conc: 0.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

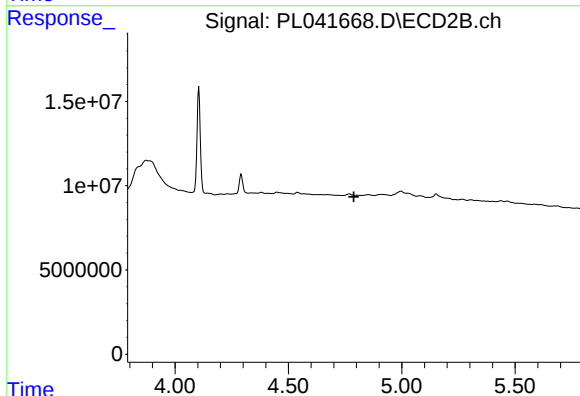


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.789 min
Response: 0
Conc: N.D.

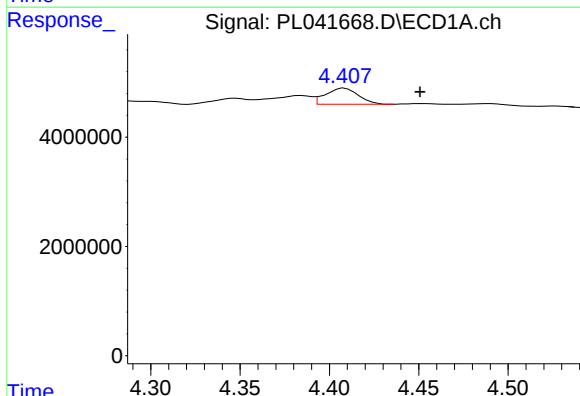


#6 beta-BHC

R.T.: 4.409 min
Delta R.T.: -0.042 min
Response: 3802161
Conc: 1.01 ng/ml

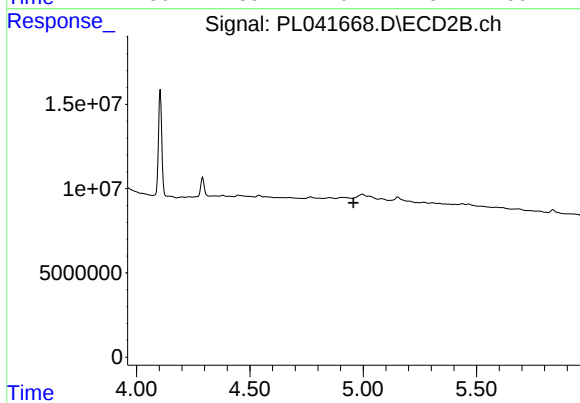

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.957 min
Response: 0
Conc: N.D.

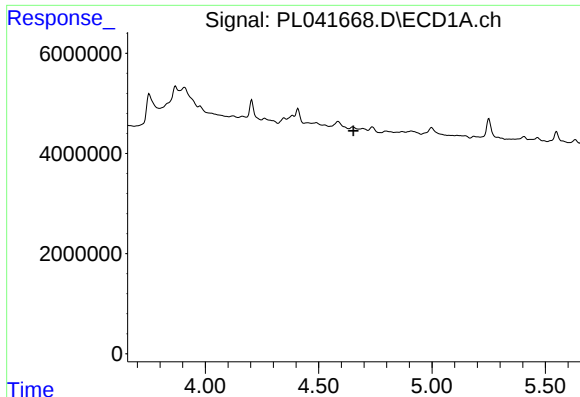

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.654 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

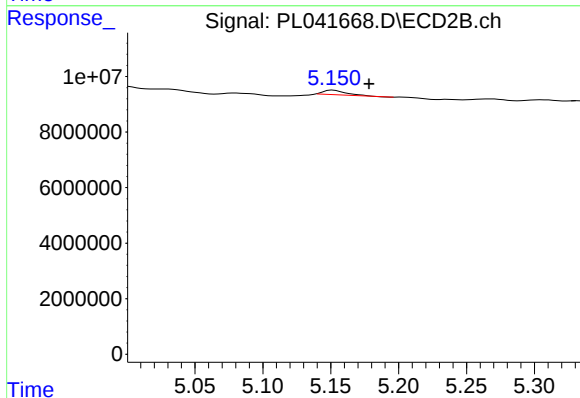


#7 delta-BHC

R.T.: 5.152 min
Delta R.T.: -0.026 min
Response: 1880408
Conc: 0.47 ng/ml

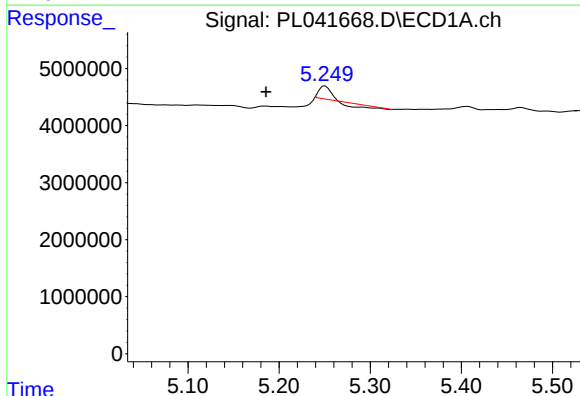


#8 Heptachlor epoxide

R.T.: 5.251 min
Delta R.T.: 0.065 min
Response: 942138
Conc: 0.12 ng/ml

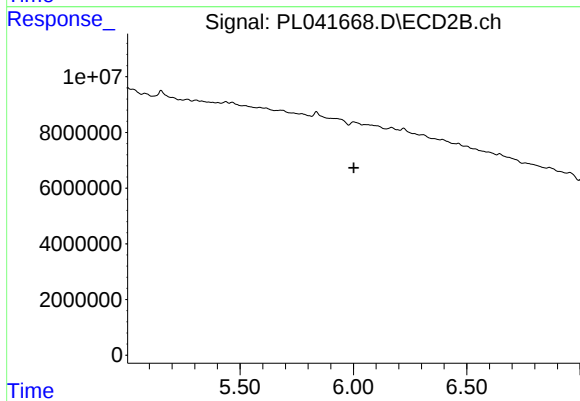

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 6.002 min
Response: 0
Conc: N.D.

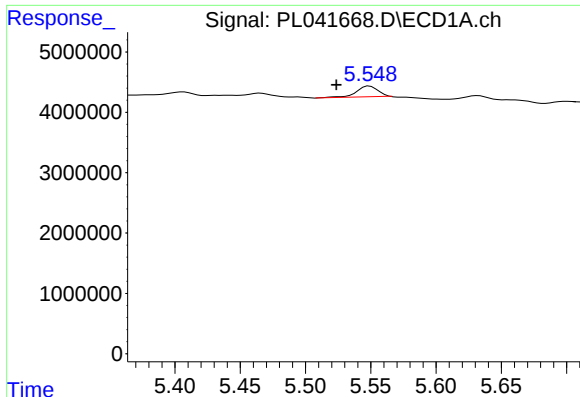

#9 Endosulfan I


R.T.: 5.549 min
Delta R.T.: 0.026 min
Response: 1830762
Conc: 0.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

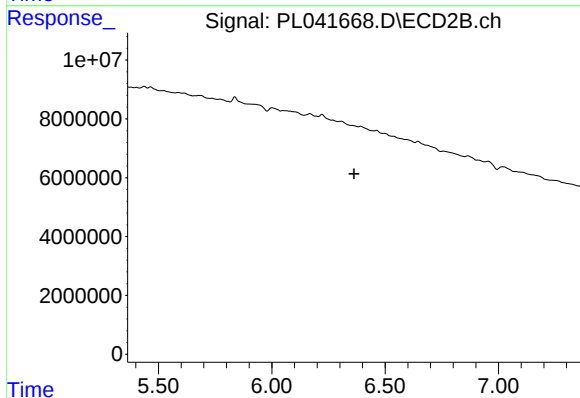


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

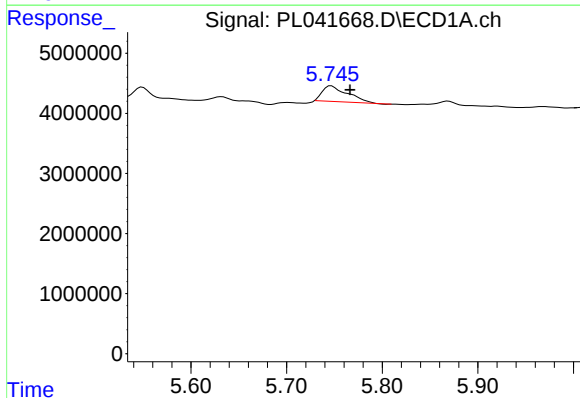


#13 Dieldrin

R.T.: 5.747 min
Delta R.T.: -0.020 min
Response: 4668644
Conc: 0.59 ng/ml

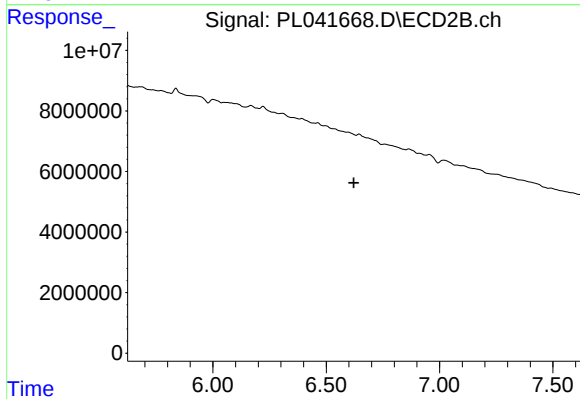

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.621 min
Response: 0
Conc: N.D.

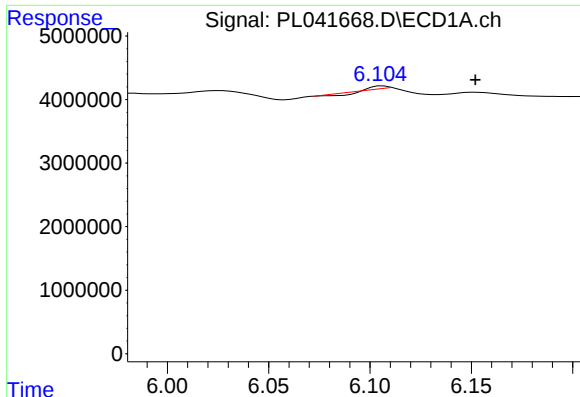

#16 4,4'-DDD


R.T.: 6.107 min
Delta R.T.: -0.045 min
Response: 103996
Conc: 0.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

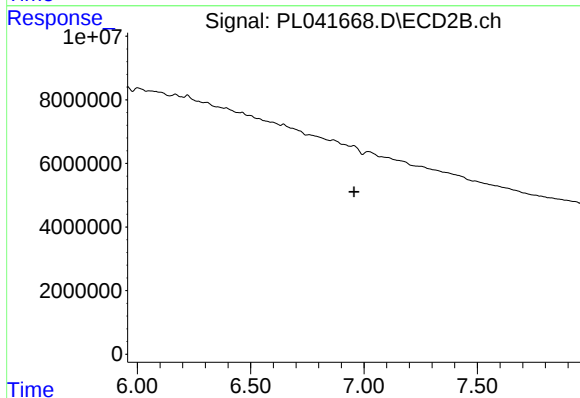


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.957 min
Response: 0
Conc: N.D.

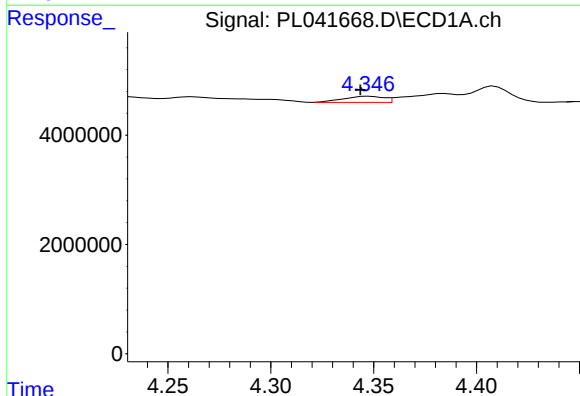


#23 Chlordane-1

R.T.: 4.348 min
Delta R.T.: 0.004 min
Response: 1507199
Conc: 5.32 ng/ml

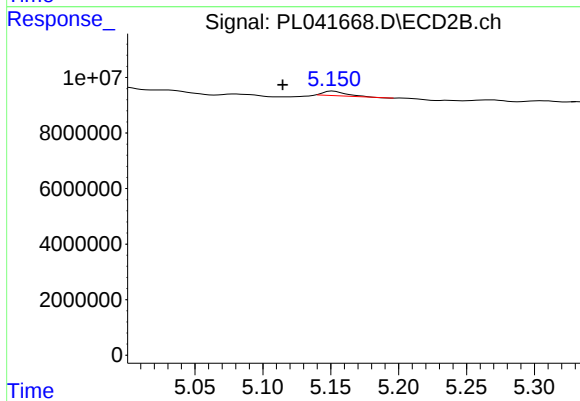

#23 Chlordane-1


R.T.: 5.152 min
Delta R.T.: 0.037 min
Response: 1880408
Conc: 13.54 ng/ml

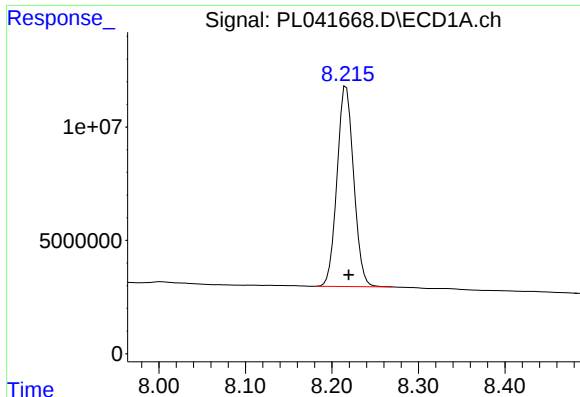

#28 Decachlorobiphenyl

R.T.: 8.217 min
Delta R.T.: -0.003 min
Response: 117432044
Conc: 17.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

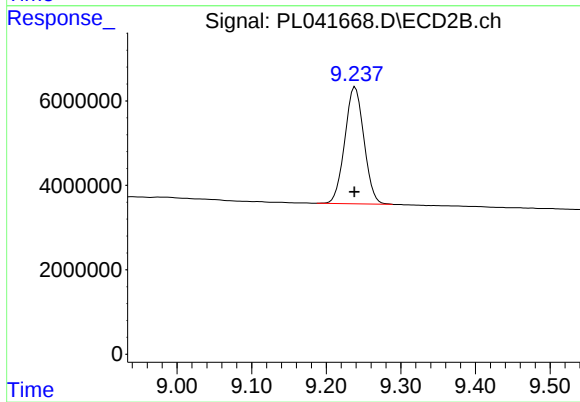

#28 Decachlorobiphenyl

R.T.: 9.239 min
Delta R.T.: 0.001 min
Response: 49253452
Conc: 19.22 ng/ml