

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110119\
 Data File : PL053988.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2019 09:00
 Operator : SG\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 22:34:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
4)	MA	Heptachlor	4.602f	0.000	5248008	0	0.333 N.D. #
8)	B	Heptachlo...	5.291	5.918	73038596	38354391	5.411 13.151 #
9)	A	Endosulfan I	5.634	0.000	58063806	0	4.724 N.D. #
10)	B	gamma-Chl...	5.513	0.000	95240081	0	6.981 N.D. #
12)	B	4,4'-DDE	5.757f	0.000	11957589	0	1.006 N.D. #
14)	MA	Endrin	6.131	6.751	23950192	7642283	2.066 3.149 #
15)	B	Endosulfa...	6.372f	0.000	10826262	0	0.968 N.D. #
17)	MA	4,4'-DDT	6.486	0.000	4430357	0	0.447 N.D. #
25)		Chlordane-3	5.513	0.000	95240081	0	82.624 N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110119\
Data File : PL053988.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2019 09:00
Operator : SG\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 22:34:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

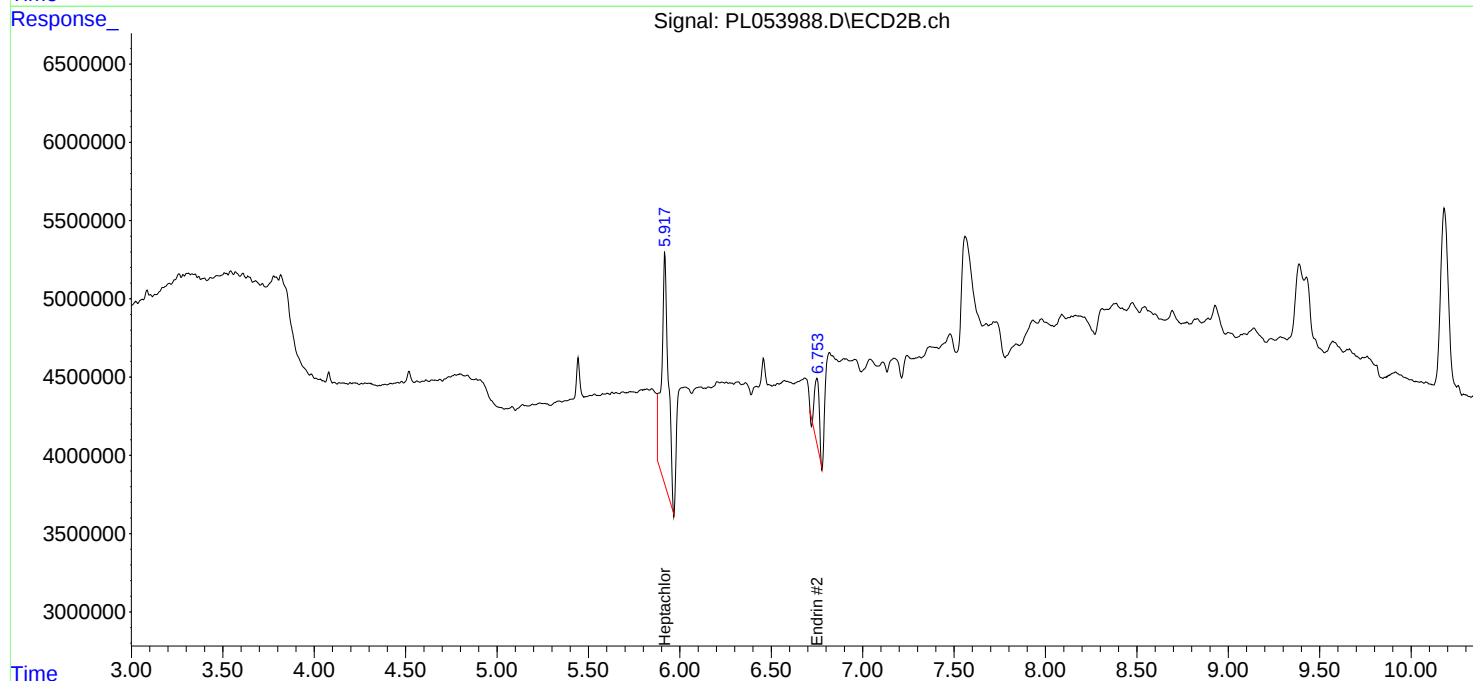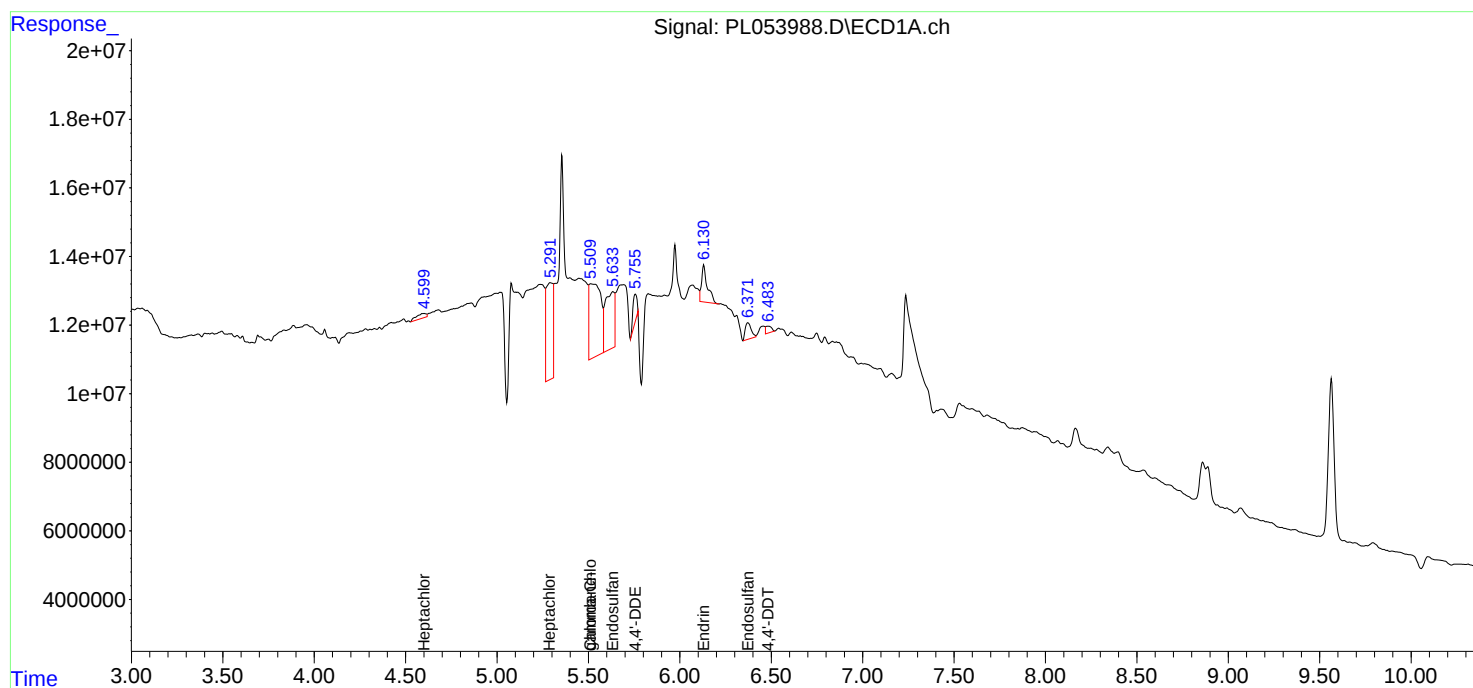


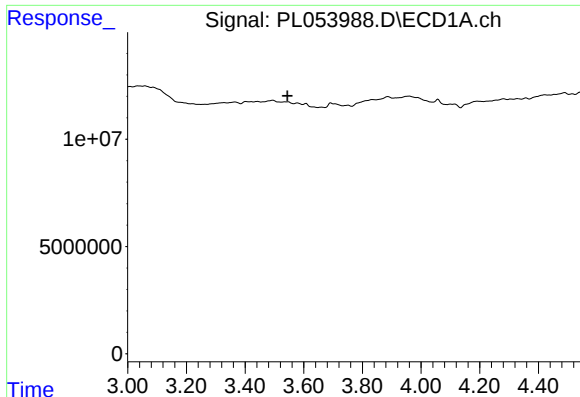

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.544 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

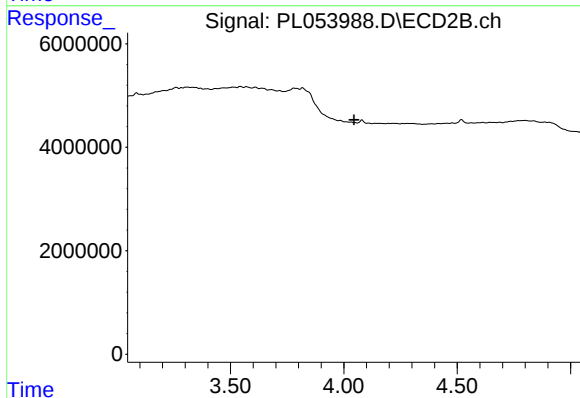


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 4.046 min
Response: 0
Conc: N.D.

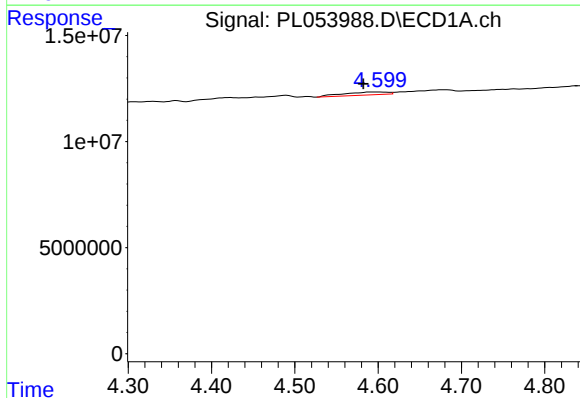


#4 Heptachlor

R.T.: 4.602 min
Delta R.T.: 0.019 min
Response: 5248008
Conc: 0.33 ng/ml

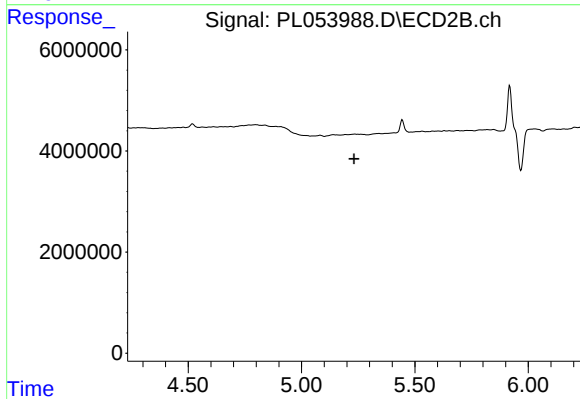

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.232 min
Response: 0
Conc: N.D.

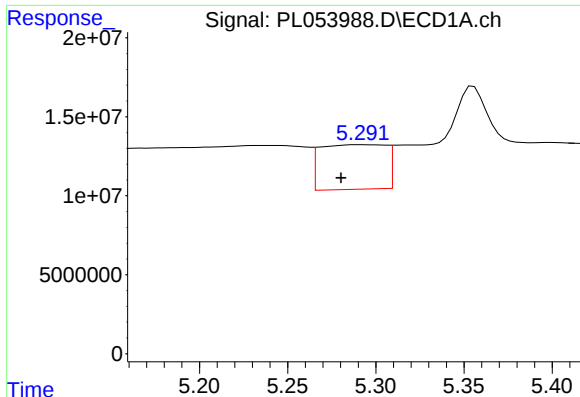

#8 Heptachlor epoxide


R.T.: 5.291 min
Delta R.T.: 0.011 min
Response: 73038596
Conc: 5.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

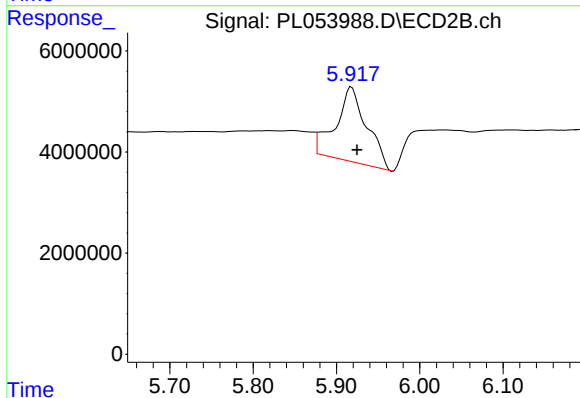


#8 Heptachlor epoxide

R.T.: 5.918 min
Delta R.T.: -0.006 min
Response: 38354391
Conc: 13.15 ng/ml

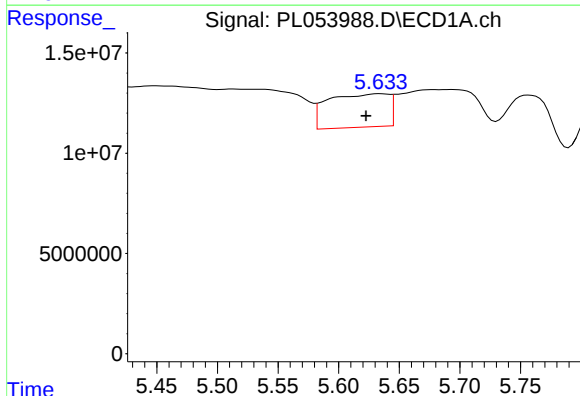


#9 Endosulfan I

R.T.: 5.634 min
Delta R.T.: 0.012 min
Response: 58063806
Conc: 4.72 ng/ml

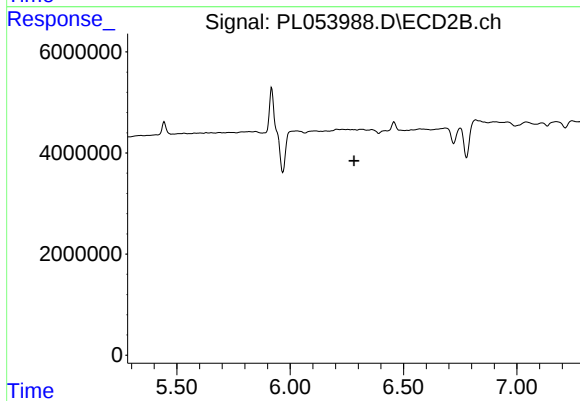

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.281 min
Response: 0
Conc: N.D.

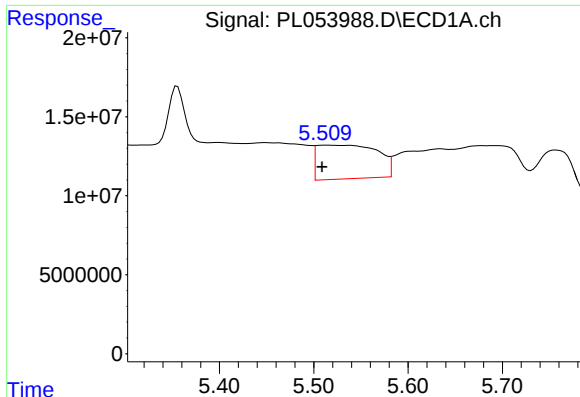

#10 gamma-Chlordane


R.T.: 5.513 min
Delta R.T.: 0.004 min
Response: 95240081
Conc: 6.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

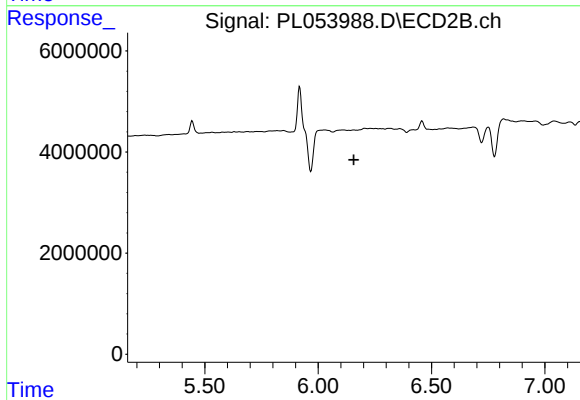


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.158 min
Response: 0
Conc: N.D.

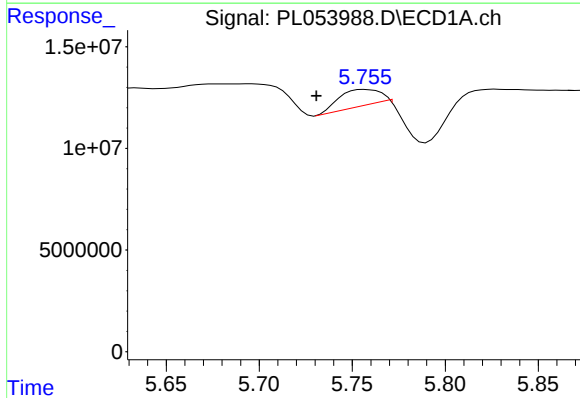


#12 4,4'-DDE

R.T.: 5.757 min
Delta R.T.: 0.026 min
Response: 11957589
Conc: 1.01 ng/ml

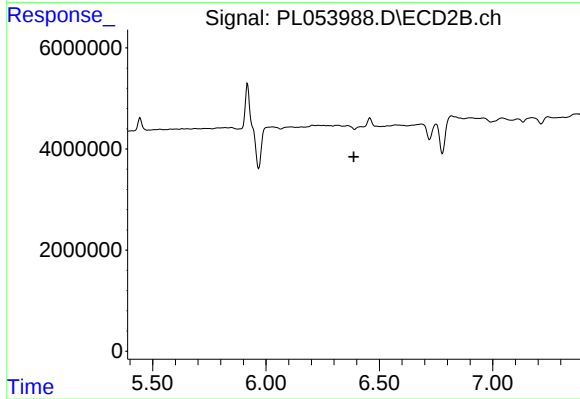

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.387 min
Response: 0
Conc: N.D.

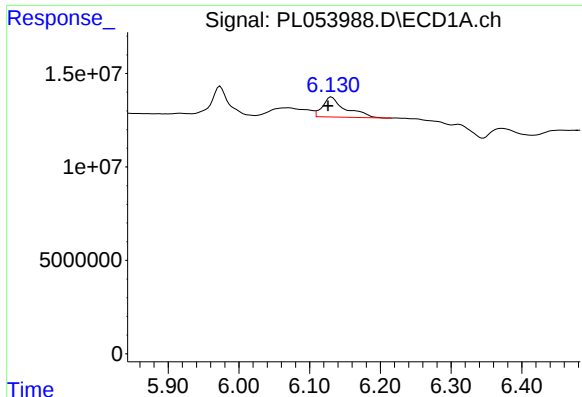

#14 Endrin


R.T.: 6.131 min
Delta R.T.: 0.005 min
Response: 23950192
Conc: 2.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

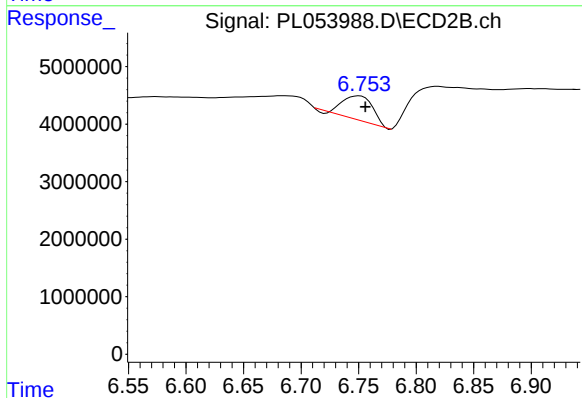


#14 Endrin

R.T.: 6.751 min
Delta R.T.: -0.005 min
Response: 7642283
Conc: 3.15 ng/ml

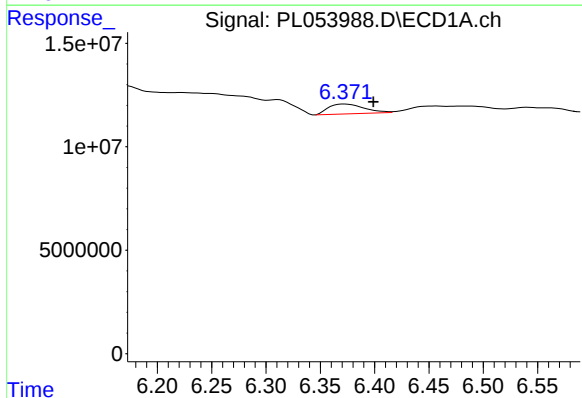


#15 Endosulfan II

R.T.: 6.372 min
Delta R.T.: -0.027 min
Response: 10826262
Conc: 0.97 ng/ml

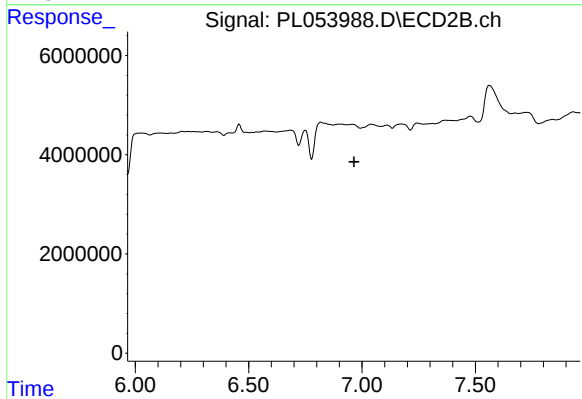

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.965 min
Response: 0
Conc: N.D.

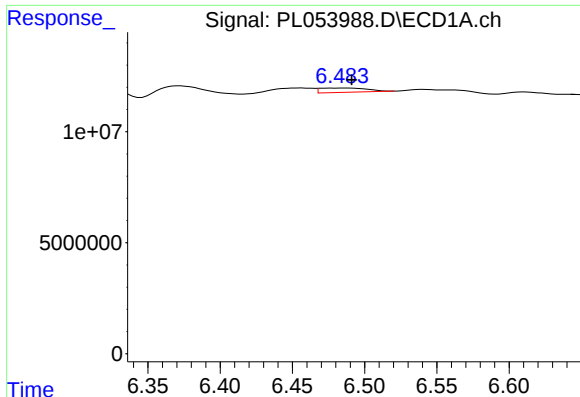

#17 4,4'-DDT


R.T.: 6.486 min
Delta R.T.: -0.005 min
Response: 4430357
Conc: 0.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

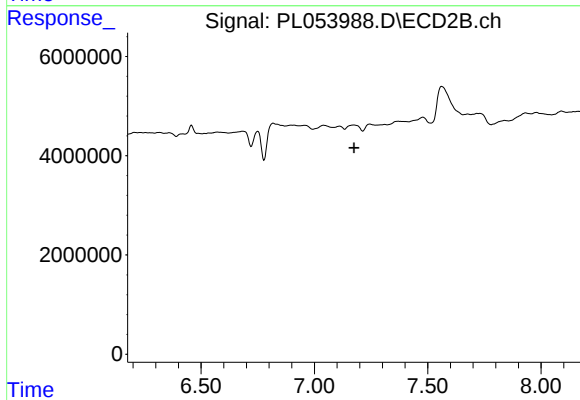


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.176 min
Response: 0
Conc: N.D.

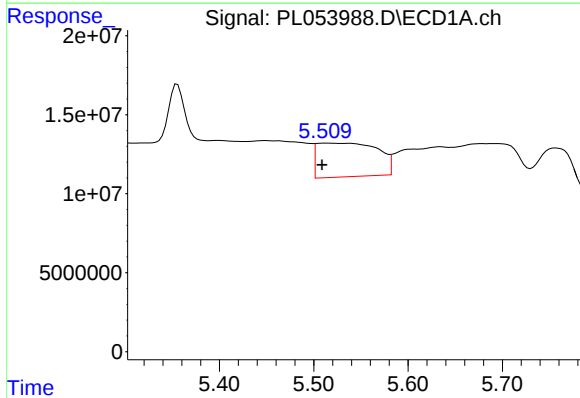


#25 Chlordane-3

R.T.: 5.513 min
Delta R.T.: 0.004 min
Response: 95240081
Conc: 82.62 ng/ml

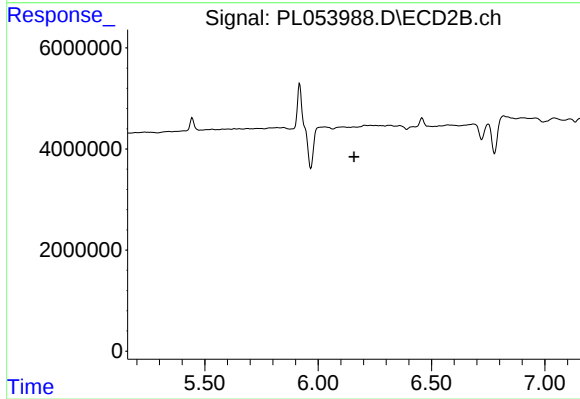

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.158 min
Response: 0
Conc: N.D.

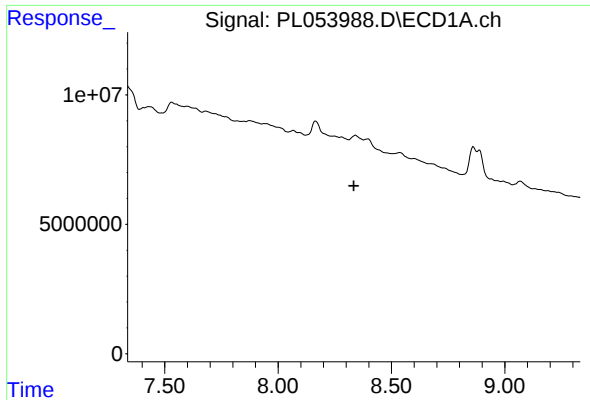

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.334 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

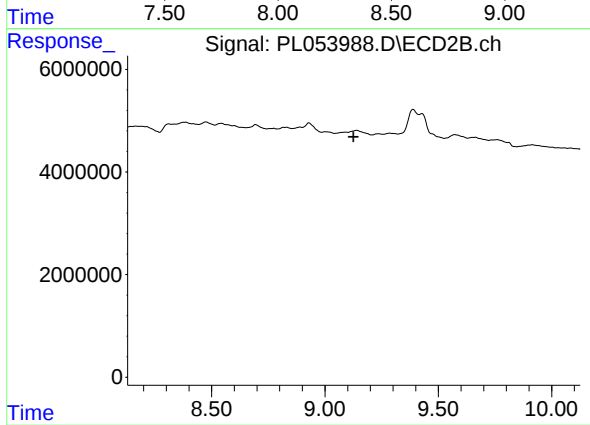

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.126 min
Response: 0
Conc: N.D.