

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110119\
 Data File : PL054001.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2019 14:29
 Operator : SG\AJ
 Sample : PB124489BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 22:37:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.548	4.045	193.3E6	46302811	17.834	18.503
28) SA Decachlor...	8.334	9.128	177.8E6	50904572	18.126	18.077
Target Compounds						
6) B beta-BHC	4.499f	0.000	9601034	0	1.457	N.D. #
23) Chlordane-1	0.000	5.032	0	3679986	N.D.	43.879 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110119\
Data File : PL054001.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2019 14:29
Operator : SG\AJ
Sample : PB124489BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 22:37:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

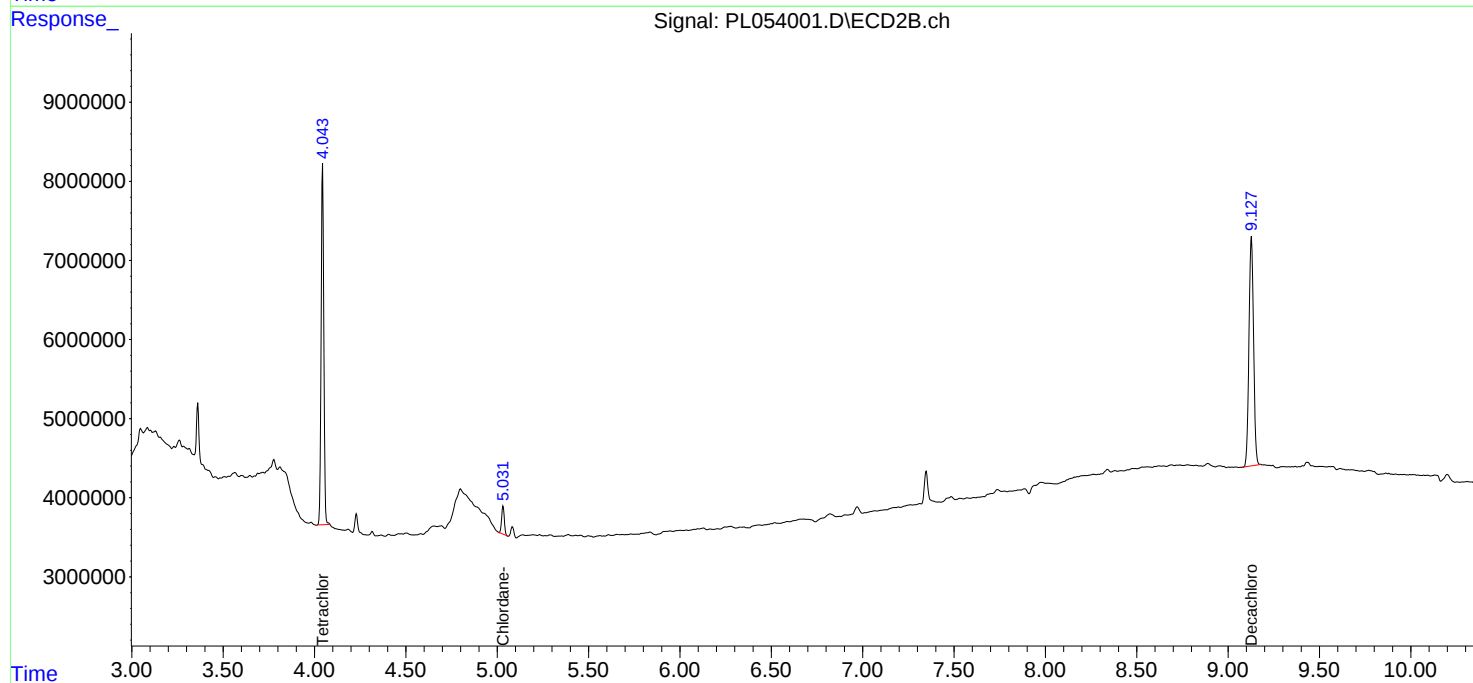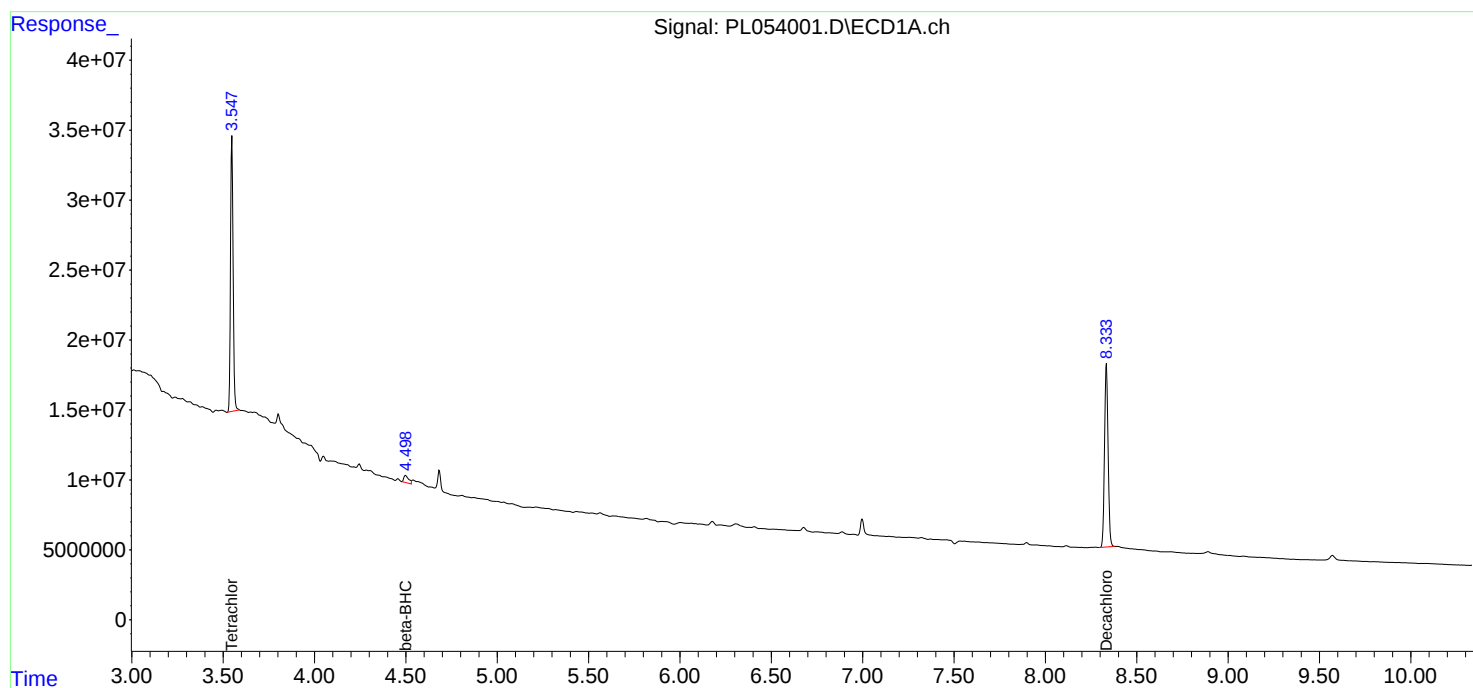


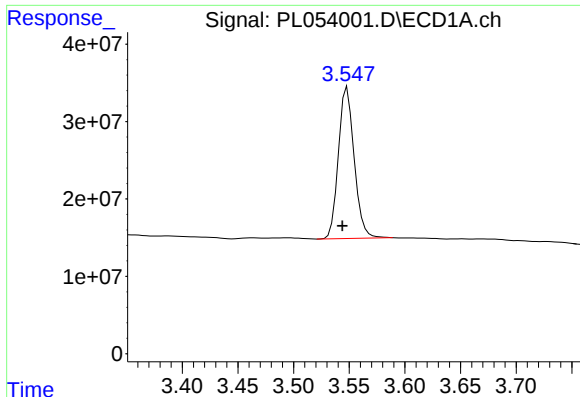

#1 Tetrachloro-m-xylene


R.T.: 3.548 min
Delta R.T.: 0.004 min
Response: 193312314
Conc: 17.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

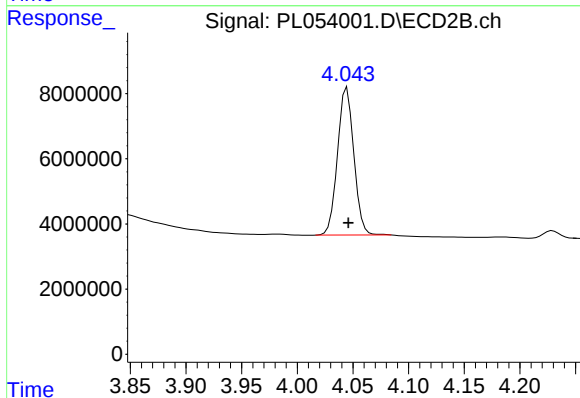


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: -0.001 min
Response: 46302811
Conc: 18.50 ng/ml

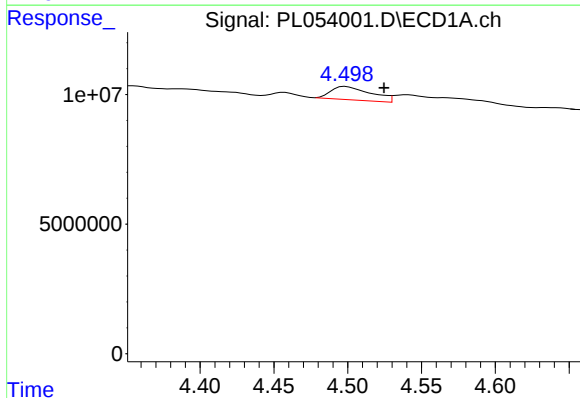


#6 beta-BHC

R.T.: 4.499 min
Delta R.T.: -0.026 min
Response: 9601034
Conc: 1.46 ng/ml

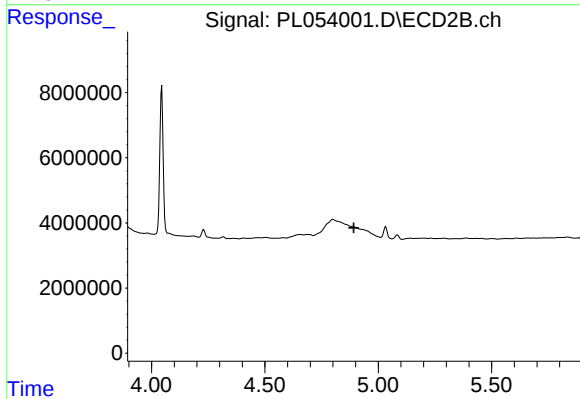

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.892 min
Response: 0
Conc: N.D.

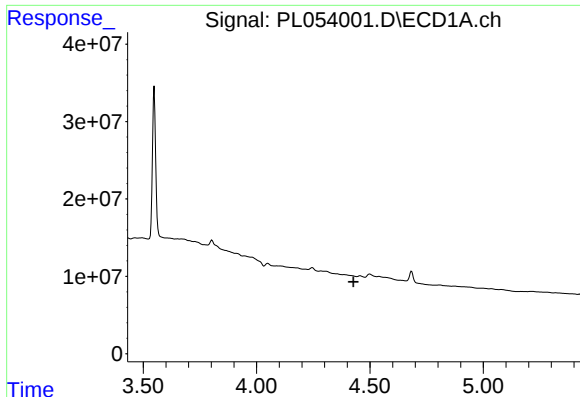

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.428 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

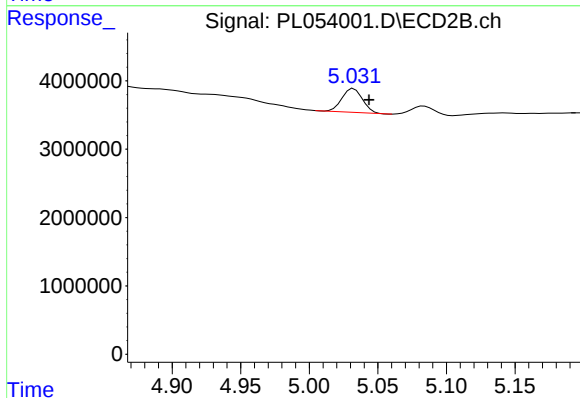


#23 Chlordane-1

R.T.: 5.032 min
Delta R.T.: -0.011 min
Response: 3679986
Conc: 43.88 ng/ml

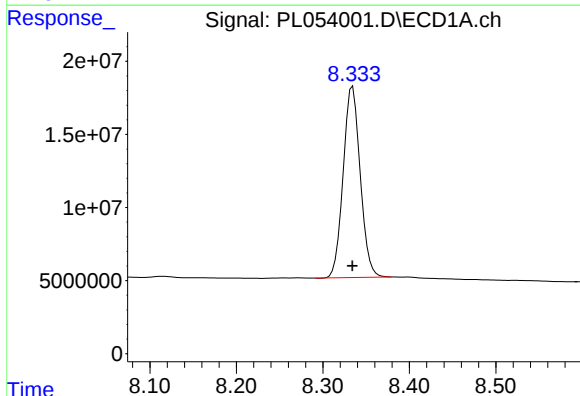

#28 Decachlorobiphenyl

R.T.: 8.334 min
Delta R.T.: 0.000 min
Response: 177841575
Conc: 18.13 ng/ml

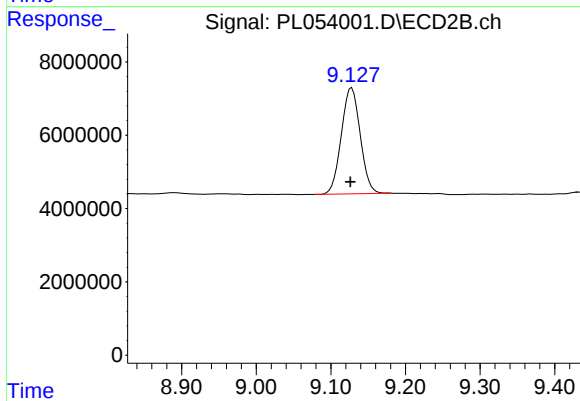

#28 Decachlorobiphenyl

R.T.: 9.128 min
Delta R.T.: 0.002 min
Response: 50904572
Conc: 18.08 ng/ml