

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110122\
 Data File : PL078695.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2022 14:02
 Operator : AR\AJ
 Sample : N5297-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BI-WEEKLY-DECANT

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/02/2022
 Supervised By :Ankita Jodhani 11/02/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 22:13:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:08:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.326	2.568	23704327	40915676	12.430	16.025 #
28) SA Decachlor...	8.775	7.635	27440844	28614560	18.241	15.107m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110122\
Data File : PL078695.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2022 14:02
Operator : AR\AJ
Sample : N5297-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-DECANT


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/02/2022
Supervised By : Ankita Jodhani 11/02/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 22:13:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:08:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

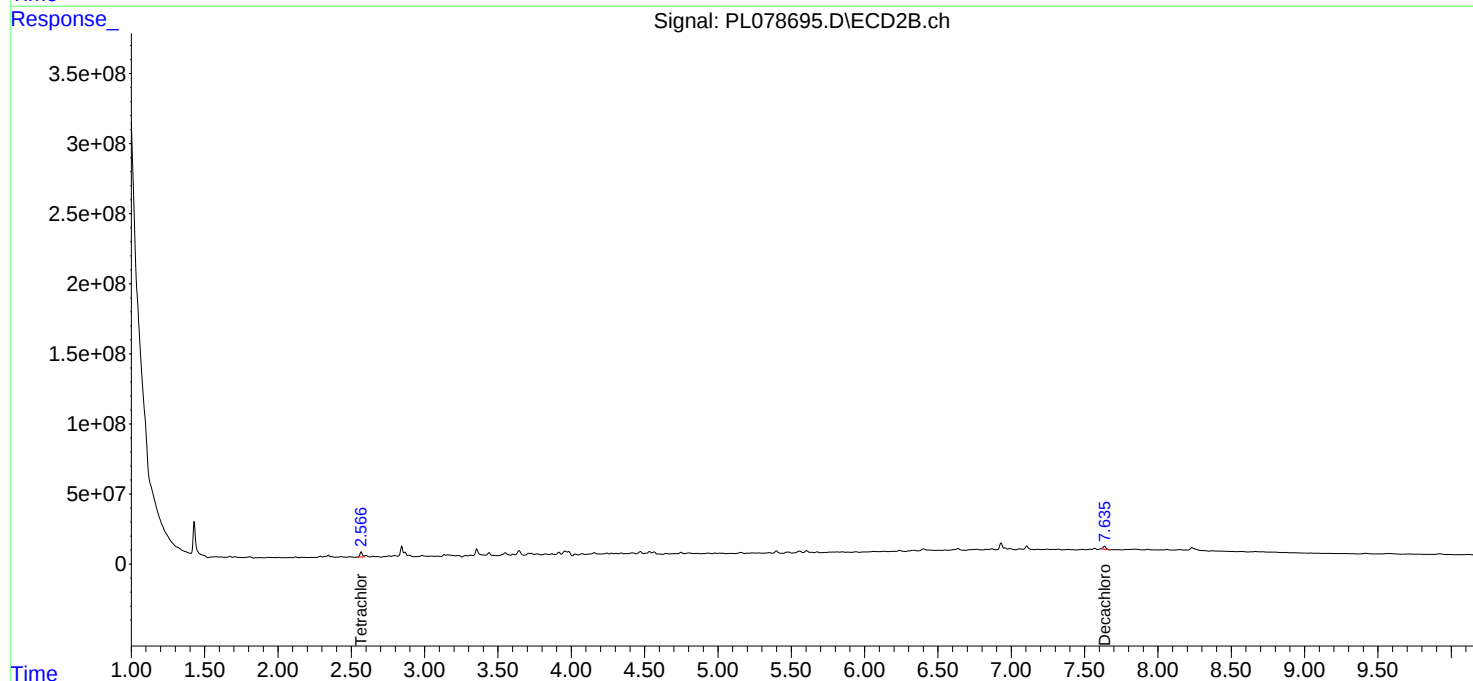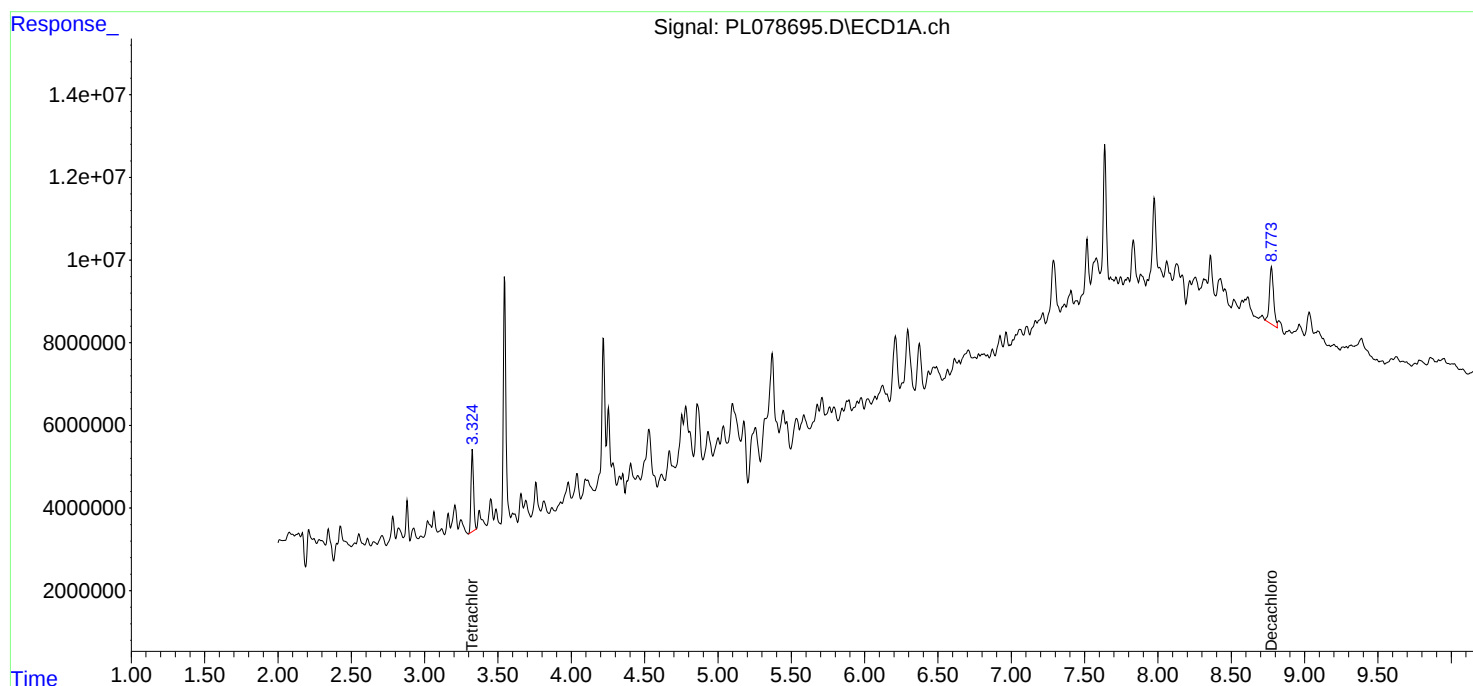

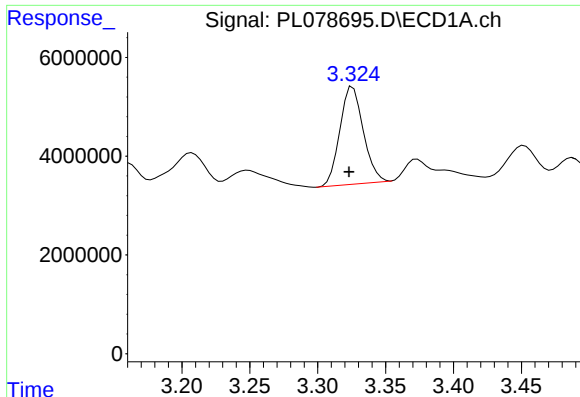


#1 Tetrachloro-m-xylene

R.T.: 3.326 min
Delta R.T.: 0.003 min
Response: 23704327
Conc: 12.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-DECANT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/02/2022
Supervised By :Ankita Jodhani 11/02/2022

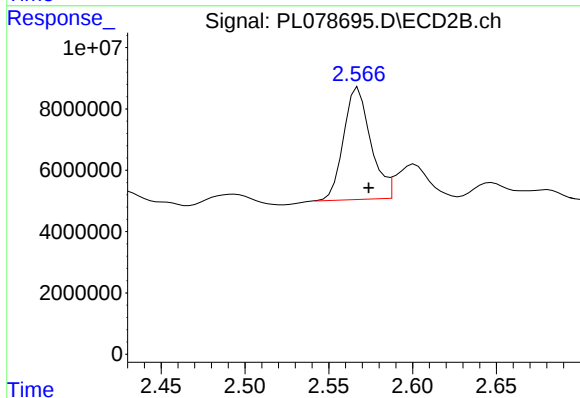


#1 Tetrachloro-m-xylene

R.T.: 2.568 min
Delta R.T.: -0.006 min
Response: 40915676
Conc: 16.03 ng/ml

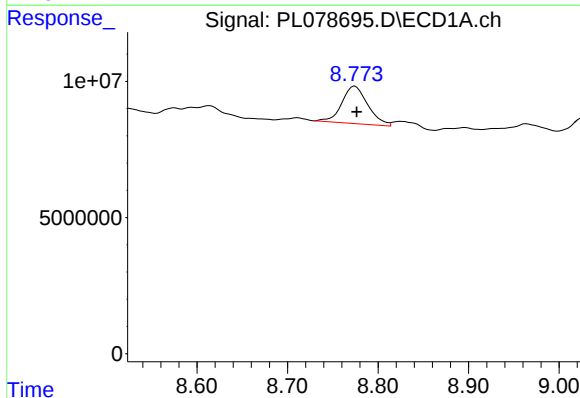

#28 Decachlorobiphenyl

R.T.: 8.775 min
Delta R.T.: -0.002 min
Response: 27440844
Conc: 18.24 ng/ml

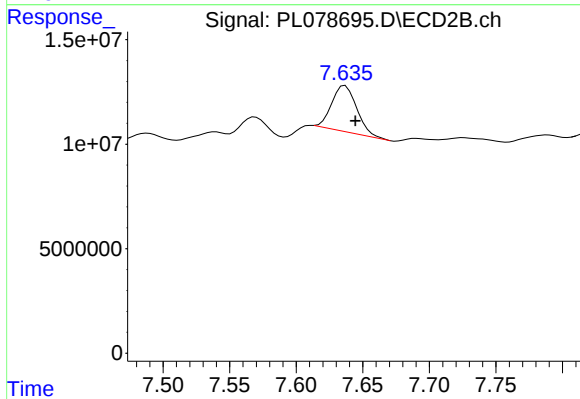

#28 Decachlorobiphenyl

R.T.: 7.635 min
Delta R.T.: -0.009 min
Response: 28614560
Conc: 15.11 ng/ml m