

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110123\
 Data File : PL086352.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2023 10:54
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 01:59:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110123.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 02 01:55:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.352	2.617	16153395	5840518	5.321	5.030
28)	SA Decachlor...	8.853	7.769	14611104	6614721	5.926	5.990
Target Compounds							
23)	Chlordane-1	4.510	3.607	7350947	1823844	54.625	53.350
24)	Chlordane-2	5.042	4.184	8706923	2539828	59.541	57.234
25)	Chlordane-3	5.754	4.813	28403527	5547308	49.801	46.559
26)	Chlordane-4	5.837	4.876	36157795	6757258	51.393	51.561
27)	Chlordane-5	6.683	5.545	6061400	1732285	55.553	50.239


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110123\
Data File : PL086352.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2023 10:54
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 01:59:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110123.M
Quant Title : GC Extractables
QLast Update : Thu Nov 02 01:55:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

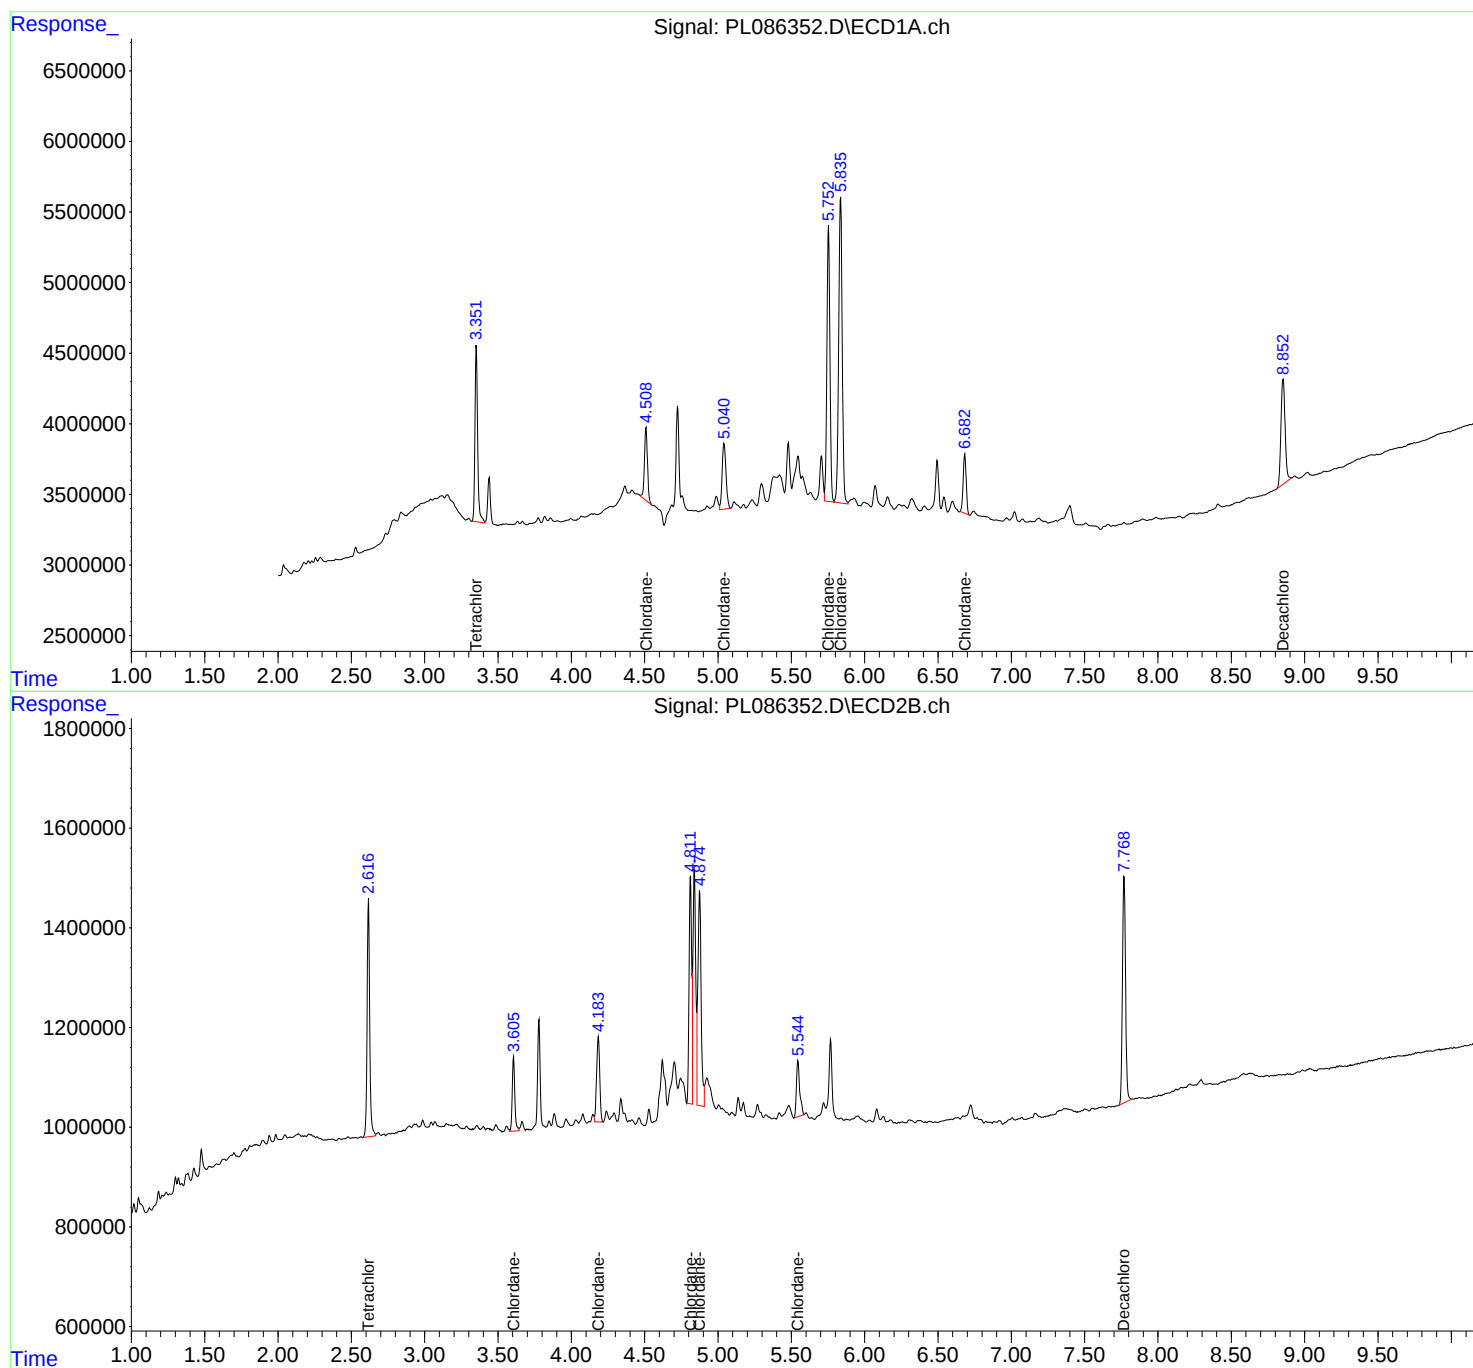


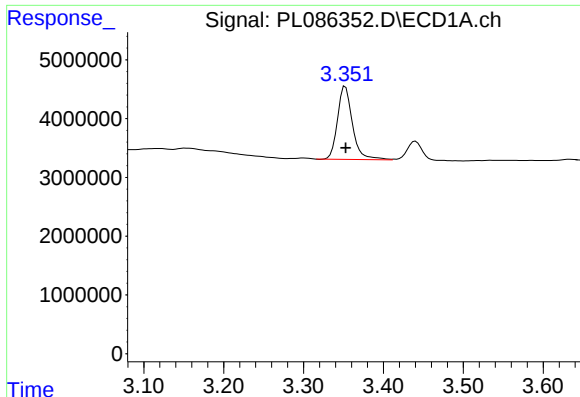

#1 Tetrachloro-m-xylene


R.T.: 3.352 min
Delta R.T.: 0.000 min
Response: 16153395
Conc: 5.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

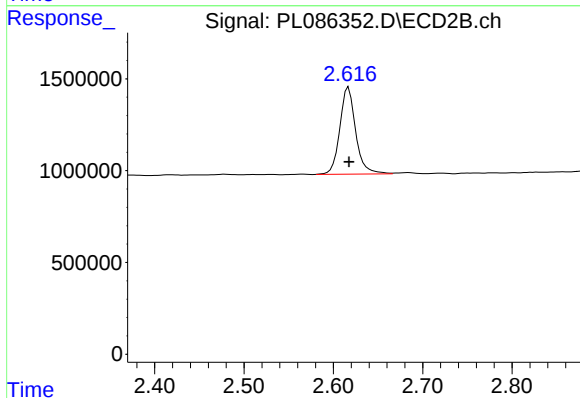


#1 Tetrachloro-m-xylene

R.T.: 2.617 min
Delta R.T.: 0.000 min
Response: 5840518
Conc: 5.03 ng/ml

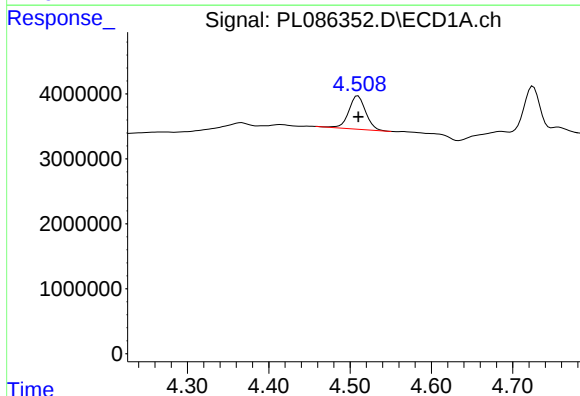


#23 Chlordane-1

R.T.: 4.510 min
Delta R.T.: 0.000 min
Response: 7350947
Conc: 54.62 ng/ml

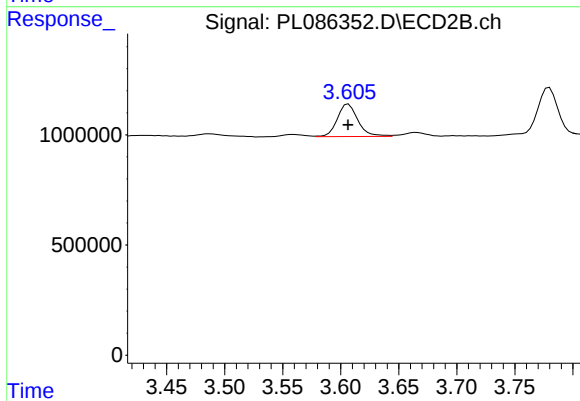

#23 Chlordane-1


R.T.: 3.607 min
Delta R.T.: 0.000 min
Response: 1823844
Conc: 53.35 ng/ml

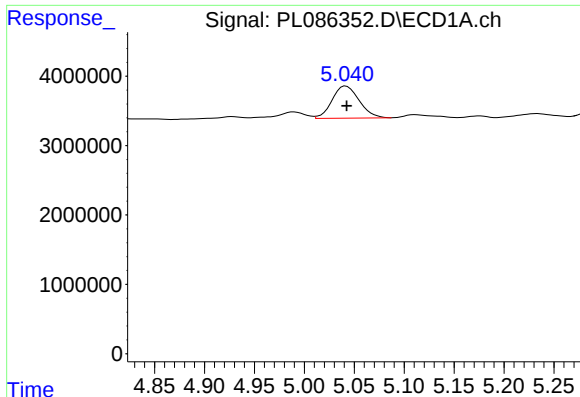

#24 Chlordane-2


R.T.: 5.042 min
Delta R.T.: 0.000 min
Response: 8706923
Conc: 59.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

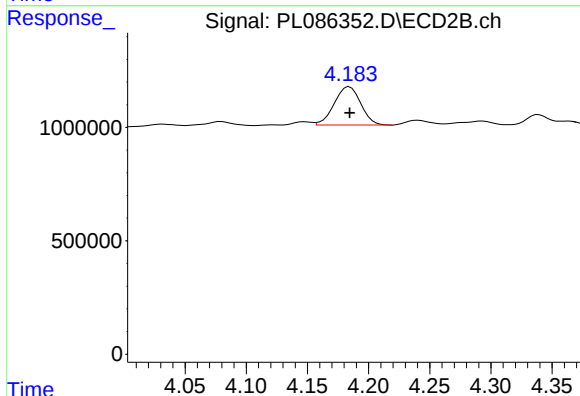


#24 Chlordane-2

R.T.: 4.184 min
Delta R.T.: 0.000 min
Response: 2539828
Conc: 57.23 ng/ml

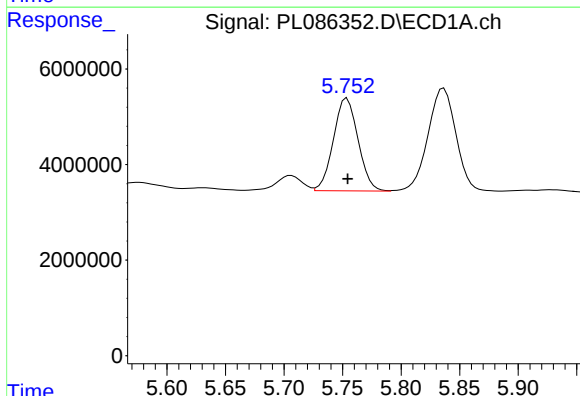


#25 Chlordane-3

R.T.: 5.754 min
Delta R.T.: 0.000 min
Response: 28403527
Conc: 49.80 ng/ml

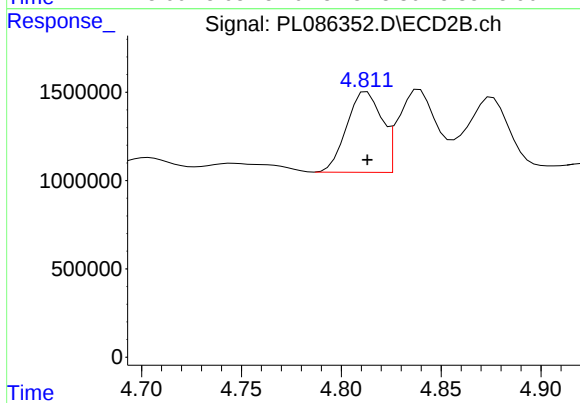

#25 Chlordane-3


R.T.: 4.813 min
Delta R.T.: 0.000 min
Response: 5547308
Conc: 46.56 ng/ml

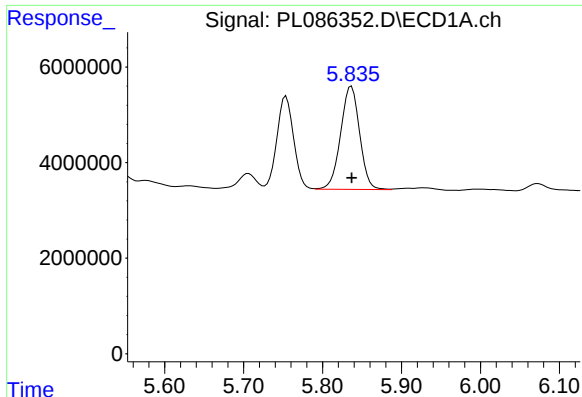

#26 Chlordane-4


R.T.: 5.837 min
Delta R.T.: 0.000 min
Response: 36157795
Conc: 51.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

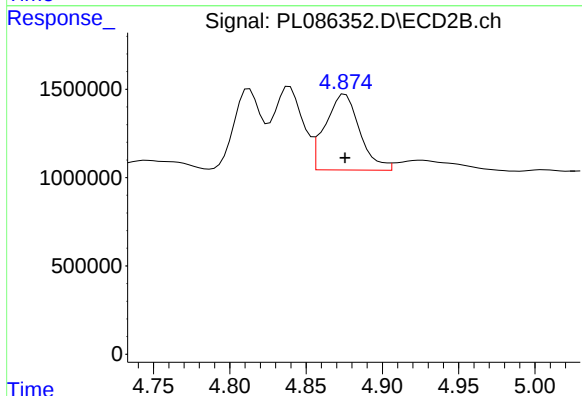


#26 Chlordane-4

R.T.: 4.876 min
Delta R.T.: 0.000 min
Response: 6757258
Conc: 51.56 ng/ml

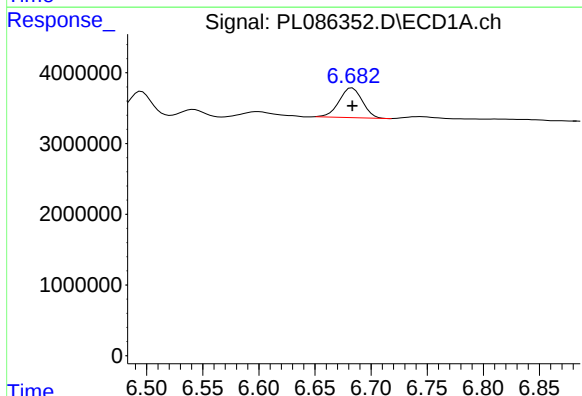


#27 Chlordane-5

R.T.: 6.683 min
Delta R.T.: 0.000 min
Response: 6061400
Conc: 55.55 ng/ml

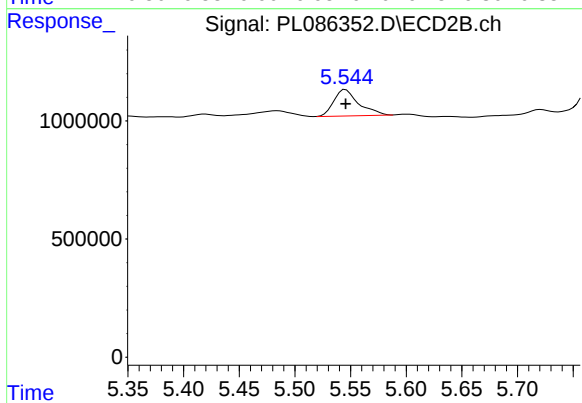

#27 Chlordane-5


R.T.: 5.545 min
Delta R.T.: 0.000 min
Response: 1732285
Conc: 50.24 ng/ml

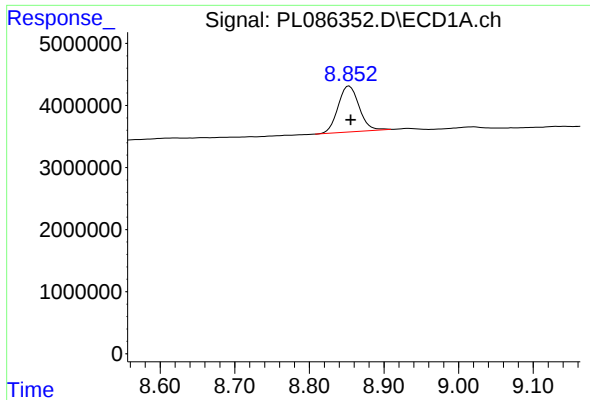

#28 Decachlorobiphenyl

R.T.: 8.853 min
Delta R.T.: -0.002 min
Response: 14611104
Conc: 5.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

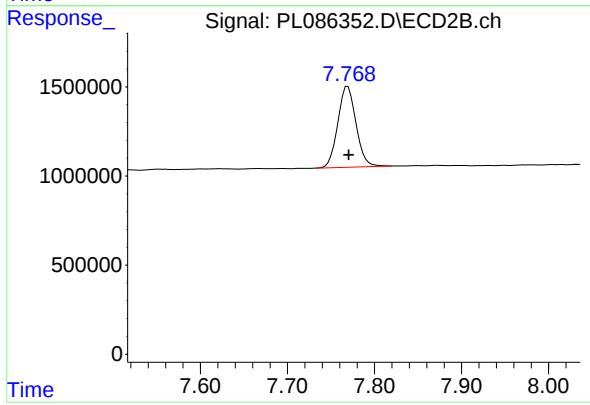

#28 Decachlorobiphenyl

R.T.: 7.769 min
Delta R.T.: 0.000 min
Response: 6614721
Conc: 5.99 ng/ml