

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110123\
 Data File : PL086348.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2023 09:58
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 02:01:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110123.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 02 02:01:21 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.353	2.617	310.1E6	119.5E6	101.063	101.424
28)	SA Decachlor...	8.854	7.770	240.2E6	106.7E6	98.696	98.305
Target Compounds							
23)	Chlordane-1	4.510	3.607	137.2E6	35001568	1009.499	1011.778
24)	Chlordane-2	5.042	4.185	142.8E6	43096615	987.946	985.369
25)	Chlordane-3	5.754	4.813	595.3E6	127.8E6	1021.459	1035.138
26)	Chlordane-4	5.836	4.874	721.7E6	138.5E6	1012.743	1027.539
27)	Chlordane-5	6.684	5.545	111.5E6	35441455	1010.944	1013.735



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110123\
Data File : PL086348.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2023 09:58
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 02:01:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110123.M
Quant Title : GC Extractables
QLast Update : Thu Nov 02 02:01:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

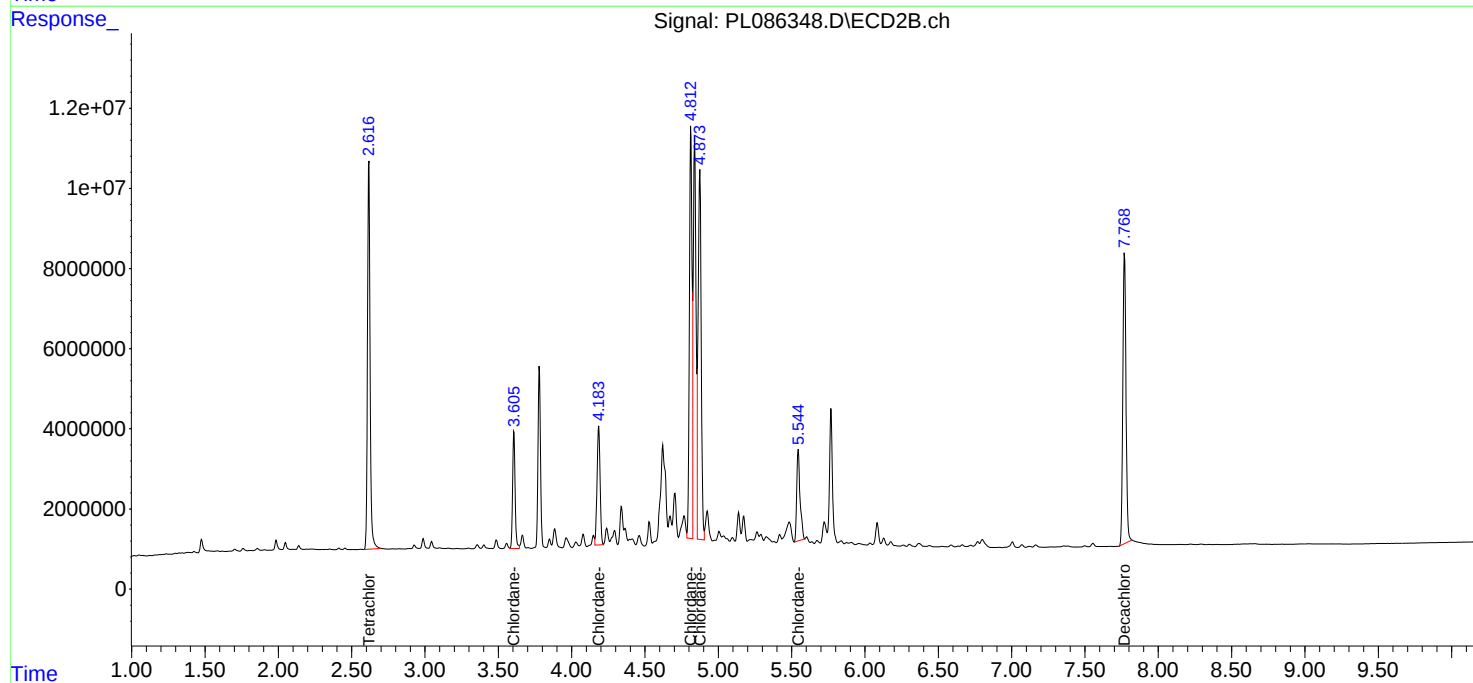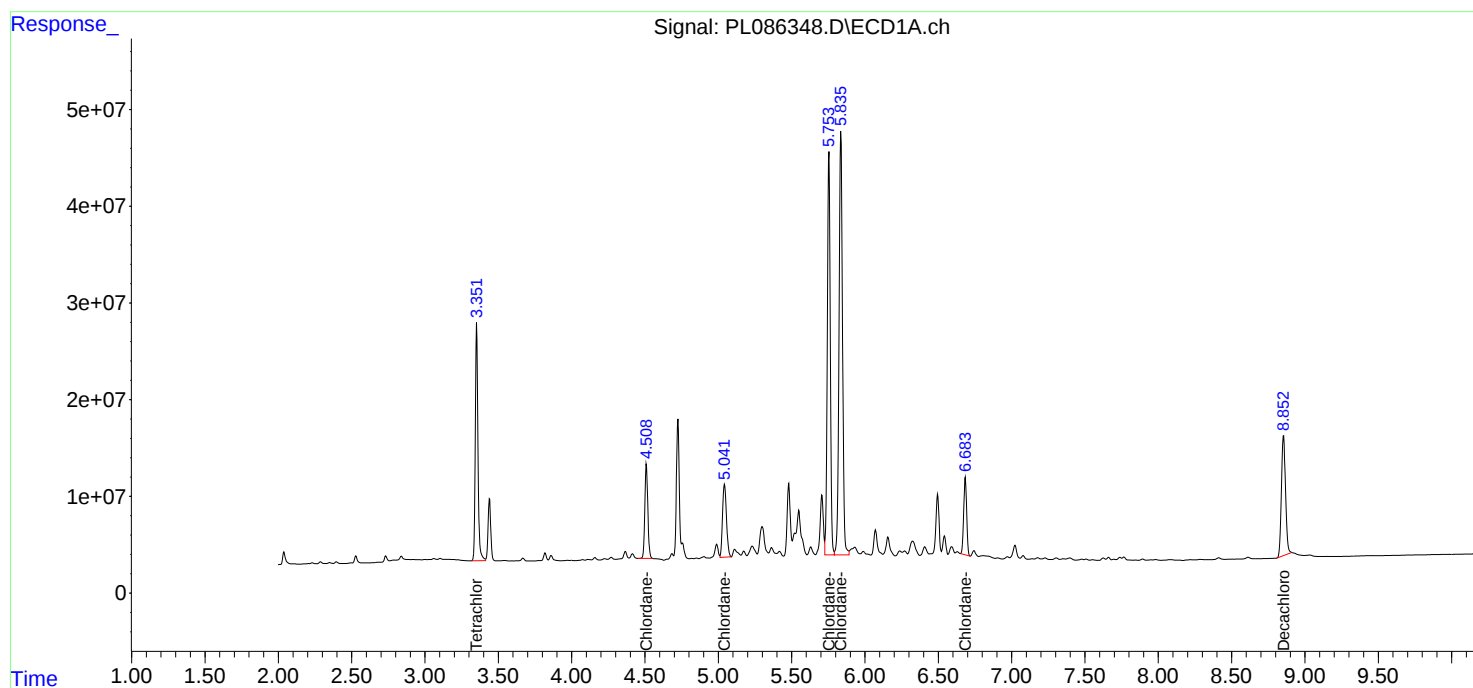


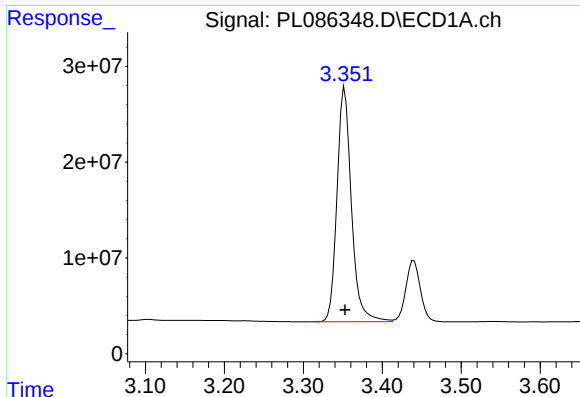

#1 Tetrachloro-m-xylene


R.T.: 3.353 min
Delta R.T.: 0.000 min
Response: 310132298
Conc: 101.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

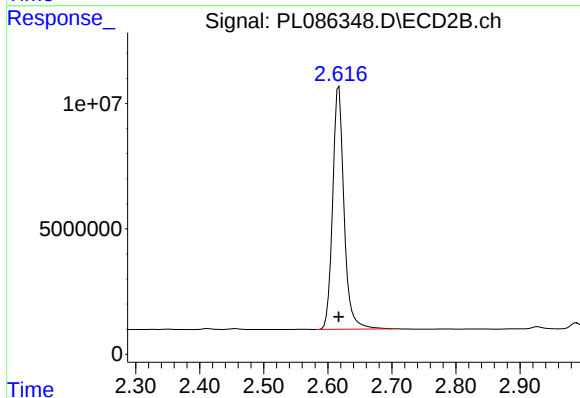


#1 Tetrachloro-m-xylene

R.T.: 2.617 min
Delta R.T.: 0.000 min
Response: 119476236
Conc: 101.42 ng/ml

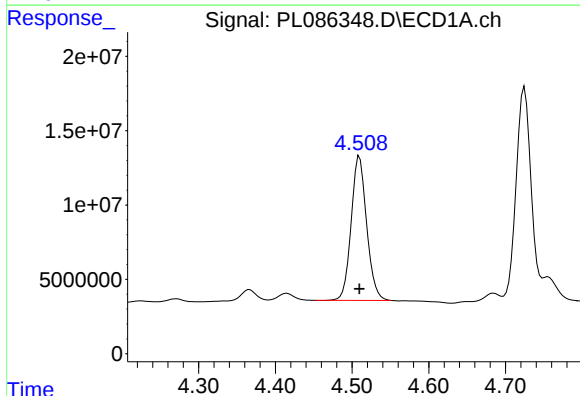


#23 Chlordane-1

R.T.: 4.510 min
Delta R.T.: 0.000 min
Response: 137153199
Conc: 1009.50 ng/ml

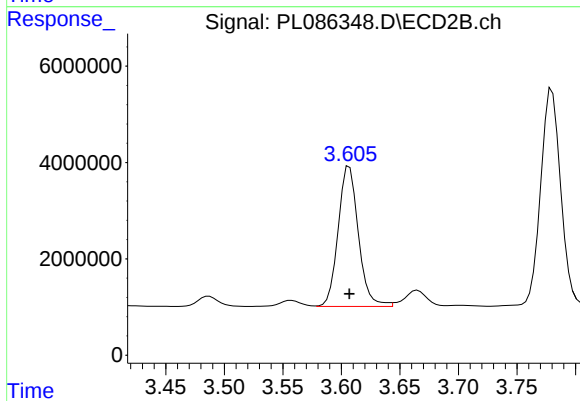

#23 Chlordane-1


R.T.: 3.607 min
Delta R.T.: 0.000 min
Response: 35001568
Conc: 1011.78 ng/ml

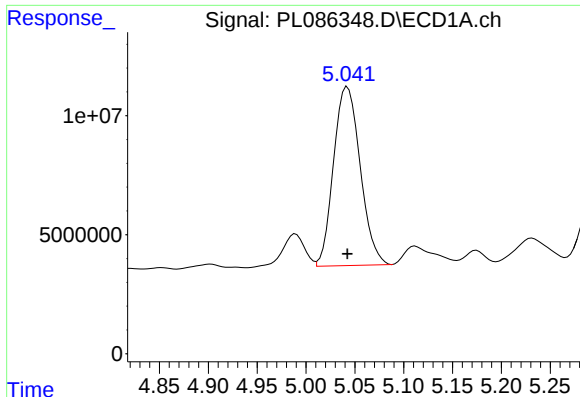

#24 Chlordane-2


R.T.: 5.042 min
Delta R.T.: 0.000 min
Response: 142751195
Conc: 987.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

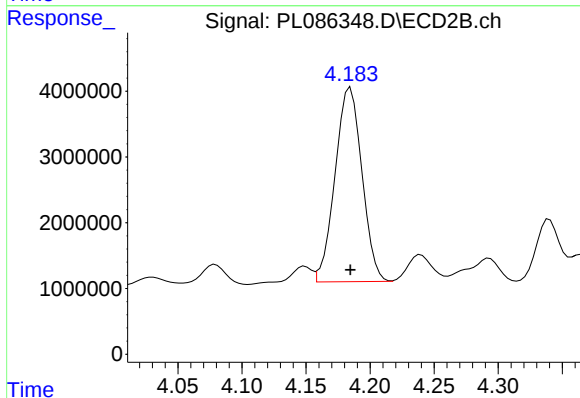


#24 Chlordane-2

R.T.: 4.185 min
Delta R.T.: 0.000 min
Response: 43096615
Conc: 985.37 ng/ml

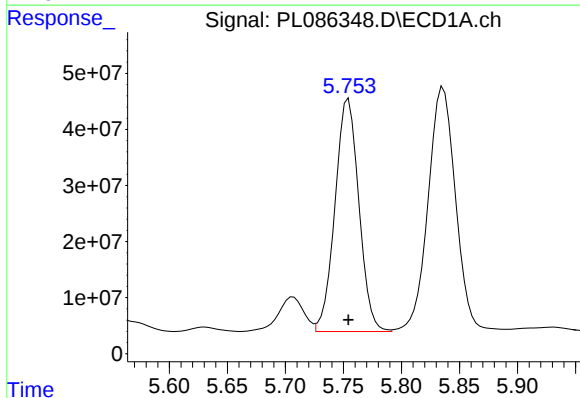


#25 Chlordane-3

R.T.: 5.754 min
Delta R.T.: 0.000 min
Response: 595349643
Conc: 1021.46 ng/ml

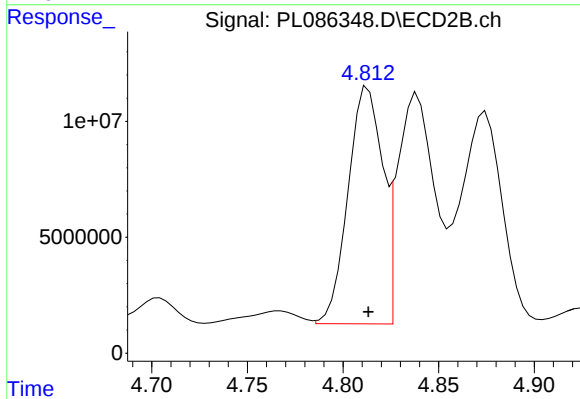

#25 Chlordane-3


R.T.: 4.813 min
Delta R.T.: 0.000 min
Response: 127824798
Conc: 1035.14 ng/ml

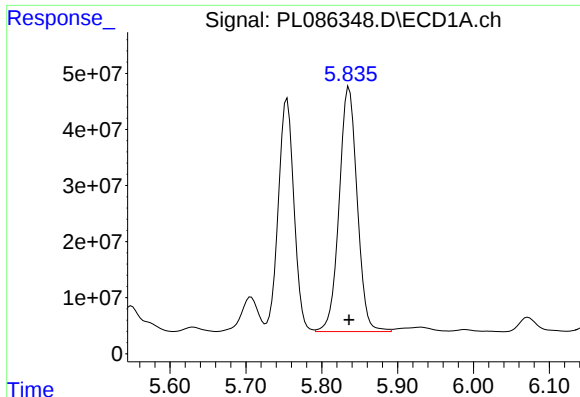

#26 Chlordane-4


R.T.: 5.836 min
Delta R.T.: 0.000 min
Response: 721724014
Conc: 1012.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

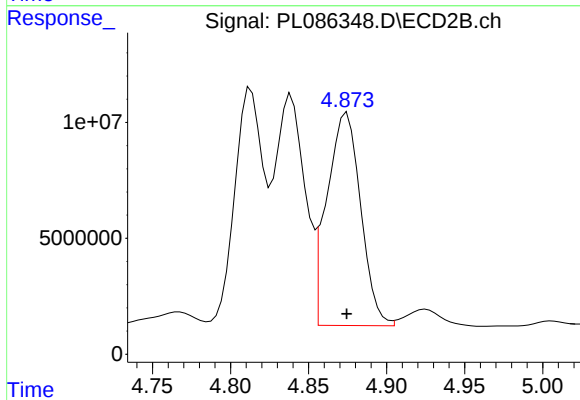


#26 Chlordane-4

R.T.: 4.874 min
Delta R.T.: 0.000 min
Response: 138474961
Conc: 1027.54 ng/ml

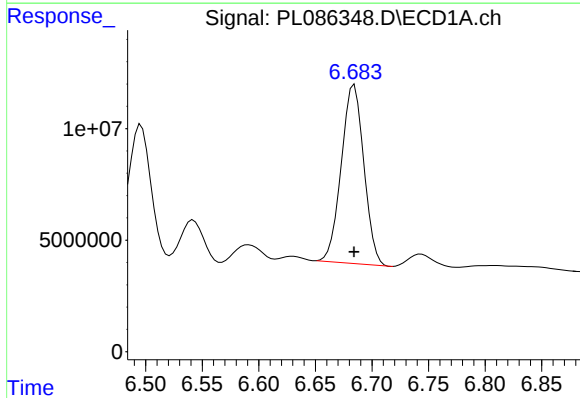


#27 Chlordane-5

R.T.: 6.684 min
Delta R.T.: 0.000 min
Response: 111524894
Conc: 1010.94 ng/ml

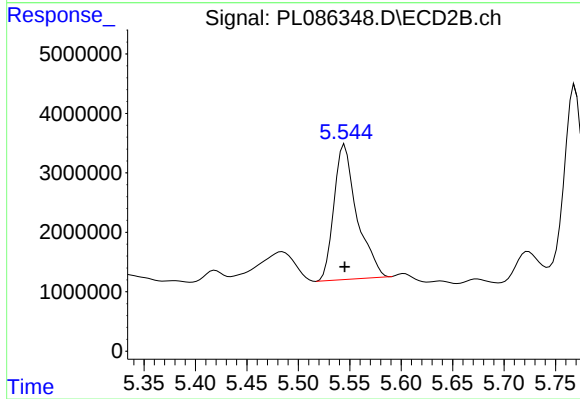

#27 Chlordane-5


R.T.: 5.545 min
Delta R.T.: 0.000 min
Response: 35441455
Conc: 1013.74 ng/ml

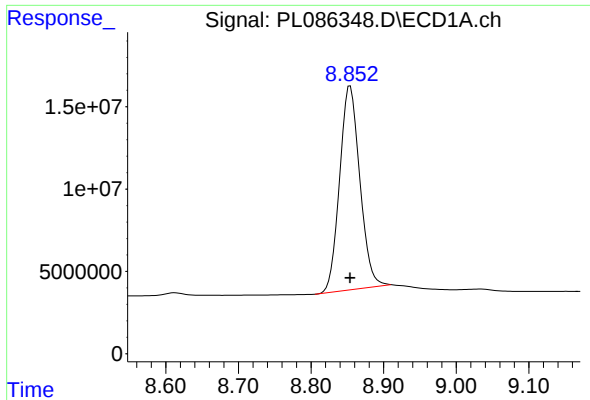

#28 Decachlorobiphenyl

R.T.: 8.854 min
Delta R.T.: 0.000 min
Response: 240216237
Conc: 98.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

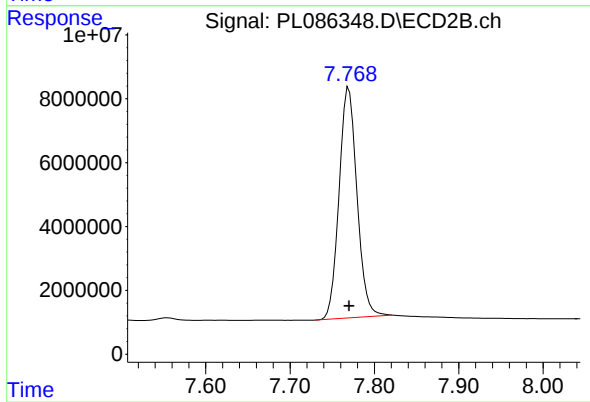

#28 Decachlorobiphenyl

R.T.: 7.770 min
Delta R.T.: 0.000 min
Response: 106741464
Conc: 98.31 ng/ml