

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110123\
 Data File : PL086350.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2023 10:26
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 01:58:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110123.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 02 01:55:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.353	2.617	151.8E6	58060773	50.000	50.000
28)	SA Decachlor...	8.856	7.770	123.3E6	55210823	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.510	3.606	67286089	17093327	500.000	500.000
24)	Chlordane-2	5.043	4.185	73117310	22188234	500.000	500.000
25)	Chlordane-3	5.754	4.813	285.2E6	59573383	500.000	500.000
26)	Chlordane-4	5.837	4.875	351.8E6	65526286	500.000	500.000
27)	Chlordane-5	6.683	5.546	54555080	17240518	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110123\
Data File : PL086350.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2023 10:26
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 01:58:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110123.M
Quant Title : GC Extractables
QLast Update : Thu Nov 02 01:55:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

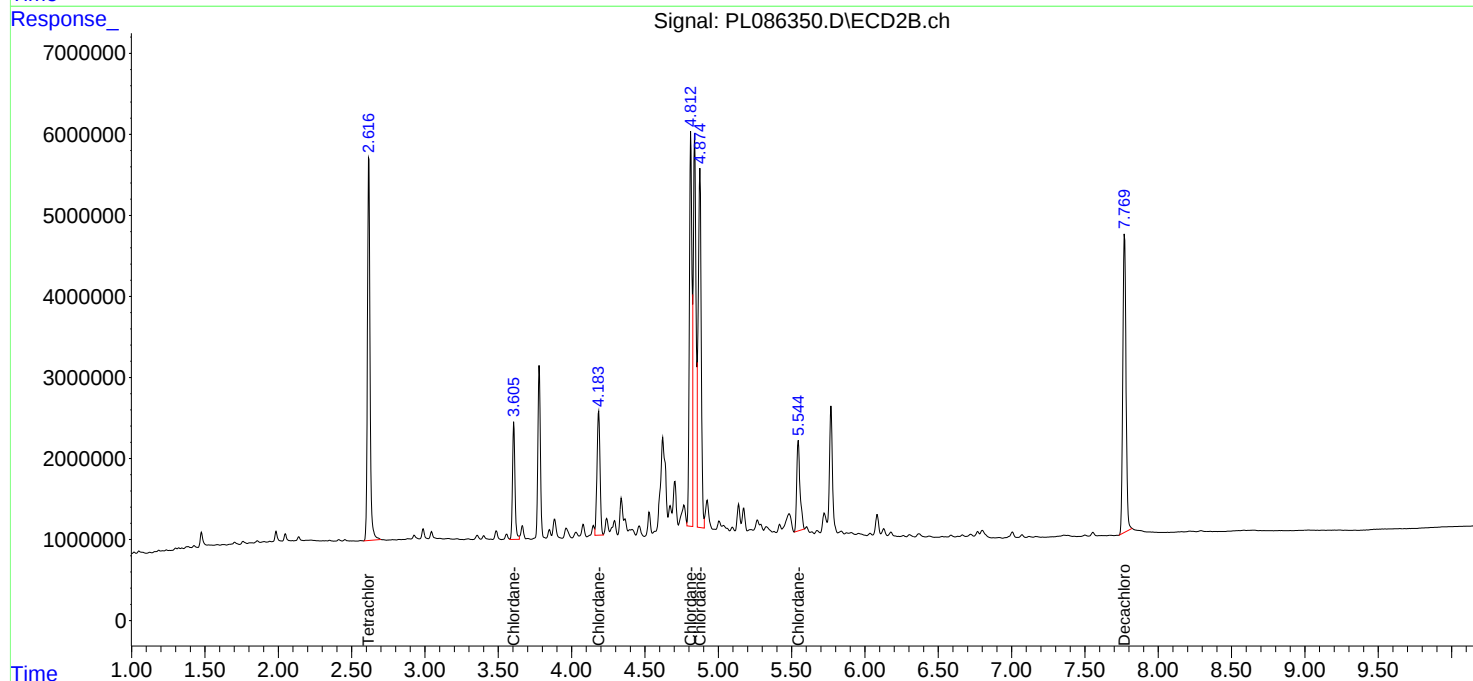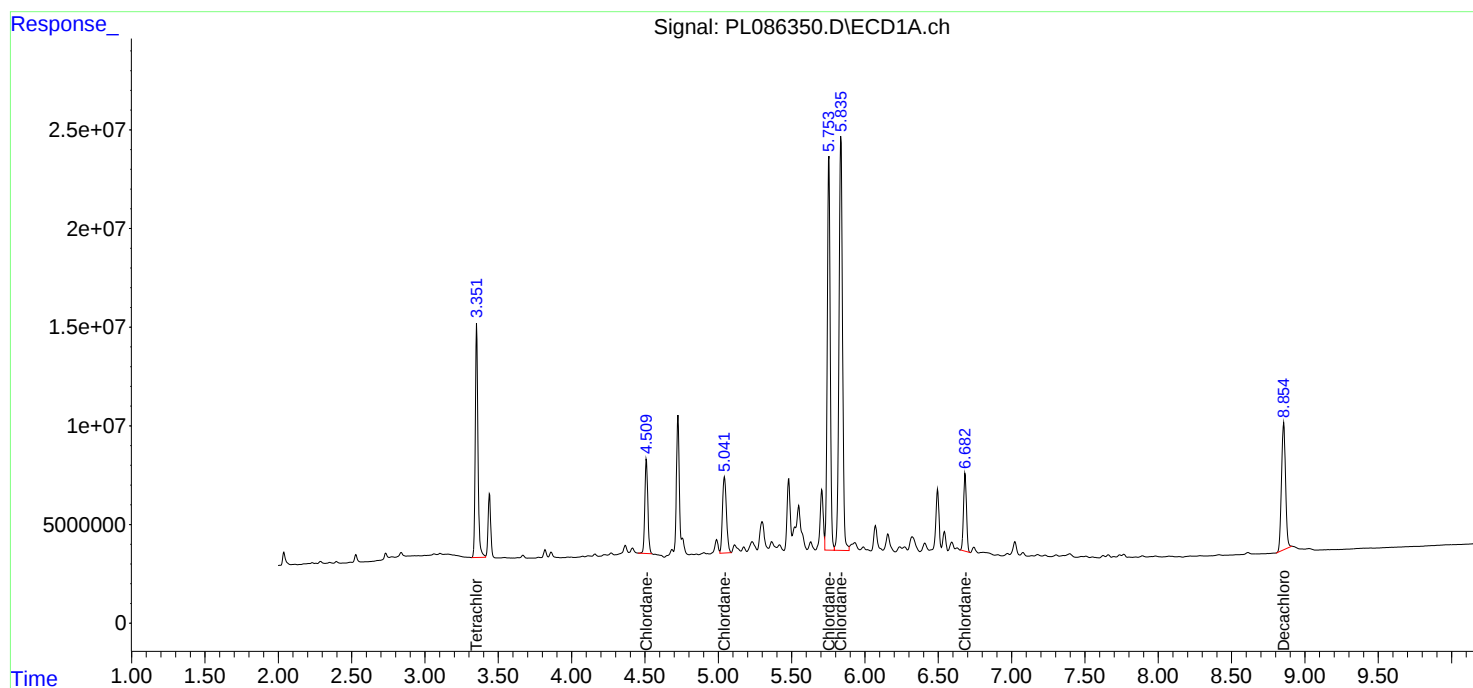


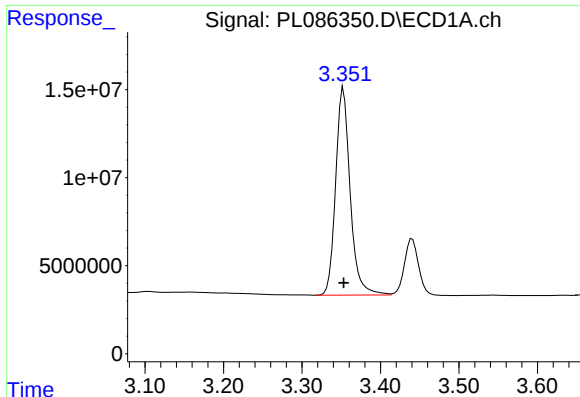

#1 Tetrachloro-m-xylene


R.T.: 3.353 min
Delta R.T.: 0.000 min
Response: 151802883
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

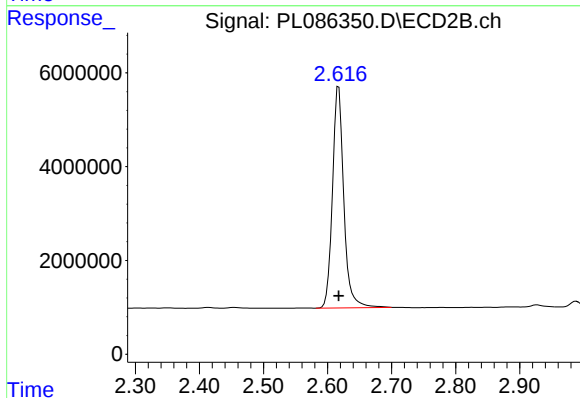


#1 Tetrachloro-m-xylene

R.T.: 2.617 min
Delta R.T.: 0.000 min
Response: 58060773
Conc: 50.00 ng/ml

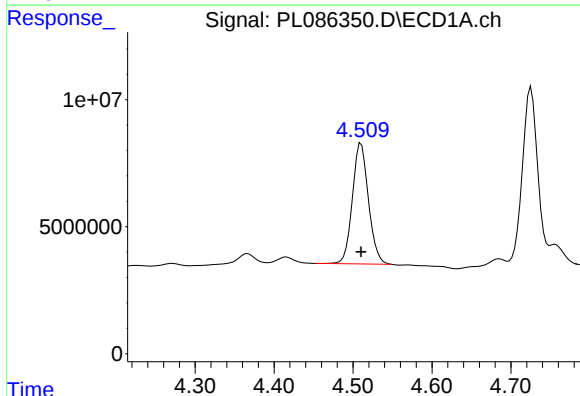


#23 Chlordane-1

R.T.: 4.510 min
Delta R.T.: 0.000 min
Response: 67286089
Conc: 500.00 ng/ml

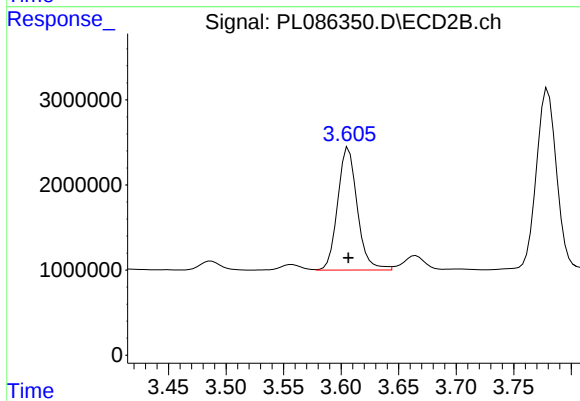

#23 Chlordane-1


R.T.: 3.606 min
Delta R.T.: 0.000 min
Response: 17093327
Conc: 500.00 ng/ml

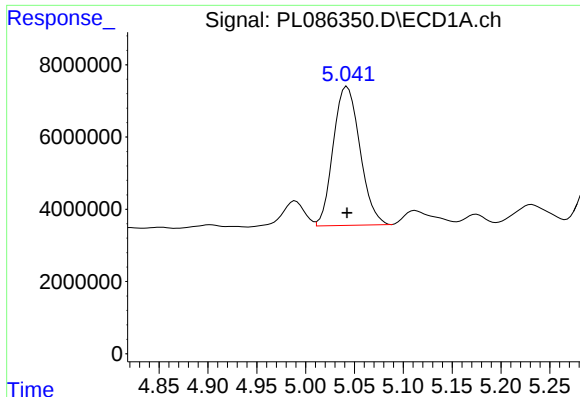

#24 Chlordane-2


R.T.: 5.043 min
Delta R.T.: 0.000 min
Response: 73117310
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

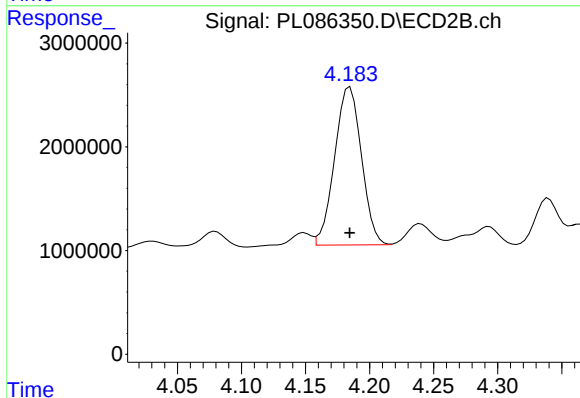


#24 Chlordane-2

R.T.: 4.185 min
Delta R.T.: 0.000 min
Response: 22188234
Conc: 500.00 ng/ml

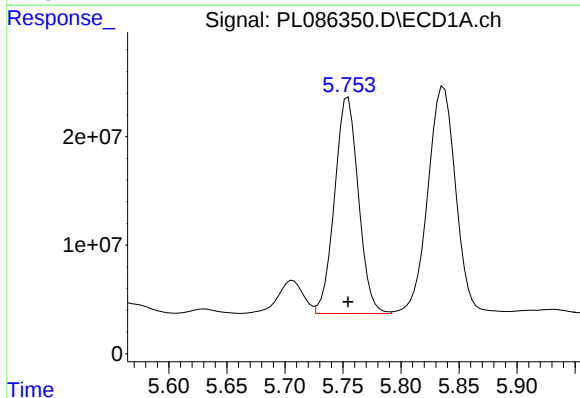


#25 Chlordane-3

R.T.: 5.754 min
Delta R.T.: 0.000 min
Response: 285167759
Conc: 500.00 ng/ml

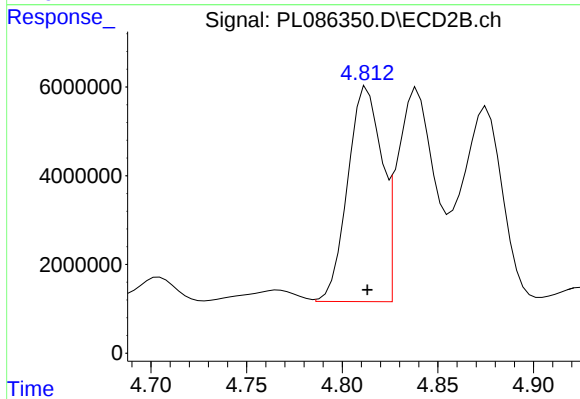

#25 Chlordane-3


R.T.: 4.813 min
Delta R.T.: 0.000 min
Response: 59573383
Conc: 500.00 ng/ml

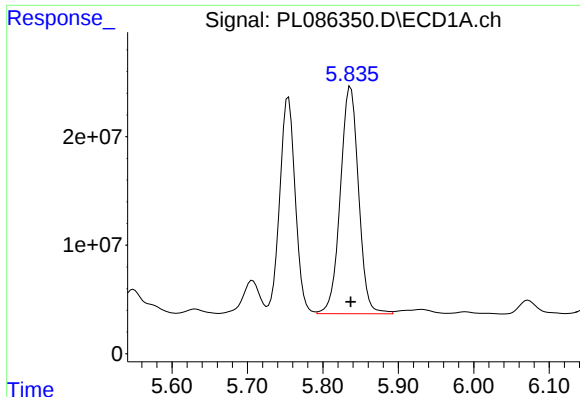

#26 Chlordane-4


R.T.: 5.837 min
Delta R.T.: 0.000 min
Response: 351780521
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

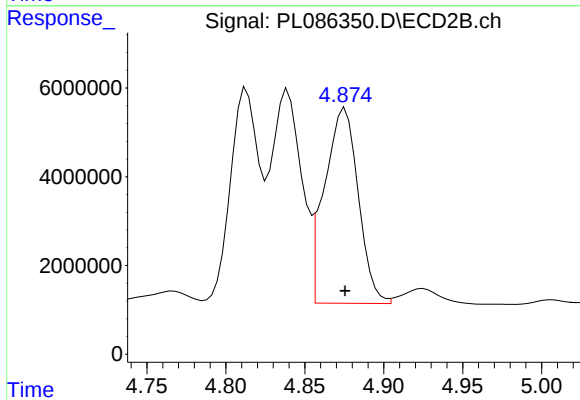


#26 Chlordane-4

R.T.: 4.875 min
Delta R.T.: 0.000 min
Response: 65526286
Conc: 500.00 ng/ml

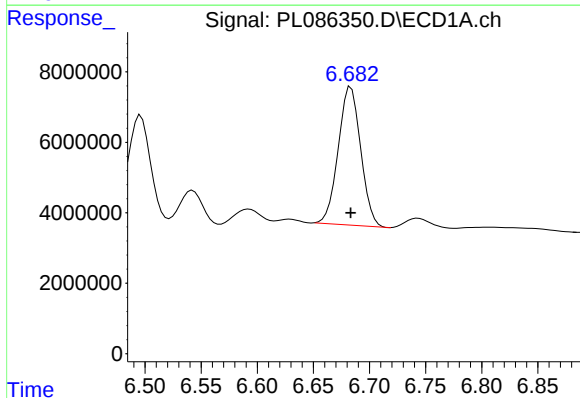


#27 Chlordane-5

R.T.: 6.683 min
Delta R.T.: 0.000 min
Response: 54555080
Conc: 500.00 ng/ml

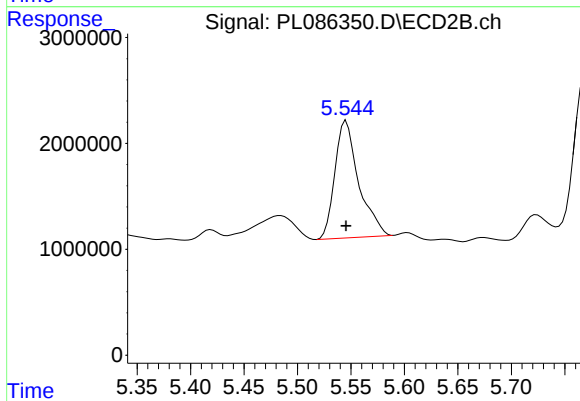

#27 Chlordane-5


R.T.: 5.546 min
Delta R.T.: 0.000 min
Response: 17240518
Conc: 500.00 ng/ml

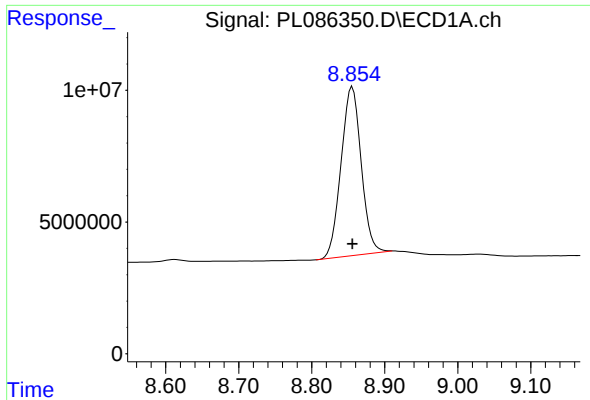

#28 Decachlorobiphenyl

R.T.: 8.856 min
Delta R.T.: 0.000 min
Response: 123281859
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

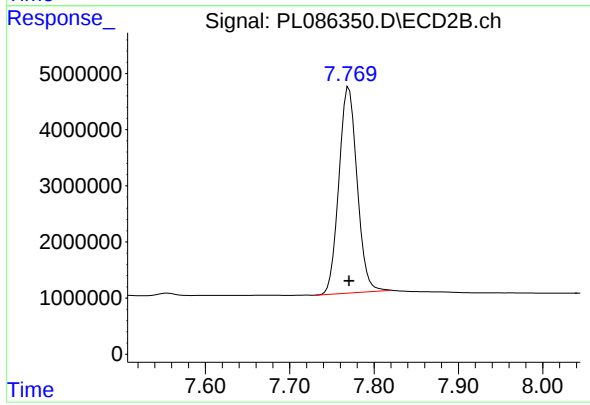

#28 Decachlorobiphenyl

R.T.: 7.770 min
Delta R.T.: 0.000 min
Response: 55210823
Conc: 50.00 ng/ml