

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110123\
 Data File : PL086351.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2023 10:40
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 02:04:55 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110123.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 02 02:04:47 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.353	2.618	77378341	29056984	25.207	24.799
28)	SA Decachlor...	8.855	7.769	65497985	29672160	26.483	26.786
Target Compounds							
23)	Chlordane-1	4.510	3.607	34652086	8738313	254.356	252.657
24)	Chlordane-2	5.043	4.185	38753523	11707084	264.343	263.976
25)	Chlordane-3	5.754	4.814	142.4E6	29350487	246.366	241.007
26)	Chlordane-4	5.837	4.875	178.3E6	32476420	250.754	243.734
27)	Chlordane-5	6.684	5.545	28227852	8648691	255.157	248.596



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110123\
Data File : PL086351.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2023 10:40
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 02:04:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110123.M
Quant Title : GC Extractables
QLast Update : Thu Nov 02 02:04:47 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

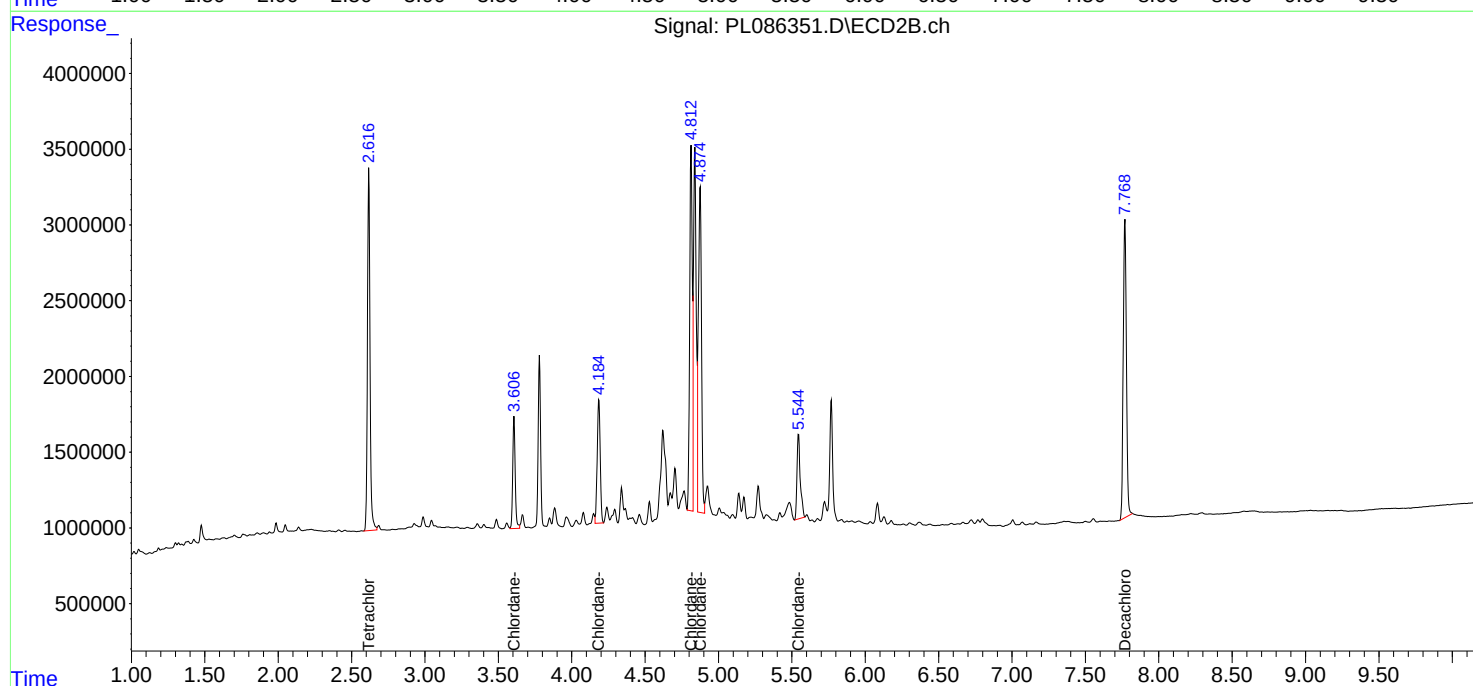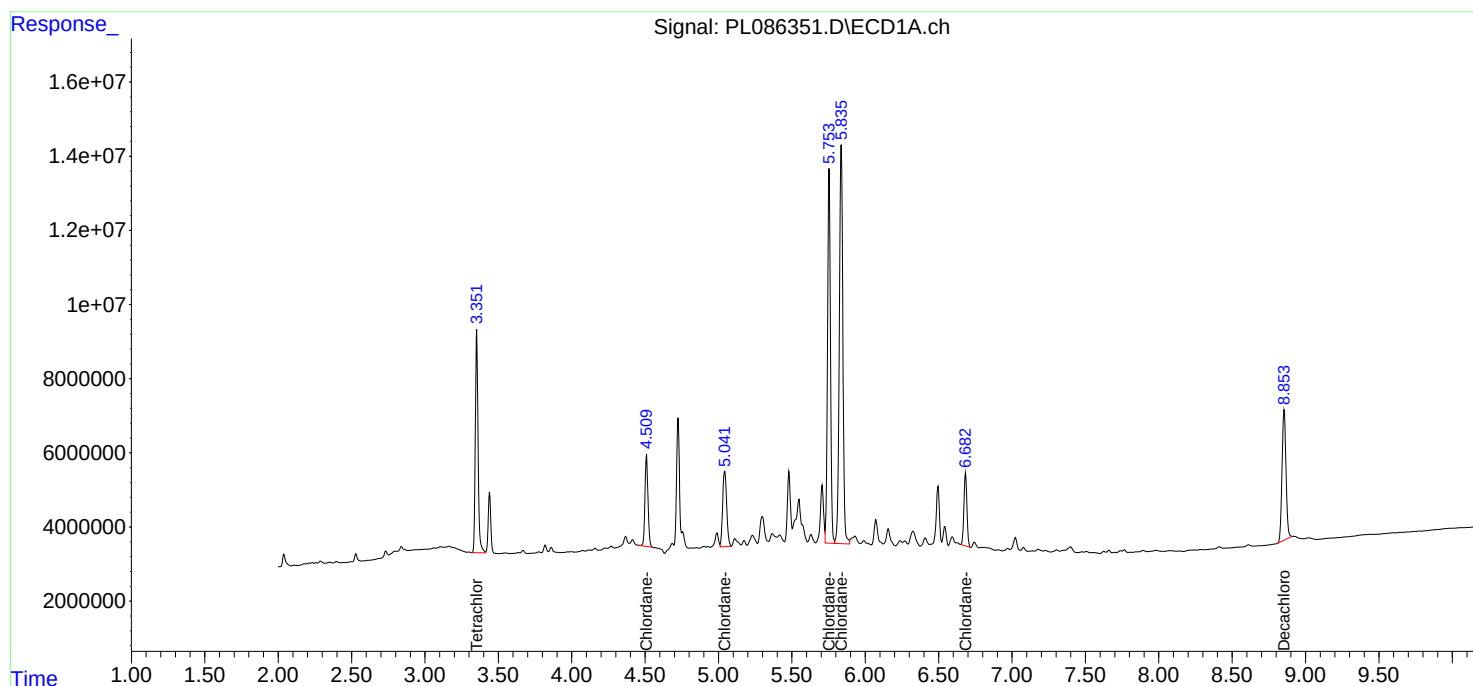


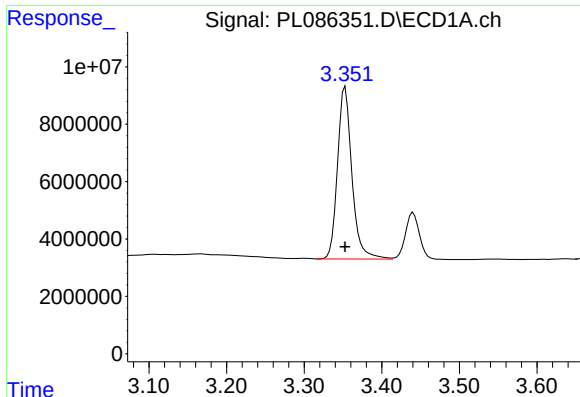

#1 Tetrachloro-m-xylene


R.T.: 3.353 min
Delta R.T.: 0.000 min
Response: 77378341
Conc: 25.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

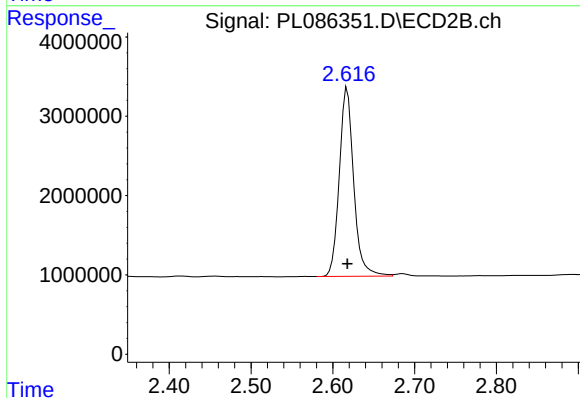


#1 Tetrachloro-m-xylene

R.T.: 2.618 min
Delta R.T.: 0.000 min
Response: 29056984
Conc: 24.80 ng/ml

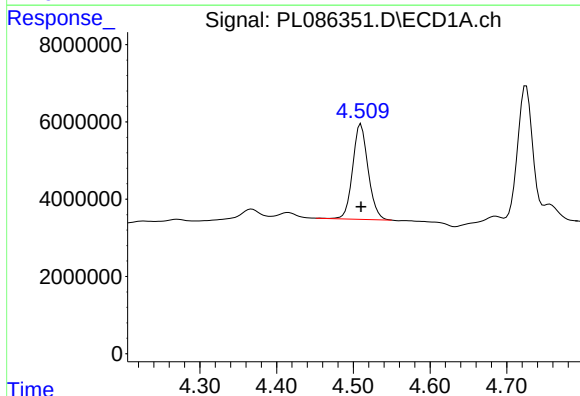


#23 Chlordane-1

R.T.: 4.510 min
Delta R.T.: 0.000 min
Response: 34652086
Conc: 254.36 ng/ml

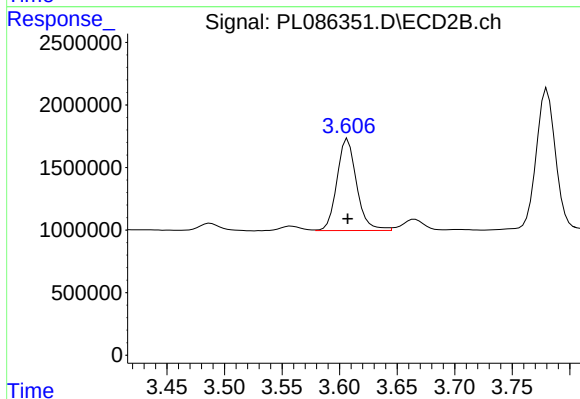

#23 Chlordane-1


R.T.: 3.607 min
Delta R.T.: 0.000 min
Response: 8738313
Conc: 252.66 ng/ml

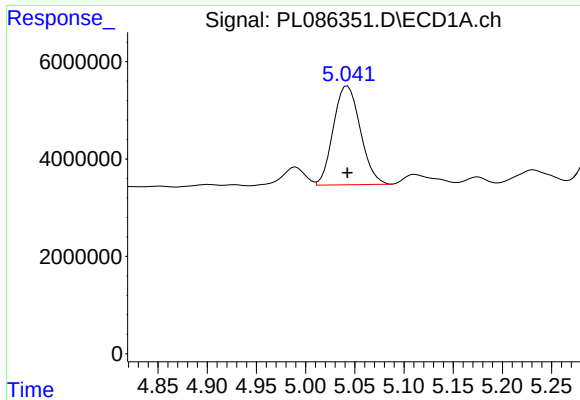

#24 Chlordane-2


R.T.: 5.043 min
Delta R.T.: 0.000 min
Response: 38753523
Conc: 264.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

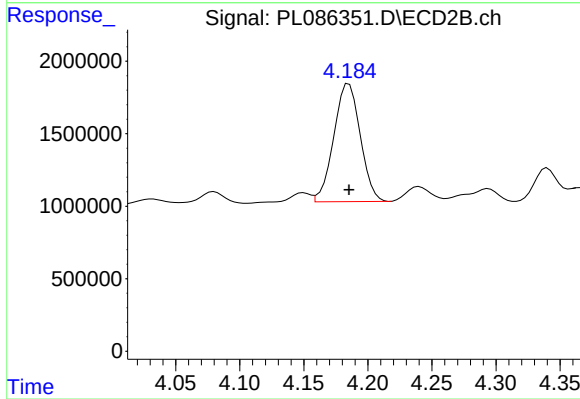


#24 Chlordane-2

R.T.: 4.185 min
Delta R.T.: 0.000 min
Response: 11707084
Conc: 263.98 ng/ml

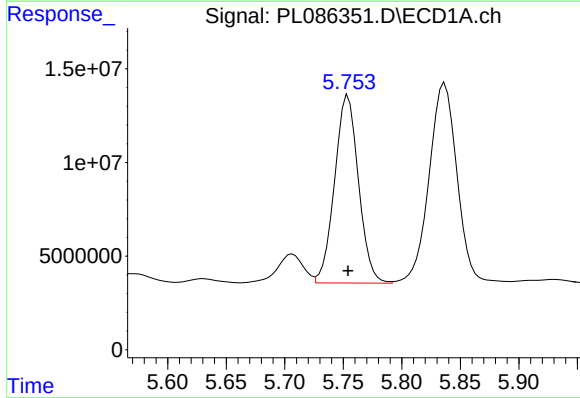


#25 Chlordane-3

R.T.: 5.754 min
Delta R.T.: 0.000 min
Response: 142431463
Conc: 246.37 ng/ml

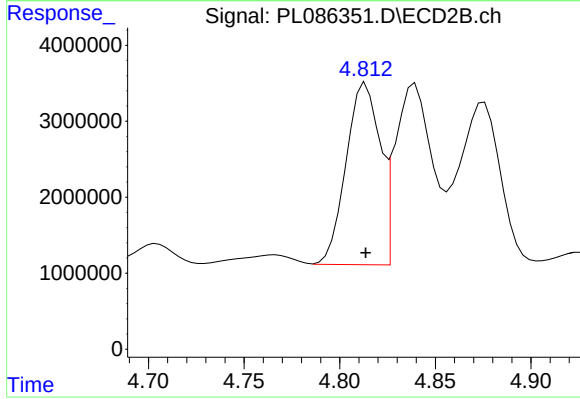

#25 Chlordane-3


R.T.: 4.814 min
Delta R.T.: 0.000 min
Response: 29350487
Conc: 241.01 ng/ml

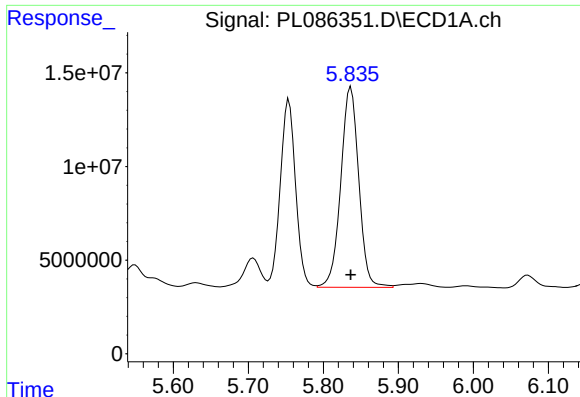

#26 Chlordane-4


R.T.: 5.837 min
Delta R.T.: 0.000 min
Response: 178287495
Conc: 250.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

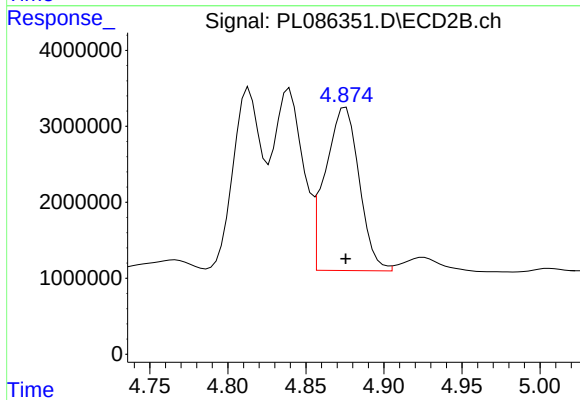


#26 Chlordane-4

R.T.: 4.875 min
Delta R.T.: 0.000 min
Response: 32476420
Conc: 243.73 ng/ml

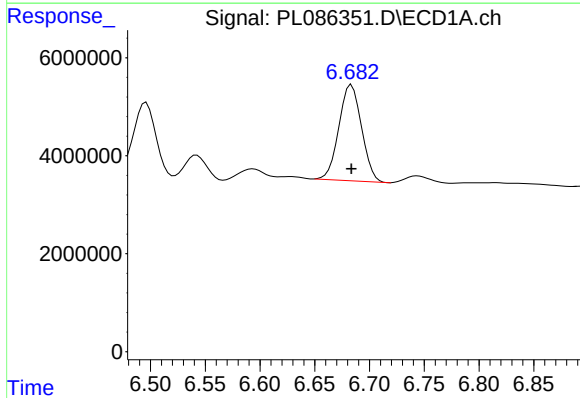


#27 Chlordane-5

R.T.: 6.684 min
Delta R.T.: 0.000 min
Response: 28227852
Conc: 255.16 ng/ml

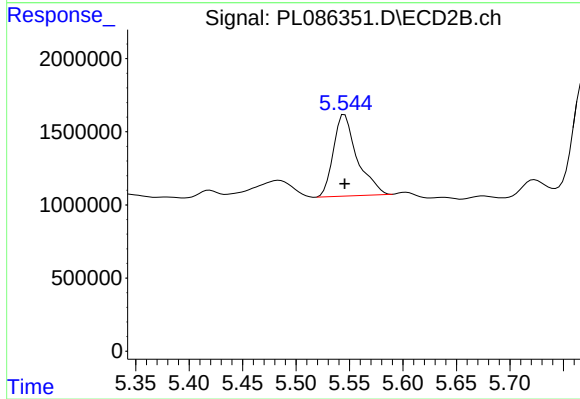

#27 Chlordane-5


R.T.: 5.545 min
Delta R.T.: 0.000 min
Response: 8648691
Conc: 248.60 ng/ml

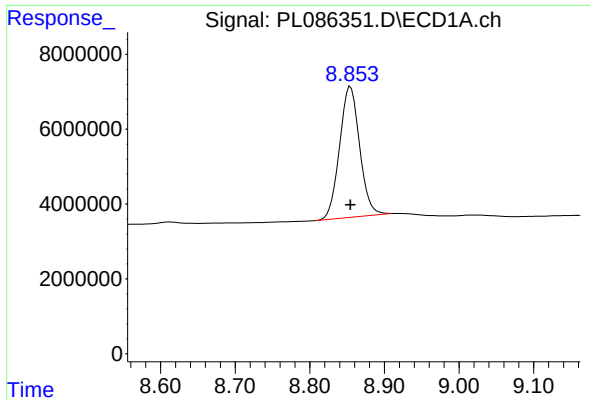

#28 Decachlorobiphenyl

R.T.: 8.855 min
Delta R.T.: 0.000 min
Response: 65497985
Conc: 26.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

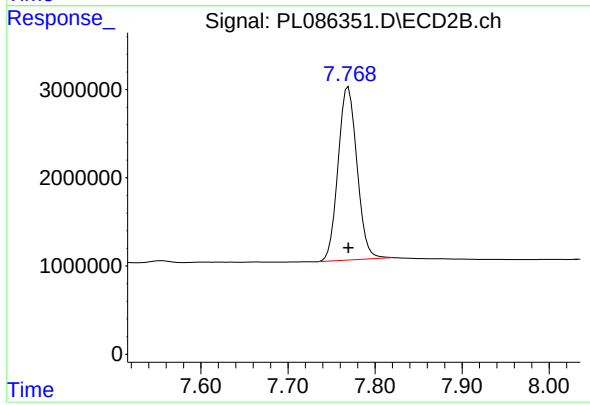

#28 Decachlorobiphenyl

R.T.: 7.769 min
Delta R.T.: 0.000 min
Response: 29672160
Conc: 26.79 ng/ml