

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110123\
 Data File : PL086359.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2023 12:30
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL110123CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 01:59:22 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110123.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 02 01:55:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.352	2.617	156.1E6	58720572	51.416	50.568
28)	SA Decachlor...	8.854	7.770	126.9E6	57270192	51.471	51.865
Target Compounds							
23)	Chlordane-1	4.509	3.607	69196989	17531017	514.200	512.803
24)	Chlordane-2	5.042	4.184	75769416	22676571	518.136	511.004
25)	Chlordane-3	5.753	4.813	295.4E6	61435072	518.018	515.625
26)	Chlordane-4	5.836	4.875	364.9E6	67255295	518.684	513.193
27)	Chlordane-5	6.683	5.545	56150179	17802593	514.619	516.301



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110123\
Data File : PL086359.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2023 12:30
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL110123CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 01:59:22 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110123.M
Quant Title : GC Extractables
QLast Update : Thu Nov 02 01:55:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

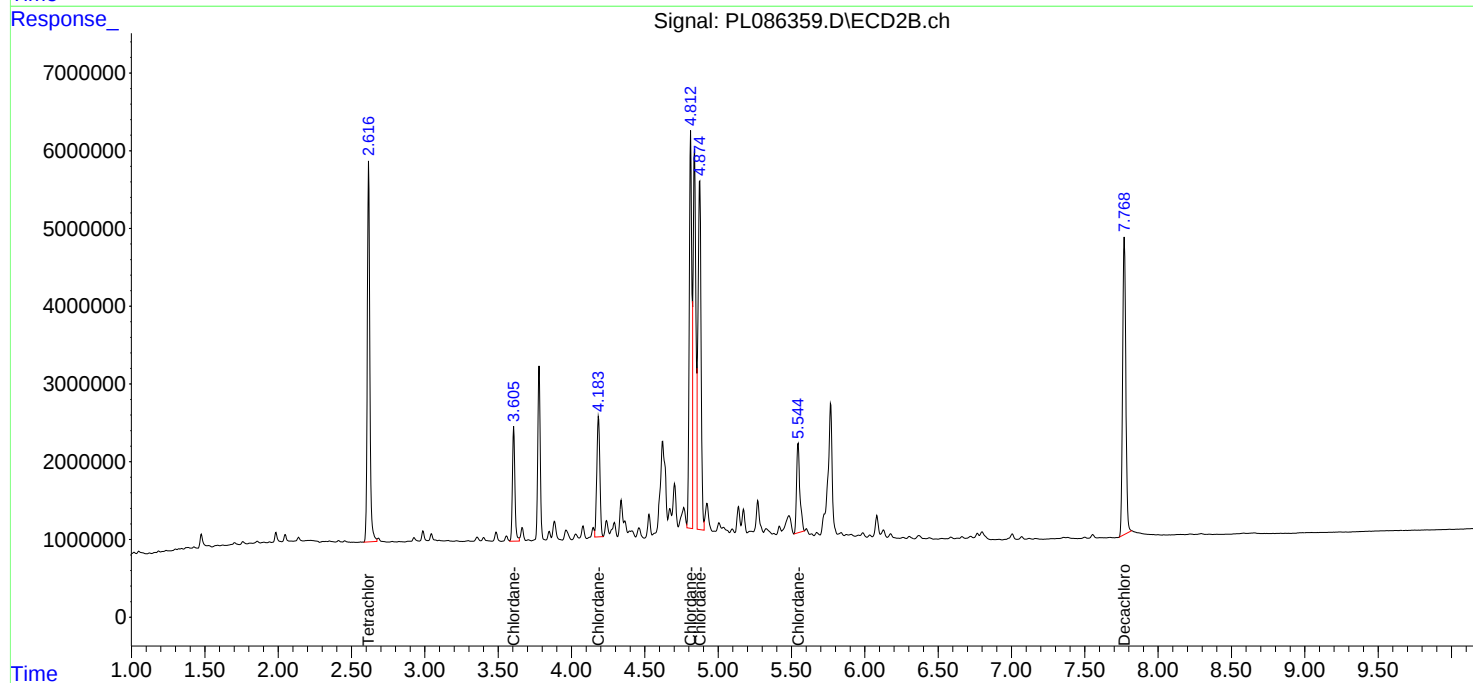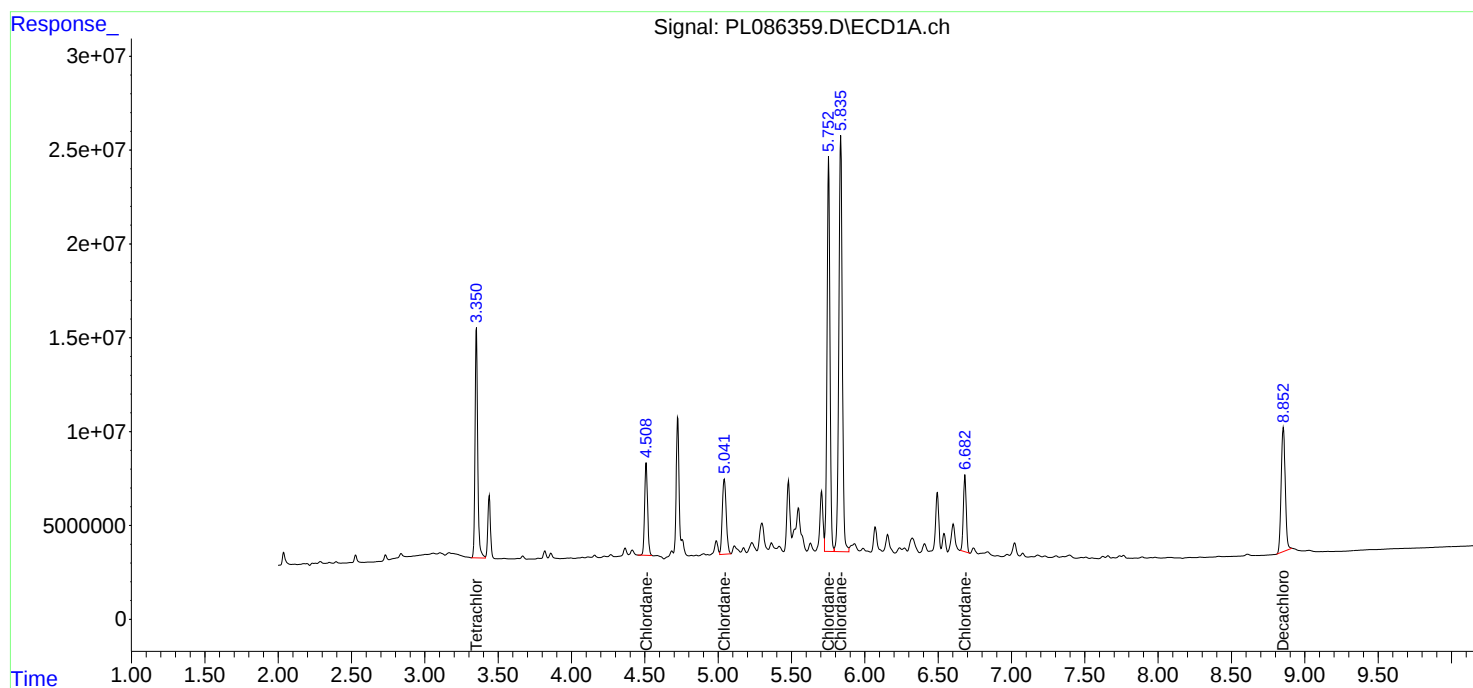


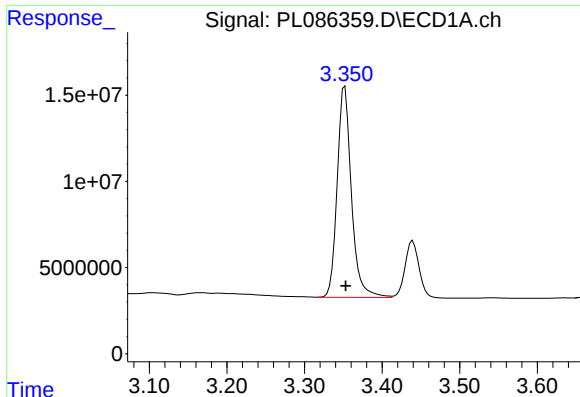

#1 Tetrachloro-m-xylene


R.T.: 3.352 min
Delta R.T.: -0.001 min
Response: 156102851
Conc: 51.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL110123CHLOR

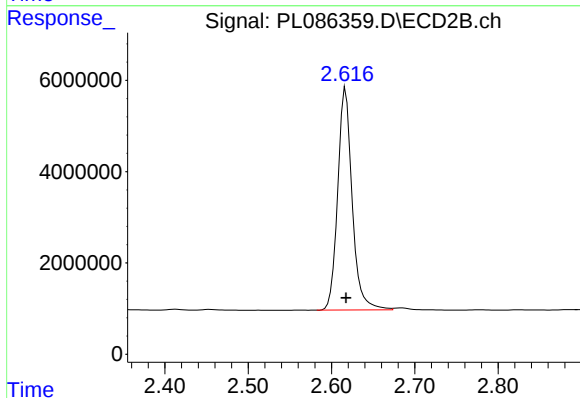


#1 Tetrachloro-m-xylene

R.T.: 2.617 min
Delta R.T.: 0.000 min
Response: 58720572
Conc: 50.57 ng/ml

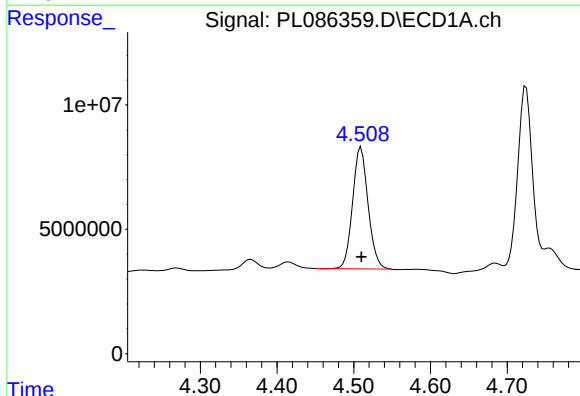


#23 Chlordane-1

R.T.: 4.509 min
Delta R.T.: 0.000 min
Response: 69196989
Conc: 514.20 ng/ml

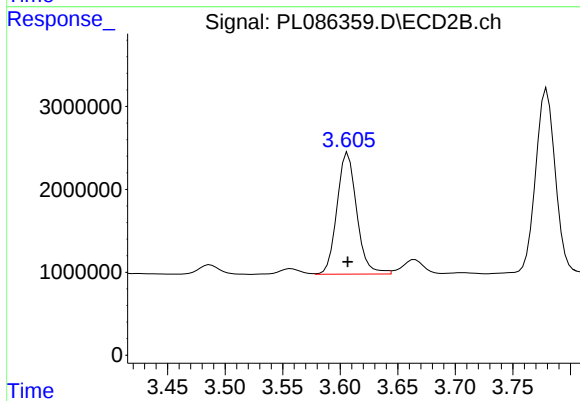

#23 Chlordane-1


R.T.: 3.607 min
Delta R.T.: 0.000 min
Response: 17531017
Conc: 512.80 ng/ml

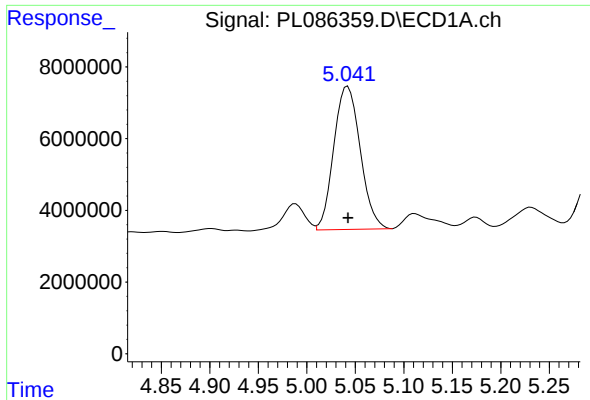

#24 Chlordane-2


R.T.: 5.042 min
Delta R.T.: 0.000 min
Response: 75769416
Conc: 518.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL110123CHLOR

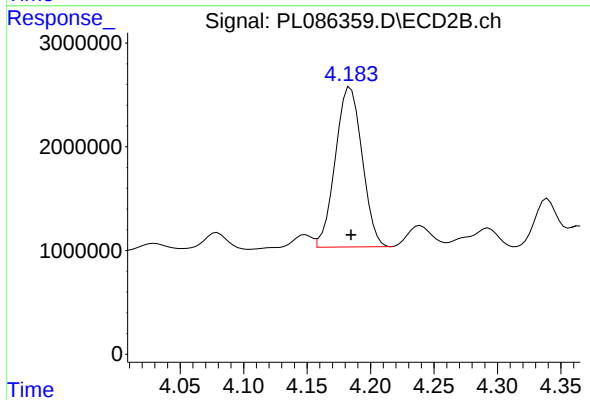


#24 Chlordane-2

R.T.: 4.184 min
Delta R.T.: 0.000 min
Response: 22676571
Conc: 511.00 ng/ml

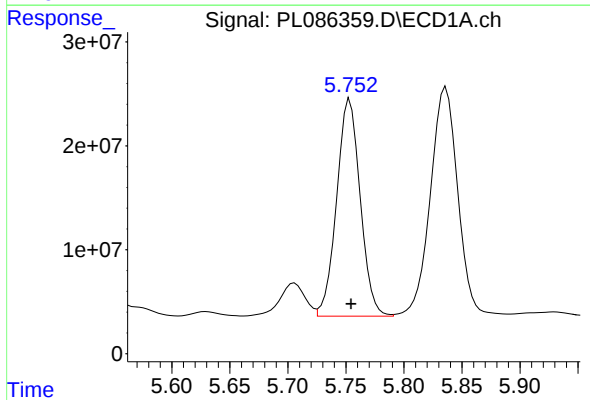


#25 Chlordane-3

R.T.: 5.753 min
Delta R.T.: 0.000 min
Response: 295444312
Conc: 518.02 ng/ml

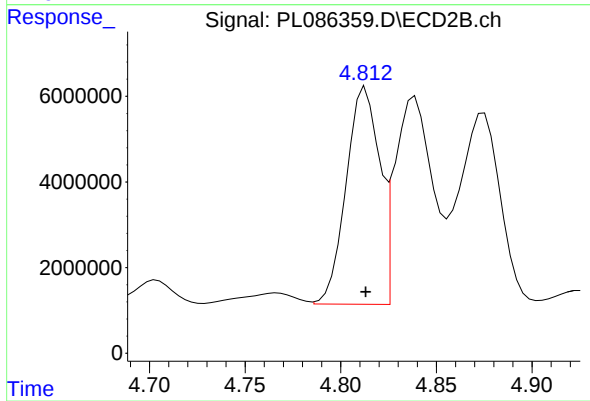

#25 Chlordane-3


R.T.: 4.813 min
Delta R.T.: 0.000 min
Response: 61435072
Conc: 515.63 ng/ml

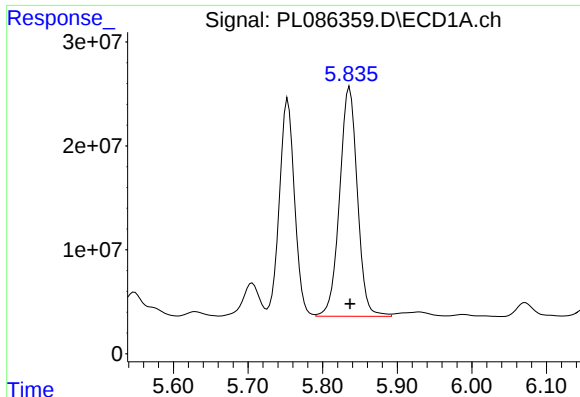

#26 Chlordane-4


R.T.: 5.836 min
Delta R.T.: 0.000 min
Response: 364925897
Conc: 518.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL110123CHLOR

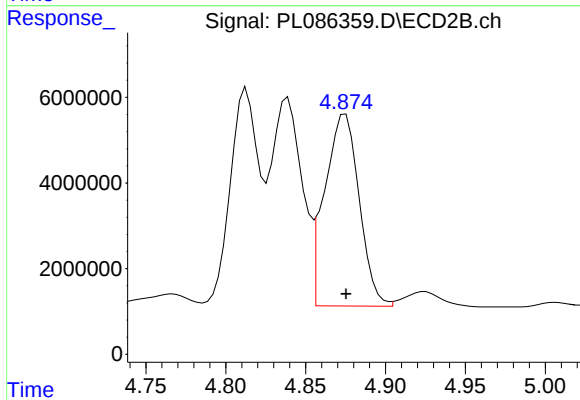


#26 Chlordane-4

R.T.: 4.875 min
Delta R.T.: 0.000 min
Response: 67255295
Conc: 513.19 ng/ml

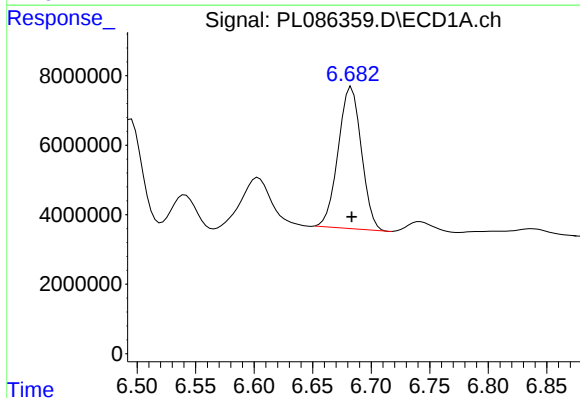


#27 Chlordane-5

R.T.: 6.683 min
Delta R.T.: 0.000 min
Response: 56150179
Conc: 514.62 ng/ml

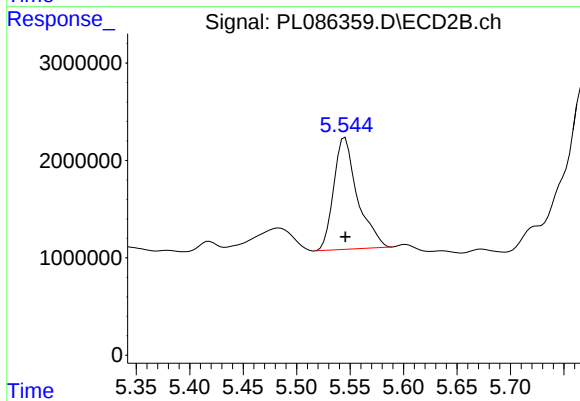

#27 Chlordane-5

R.T.: 5.545 min
Delta R.T.: 0.000 min
Response: 17802593
Conc: 516.30 ng/ml

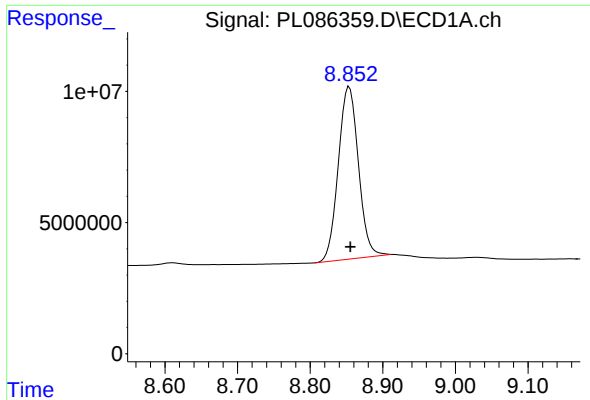

#28 Decachlorobiphenyl


R.T.: 8.854 min

Delta R.T.: -0.002 min

Response: 126907862

Conc: 51.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL110123CHLOR

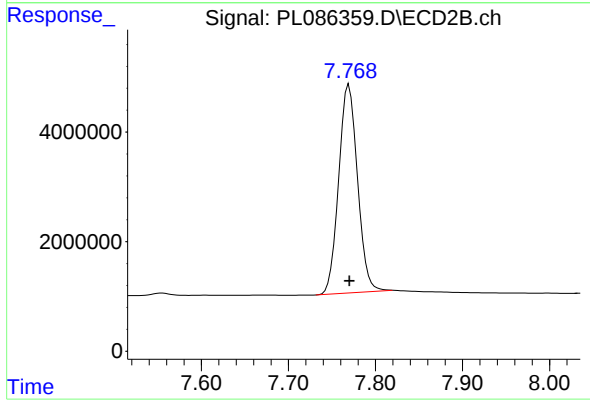

#28 Decachlorobiphenyl

R.T.: 7.770 min

Delta R.T.: 0.000 min

Response: 57270192

Conc: 51.87 ng/ml