

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110124\
 Data File : PL092801.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2024 14:47
 Operator : AR\AJ
 Sample : PB164592BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB164592BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 01:41:46 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.779	48927386	51903561	19.968	19.074
28)	SA Decachlor...	9.063	7.920	40833698	60045385	21.217	22.001
Target Compounds							
2)	A alpha-BHC	0.000	3.293	0	138037	N.D.	0.035 #
4)	MA Heptachlor	0.000	3.950	0	181409	N.D.	0.048 #
5)	MB Aldrin	0.000	4.212f	0	128494	N.D.	0.035 #
6)	B beta-BHC	0.000	3.920	0	212854	N.D.	0.129 #
7)	B delta-BHC	4.772	4.140	2793008	159528	0.892	0.042 #
10)	B gamma-Chl...	0.000	4.975	0	752112	N.D.	0.224 #
12)	B 4,4'-DDE	0.000	5.258f	0	330653	N.D.	0.103 #
14)	MA Endrin	0.000	5.664f	0	310807	N.D.	0.107 #
22)	Mirex	0.000	7.047f	0	4171	N.D.	0.002 #
23)	Chlordane-1	0.000	3.777	0	36857	N.D.	0.347 #
24)	Chlordane-2	0.000	4.342	0	279895	N.D.	2.260 #
25)	Chlordane-3	0.000	4.975	0	752112	N.D.	2.074 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110124\
Data File : PL092801.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2024 14:47
Operator : AR\AJ
Sample : PB164592BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB164592BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 01:41:46 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

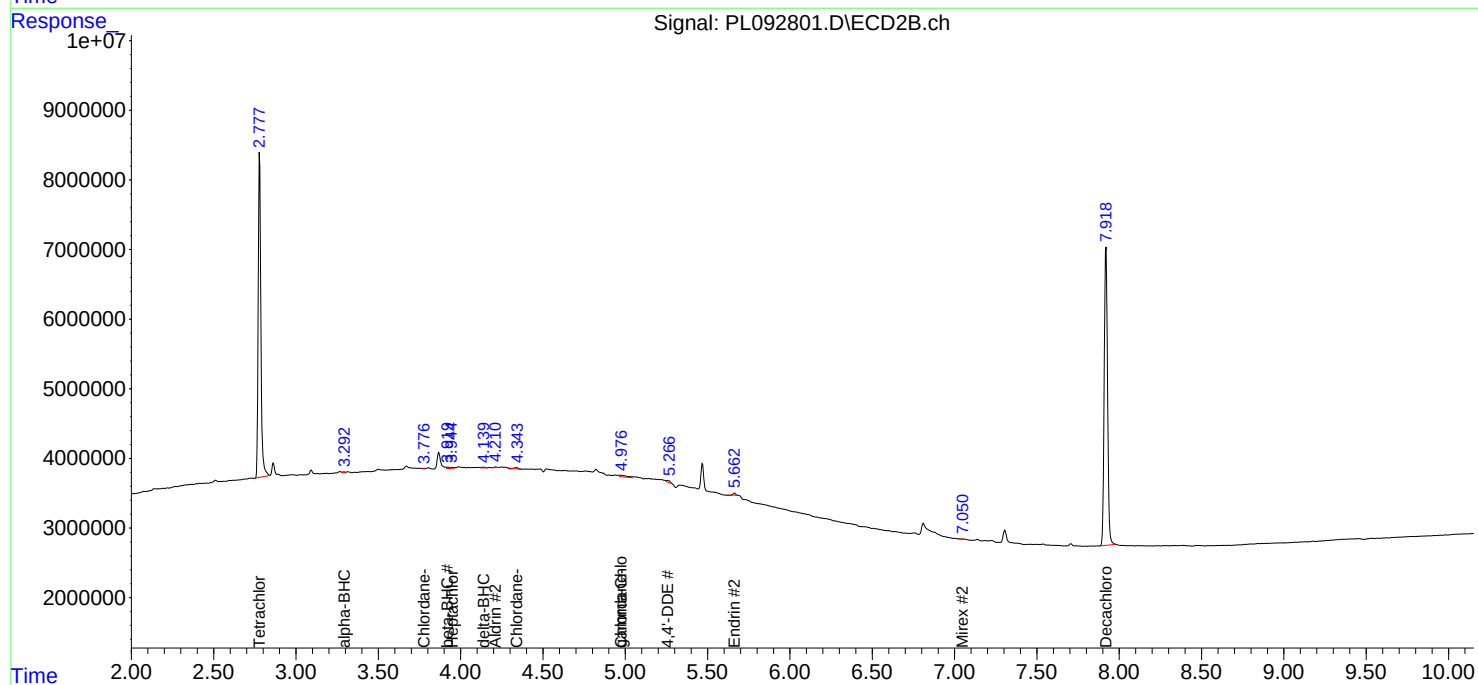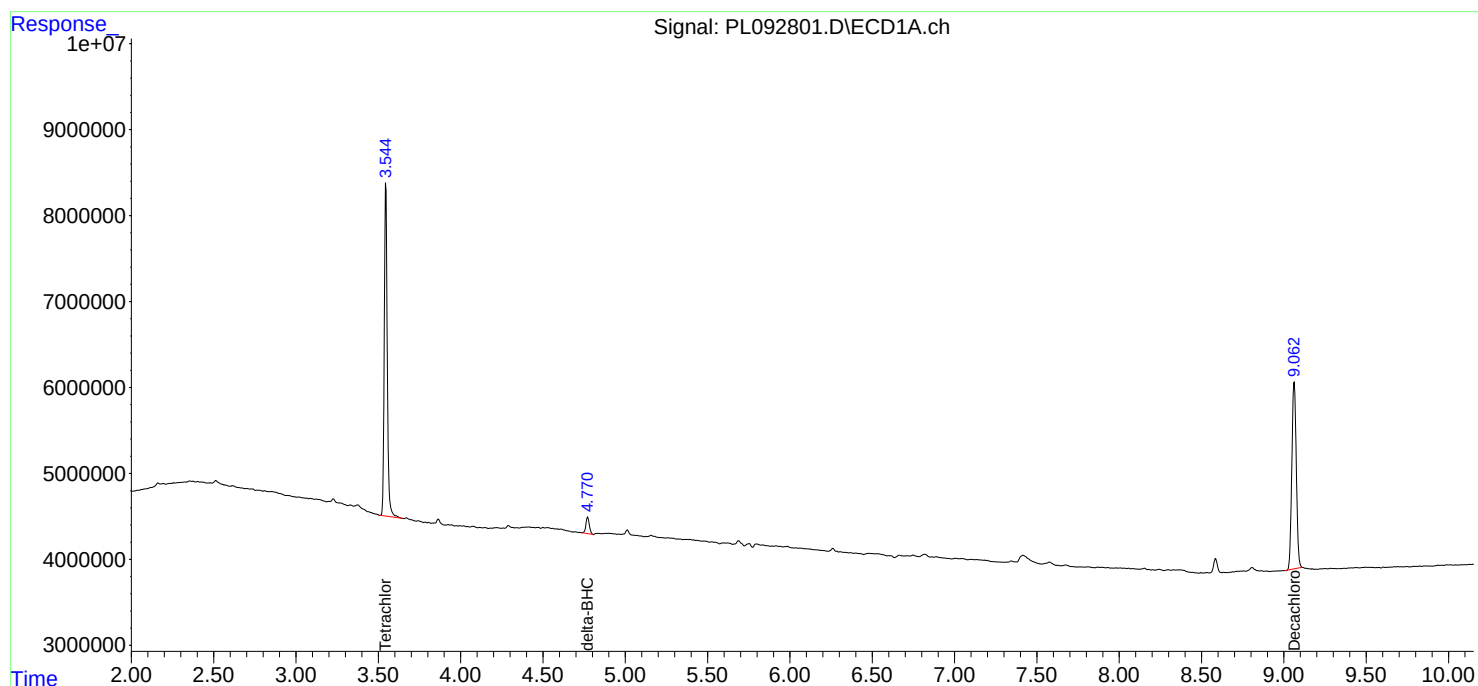


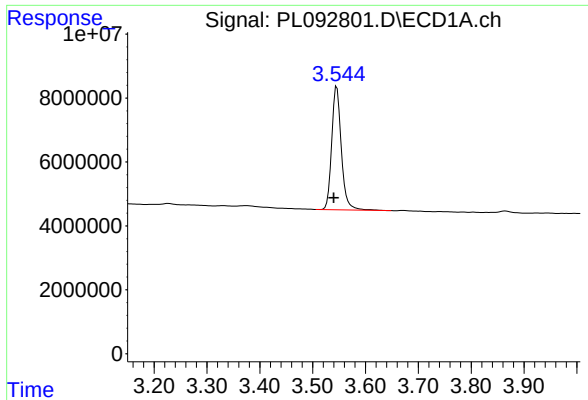

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: 0.006 min
Response: 48927386
Conc: 19.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB164592BL

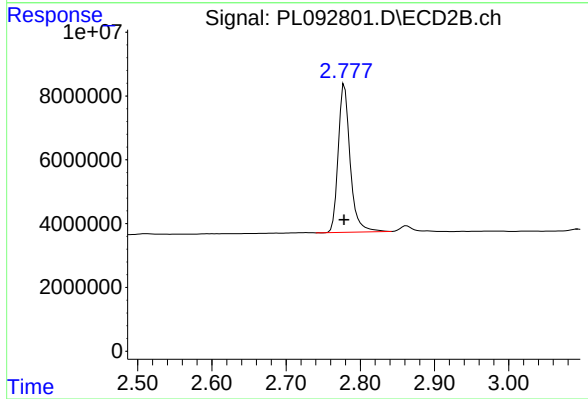


#1 Tetrachloro-m-xylene

R.T.: 2.779 min
Delta R.T.: 0.000 min
Response: 51903561
Conc: 19.07 ng/ml

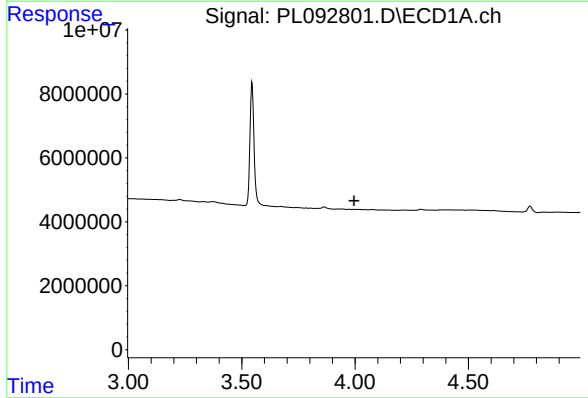


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.996 min
Response: 0
Conc: N.D.

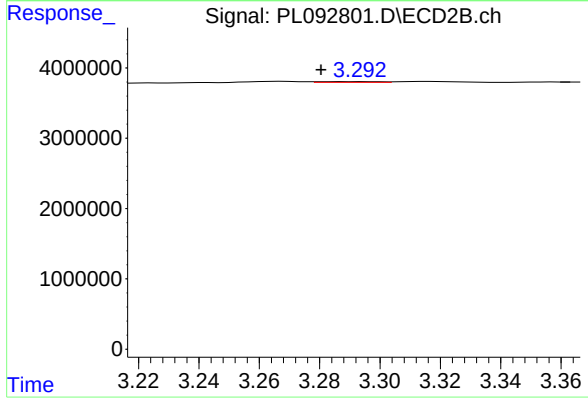

#2 alpha-BHC


R.T.: 3.293 min
Delta R.T.: 0.013 min
Response: 138037
Conc: 0.03 ng/ml

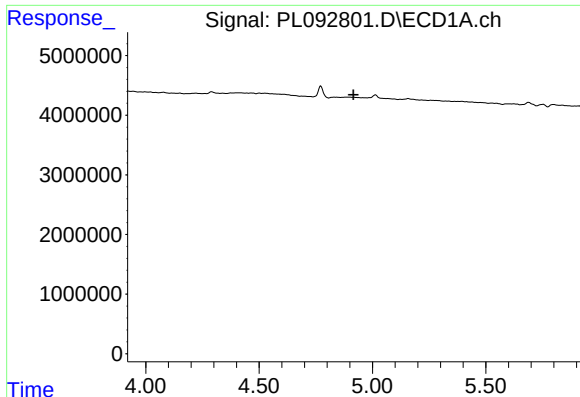

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.917 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB164592BL

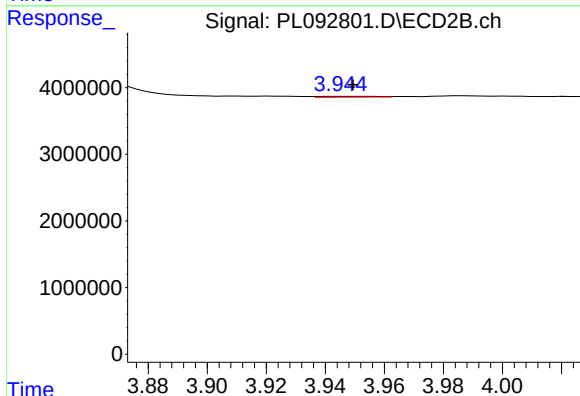


#4 Heptachlor

R.T.: 3.950 min
Delta R.T.: 0.000 min
Response: 181409
Conc: 0.05 ng/ml

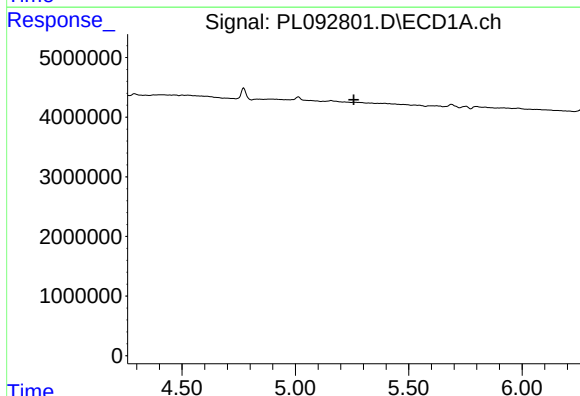


#5 Aldrin

R.T.: 0.000 min
Exp R.T.: 5.258 min
Response: 0
Conc: N.D.

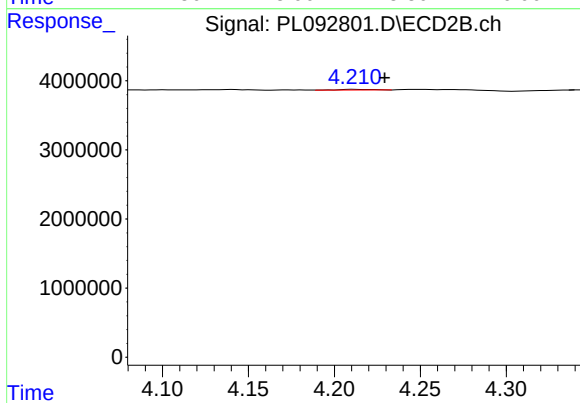

#5 Aldrin


R.T.: 4.212 min
Delta R.T.: -0.018 min
Response: 128494
Conc: 0.04 ng/ml

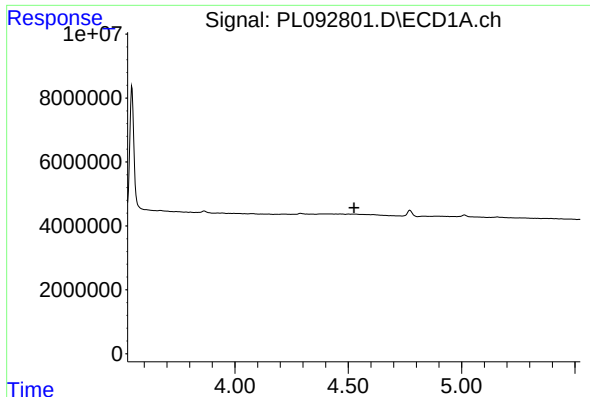

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.525 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB164592BL

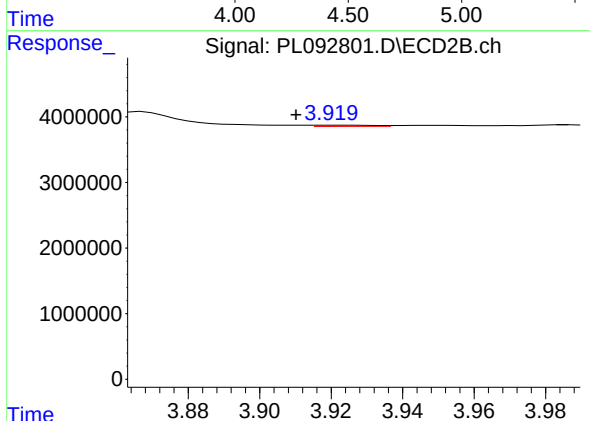


#6 beta-BHC

R.T.: 3.920 min
Delta R.T.: 0.010 min
Response: 212854
Conc: 0.13 ng/ml

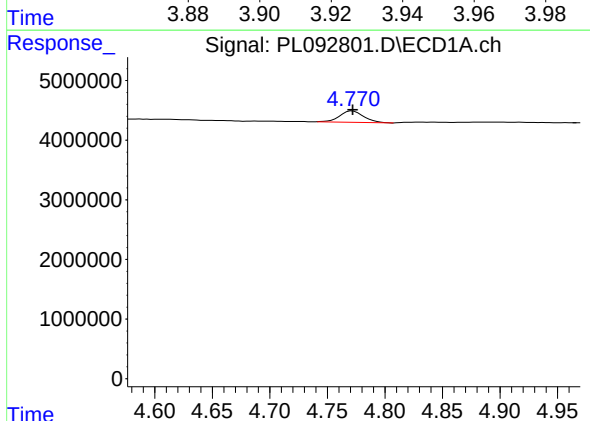


#7 delta-BHC

R.T.: 4.772 min
Delta R.T.: 0.000 min
Response: 2793008
Conc: 0.89 ng/ml

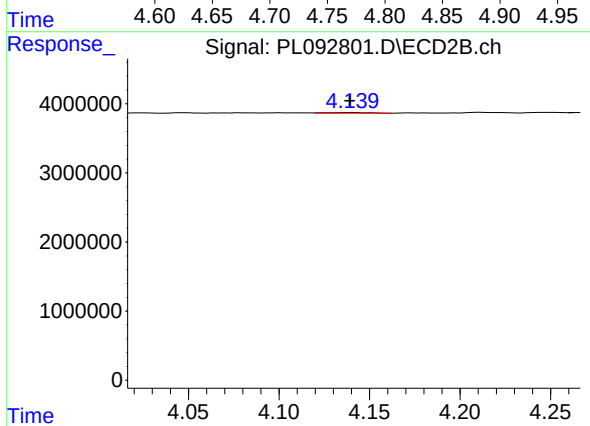

#7 delta-BHC


R.T.: 4.140 min
Delta R.T.: 0.001 min
Response: 159528
Conc: 0.04 ng/ml

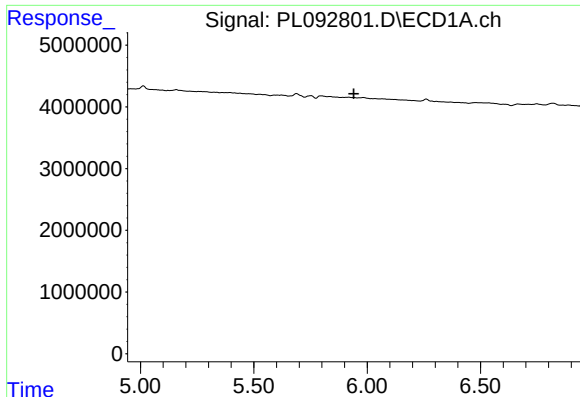

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.941 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB164592BL

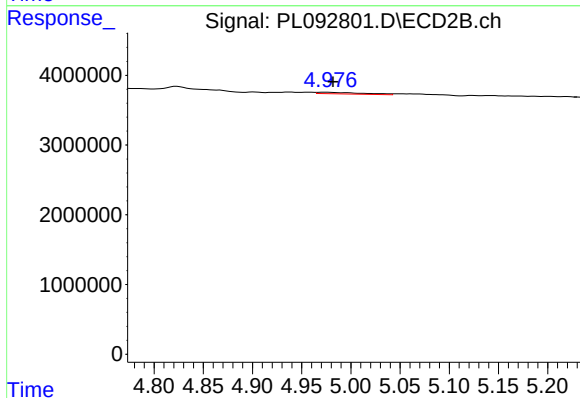


#10 gamma-Chlordane

R.T.: 4.975 min
Delta R.T.: -0.007 min
Response: 752112
Conc: 0.22 ng/ml

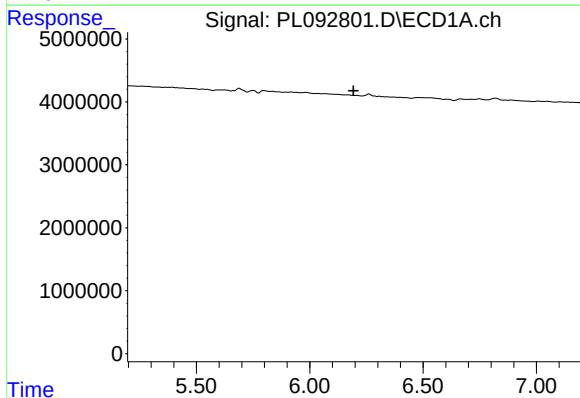


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 6.193 min
Response: 0
Conc: N.D.

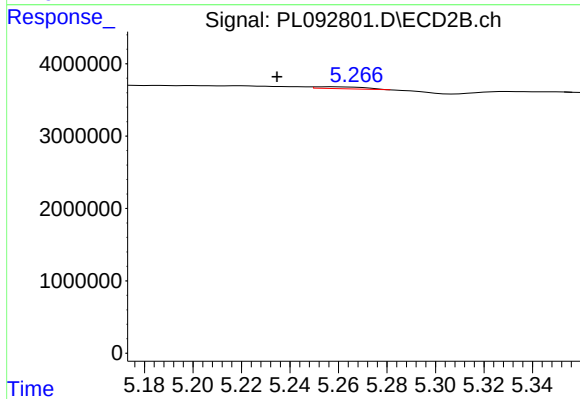

#12 4,4'-DDE


R.T.: 5.258 min
Delta R.T.: 0.024 min
Response: 330653
Conc: 0.10 ng/ml

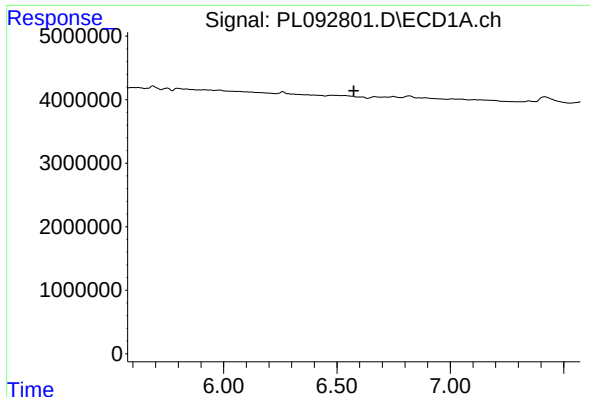

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.574 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB164592BL

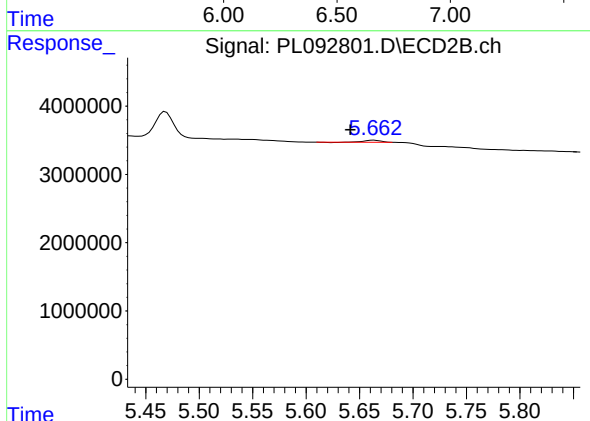


#14 Endrin

R.T.: 5.664 min
Delta R.T.: 0.022 min
Response: 310807
Conc: 0.11 ng/ml

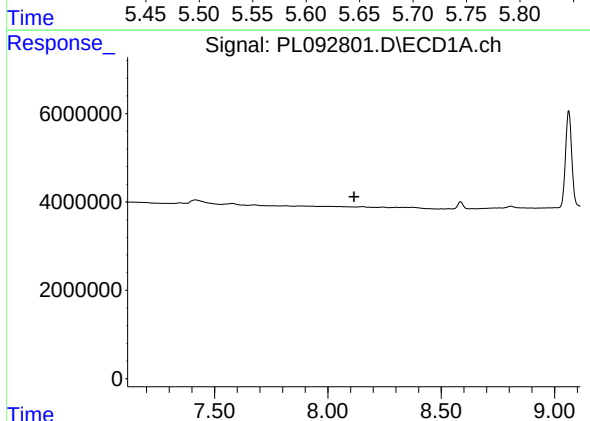


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 8.116 min
Response: 0
Conc: N.D.

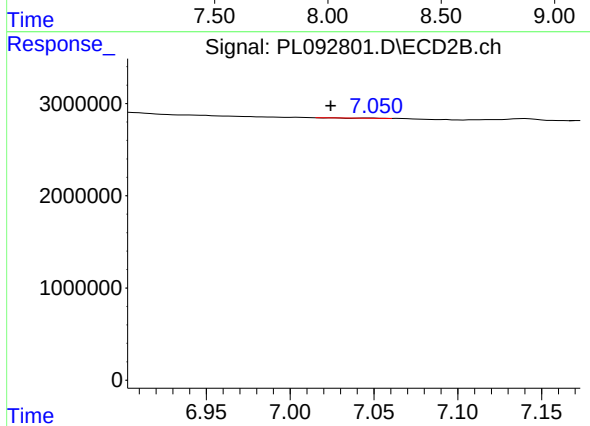

#22 Mirex


R.T.: 7.047 min
Delta R.T.: 0.023 min
Response: 4171
Conc: 0.00 ng/ml

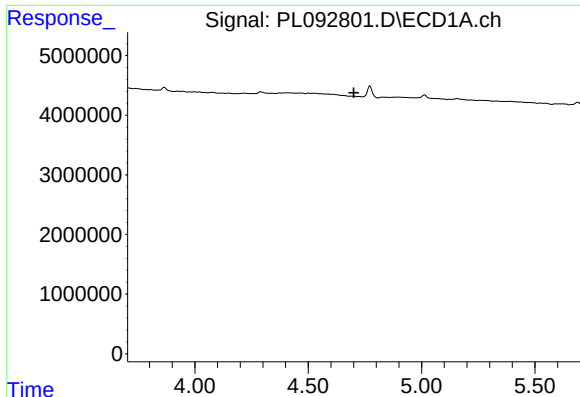

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.702 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB164592BL

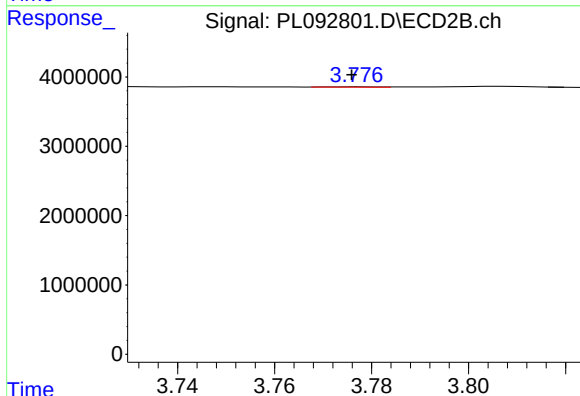


#23 Chlordane-1

R.T.: 3.777 min
Delta R.T.: 0.000 min
Response: 36857
Conc: 0.35 ng/ml

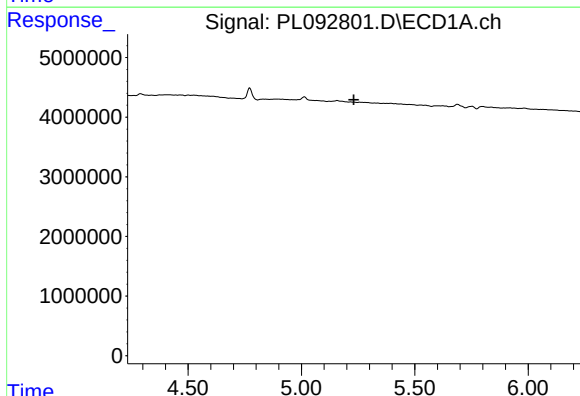


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 5.231 min
Response: 0
Conc: N.D.

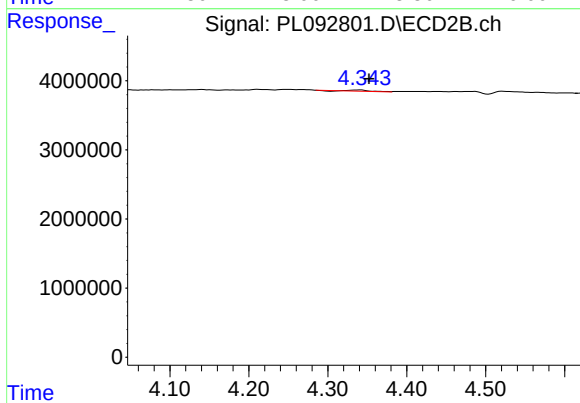

#24 Chlordane-2


R.T.: 4.342 min
Delta R.T.: -0.010 min
Response: 279895
Conc: 2.26 ng/ml

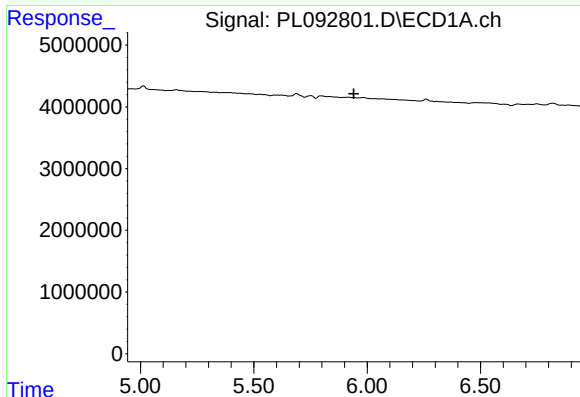

#25 Chlorine-3


R.T.: 0.000 min
Exp R.T.: 5.941 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB164592BL

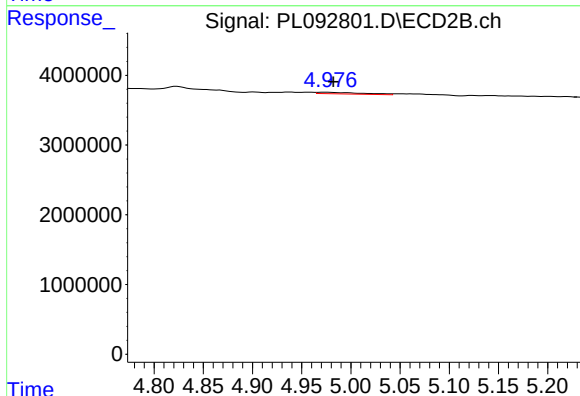


#25 Chlorine-3

R.T.: 4.975 min
Delta R.T.: -0.008 min
Response: 752112
Conc: 2.07 ng/ml

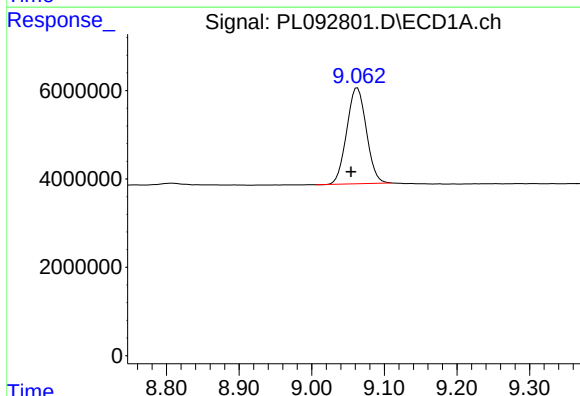

#28 Decachlorobiphenyl

R.T.: 9.063 min
Delta R.T.: 0.009 min
Response: 40833698
Conc: 21.22 ng/ml

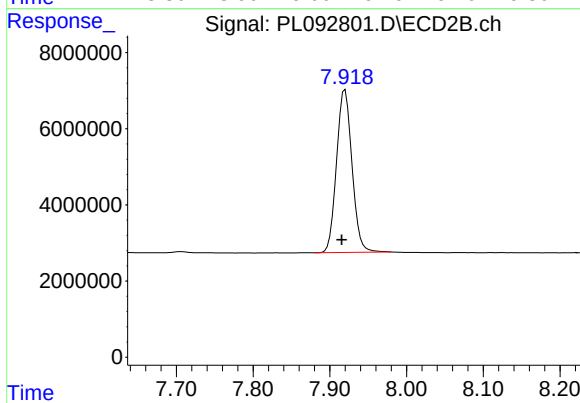

#28 Decachlorobiphenyl

R.T.: 7.920 min
Delta R.T.: 0.004 min
Response: 60045385
Conc: 22.00 ng/ml