

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110124\
 Data File : PL092807.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2024 16:10
 Operator : AR\AJ
 Sample : P4663-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RES-BUILDING-PAD-NO-11

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/04/2024
 Supervised By :Ankita Jodhani 11/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 01:44:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.541	2.778	35005478	35930823	14.287	13.204
28) SA Decachlor...	9.056	7.918	24606013	31940307	12.785m	11.703
Target Compounds						
12) B 4,4'-DDE	6.191	5.233	1443343	1644831	0.609m	0.511m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110124\
Data File : PL092807.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2024 16:10
Operator : AR\AJ
Sample : P4663-04
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
RES-BUILDING-PAD-NO-11


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/04/2024
Supervised By : Ankita Jodhani 11/04/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 01:44:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

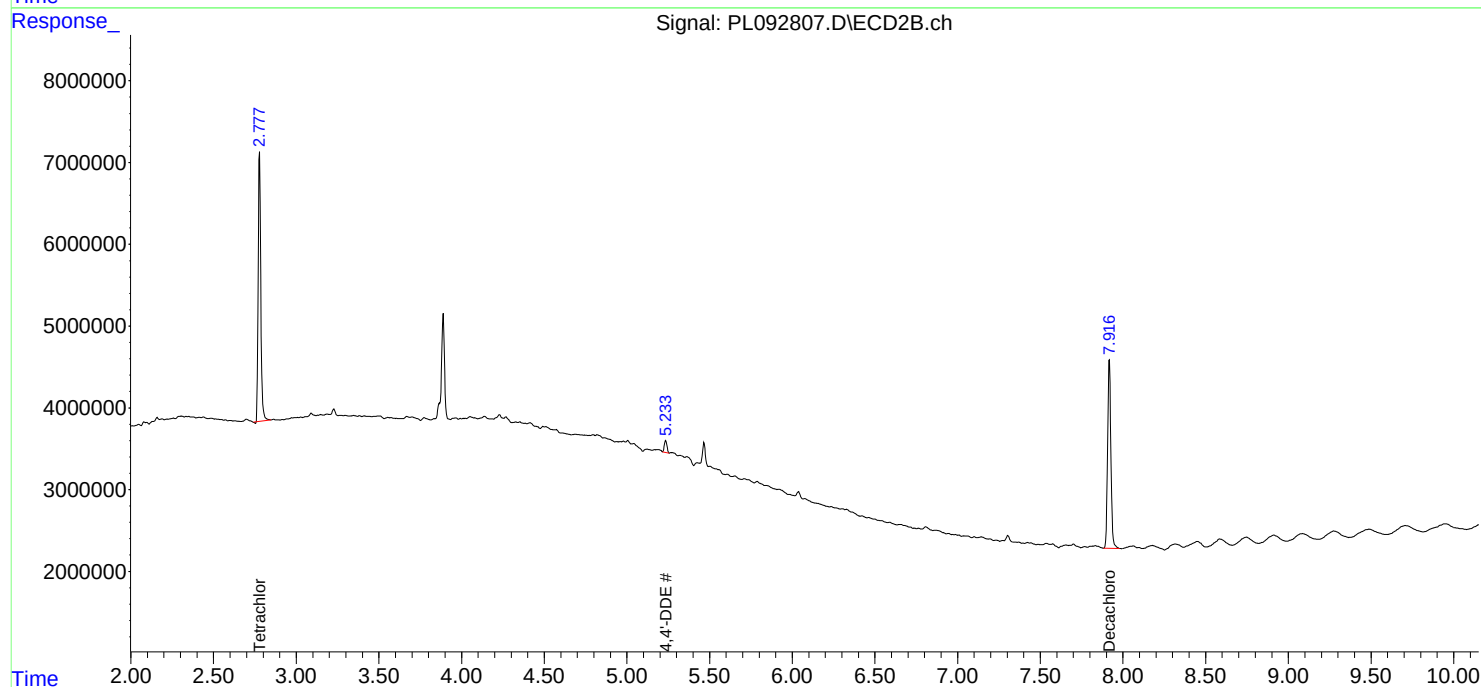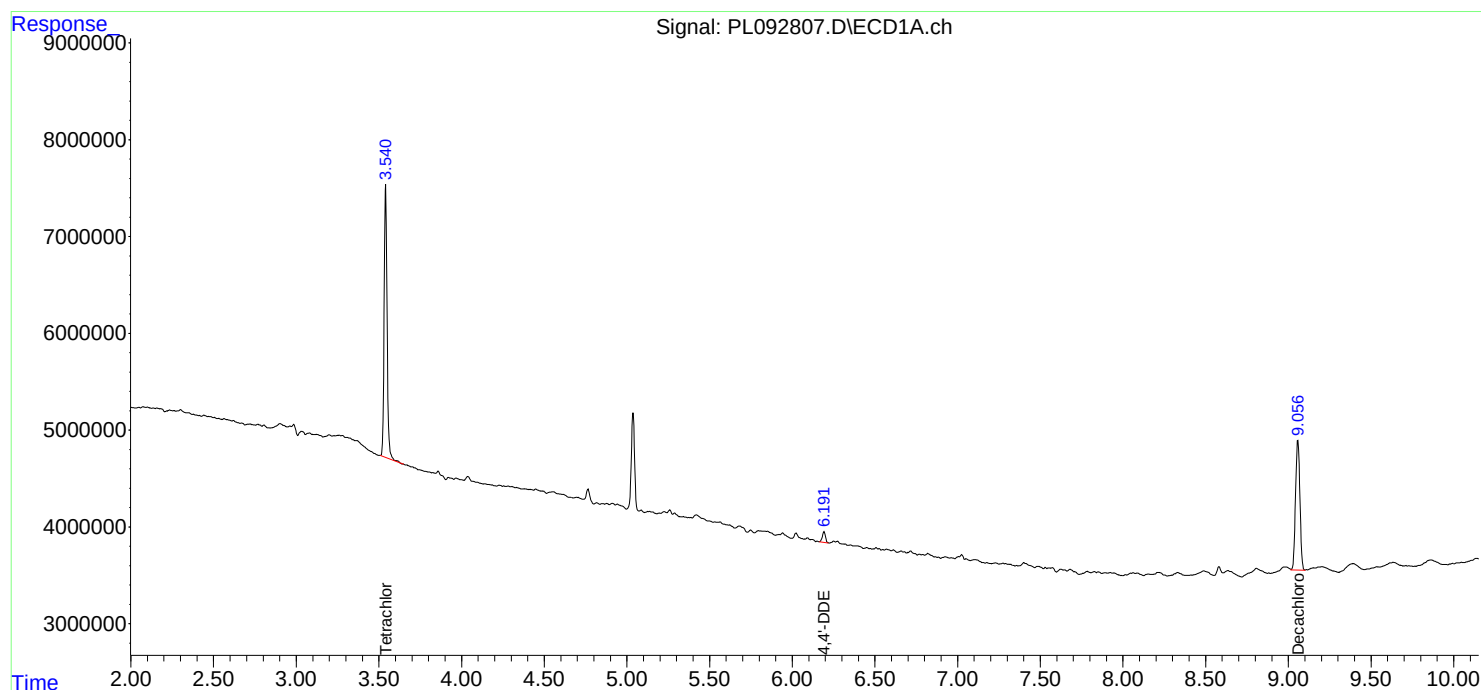

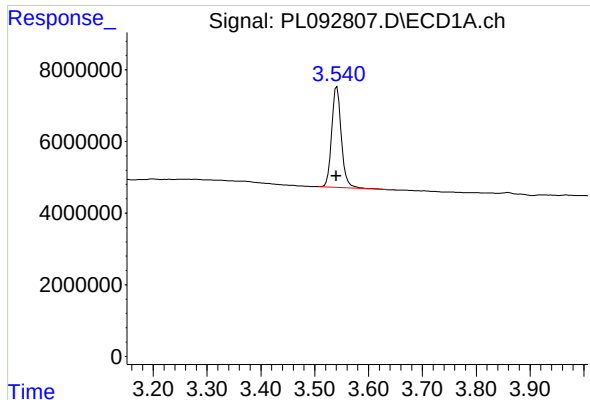


#1 Tetrachloro-m-xylene

R.T.: 3.541 min
Delta R.T.: 0.001 min
Response: 35005478
Conc: 14.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
RES-BUILDING-PAD-NO-11


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/04/2024
Supervised By :Ankita Jodhani 11/04/2024

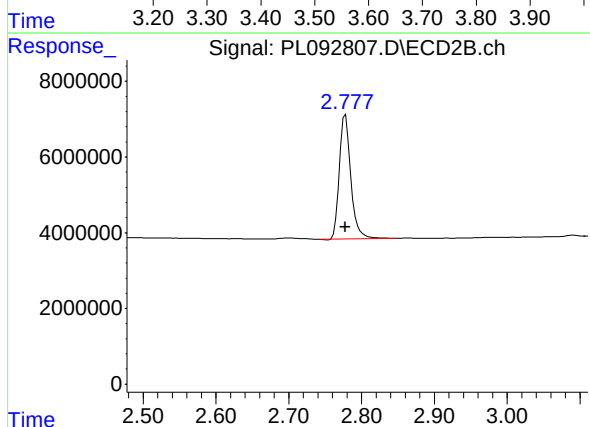


#1 Tetrachloro-m-xylene

R.T.: 2.778 min
Delta R.T.: 0.000 min
Response: 35930823
Conc: 13.20 ng/ml

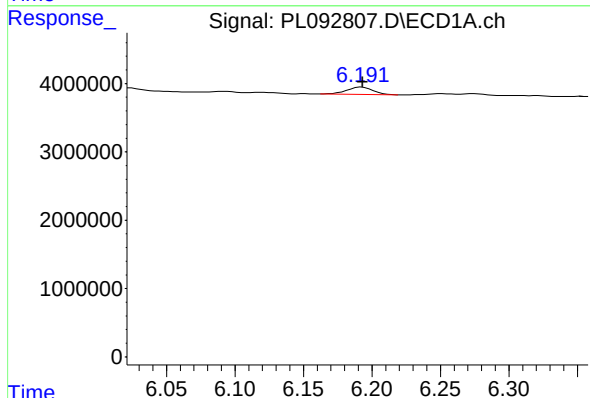


#12 4,4'-DDE

R.T.: 6.191 min
Delta R.T.: -0.002 min
Response: 1443343
Conc: 0.61 ng/ml m

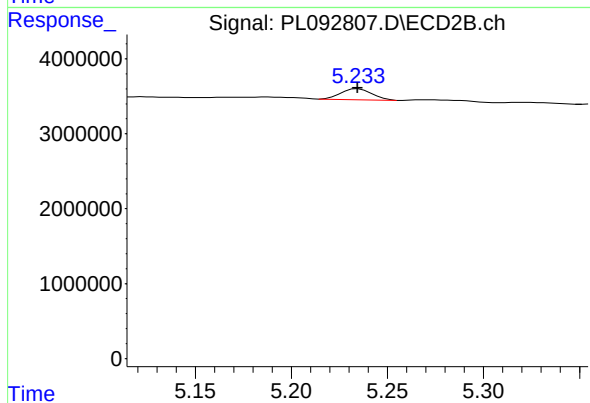

#12 4,4'-DDE

R.T.: 5.233 min
Delta R.T.: -0.001 min
Response: 1644831
Conc: 0.51 ng/ml m

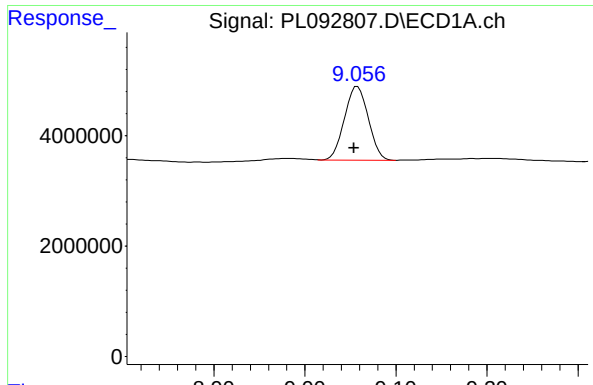


#28 Decachlorobiphenyl

R.T.: 9.056 min
Delta R.T.: 0.002 min
Response: 24606013
Conc: 12.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
RES-BUILDING-PAD-NO-11

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/04/2024
Supervised By :Ankita Jodhani 11/04/2024

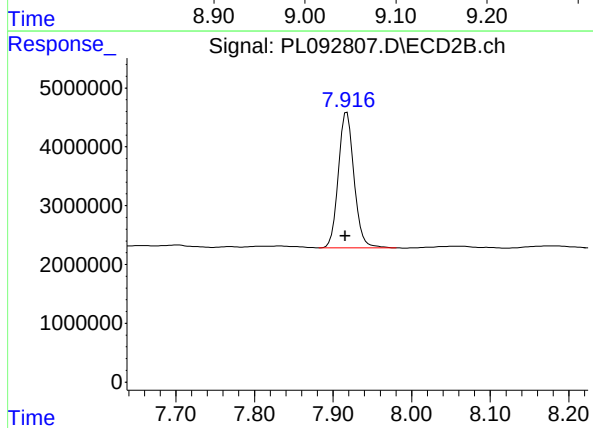

#28 Decachlorobiphenyl

R.T.: 7.918 min
Delta R.T.: 0.002 min
Response: 31940307
Conc: 11.70 ng/ml