

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110124\
 Data File : PL092808.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2024 16:24
 Operator : AR\AJ
 Sample : P4663-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RES-BUILDING-PAD-NO-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 01:44:21 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.542	2.778	36490088	39737059	14.892	14.603
28) SA Decachlor...	9.059	7.918	28504404	32312205	14.811	11.839

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110124\
Data File : PL092808.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2024 16:24
Operator : AR\AJ
Sample : P4663-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RES-BUILDING-PAD-NO-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 01:44:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

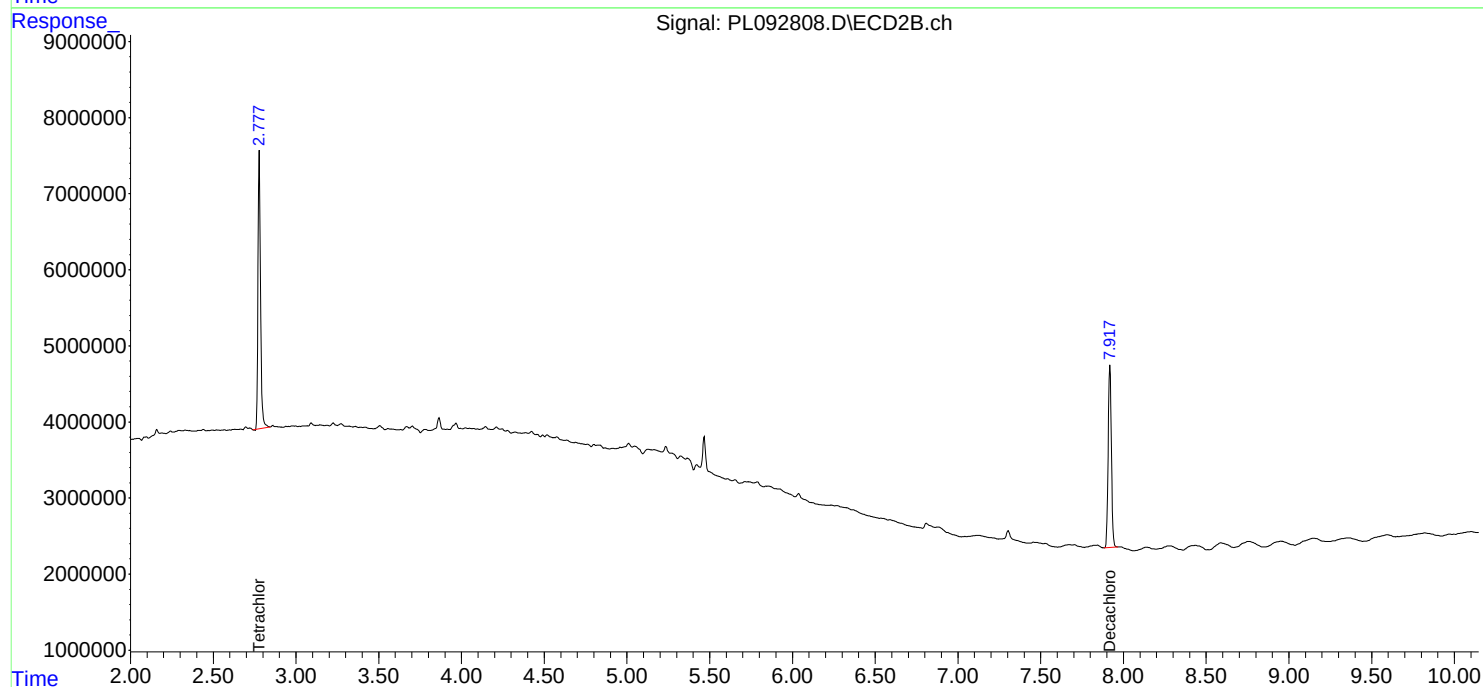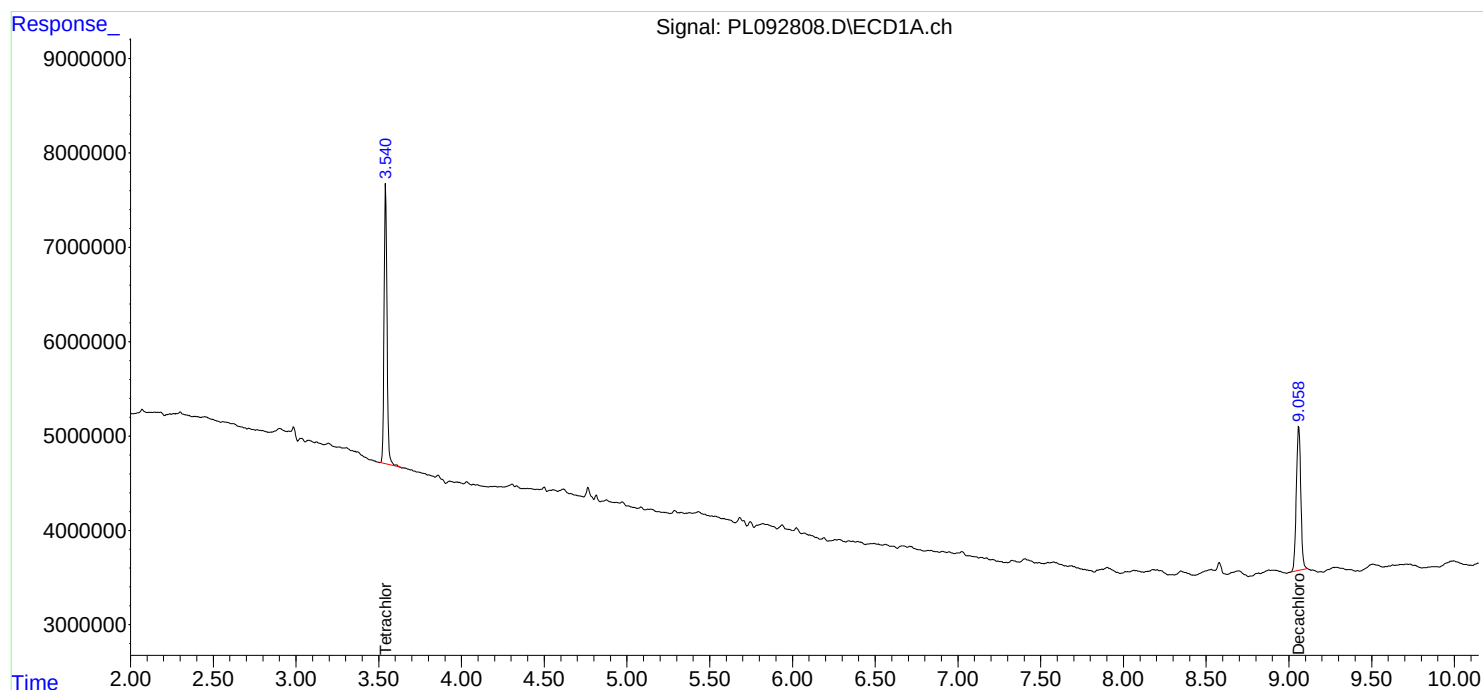


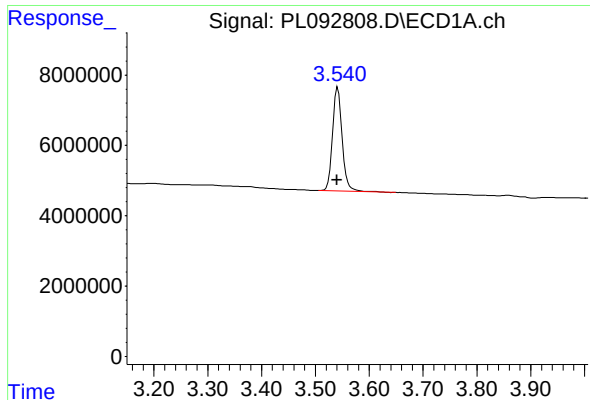

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: 0.002 min
Response: 36490088
Conc: 14.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
RES-BUILDING-PAD-NO-3

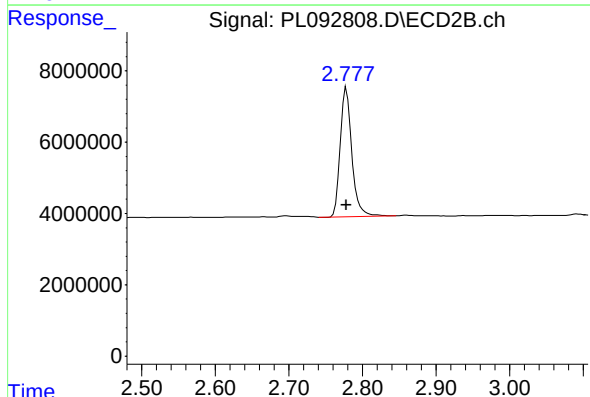


#1 Tetrachloro-m-xylene

R.T.: 2.778 min
Delta R.T.: 0.000 min
Response: 39737059
Conc: 14.60 ng/ml

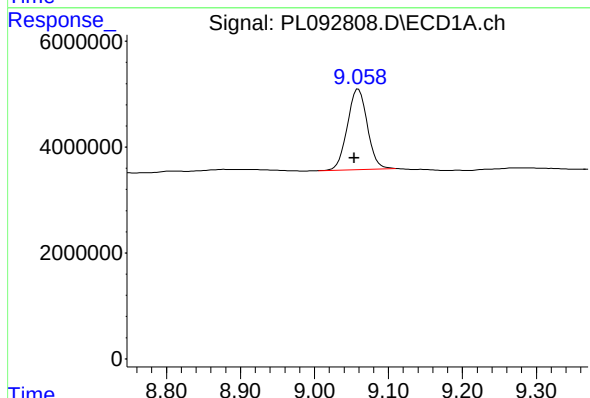

#28 Decachlorobiphenyl

R.T.: 9.059 min
Delta R.T.: 0.005 min
Response: 28504404
Conc: 14.81 ng/ml

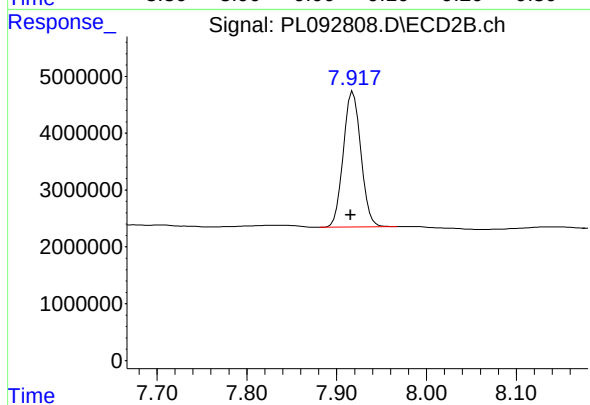

#28 Decachlorobiphenyl

R.T.: 7.918 min
Delta R.T.: 0.003 min
Response: 32312205
Conc: 11.84 ng/ml