

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110124\
 Data File : PL092809.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2024 16:38
 Operator : AR\AJ
 Sample : P4663-08
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RES-BUILDING-PAD-NO-2

Manual Integrations APPROVED

Reviewed By :Abdul Mirza 11/04/2024
 Supervised By :Ankita Jodhani 11/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 01:44:43 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.540	2.795	44171610	46707131	18.027m	17.164
28) SA Decachlor...	9.059	7.933	30794001	39266070	16.001	14.387m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110124\
Data File : PL092809.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2024 16:38
Operator : AR\AJ
Sample : P4663-08
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
RES-BUILDING-PAD-NO-2


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/04/2024
Supervised By : Ankita Jodhani 11/04/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 01:44:43 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

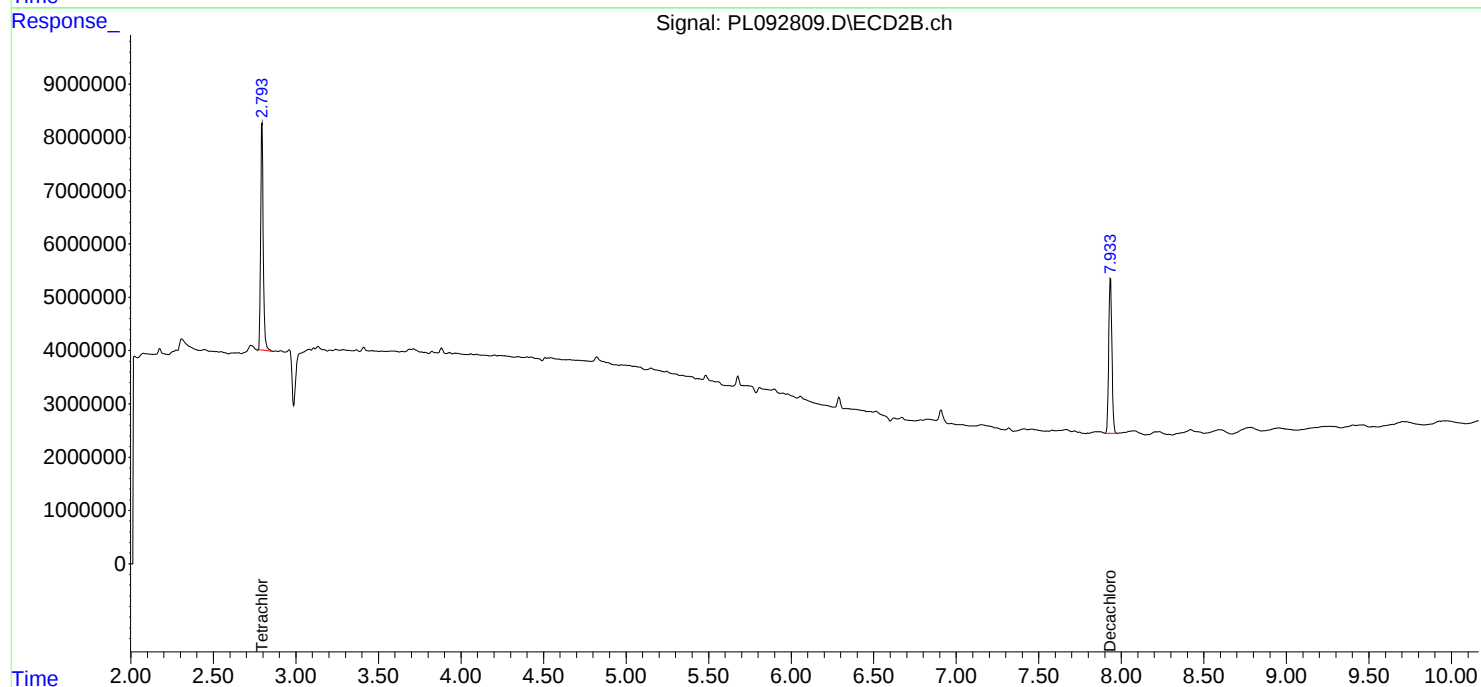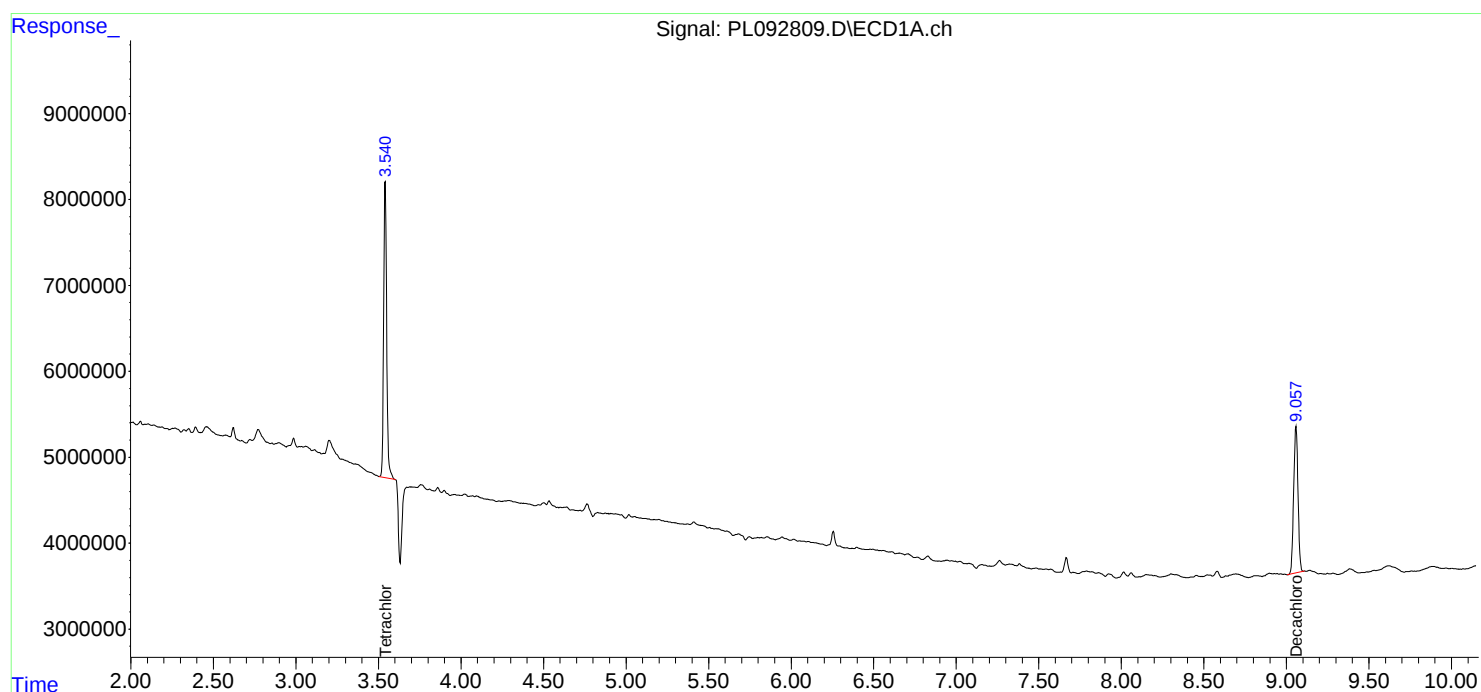

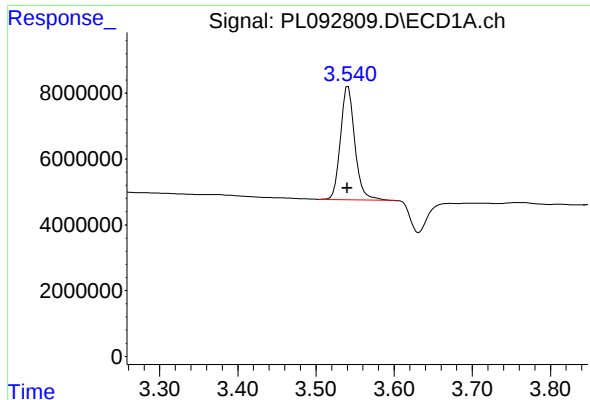


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: 0.000 min
Response: 44171610
Conc: 18.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
RES-BUILDING-PAD-NO-2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/04/2024
Supervised By :Ankita Jodhani 11/04/2024

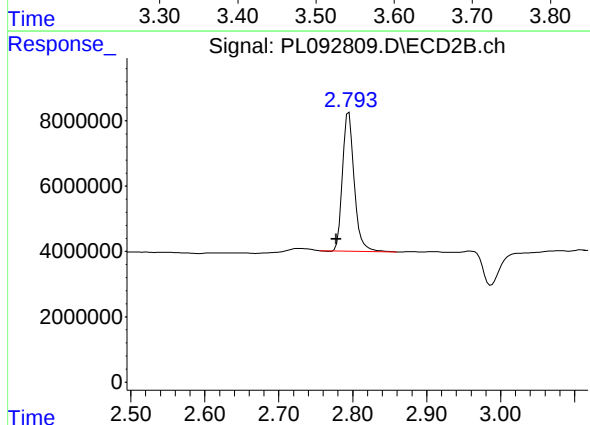


#1 Tetrachloro-m-xylene

R.T.: 2.795 min
Delta R.T.: 0.017 min
Response: 46707131
Conc: 17.16 ng/ml

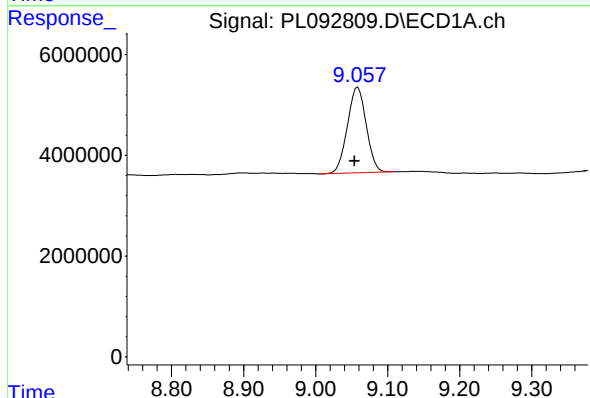

#28 Decachlorobiphenyl

R.T.: 9.059 min
Delta R.T.: 0.005 min
Response: 30794001
Conc: 16.00 ng/ml

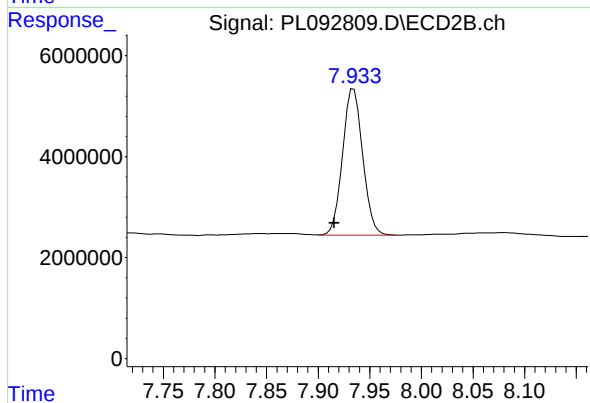

#28 Decachlorobiphenyl

R.T.: 7.933 min
Delta R.T.: 0.017 min
Response: 39266070
Conc: 14.39 ng/ml m