

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110218\
 Data File : PL041699.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2018 17:37
 Operator : AJ\SJ
 Sample : J5755-13
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-2A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 23:08:34 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.473	4.105	91091253	30393084	14.300	9.867 #
28)	SA Decachlor...	8.217	9.239	66485958	25887264	10.037	10.104
Target Compounds							
2)	A alpha-BHC	3.867f	0.000	11950610	0	1.230	N.D. #
6)	B beta-BHC	4.410f	0.000	6813773	0	1.808	N.D. #
7)	B delta-BHC	0.000	5.152f	0	1544927	N.D.	0.383 #
9)	A Endosulfan I	5.502	0.000	915458	0	0.123	N.D. #
11)	B alpha-Chl...	5.502	0.000	915458	0	0.113	N.D. #
23)	Chlordane-1	4.345	5.152	1993561	1544927	7.031	11.123 #
24)	Chlordane-2	0.000	5.546	0	2347830	N.D.	17.668 #
26)	Chlordane-4	5.502	0.000	915458	0	1.169	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110218\
Data File : PL041699.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2018 17:37
Operator : AJ\SJ
Sample : J5755-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP-2A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 23:08:34 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

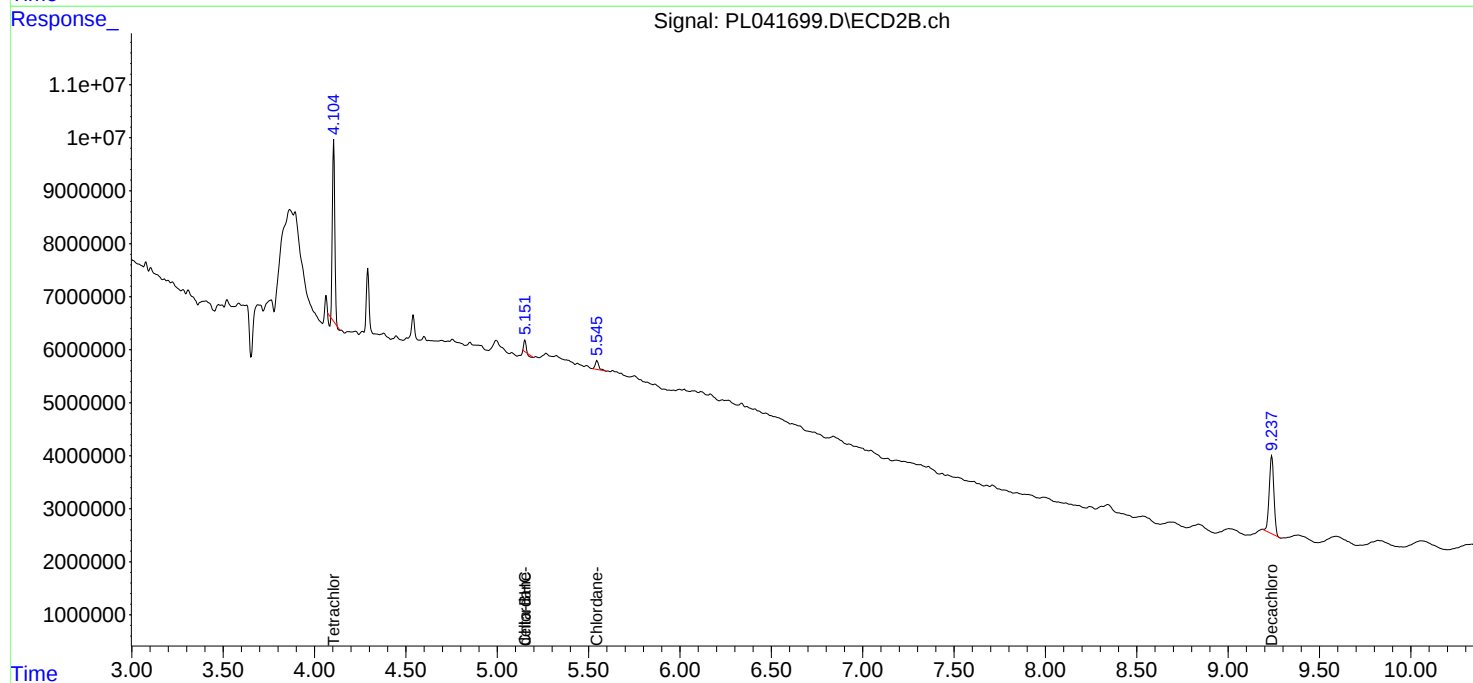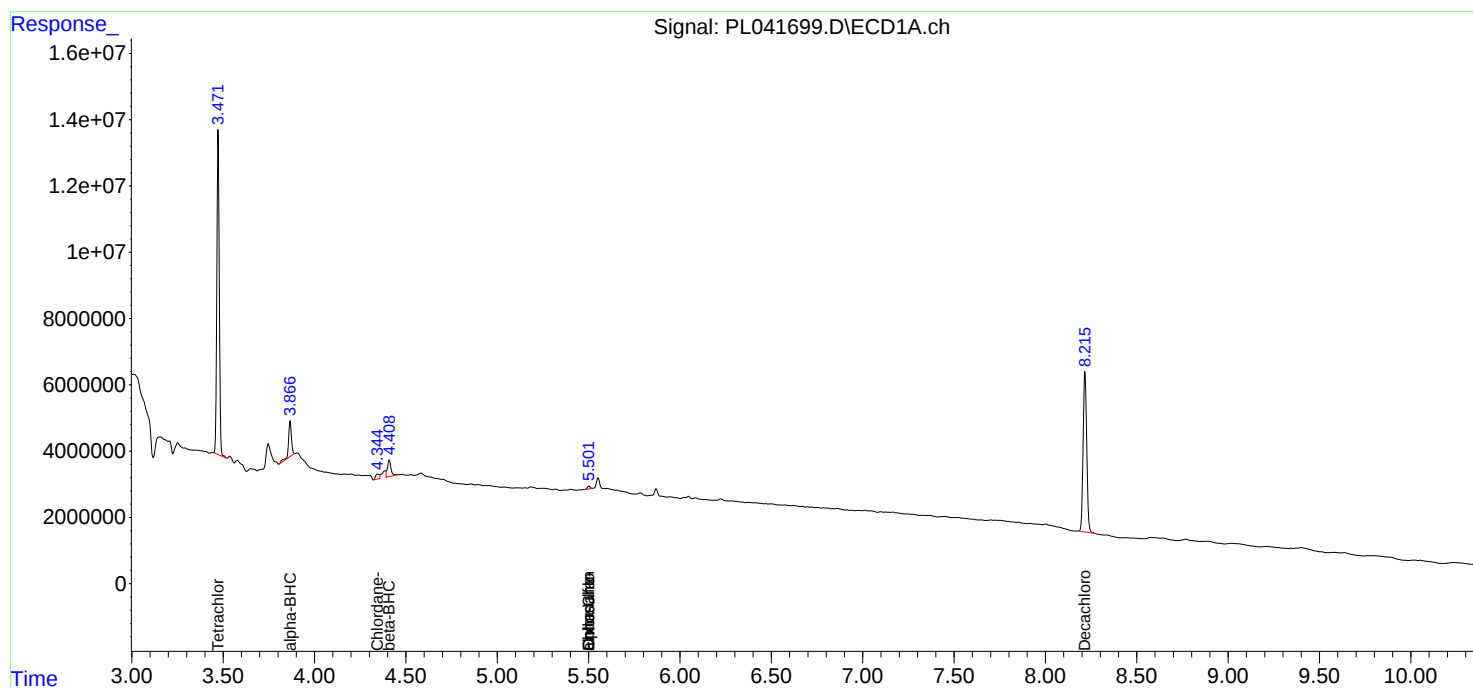


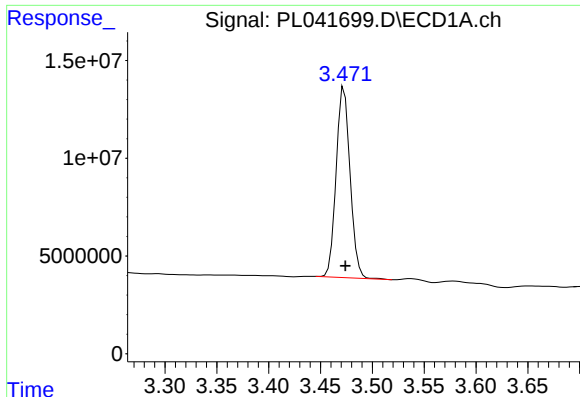

#1 Tetrachloro-m-xylene


R.T.: 3.473 min
Delta R.T.: -0.001 min
Response: 91091253
Conc: 14.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2A

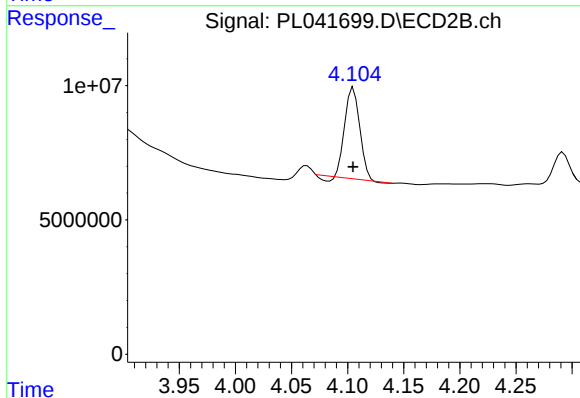


#1 Tetrachloro-m-xylene

R.T.: 4.105 min
Delta R.T.: 0.000 min
Response: 30393084
Conc: 9.87 ng/ml

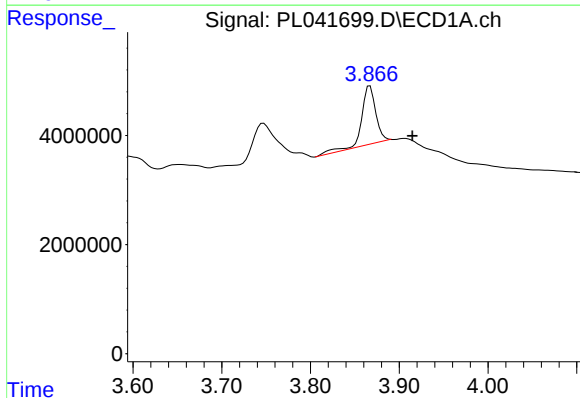


#2 alpha-BHC

R.T.: 3.867 min
Delta R.T.: -0.048 min
Response: 11950610
Conc: 1.23 ng/ml

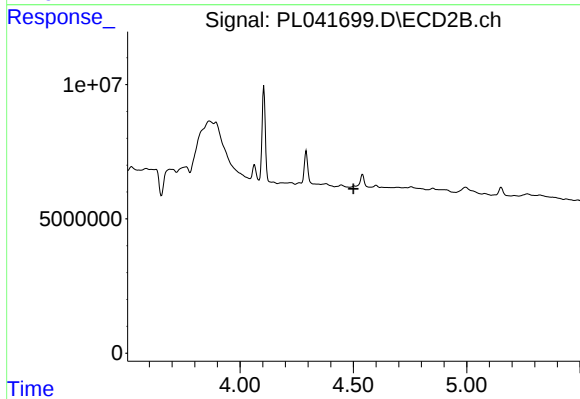

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.501 min
Response: 0
Conc: N.D.

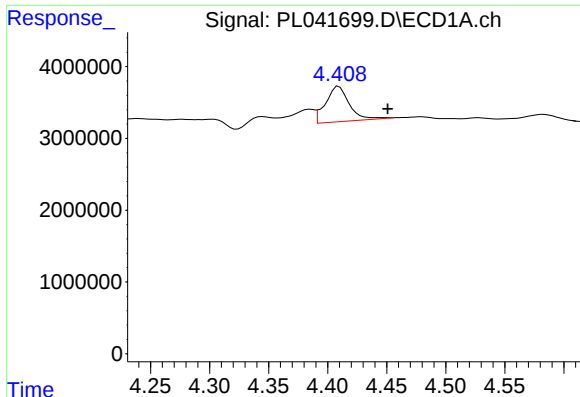

#6 beta-BHC


R.T.: 4.410 min
Delta R.T.: -0.041 min
Response: 6813773
Conc: 1.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2A

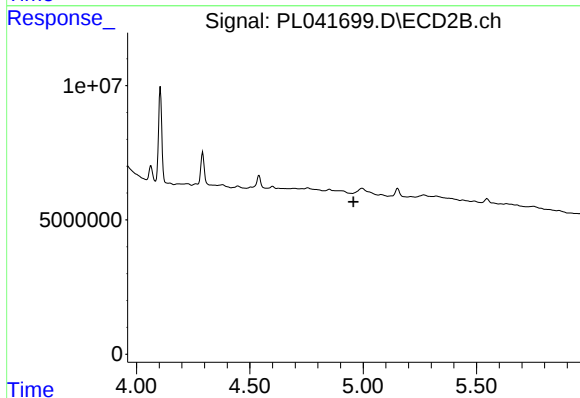


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.957 min
Response: 0
Conc: N.D.

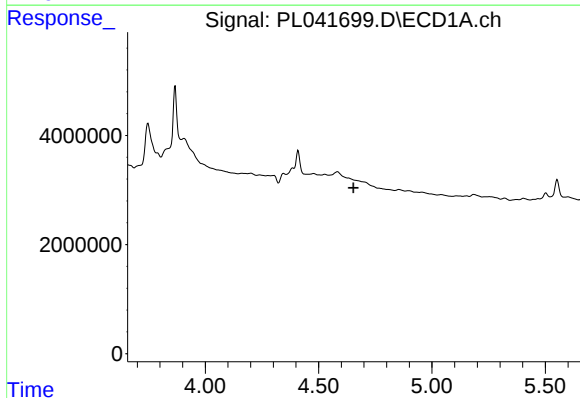


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.654 min
Response: 0
Conc: N.D.

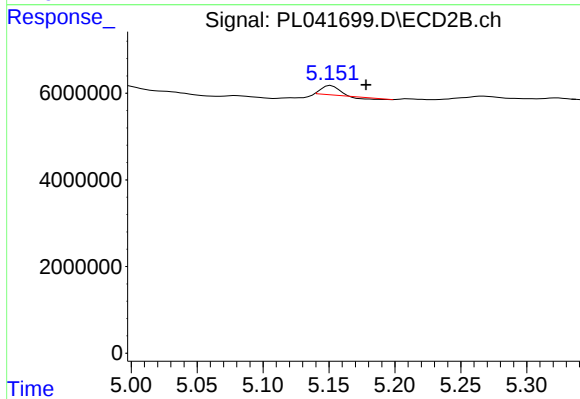

#7 delta-BHC


R.T.: 5.152 min
Delta R.T.: -0.027 min
Response: 1544927
Conc: 0.38 ng/ml

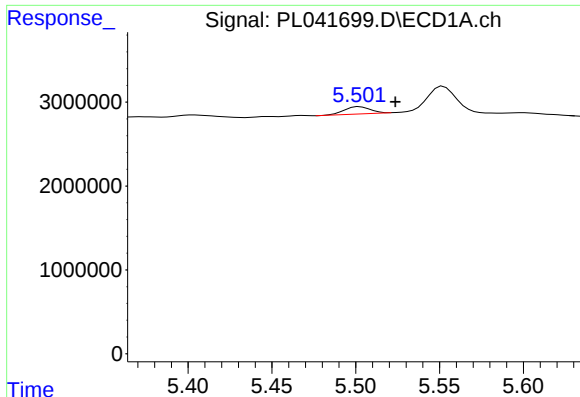

#9 Endosulfan I


R.T.: 5.502 min
Delta R.T.: -0.021 min
Response: 915458
Conc: 0.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2A

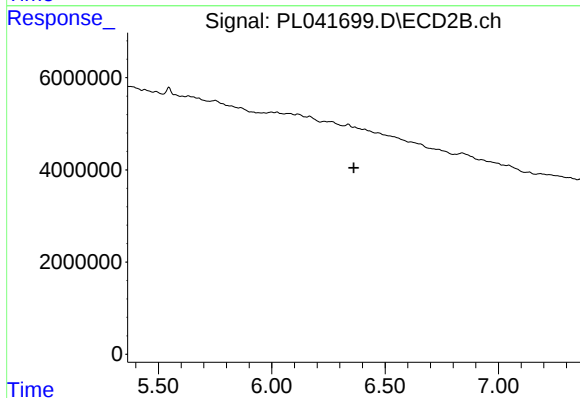


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

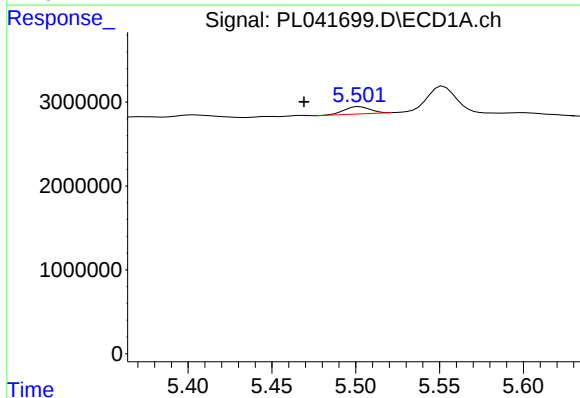


#11 alpha-Chlordane

R.T.: 5.502 min
Delta R.T.: 0.033 min
Response: 915458
Conc: 0.11 ng/ml

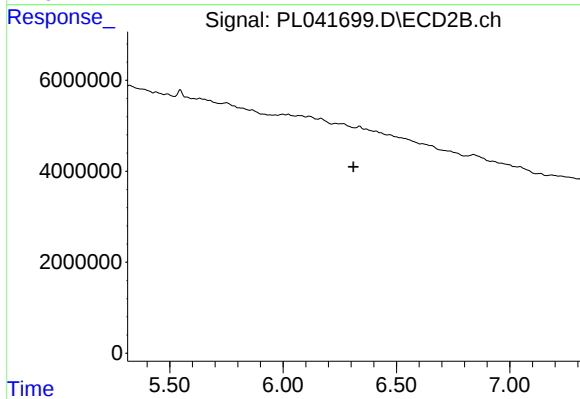

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.311 min
Response: 0
Conc: N.D.

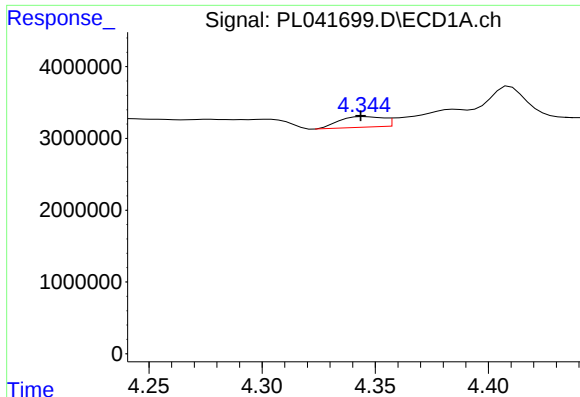

#23 Chlordane-1


R.T.: 4.345 min
Delta R.T.: 0.002 min
Response: 1993561
Conc: 7.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2A

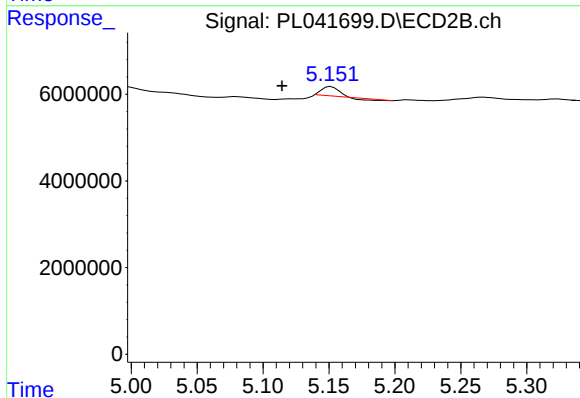


#23 Chlordane-1

R.T.: 5.152 min
Delta R.T.: 0.037 min
Response: 1544927
Conc: 11.12 ng/ml

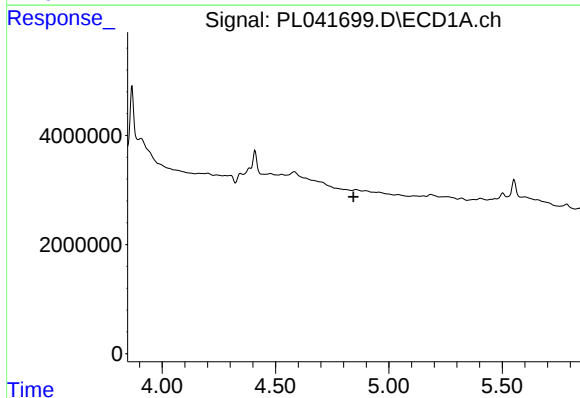


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.844 min
Response: 0
Conc: N.D.

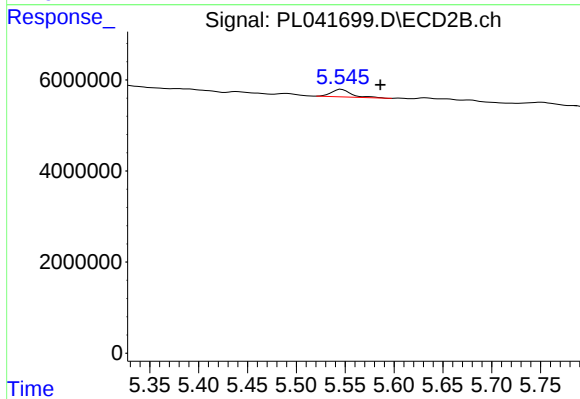

#24 Chlordane-2


R.T.: 5.546 min
Delta R.T.: -0.040 min
Response: 2347830
Conc: 17.67 ng/ml

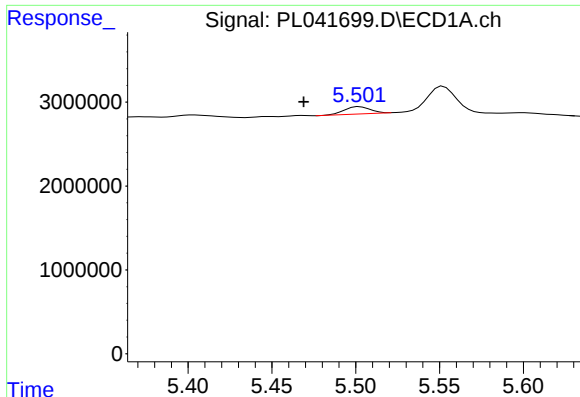

#26 Chlordane-4


R.T.: 5.502 min
Delta R.T.: 0.033 min
Response: 915458
Conc: 1.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2A

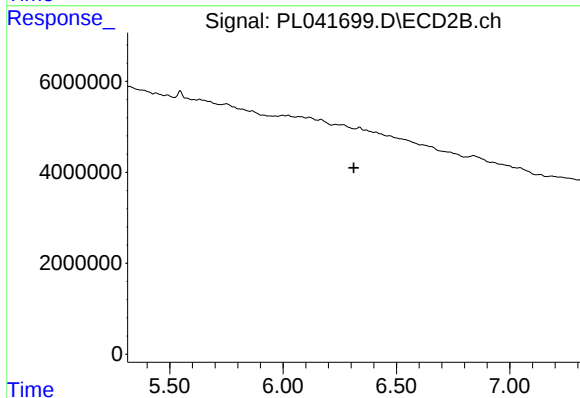


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.311 min
Response: 0
Conc: N.D.

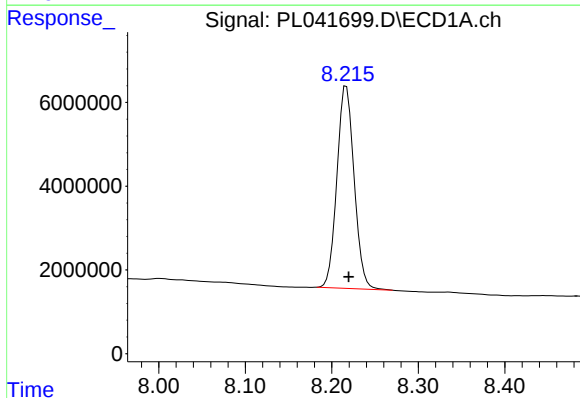

#28 Decachlorobiphenyl

R.T.: 8.217 min
Delta R.T.: -0.003 min
Response: 66485958
Conc: 10.04 ng/ml

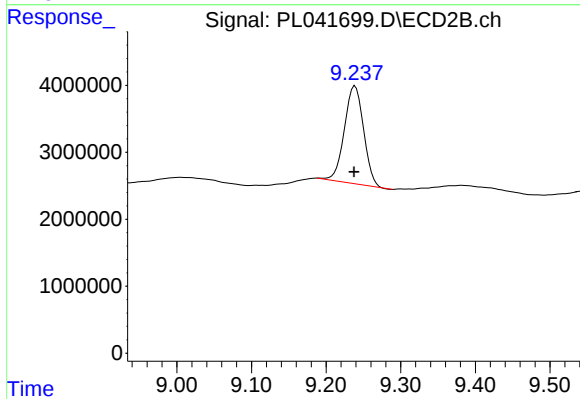

#28 Decachlorobiphenyl

R.T.: 9.239 min
Delta R.T.: 0.001 min
Response: 25887264
Conc: 10.10 ng/ml