

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110218\
 Data File : PL041722.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2018 23:02
 Operator : AJ\SJ
 Sample : J5794-11
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-10B-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 00:52:42 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.472	4.105	62037473	33414373	9.739	10.848
28)	SA Decachlor...	8.218	9.240	67689373	27588676	10.219	10.768
Target Compounds							
2)	A alpha-BHC	3.908	0.000	2481423	0	0.255	N.D. #
6)	B beta-BHC	4.409f	4.909f	4377939	1677914	1.162	0.977
8)	B Heptachlo...	5.236f	0.000	13125	0	0.002	N.D. #
13)	MA Dieldrin	5.758	0.000	2372074	0	0.298	N.D. #
16)	A 4,4'-DDD	6.221f	0.000	2776603	0	0.478	N.D. #
17)	MA 4,4'-DDT	6.383	0.000	2462597	0	0.405	N.D. #
23)	Chlordane-1	4.409	0.000	4377939	0	15.440	N.D. #
24)	Chlordane-2	4.824	0.000	1848095	0	6.275	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110218\
Data File : PL041722.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2018 23:02
Operator : AJ\SJ
Sample : J5794-11
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-10B-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 00:52:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

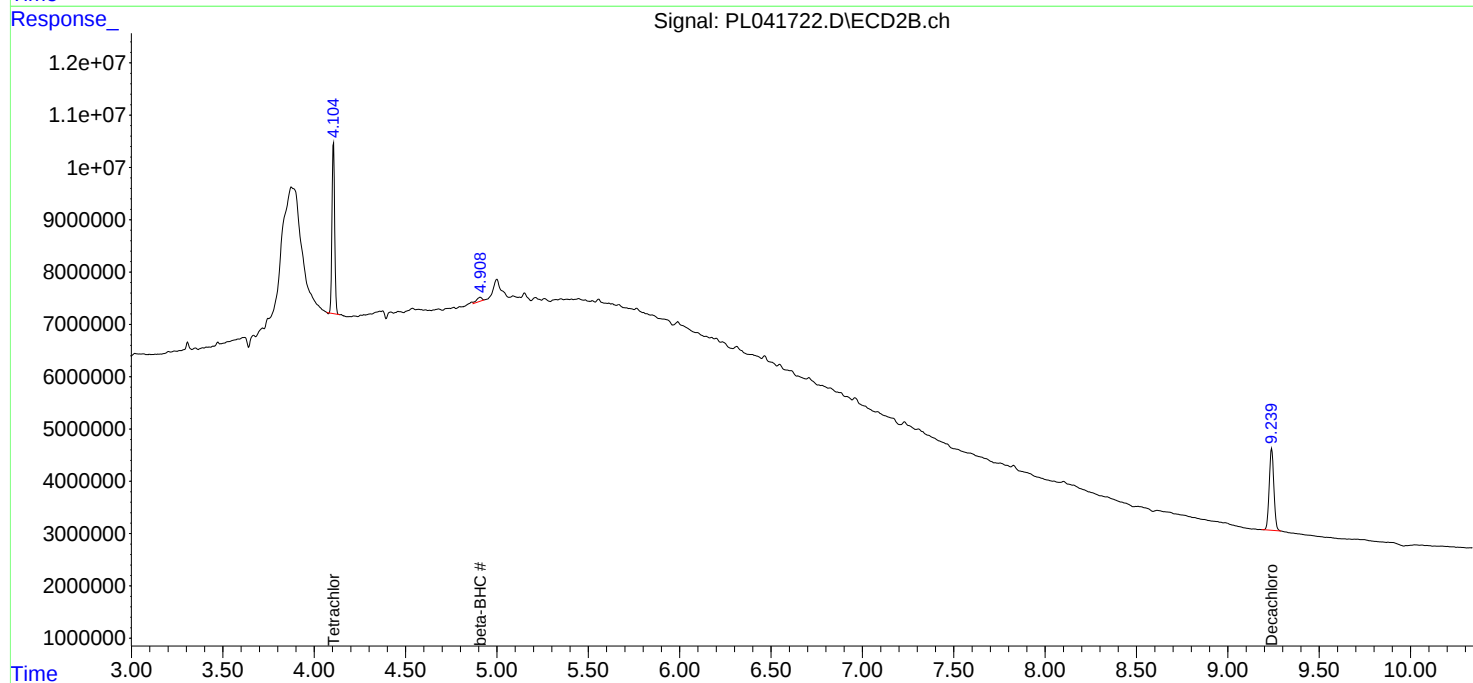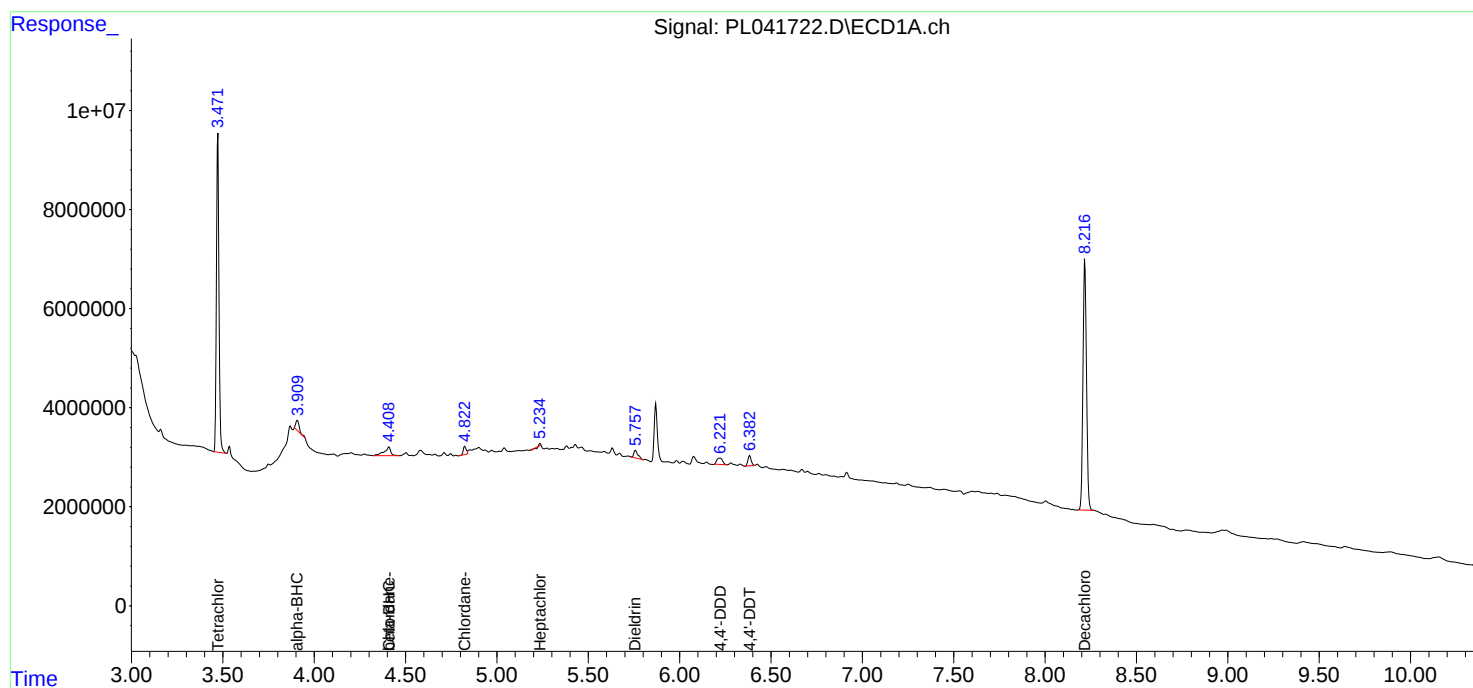


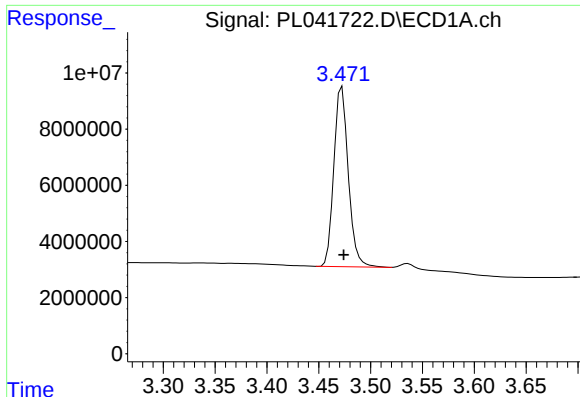

#1 Tetrachloro-m-xylene


R.T.: 3.472 min
Delta R.T.: -0.002 min
Response: 62037473
Conc: 9.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-10B-S

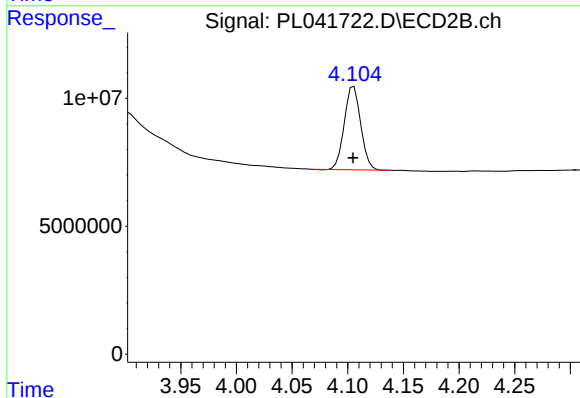


#1 Tetrachloro-m-xylene

R.T.: 4.105 min
Delta R.T.: 0.000 min
Response: 33414373
Conc: 10.85 ng/ml

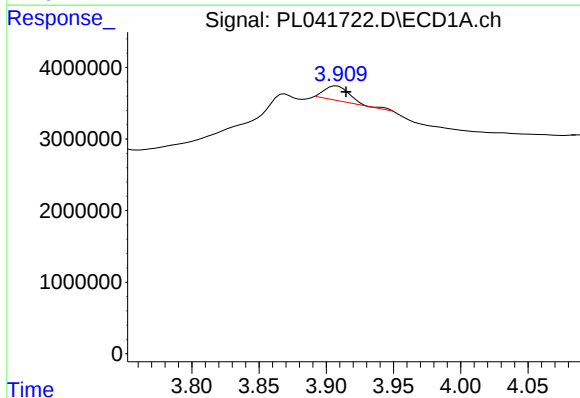


#2 alpha-BHC

R.T.: 3.908 min
Delta R.T.: -0.007 min
Response: 2481423
Conc: 0.26 ng/ml

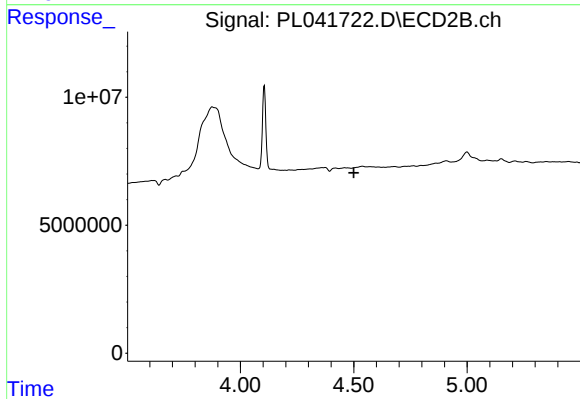

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.501 min
Response: 0
Conc: N.D.

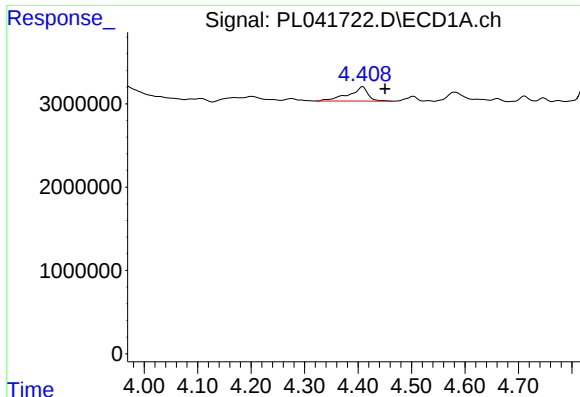

#6 beta-BHC


R.T.: 4.409 min
Delta R.T.: -0.042 min
Response: 4377939
Conc: 1.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-10B-S

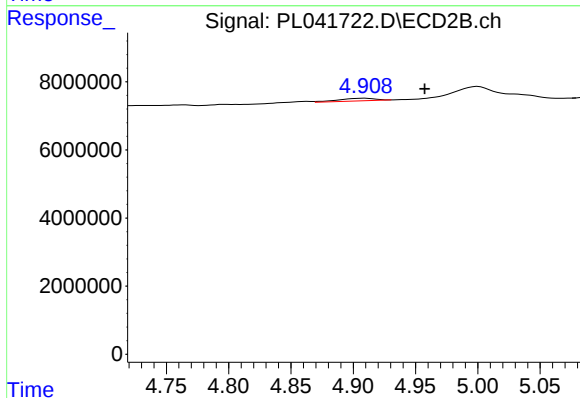


#6 beta-BHC

R.T.: 4.909 min
Delta R.T.: -0.048 min
Response: 1677914
Conc: 0.98 ng/ml

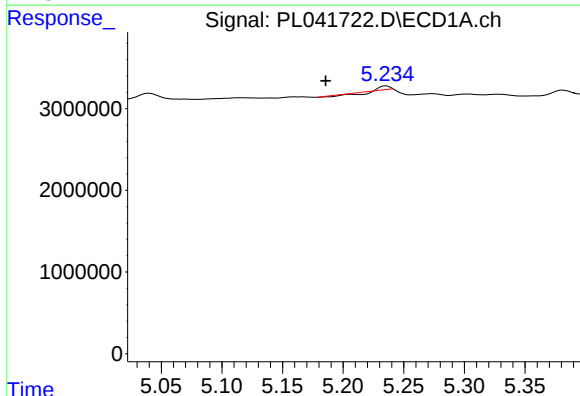


#8 Heptachlor epoxide

R.T.: 5.236 min
Delta R.T.: 0.050 min
Response: 13125
Conc: 0.00 ng/ml

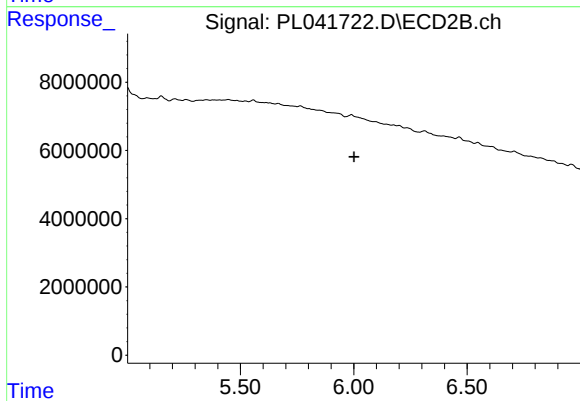

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 6.002 min
Response: 0
Conc: N.D.

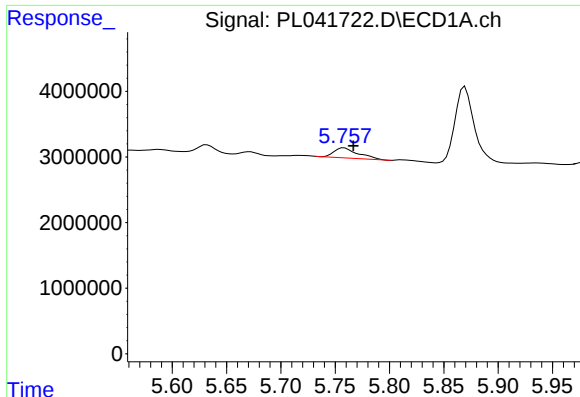

#13 Dieldrin


R.T.: 5.758 min
Delta R.T.: -0.008 min
Response: 2372074
Conc: 0.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-10B-S

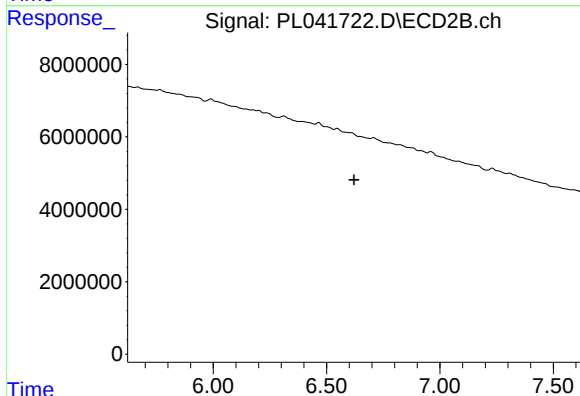


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.621 min
Response: 0
Conc: N.D.

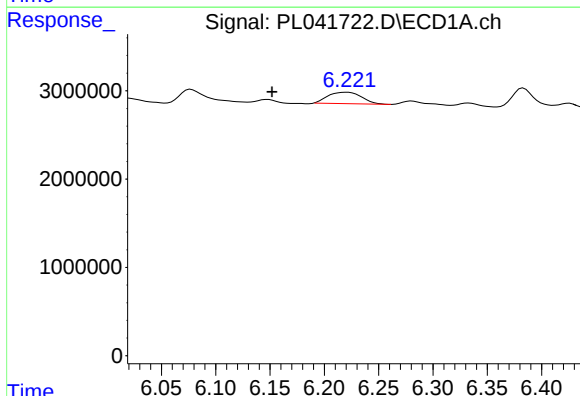


#16 4,4'-DDD

R.T.: 6.221 min
Delta R.T.: 0.069 min
Response: 2776603
Conc: 0.48 ng/ml

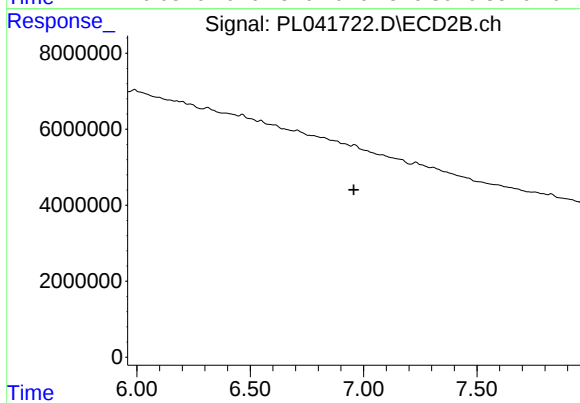

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.957 min
Response: 0
Conc: N.D.

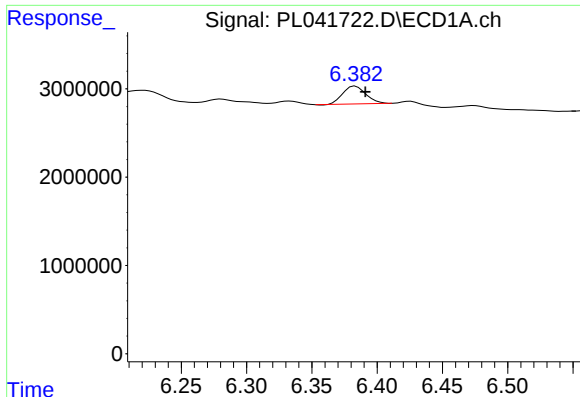

#17 4,4'-DDT


R.T.: 6.383 min
Delta R.T.: -0.008 min
Response: 2462597
Conc: 0.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-10B-S

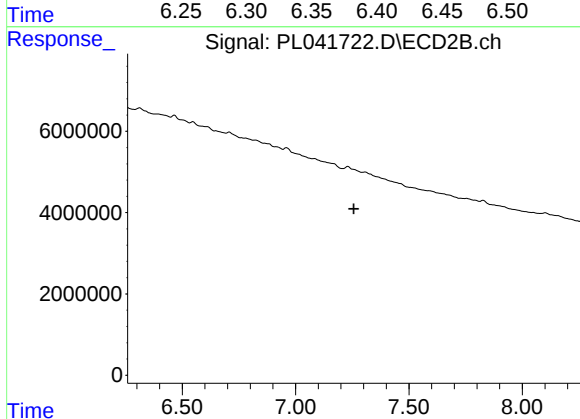


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.258 min
Response: 0
Conc: N.D.

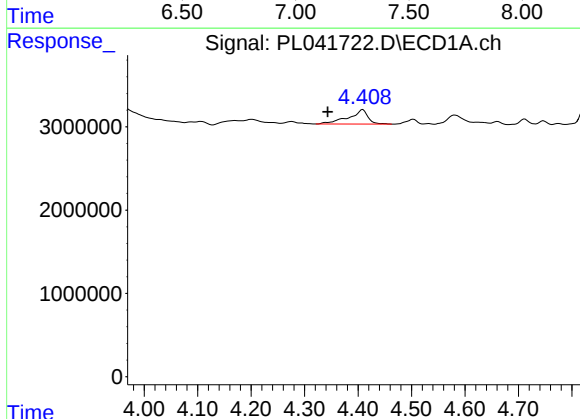


#23 Chlordane-1

R.T.: 4.409 min
Delta R.T.: 0.065 min
Response: 4377939
Conc: 15.44 ng/ml

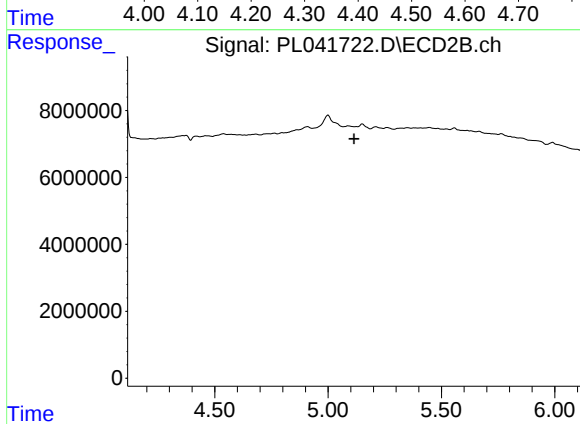

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.115 min
Response: 0
Conc: N.D.

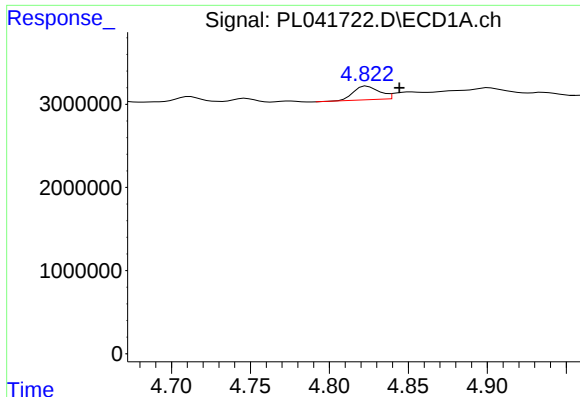

#24 Chlordane-2


R.T.: 4.824 min
Delta R.T.: -0.020 min
Response: 1848095
Conc: 6.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-10B-S

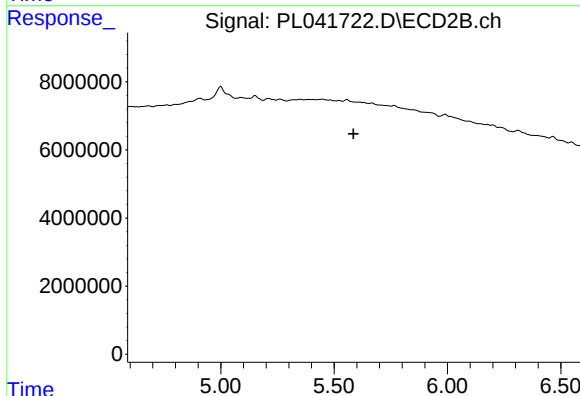


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.586 min
Response: 0
Conc: N.D.

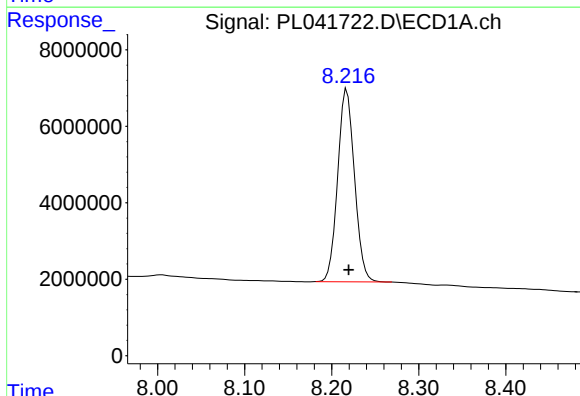

#28 Decachlorobiphenyl

R.T.: 8.218 min
Delta R.T.: -0.002 min
Response: 67689373
Conc: 10.22 ng/ml

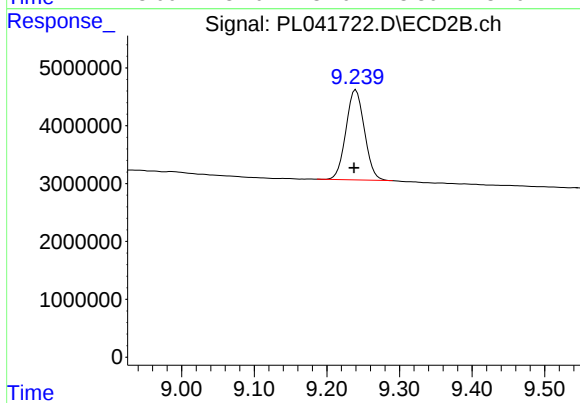

#28 Decachlorobiphenyl

R.T.: 9.240 min
Delta R.T.: 0.002 min
Response: 27588676
Conc: 10.77 ng/ml