

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110218\
 Data File : PL041736.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2018 02:20
 Operator : AJ\SJ
 Sample : J5759-16
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 02:48:41 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.473	4.106	115.4E6	61258565	18.113	19.888
28)	SA Decachlor...	8.218	9.241	108.0E6	44528921	16.305	17.379
Target Compounds							
3)	MA gamma-BHC...	4.205	4.775	24210813	14555331	2.710	3.433 #
4)	MA Heptachlor	4.481	0.000	2230680	0	0.243	N.D. #
6)	B beta-BHC	4.421f	0.000	6244125	0	1.657	N.D. #
7)	B delta-BHC	0.000	5.152f	0	5021226	N.D.	1.243 #
8)	B Heptachlo...	5.250f	0.000	3857881	0	0.478	N.D. #
9)	A Endosulfan I	5.550	0.000	4062925	0	0.546	N.D. #
10)	B gamma-Chl...	0.000	6.169f	0	2119048	N.D.	0.628 #
13)	MA Dieldrin	5.768	0.000	4014056	0	0.505	N.D. #
23)	Chlordane-1	4.348	5.152	2631881	5021226	9.282	36.153 #
25)	Chlordane-3	0.000	6.169	0	2119048	N.D.	4.709 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110218\
Data File : PL041736.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2018 02:20
Operator : AJ\SJ
Sample : J5759-16
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP-4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 02:48:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

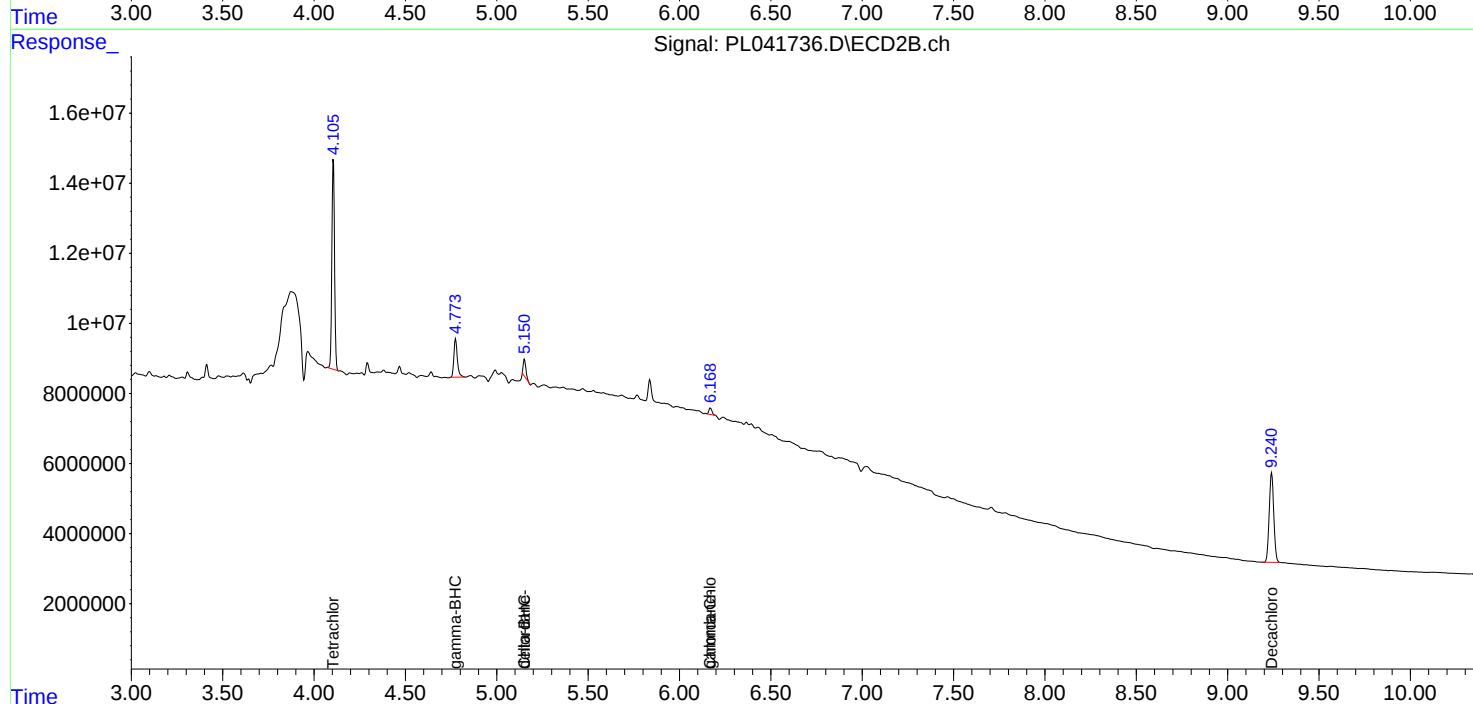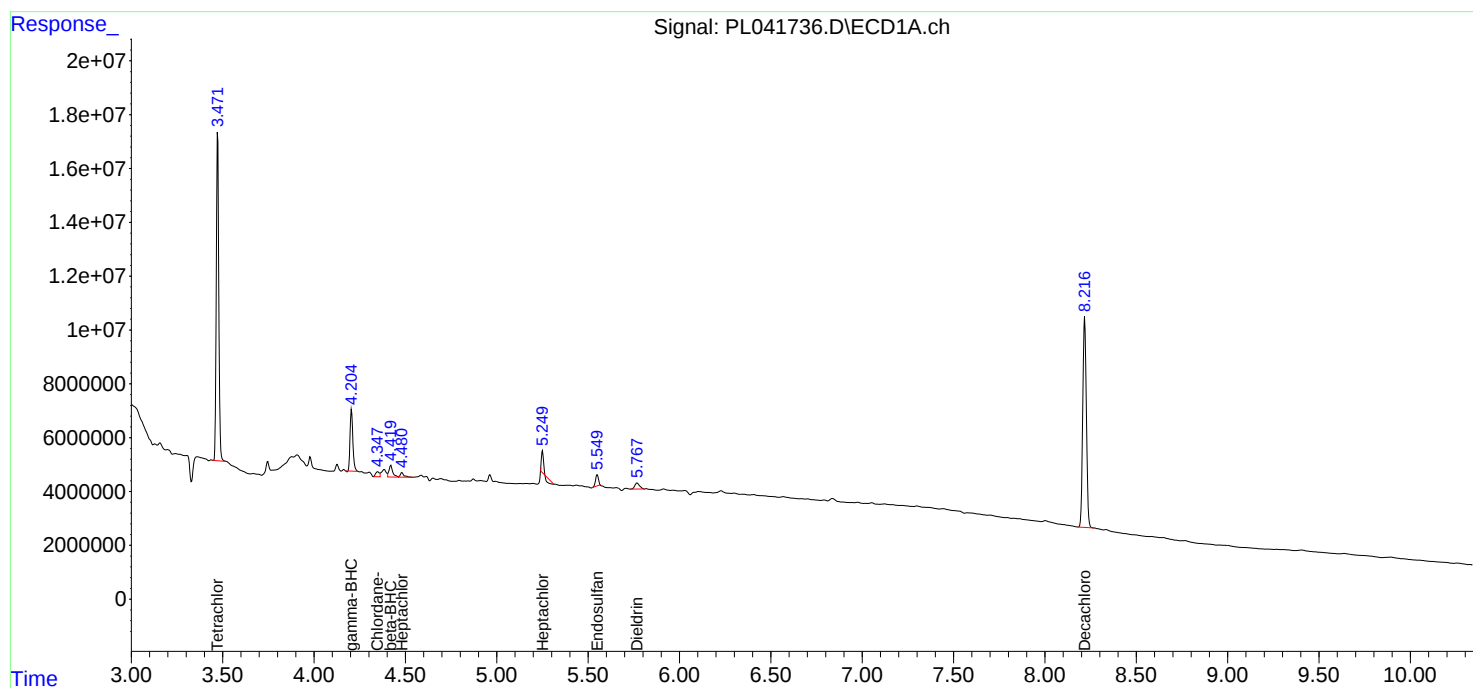


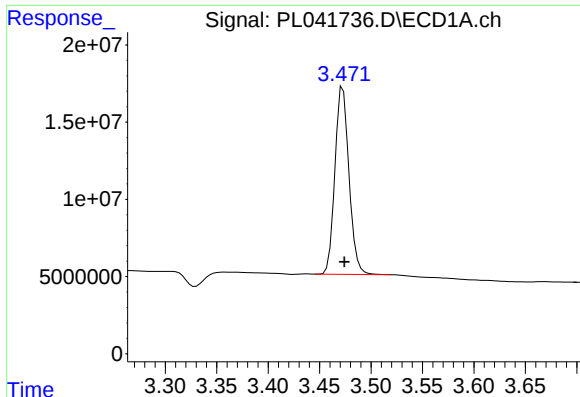

#1 Tetrachloro-m-xylene


R.T.: 3.473 min
Delta R.T.: -0.001 min
Response: 115386825
Conc: 18.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4

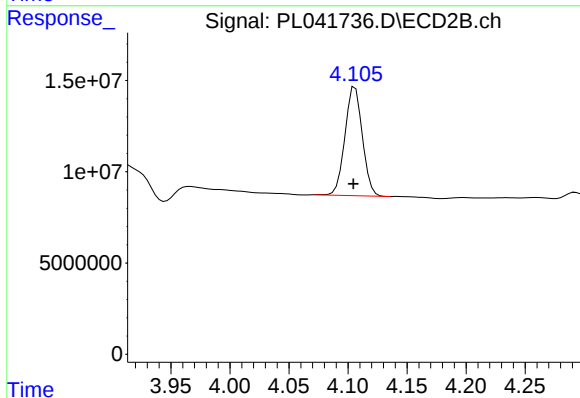


#1 Tetrachloro-m-xylene

R.T.: 4.106 min
Delta R.T.: 0.001 min
Response: 61258565
Conc: 19.89 ng/ml

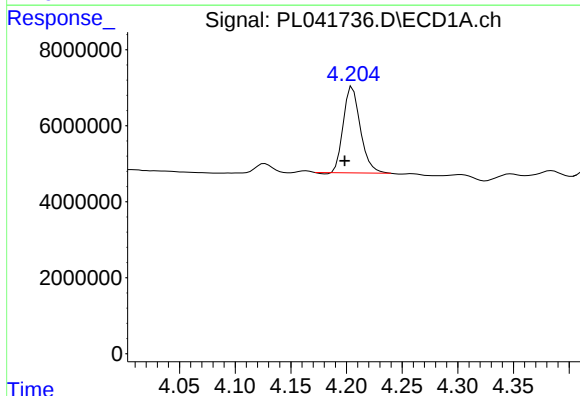


#3 gamma-BHC (Lindane)

R.T.: 4.205 min
Delta R.T.: 0.007 min
Response: 24210813
Conc: 2.71 ng/ml

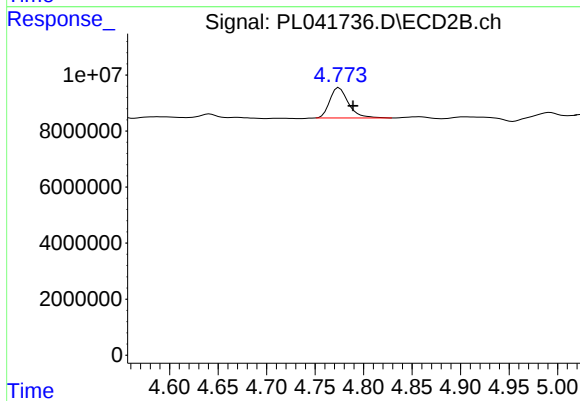

#3 gamma-BHC (Lindane)


R.T.: 4.775 min
Delta R.T.: -0.014 min
Response: 14555331
Conc: 3.43 ng/ml

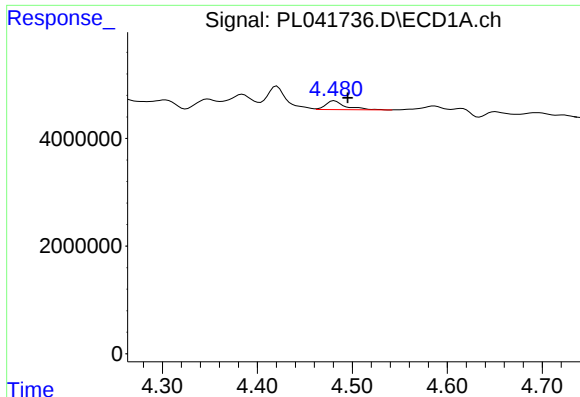

#4 Heptachlor


R.T.: 4.481 min
Delta R.T.: -0.014 min
Response: 2230680
Conc: 0.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4

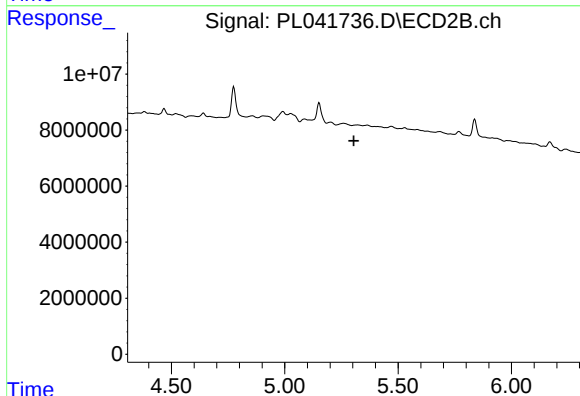


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.305 min
Response: 0
Conc: N.D.

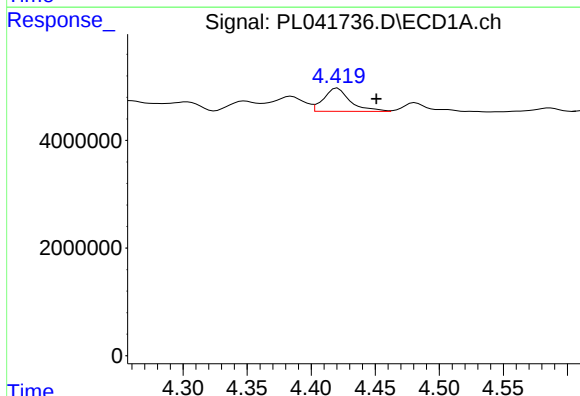


#6 beta-BHC

R.T.: 4.421 min
Delta R.T.: -0.030 min
Response: 6244125
Conc: 1.66 ng/ml

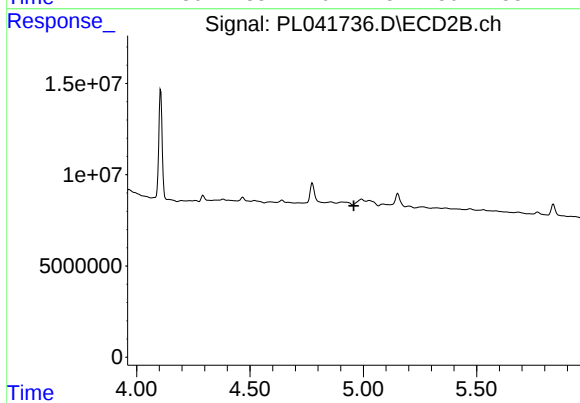

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.957 min
Response: 0
Conc: N.D.

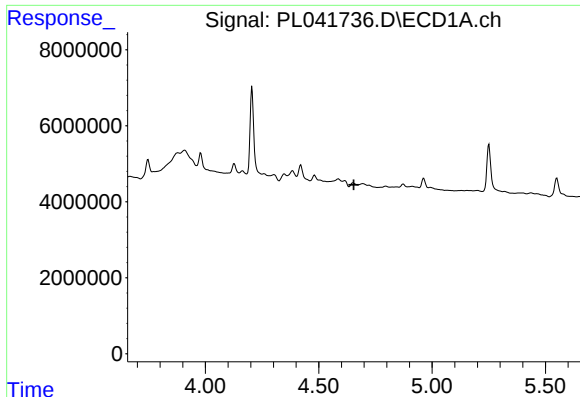

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.654 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-4

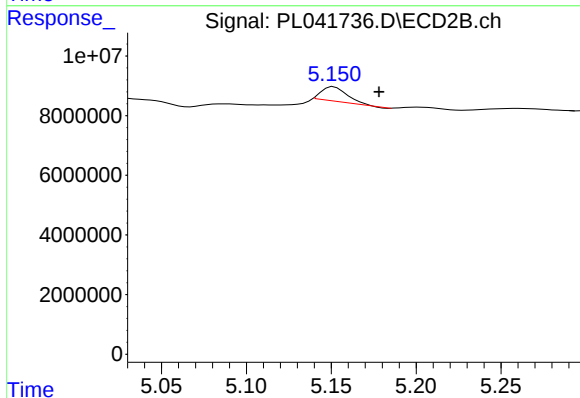


#7 delta-BHC

R.T.: 5.152 min
Delta R.T.: -0.027 min
Response: 5021226
Conc: 1.24 ng/ml

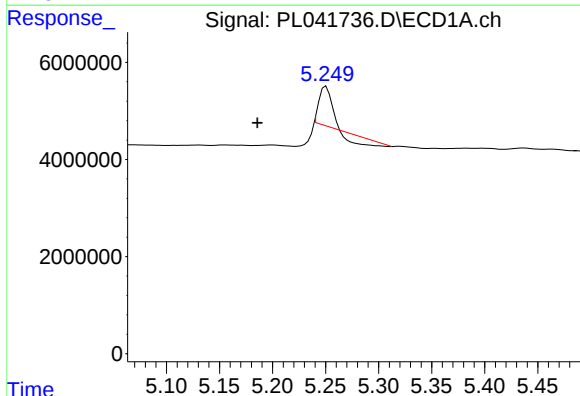


#8 Heptachlor epoxide

R.T.: 5.250 min
Delta R.T.: 0.065 min
Response: 3857881
Conc: 0.48 ng/ml

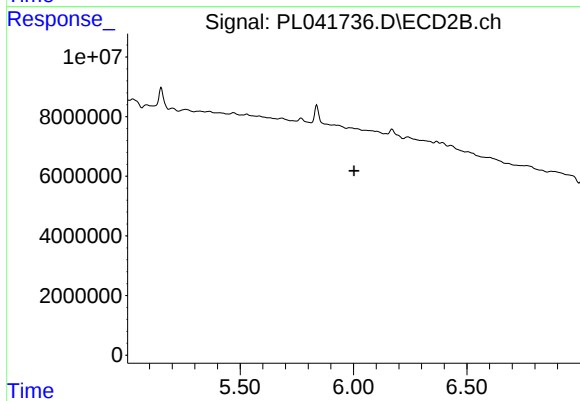

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 6.002 min
Response: 0
Conc: N.D.

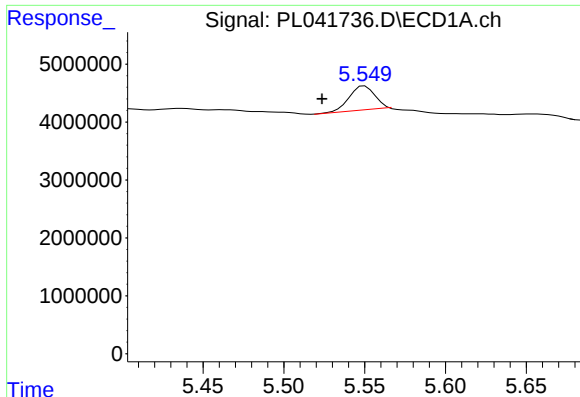

#9 Endosulfan I


R.T.: 5.550 min
Delta R.T.: 0.026 min
Response: 4062925
Conc: 0.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4

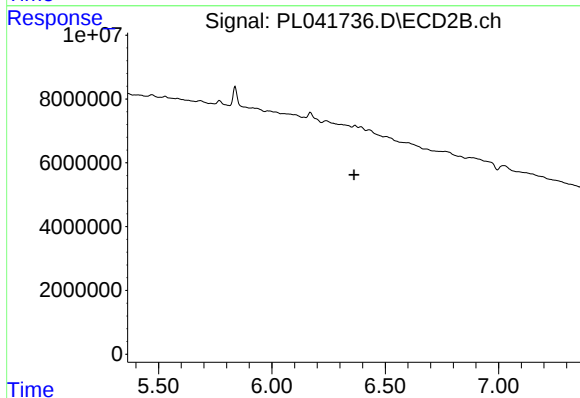


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

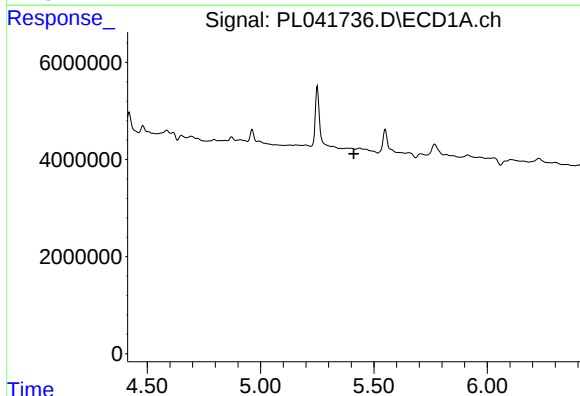


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.412 min
Response: 0
Conc: N.D.

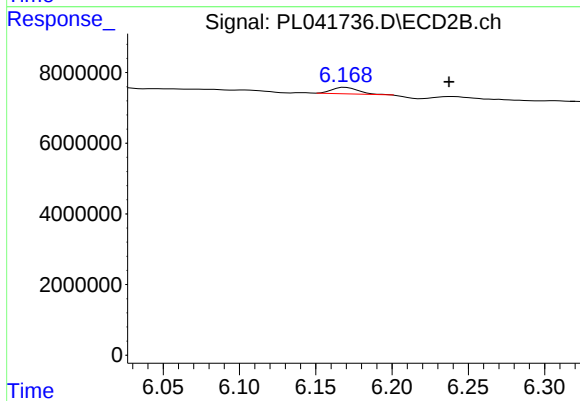

#10 gamma-Chlordane


R.T.: 6.169 min
Delta R.T.: -0.068 min
Response: 2119048
Conc: 0.63 ng/ml

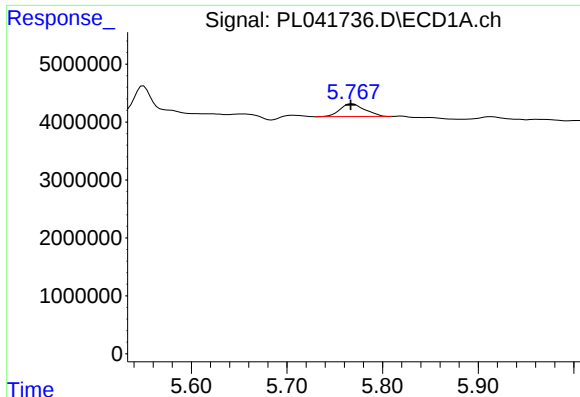

#13 Dieldrin


R.T.: 5.768 min
Delta R.T.: 0.002 min
Response: 4014056
Conc: 0.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4

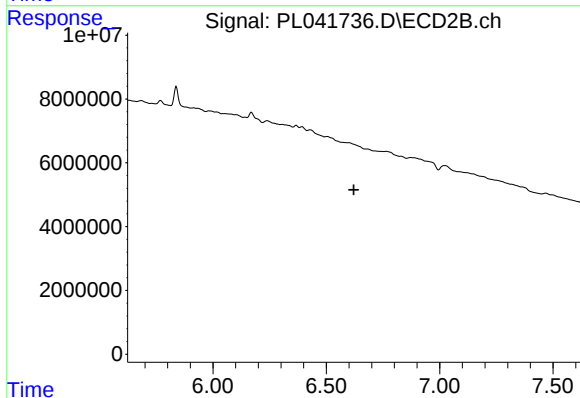


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.621 min
Response: 0
Conc: N.D.

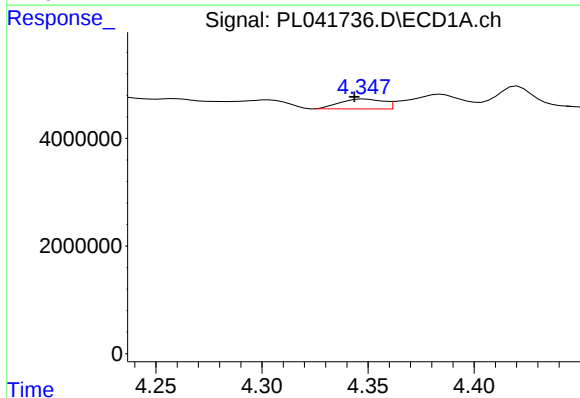


#23 Chlordane-1

R.T.: 4.348 min
Delta R.T.: 0.005 min
Response: 2631881
Conc: 9.28 ng/ml

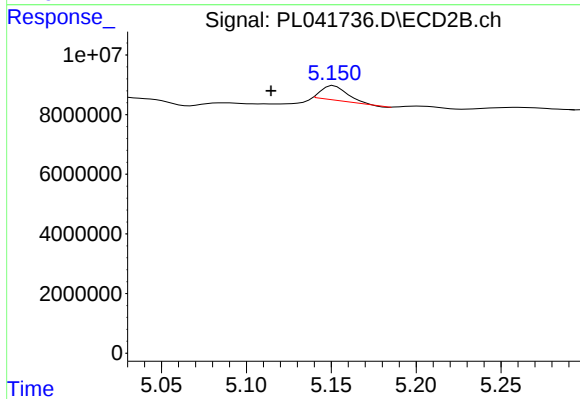

#23 Chlordane-1


R.T.: 5.152 min
Delta R.T.: 0.037 min
Response: 5021226
Conc: 36.15 ng/ml

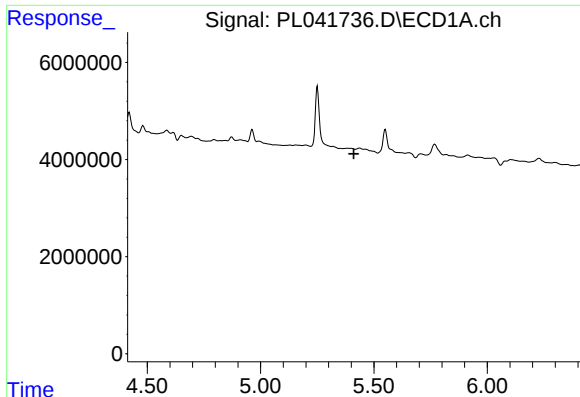

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.412 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-4

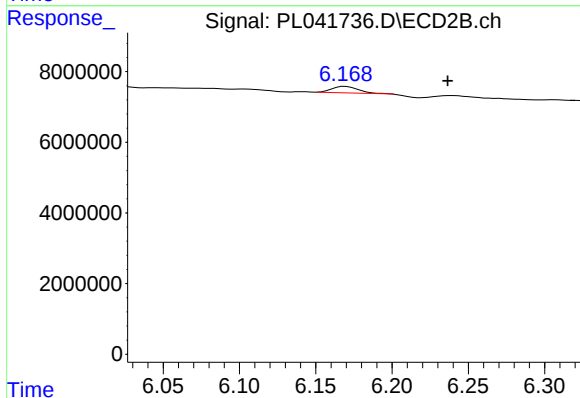


#25 Chlordane-3

R.T.: 6.169 min
Delta R.T.: -0.067 min
Response: 2119048
Conc: 4.71 ng/ml

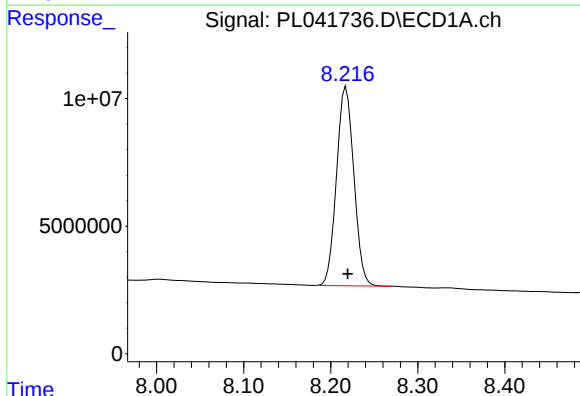

#28 Decachlorobiphenyl

R.T.: 8.218 min
Delta R.T.: -0.002 min
Response: 108005263
Conc: 16.31 ng/ml

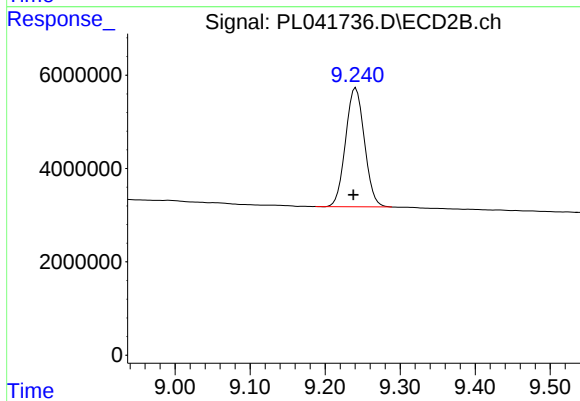

#28 Decachlorobiphenyl

R.T.: 9.241 min
Delta R.T.: 0.003 min
Response: 44528921
Conc: 17.38 ng/ml