

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110218\
 Data File : PL041745.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2018 04:28
 Operator : AJ\SJ
 Sample : J5755-08
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-2A-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 04:53:46 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.473	4.106	119.4E6	62868588	18.741	20.410
28)	SA Decachlor...	8.218	9.241	116.9E6	48089837	17.646	18.769
Target Compounds							
6)	B beta-BHC	4.409f	0.000	3589190	0	0.952	N.D. #
23)	Chlordane-1	4.386	0.000	2726591	0	9.616	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110218\
Data File : PL041745.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2018 04:28
Operator : AJ\SJ
Sample : J5755-08
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-2A-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 04:53:46 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

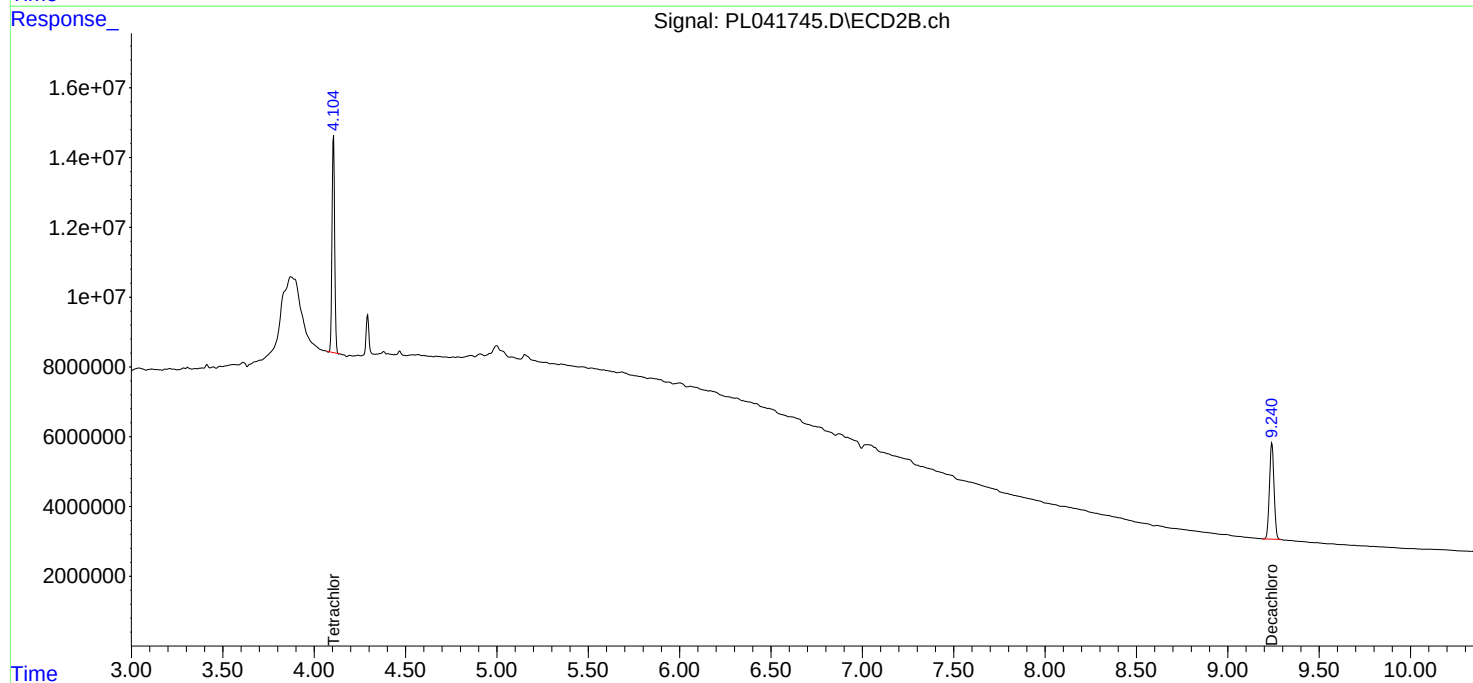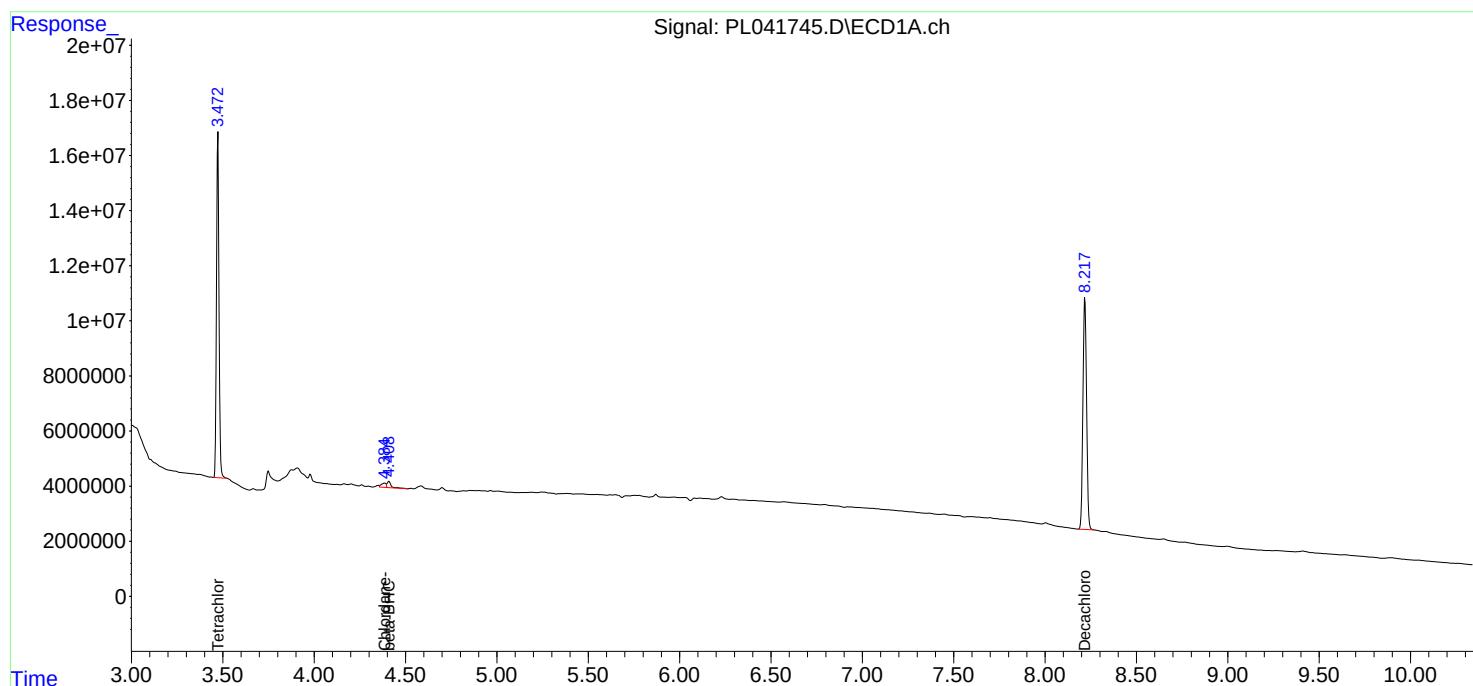


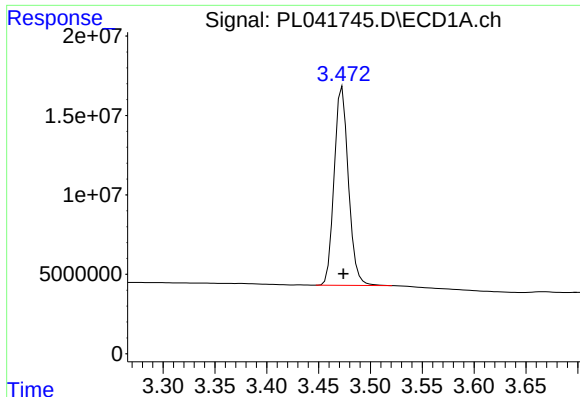

#1 Tetrachloro-m-xylene


R.T.: 3.473 min
Delta R.T.: -0.001 min
Response: 119386946
Conc: 18.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2A-S

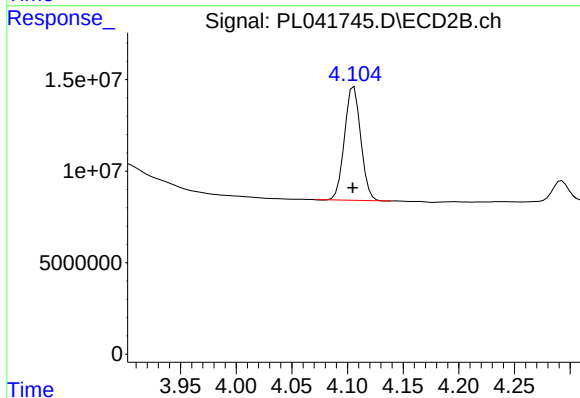


#1 Tetrachloro-m-xylene

R.T.: 4.106 min
Delta R.T.: 0.001 min
Response: 62868588
Conc: 20.41 ng/ml

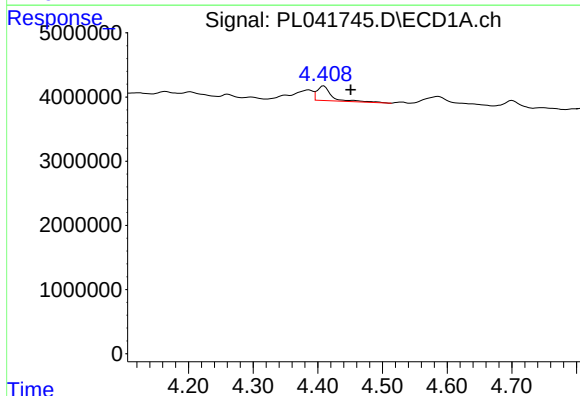


#6 beta-BHC

R.T.: 4.409 min
Delta R.T.: -0.042 min
Response: 3589190
Conc: 0.95 ng/ml

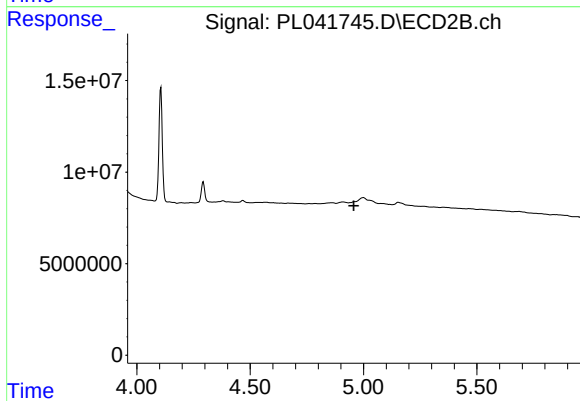

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.957 min
Response: 0
Conc: N.D.

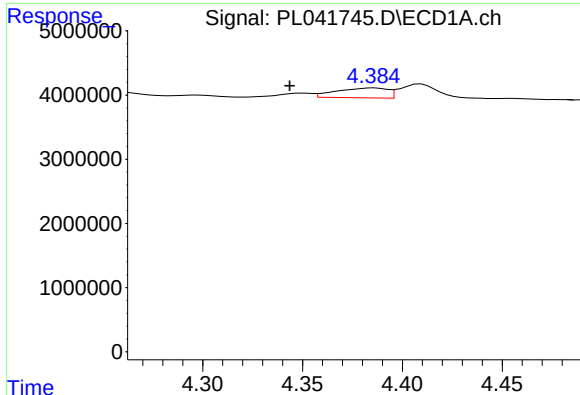

#23 Chlordane-1


R.T.: 4.386 min
Delta R.T.: 0.042 min
Response: 2726591
Conc: 9.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2A-S

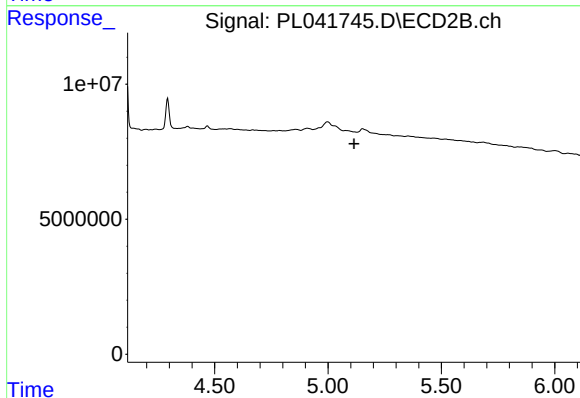


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.115 min
Response: 0
Conc: N.D.

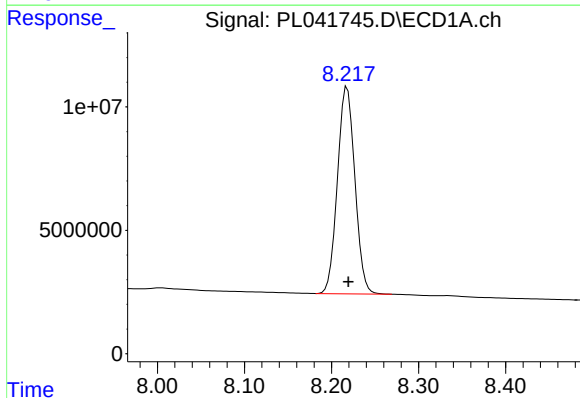

#28 Decachlorobiphenyl

R.T.: 8.218 min
Delta R.T.: -0.001 min
Response: 116886816
Conc: 17.65 ng/ml

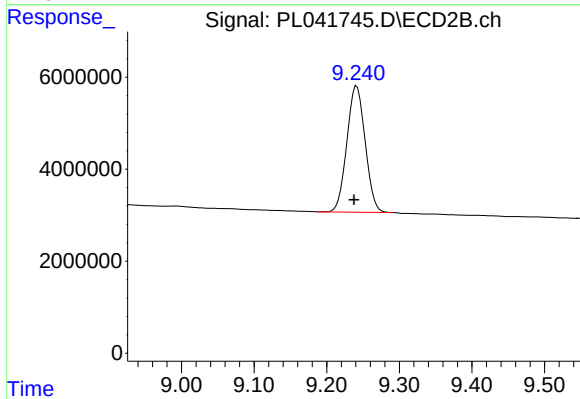

#28 Decachlorobiphenyl

R.T.: 9.241 min
Delta R.T.: 0.004 min
Response: 48089837
Conc: 18.77 ng/ml