

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110218\
Data File : PL041689.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2018 15:16
Operator : AJ\SJ
Sample : J5769-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
LEFT-CORNER-BULDG-85

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 23:06:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.473	4.105	58550547	29894173	9.191	9.705
28)	SA Decachlor...	8.217	9.239	69583689	26716142	10.505	10.427

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110218\
Data File : PL041689.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2018 15:16
Operator : AJ\SJ
Sample : J5769-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
LEFT-CORNER-BULDG-85

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 23:06:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

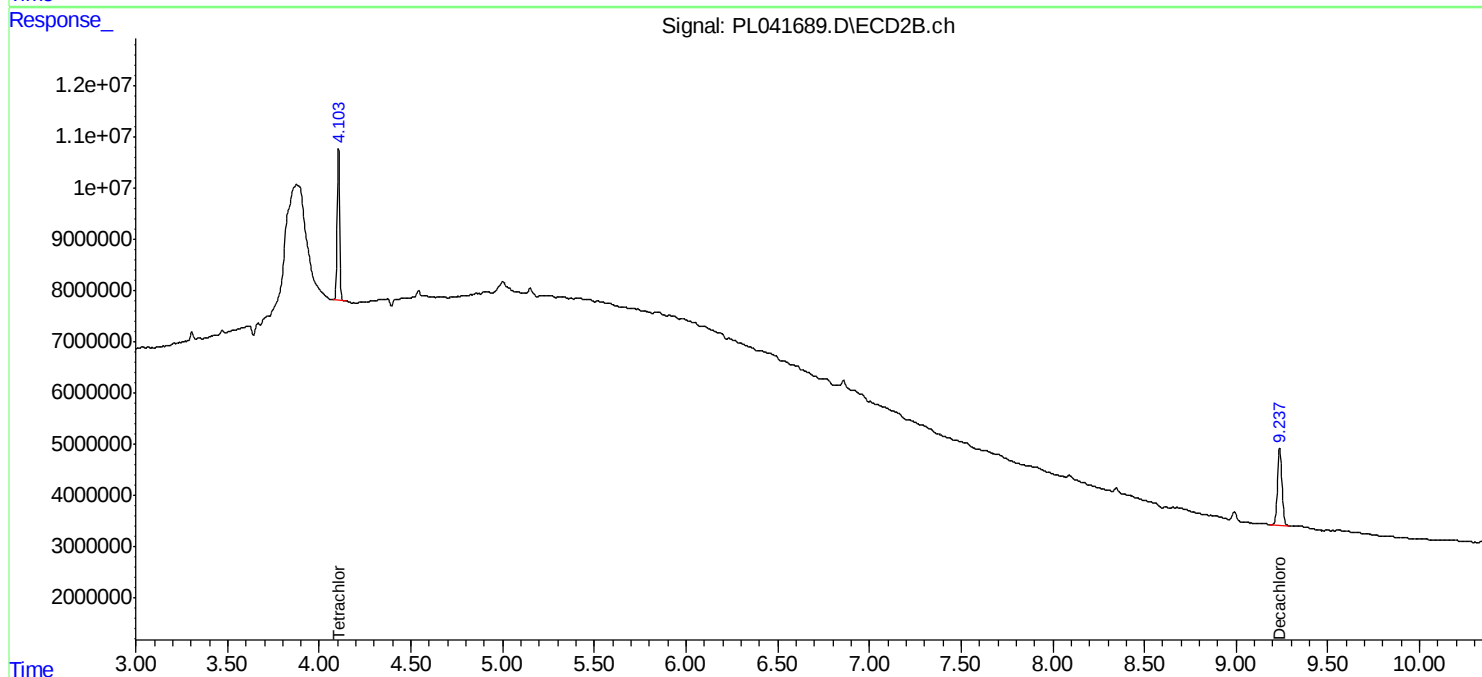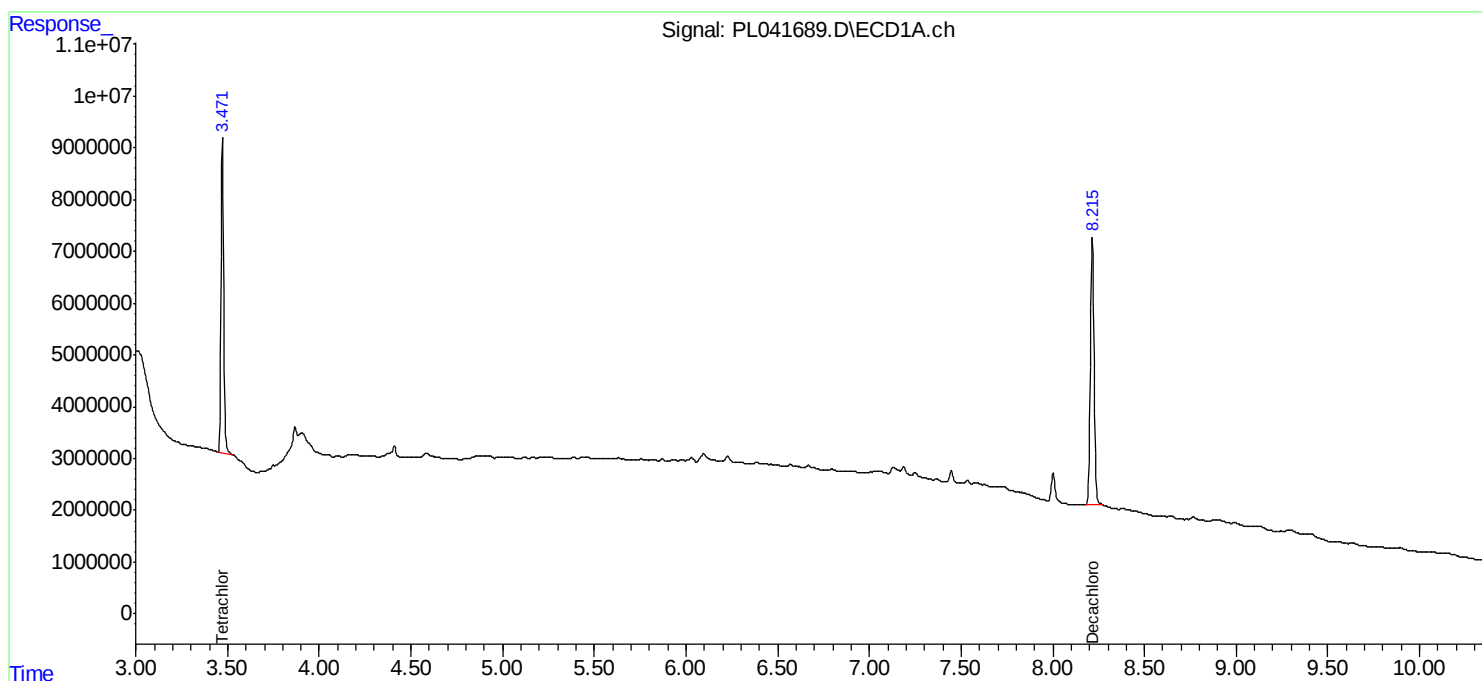


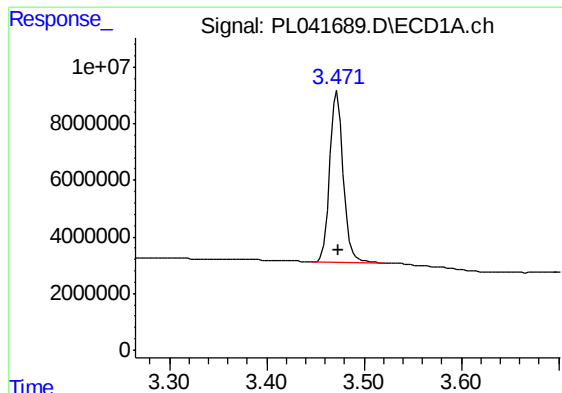

#1 Tetrachloro-m-xylene


R.T.: 3.473 min
Delta R.T.: -0.001 min
Response: 58550547
Conc: 9.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
LEFT-CORNER-BULDG-85

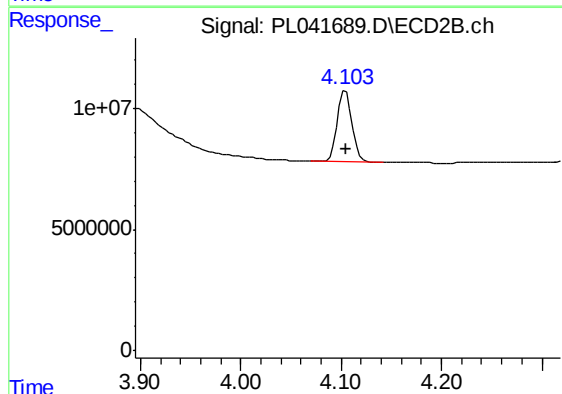


#1 Tetrachloro-m-xylene

R.T.: 4.105 min
Delta R.T.: 0.000 min
Response: 29894173
Conc: 9.71 ng/ml

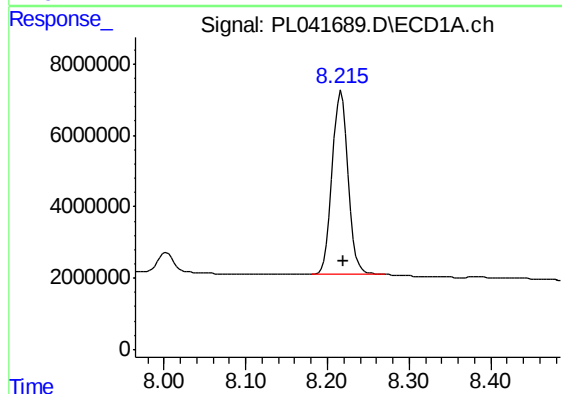

#28 Decachlorobiphenyl

R.T.: 8.217 min
Delta R.T.: -0.003 min
Response: 69583689
Conc: 10.50 ng/ml

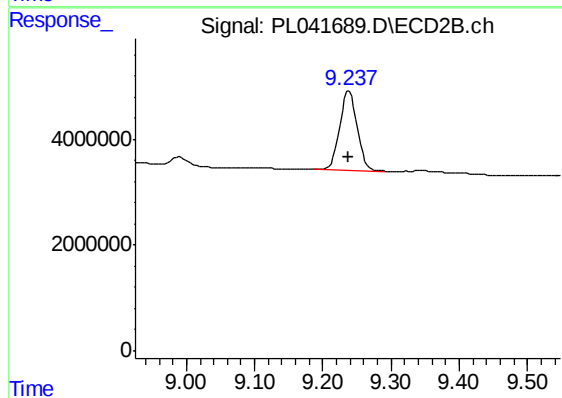

#28 Decachlorobiphenyl

R.T.: 9.239 min
Delta R.T.: 0.001 min
Response: 26716142
Conc: 10.43 ng/ml