

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110220\
 Data File : PL062752.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2020 11:00
 Operator : DD\AJ
 Sample : PB132731BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB132731BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 02:59:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.417	3.952	32657866	56281008	18.986	19.152
28)	SA Decachlor...	8.135	8.998	37035024	47640261	23.085	22.762
Target Compounds							
6)	B beta-BHC	0.000	4.812f	0	15523069	N.D.	8.244 #
8)	B Heptachlo...	0.000	5.835f	0	10890140	N.D.	3.363 #
9)	A Endosulfan I	5.451	0.000	2955050	0	1.768	N.D. #
10)	B gamma-Chl...	0.000	6.076f	0	5221252	N.D.	1.551 #
12)	B 4,4'-DDE	0.000	6.281	0	9143176	N.D.	2.838 #
15)	B Endosulfa...	0.000	6.869f	0	3770002	N.D.	1.319 #
17)	MA 4,4'-DDT	0.000	7.043f	0	4997407	N.D.	2.226 #
18)	B Endrin al...	0.000	6.976	0	5274977	N.D.	2.313 #
19)	B Endosulfa...	6.574	0.000	3329598	0	2.018	N.D. #
21)	B Endrin ke...	7.088f	0.000	14637236	0	8.118	N.D. #
25)	Chlordane-3	0.000	6.076f	0	5221252	N.D.	12.926 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110220\
Data File : PL062752.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2020 11:00
Operator : DD\AJ
Sample : PB132731BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleID :
PB132731BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 02:59:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

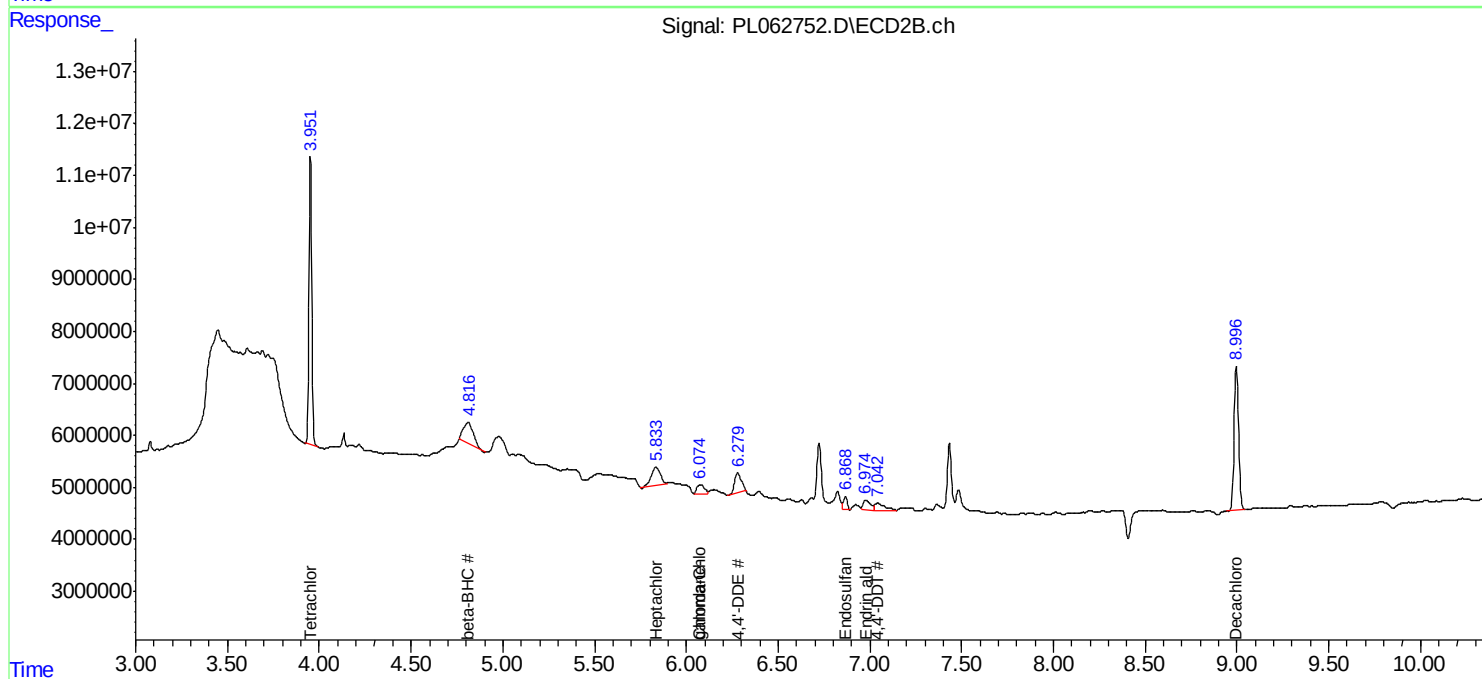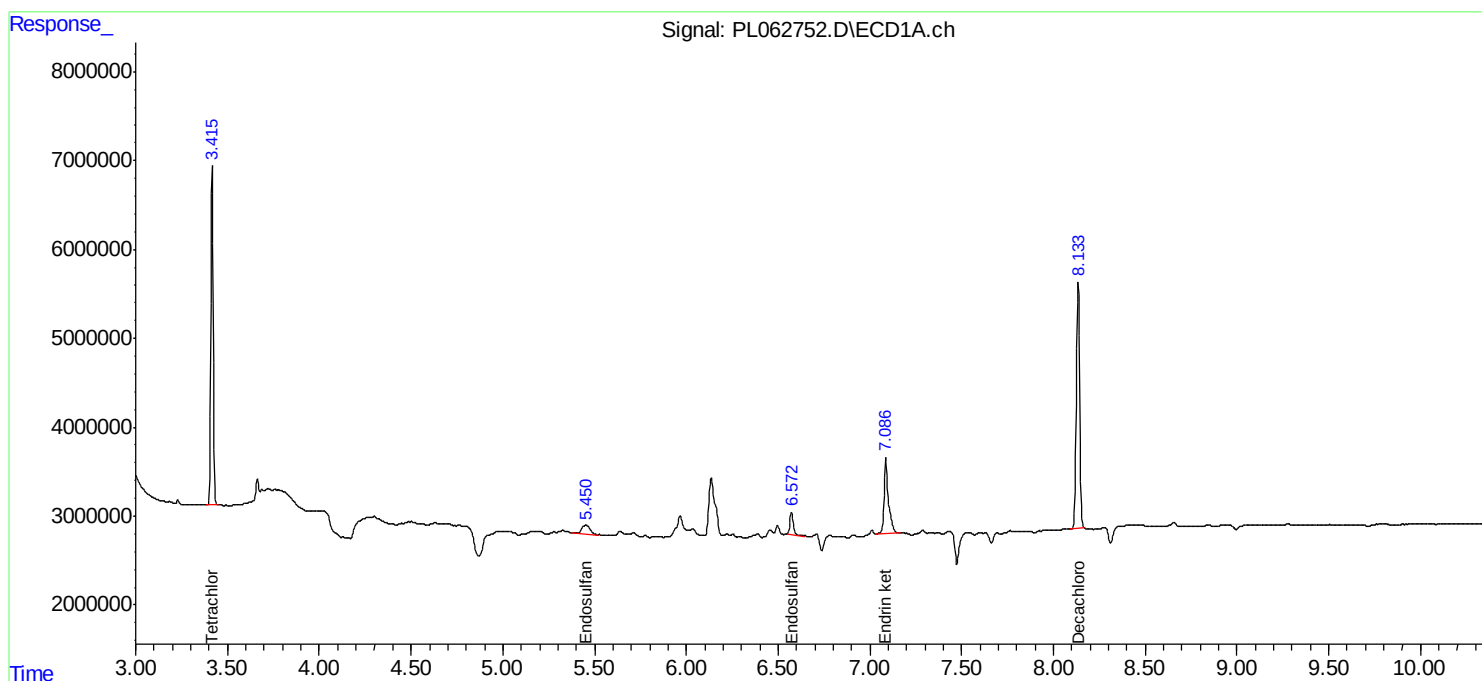


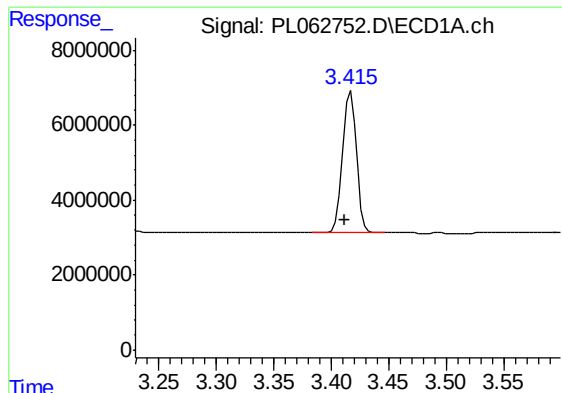

#1 Tetrachloro-m-xylene


R.T.: 3.417 min
Delta R.T.: 0.005 min
Response: 32657866
Conc: 18.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB132731BL

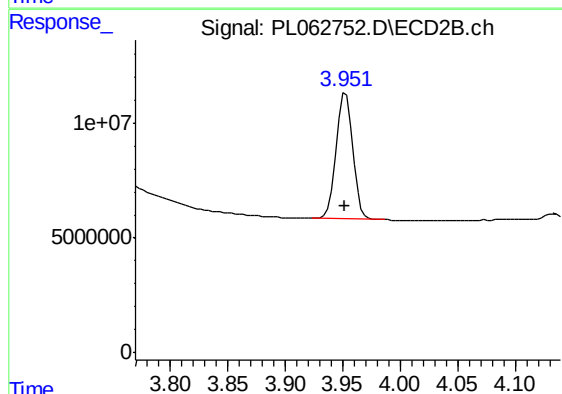


#1 Tetrachloro-m-xylene

R.T.: 3.952 min
Delta R.T.: 0.000 min
Response: 56281008
Conc: 19.15 ng/ml

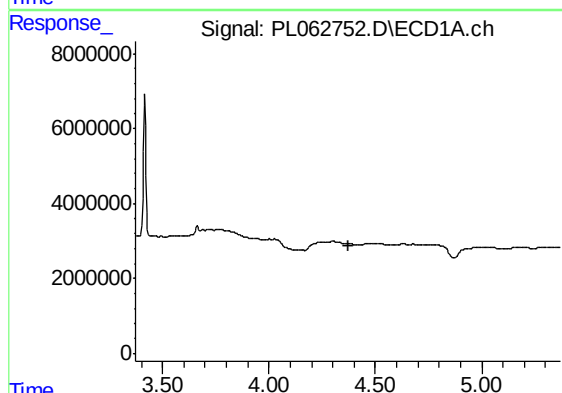


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.372 min
Response: 0
Conc: N.D.

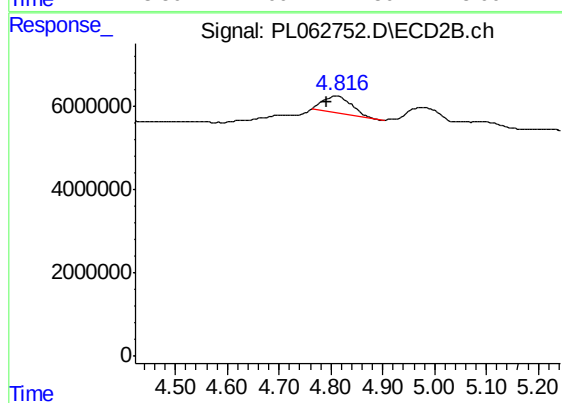

#6 beta-BHC


R.T.: 4.812 min
Delta R.T.: 0.020 min
Response: 15523069
Conc: 8.24 ng/ml

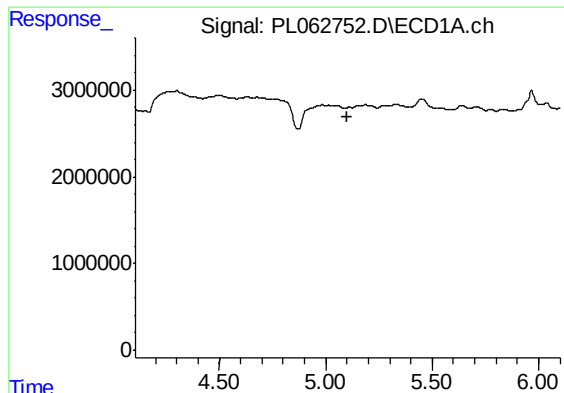

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.103 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB132731BL

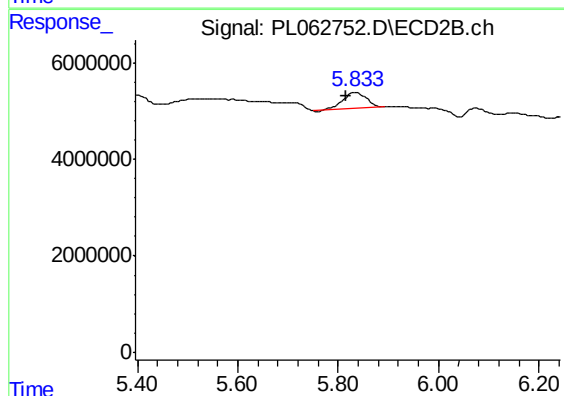


#8 Heptachlor epoxide

R.T.: 5.835 min
Delta R.T.: 0.021 min
Response: 10890140
Conc: 3.36 ng/ml

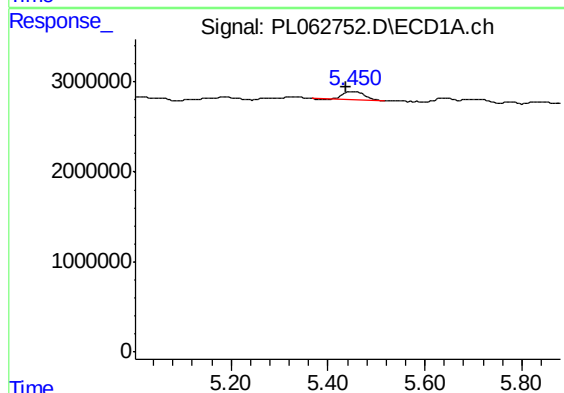


#9 Endosulfan I

R.T.: 5.451 min
Delta R.T.: 0.014 min
Response: 2955050
Conc: 1.77 ng/ml

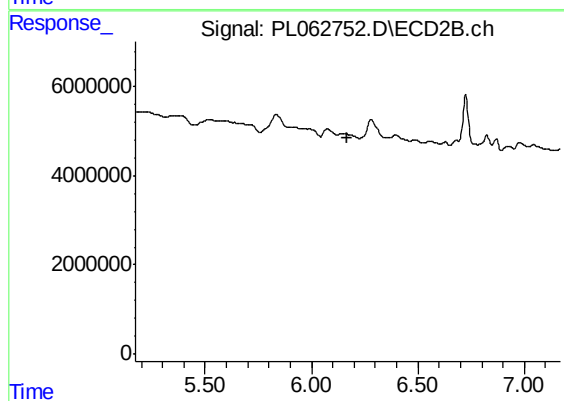

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.170 min
Response: 0
Conc: N.D.

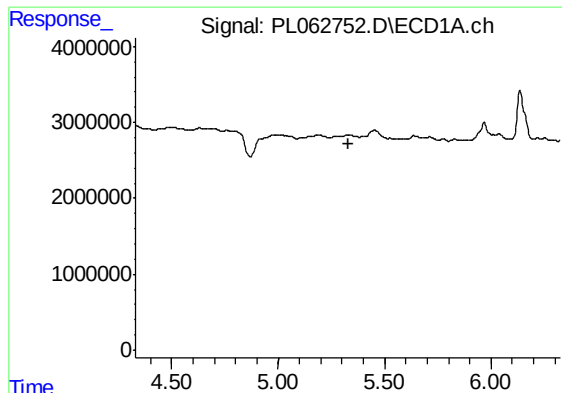

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB132731BL

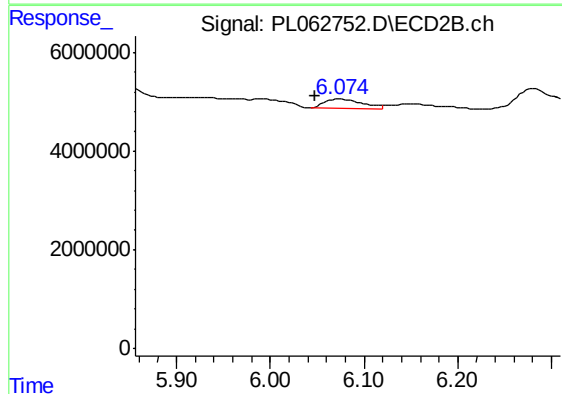


#10 gamma-Chlordane

R.T.: 6.076 min
Delta R.T.: 0.027 min
Response: 5221252
Conc: 1.55 ng/ml

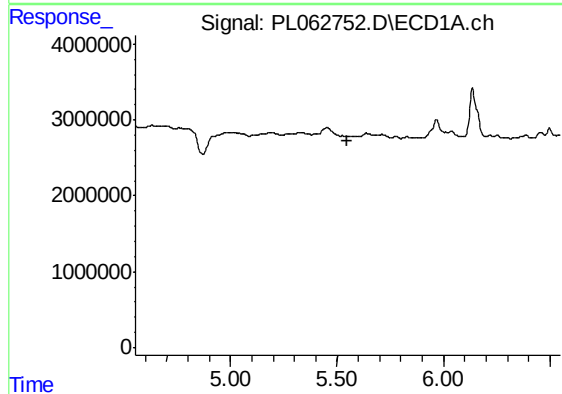


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 5.550 min
Response: 0
Conc: N.D.

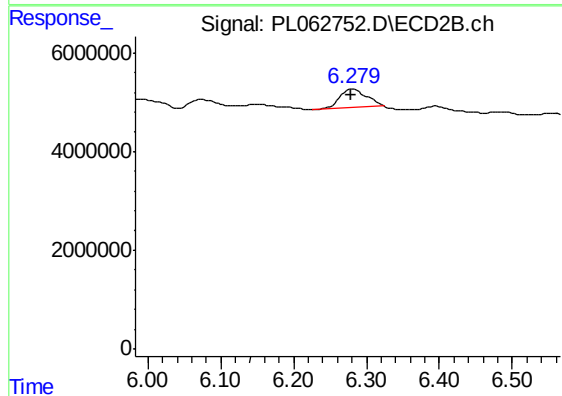

#12 4,4'-DDE


R.T.: 6.281 min
Delta R.T.: 0.002 min
Response: 9143176
Conc: 2.84 ng/ml

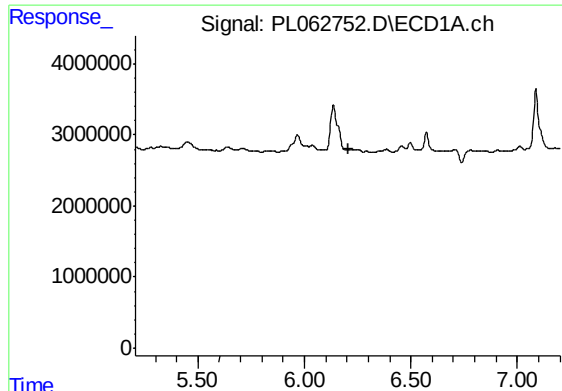

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.205 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB132731BL

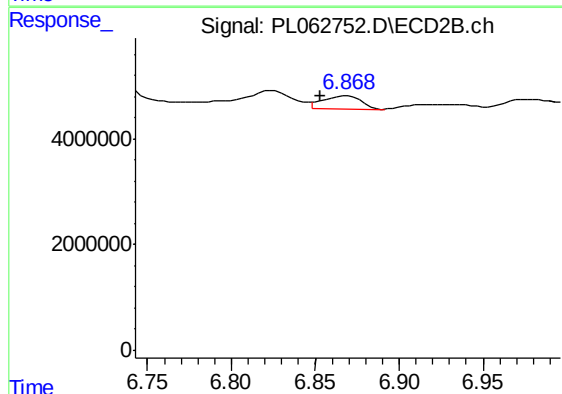


#15 Endosulfan II

R.T.: 6.869 min
Delta R.T.: 0.017 min
Response: 3770002
Conc: 1.32 ng/ml

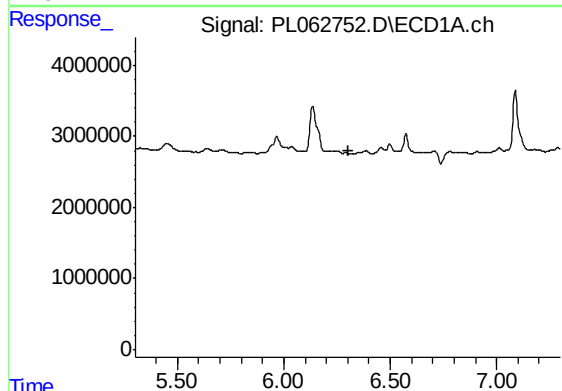


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.301 min
Response: 0
Conc: N.D.

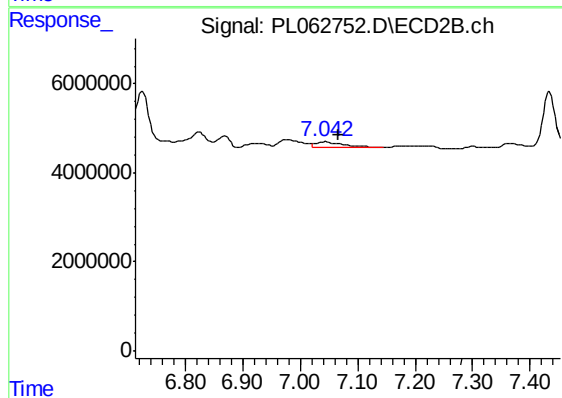

#17 4,4'-DDT


R.T.: 7.043 min
Delta R.T.: -0.023 min
Response: 4997407
Conc: 2.23 ng/ml

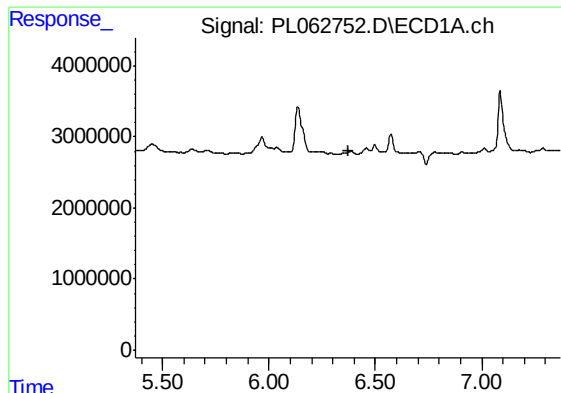

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB132731BL

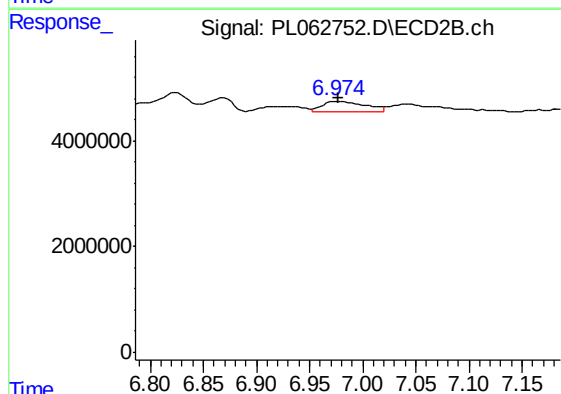


#18 Endrin aldehyde

R.T.: 6.976 min
Delta R.T.: 0.000 min
Response: 5274977
Conc: 2.31 ng/ml

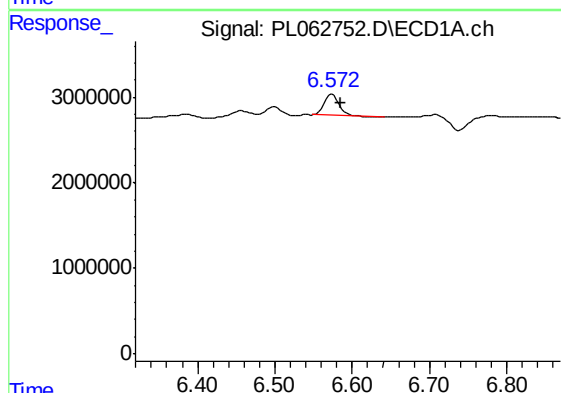


#19 Endosulfan Sulfate

R.T.: 6.574 min
Delta R.T.: -0.011 min
Response: 3329598
Conc: 2.02 ng/ml

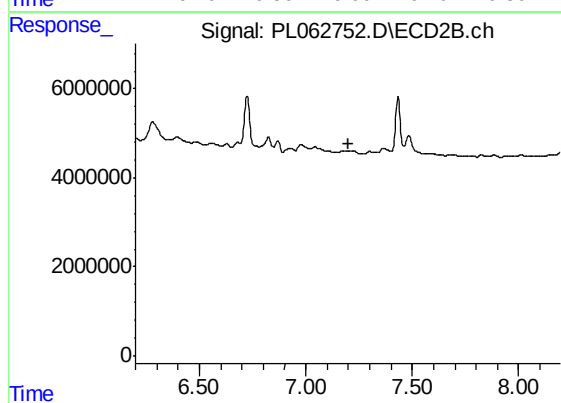

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.199 min
Response: 0
Conc: N.D.

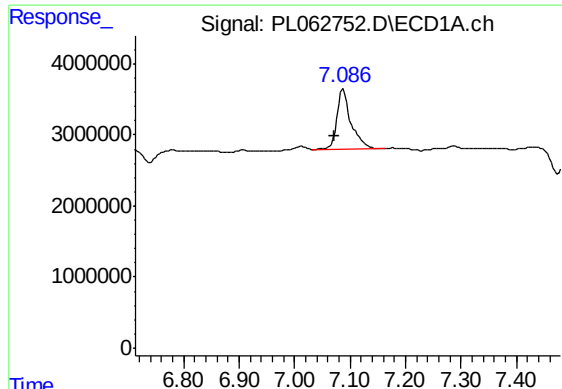

#21 Endrin ketone


R.T.: 7.088 min
Delta R.T.: 0.017 min
Response: 14637236
Conc: 8.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB132731BL

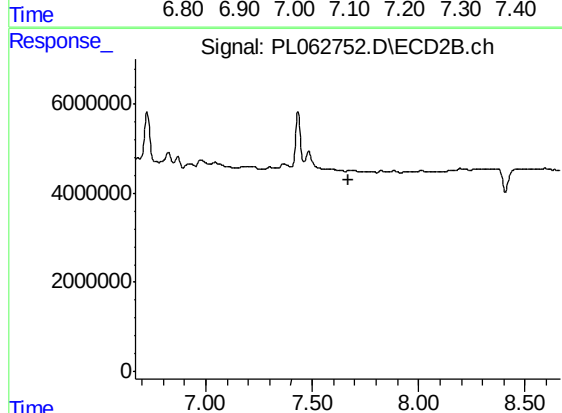


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.668 min
Response: 0
Conc: N.D.

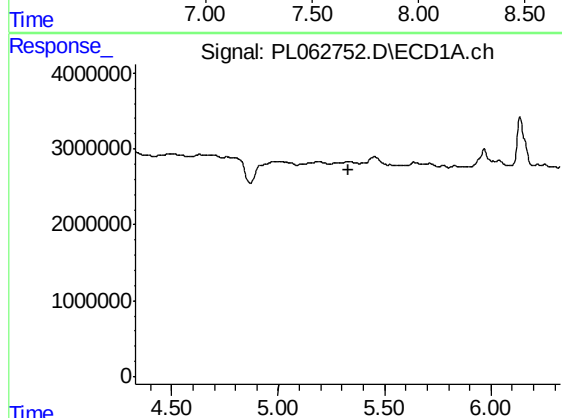


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.328 min
Response: 0
Conc: N.D.

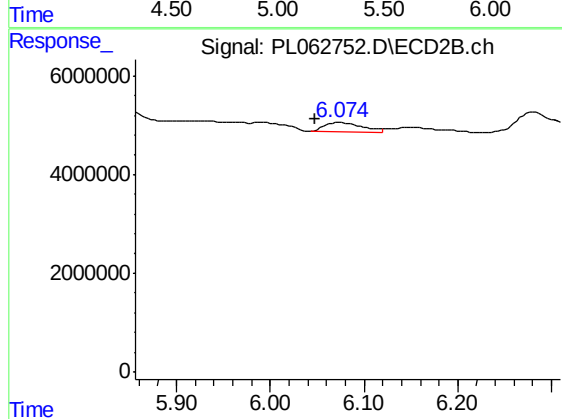

#25 Chlordane-3


R.T.: 6.076 min
Delta R.T.: 0.028 min
Response: 5221252
Conc: 12.93 ng/ml

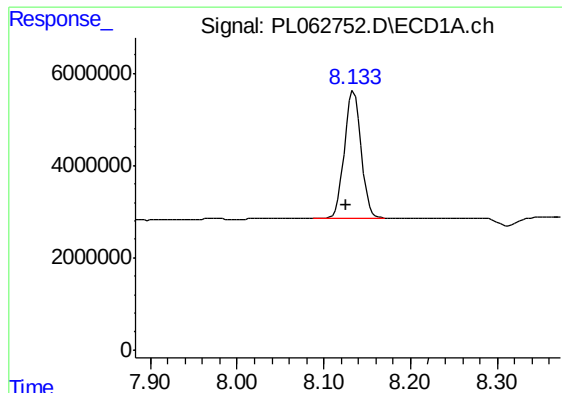

#28 Decachlorobiphenyl

R.T.: 8.135 min
Delta R.T.: 0.008 min
Response: 37035024
Conc: 23.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB132731BL

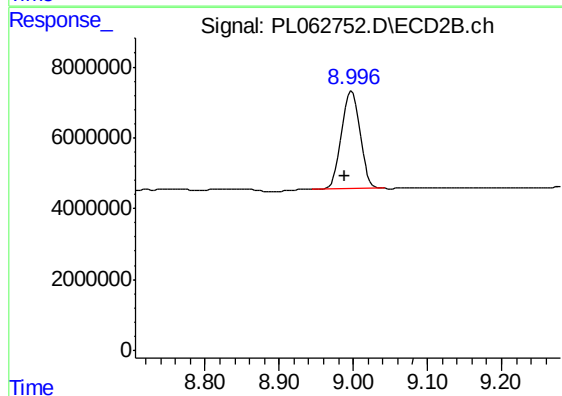

#28 Decachlorobiphenyl

R.T.: 8.998 min
Delta R.T.: 0.009 min
Response: 47640261
Conc: 22.76 ng/ml