

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110220\
 Data File : PL062754.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2020 11:28
 Operator : DD\AJ
 Sample : L4215-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 AU-05-102820

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 02:59:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.951	26997658	48029376	15.696	16.344
28)	SA Decachlor...	8.128	8.993	26126287	34979342	16.285	16.713
Target Compounds							
5)	MB Aldrin	4.645f	0.000	1198245	0	0.628	N.D. #
7)	B delta-BHC	0.000	5.006	0	3154321	N.D.	0.901 #
8)	B Heptachlo...	5.089	0.000	6786867	0	3.720	N.D. #
9)	A Endosulfan I	5.453f	0.000	1394972	0	0.835	N.D. #
12)	B 4,4'-DDE	0.000	6.277	0	2055131	N.D.	0.638 #
15)	B Endosulfa...	0.000	6.869f	0	1952007	N.D.	0.683 #
19)	B Endosulfa...	6.571	0.000	873043	0	0.529	N.D. #
21)	B Endrin ke...	7.084	0.000	5560474	0	3.084	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110220\
Data File : PL062754.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2020 11:28
Operator : DD\AJ
Sample : L4215-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
AU-05-102820

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 02:59:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

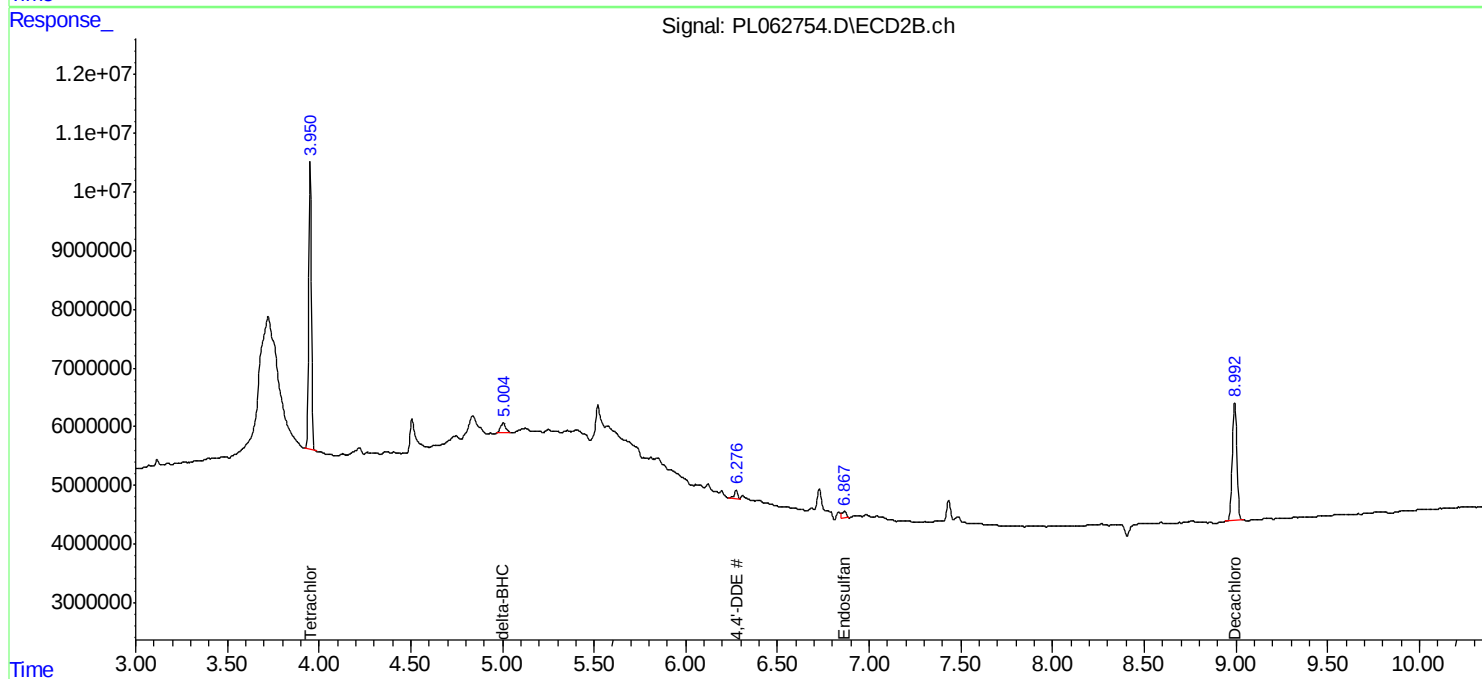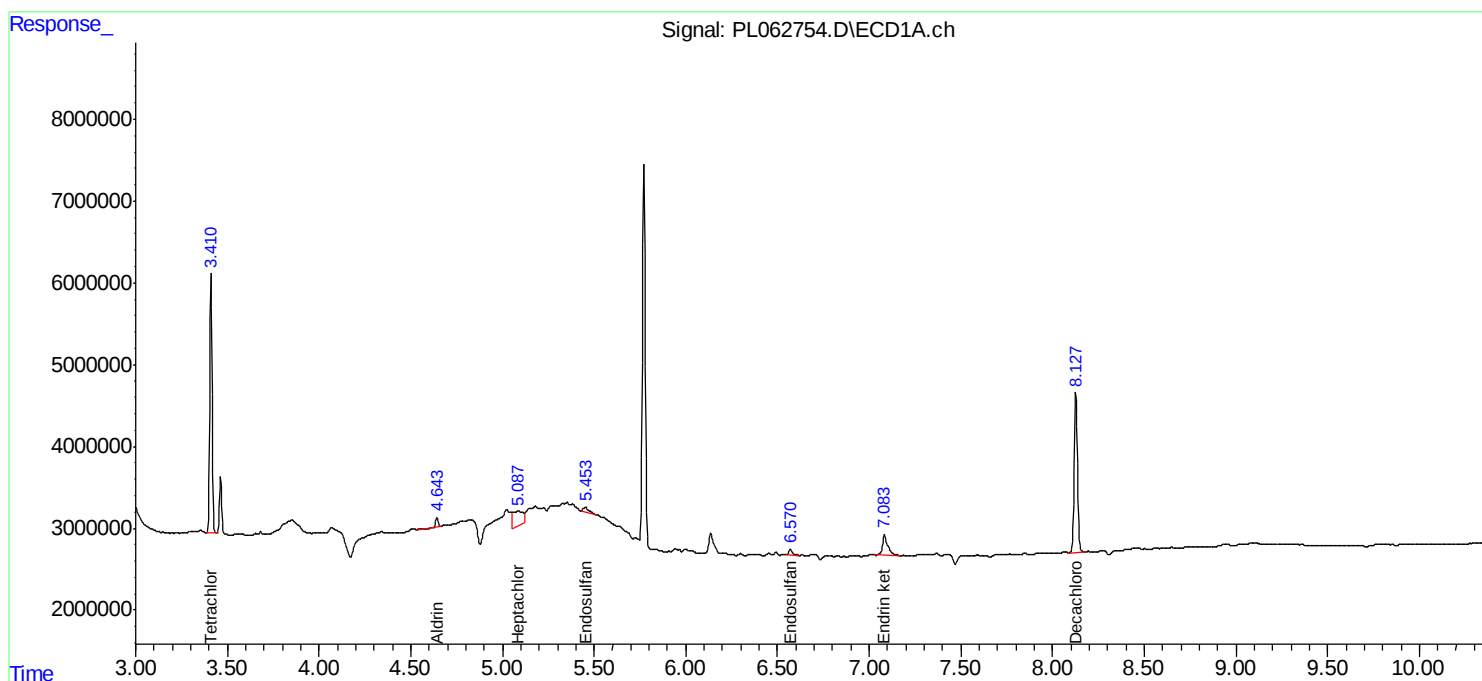


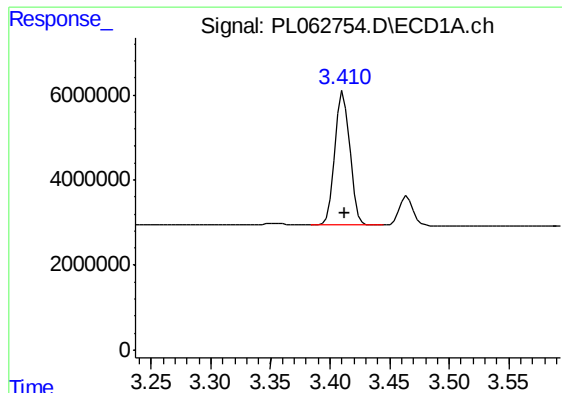

#1 Tetrachloro-m-xylene


R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 26997658
Conc: 15.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-05-102820

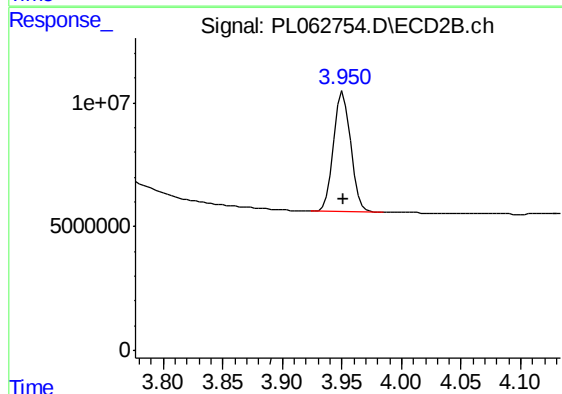


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 48029376
Conc: 16.34 ng/ml

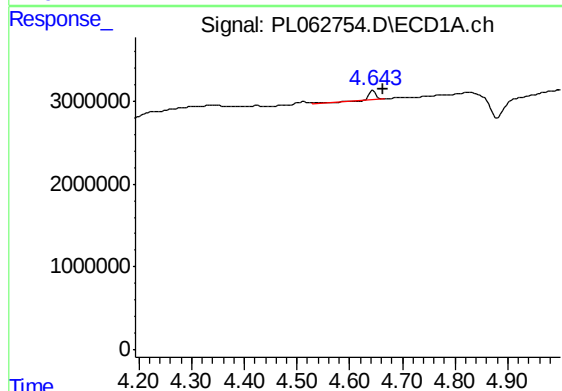


#5 Aldrin

R.T.: 4.645 min
Delta R.T.: -0.020 min
Response: 1198245
Conc: 0.63 ng/ml

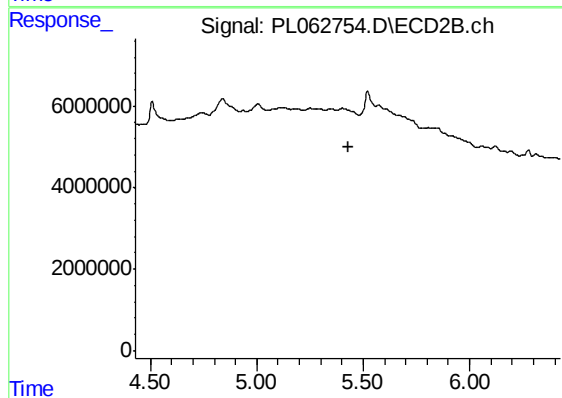

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 5.429 min
Response: 0
Conc: N.D.

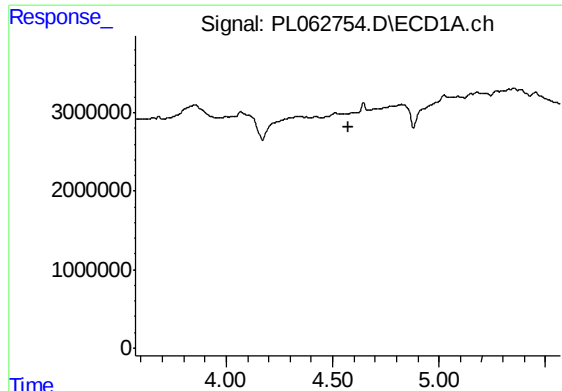

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.573 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
AU-05-102820

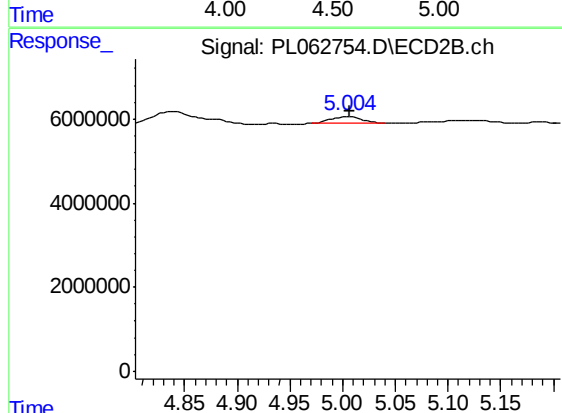


#7 delta-BHC

R.T.: 5.006 min
Delta R.T.: 0.000 min
Response: 3154321
Conc: 0.90 ng/ml

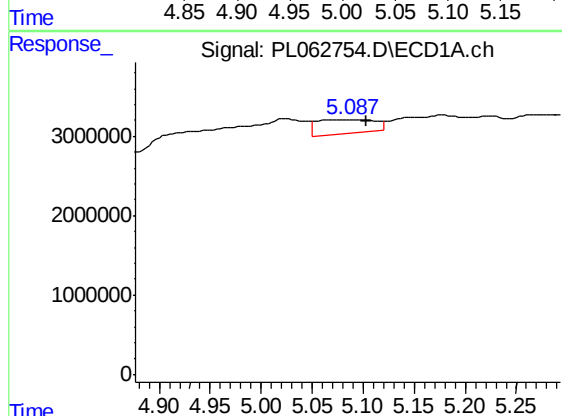


#8 Heptachlor epoxide

R.T.: 5.089 min
Delta R.T.: -0.015 min
Response: 6786867
Conc: 3.72 ng/ml

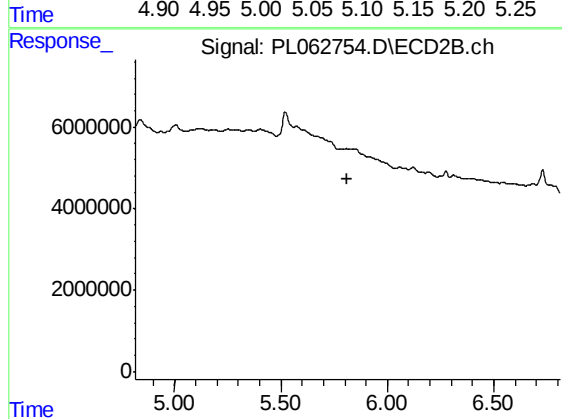

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.815 min
Response: 0
Conc: N.D.

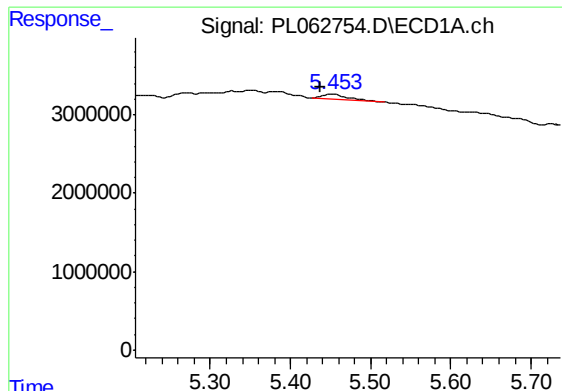

#9 Endosulfan I


R.T.: 5.453 min
Delta R.T.: 0.015 min
Response: 1394972
Conc: 0.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-05-102820

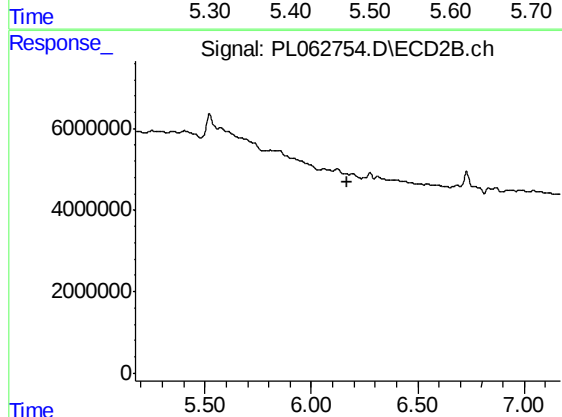


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.170 min
Response: 0
Conc: N.D.

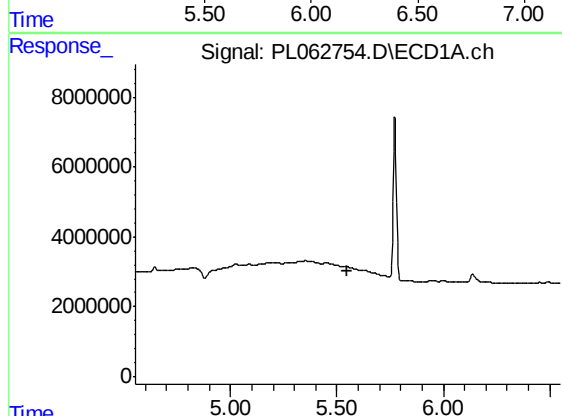


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 5.550 min
Response: 0
Conc: N.D.

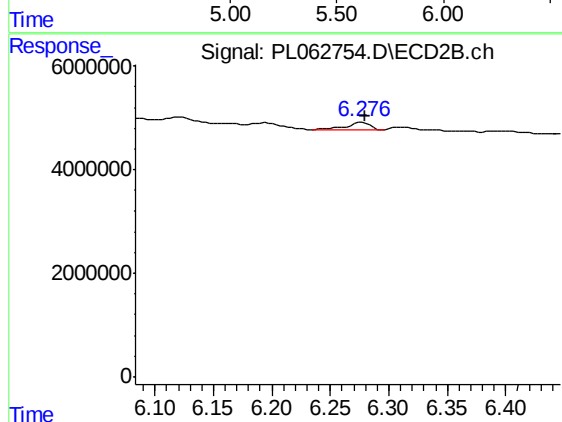

#12 4,4'-DDE


R.T.: 6.277 min
Delta R.T.: -0.002 min
Response: 2055131
Conc: 0.64 ng/ml

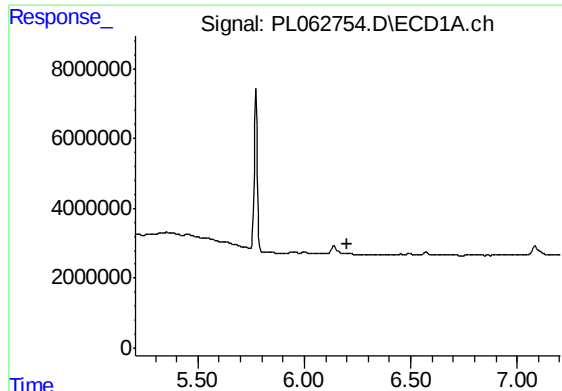

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.205 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
AU-05-102820

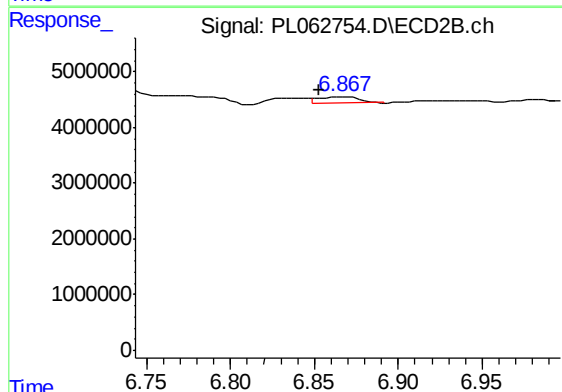


#15 Endosulfan II

R.T.: 6.869 min
Delta R.T.: 0.016 min
Response: 1952007
Conc: 0.68 ng/ml

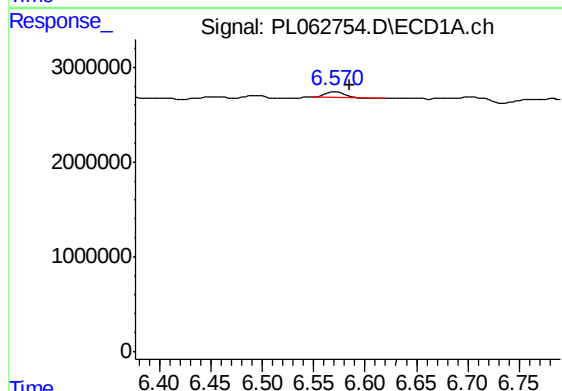


#19 Endosulfan Sulfate

R.T.: 6.571 min
Delta R.T.: -0.014 min
Response: 873043
Conc: 0.53 ng/ml

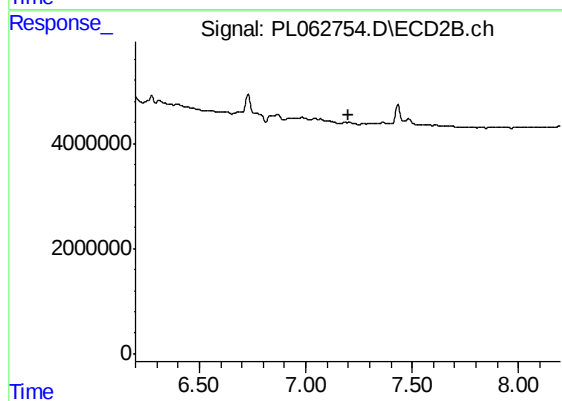

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.199 min
Response: 0
Conc: N.D.

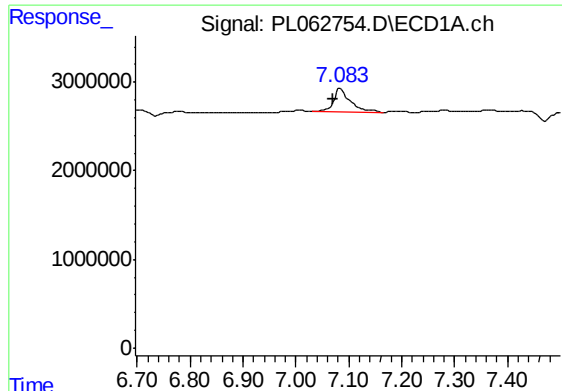

#21 Endrin ketone


R.T.: 7.084 min
Delta R.T.: 0.013 min
Response: 5560474
Conc: 3.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-05-102820

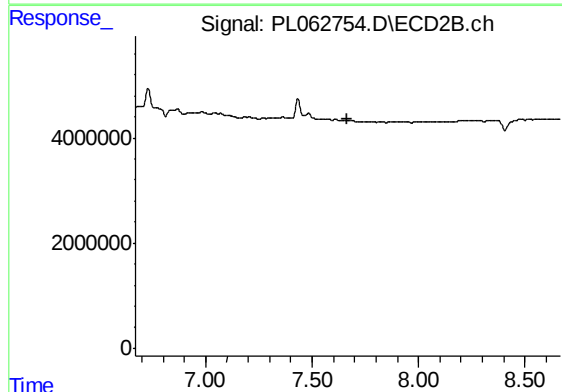


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.668 min
Response: 0
Conc: N.D.

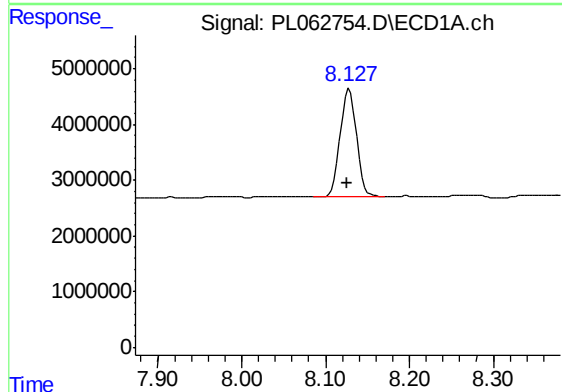

#28 Decachlorobiphenyl

R.T.: 8.128 min
Delta R.T.: 0.002 min
Response: 26126287
Conc: 16.29 ng/ml

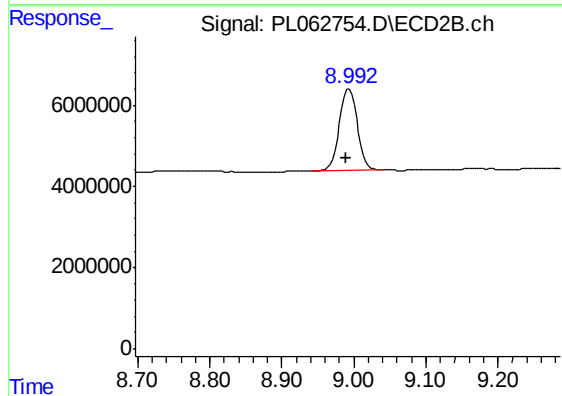

#28 Decachlorobiphenyl

R.T.: 8.993 min
Delta R.T.: 0.005 min
Response: 34979342
Conc: 16.71 ng/ml