

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110220\
 Data File : PL062761.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2020 13:08
 Operator : DD\AJ
 Sample : L4541-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20-105

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 03:02:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.411	3.951	12721124	20524324	7.396	6.984
28)	SA Decachlor...	8.127	8.992	5423892	5712919	3.381	2.730
Target Compounds							
2)	A alpha-BHC	3.842	0.000	1424869	0	0.559	N.D. #
4)	MA Heptachlor	0.000	5.146f	0	1448260	N.D.	0.363 #
7)	B delta-BHC	0.000	5.002	0	4410222	N.D.	1.260 #
8)	B Heptachlo...	5.109	0.000	2580781	0	1.414	N.D. #
9)	A Endosulfan I	5.459f	0.000	1934925	0	1.158	N.D. #
15)	B Endosulfa...	0.000	6.870f	0	5369276	N.D.	1.878 #
21)	B Endrin ke...	7.082	0.000	1597206	0	0.886	N.D. #
23)	Chlordane-1	4.275	0.000	1442434	0	27.981	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110220\
Data File : PL062761.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2020 13:08
Operator : DD\AJ
Sample : L4541-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
20-105

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 03:02:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

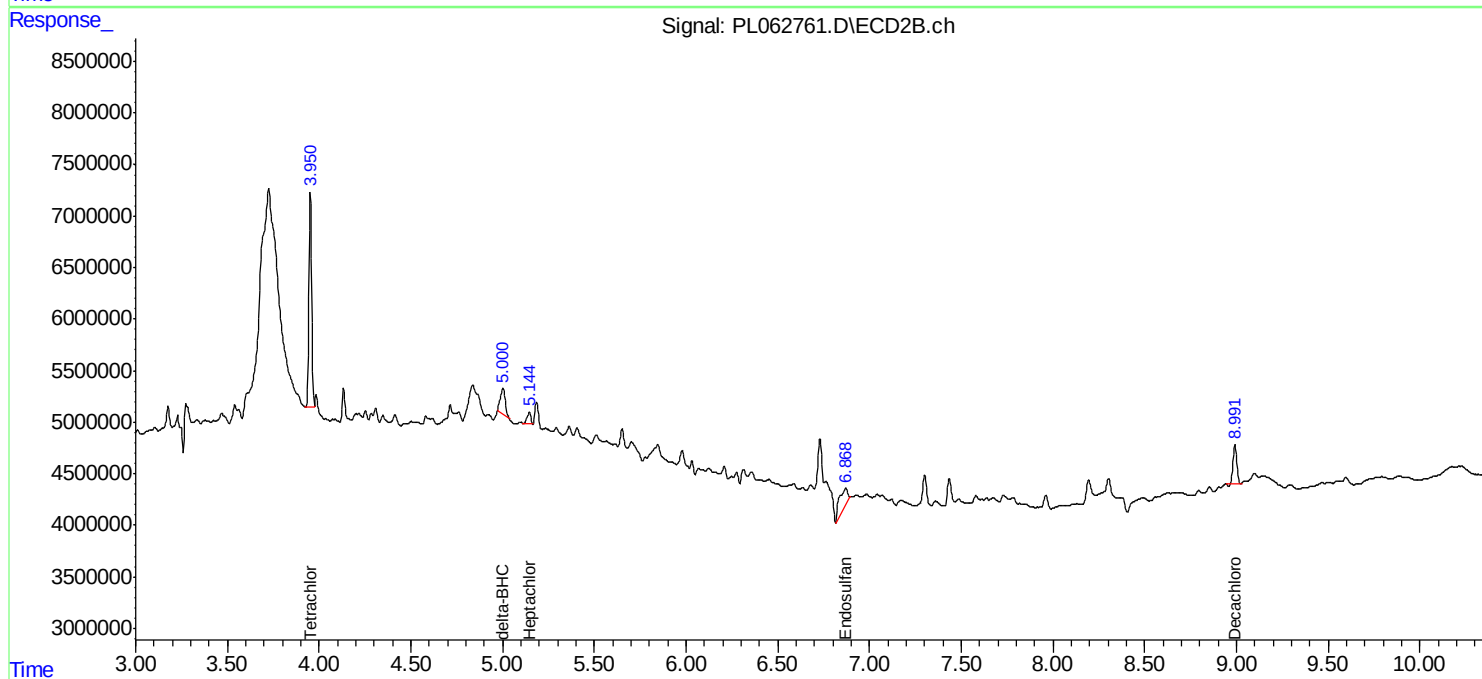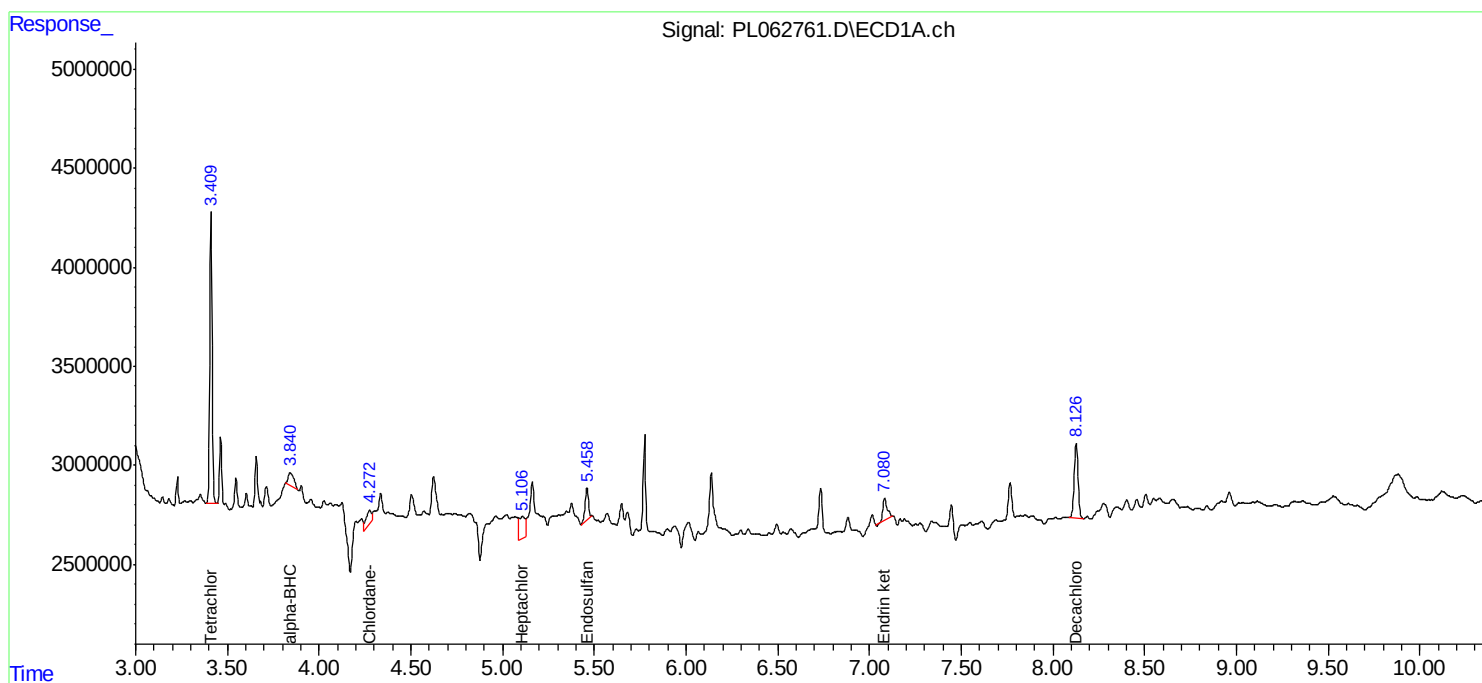


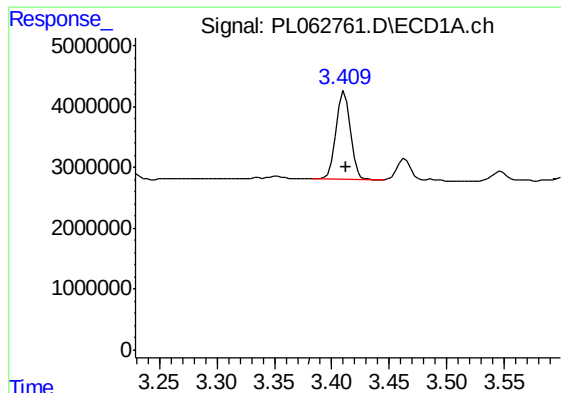

#1 Tetrachloro-m-xylene


R.T.: 3.411 min
Delta R.T.: -0.001 min
Response: 12721124
Conc: 7.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
20-105

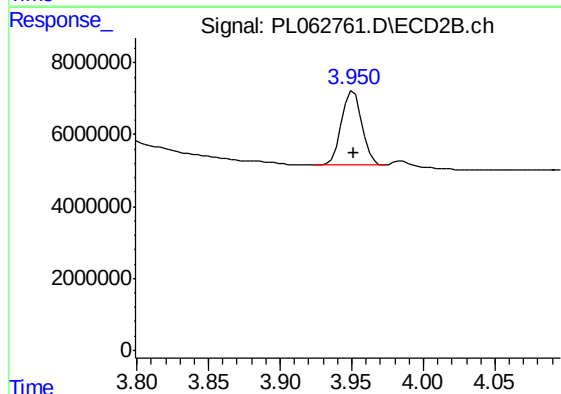


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 20524324
Conc: 6.98 ng/ml

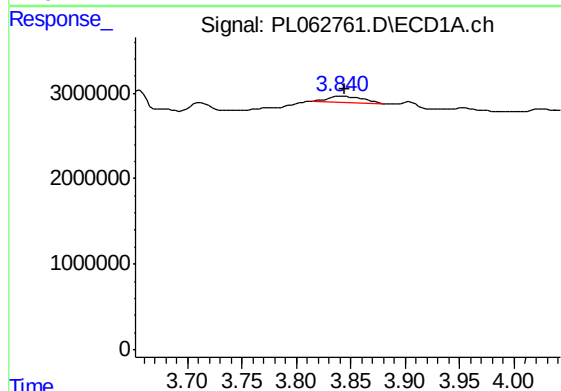


#2 alpha-BHC

R.T.: 3.842 min
Delta R.T.: -0.003 min
Response: 1424869
Conc: 0.56 ng/ml

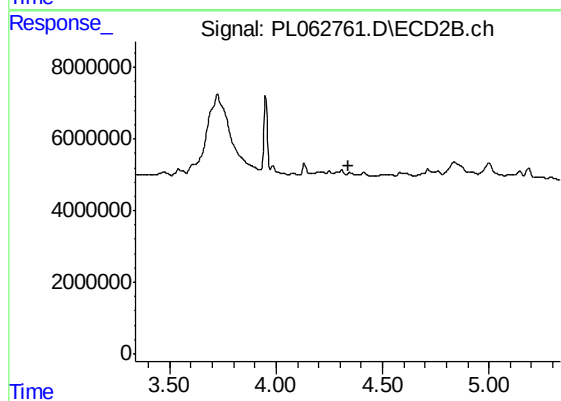

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.338 min
Response: 0
Conc: N.D.

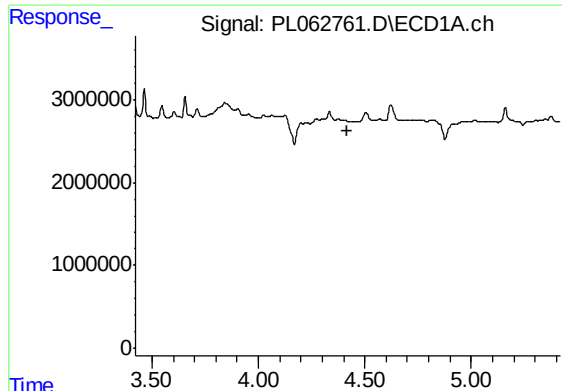

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 4.420 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20-105

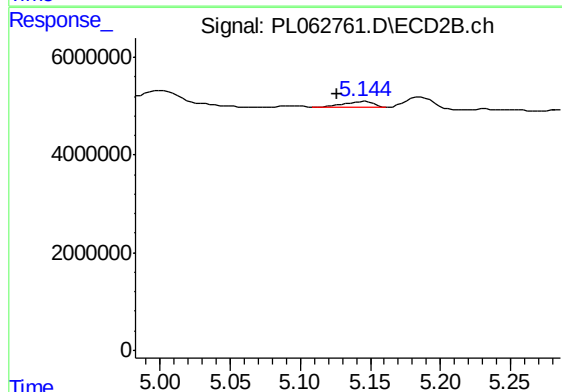


#4 Heptachlor

R.T.: 5.146 min
Delta R.T.: 0.020 min
Response: 1448260
Conc: 0.36 ng/ml

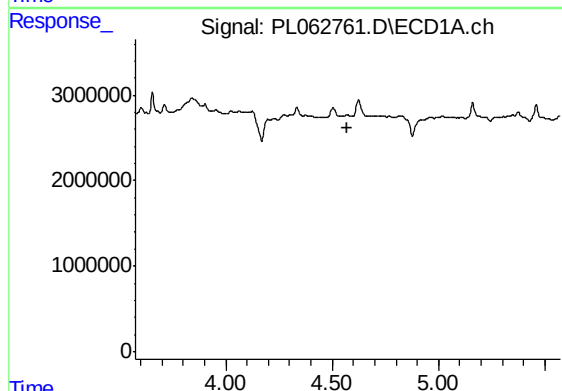


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.573 min
Response: 0
Conc: N.D.

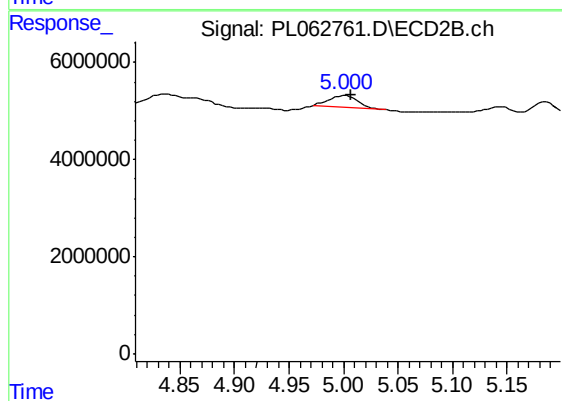

#7 delta-BHC


R.T.: 5.002 min
Delta R.T.: -0.005 min
Response: 4410222
Conc: 1.26 ng/ml

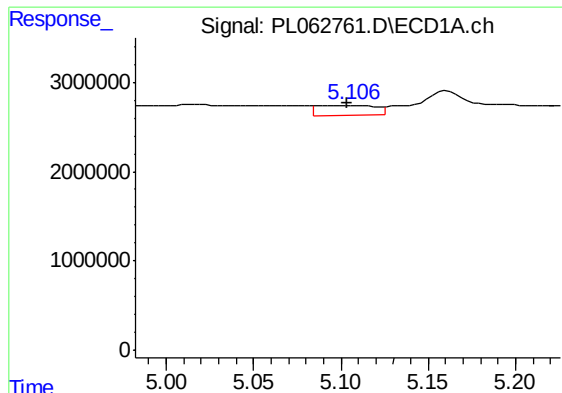

#8 Heptachlor epoxide


R.T.: 5.109 min
Delta R.T.: 0.005 min
Response: 2580781
Conc: 1.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
20-105

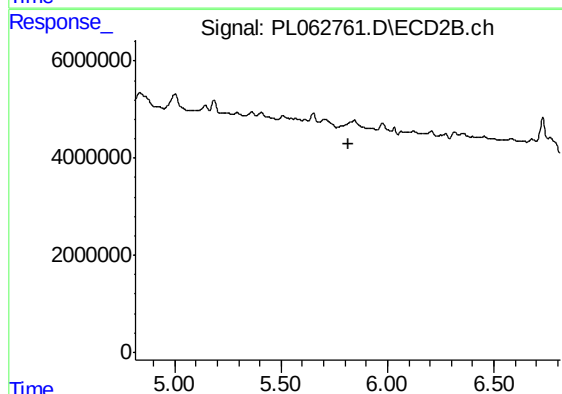


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.815 min
Response: 0
Conc: N.D.

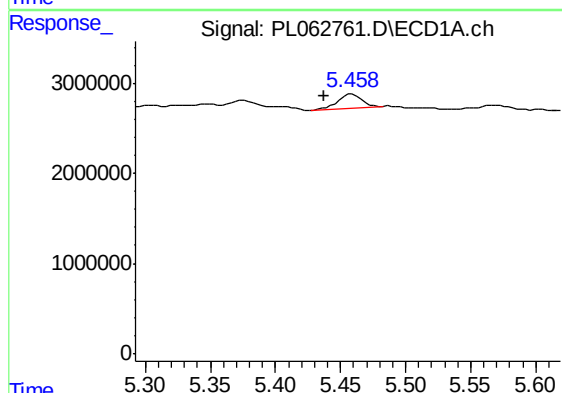


#9 Endosulfan I

R.T.: 5.459 min
Delta R.T.: 0.021 min
Response: 1934925
Conc: 1.16 ng/ml

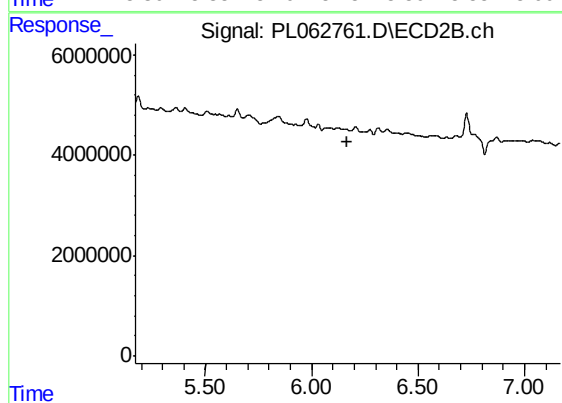

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.170 min
Response: 0
Conc: N.D.

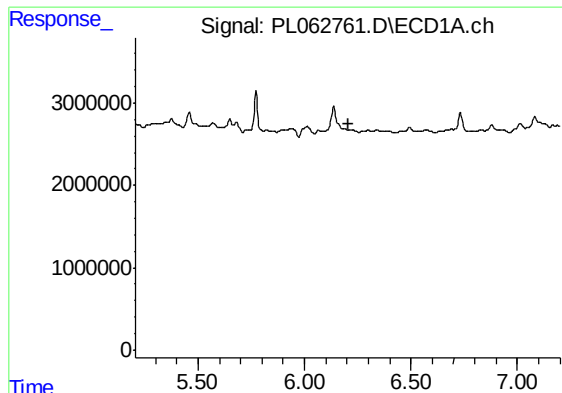

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.205 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20-105

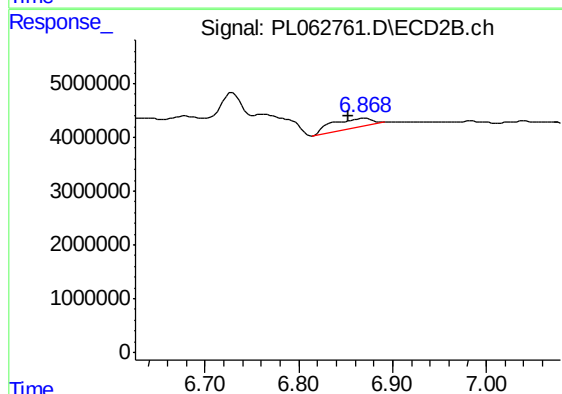


#15 Endosulfan II

R.T.: 6.870 min
Delta R.T.: 0.017 min
Response: 5369276
Conc: 1.88 ng/ml

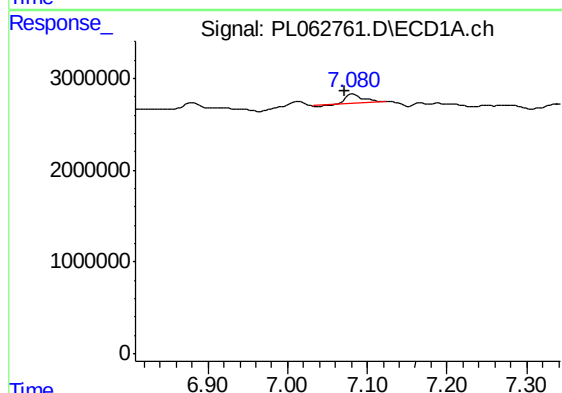


#21 Endrin ketone

R.T.: 7.082 min
Delta R.T.: 0.011 min
Response: 1597206
Conc: 0.89 ng/ml

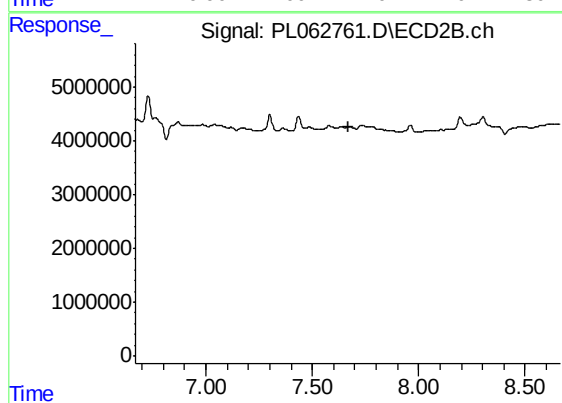

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.668 min
Response: 0
Conc: N.D.

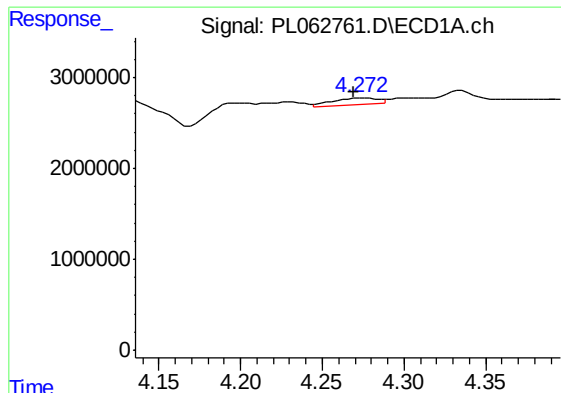

#23 Chlordane-1


R.T.: 4.275 min
Delta R.T.: 0.006 min
Response: 1442434
Conc: 27.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
20-105

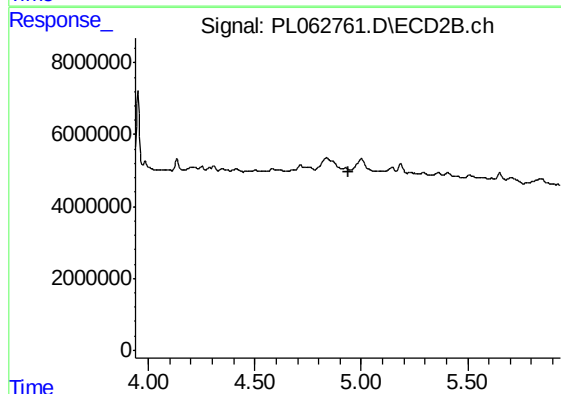


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.938 min
Response: 0
Conc: N.D.

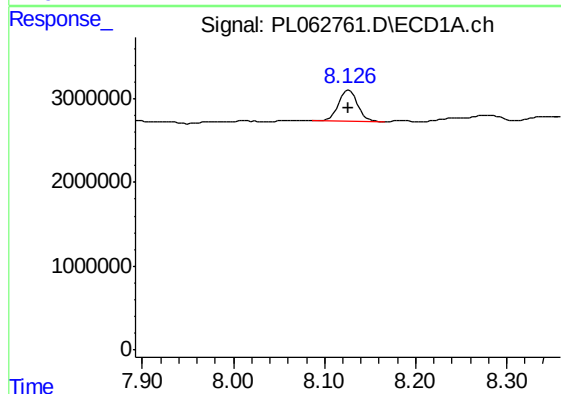

#28 Decachlorobiphenyl

R.T.: 8.127 min
Delta R.T.: 0.000 min
Response: 5423892
Conc: 3.38 ng/ml

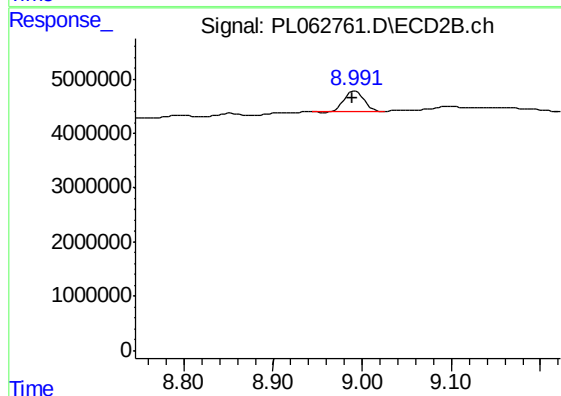

#28 Decachlorobiphenyl

R.T.: 8.992 min
Delta R.T.: 0.003 min
Response: 5712919
Conc: 2.73 ng/ml