

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110220\
 Data File : PL062779.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2020 17:45
 Operator : DD\AJ
 Sample : L4549-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BUS-WASH-RECLAMATION-PIT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 03:08:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	3.411	3.951	33550204	50505235	19.505	17.186
28) SA	Decachlor...	8.127	8.993	34423634	44968850	21.457	21.486
Target Compounds							
2) A	alpha-BHC	0.000	4.338	0	3481533	N.D.	0.784 #
7) B	delta-BHC	0.000	4.983f	0	1582379	N.D.	0.452 #
8) B	Heptachlo...	5.081f	0.000	3681795	0	2.018	N.D. #
11) B	alpha-Chl...	5.375	0.000	1107444	0	0.613	N.D. #
21) B	Endrin ke...	7.083	0.000	1507655	0	0.836	N.D. #
23) B	Chlordane-1	4.276	0.000	934486	0	18.128	N.D. #
26) B	Chlordane-4	5.375	0.000	1107444	0	8.502	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110220\
Data File : PL062779.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2020 17:45
Operator : DD\AJ
Sample : L4549-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
BUS-WASH-RECLAMATION-PIT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 03:08:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

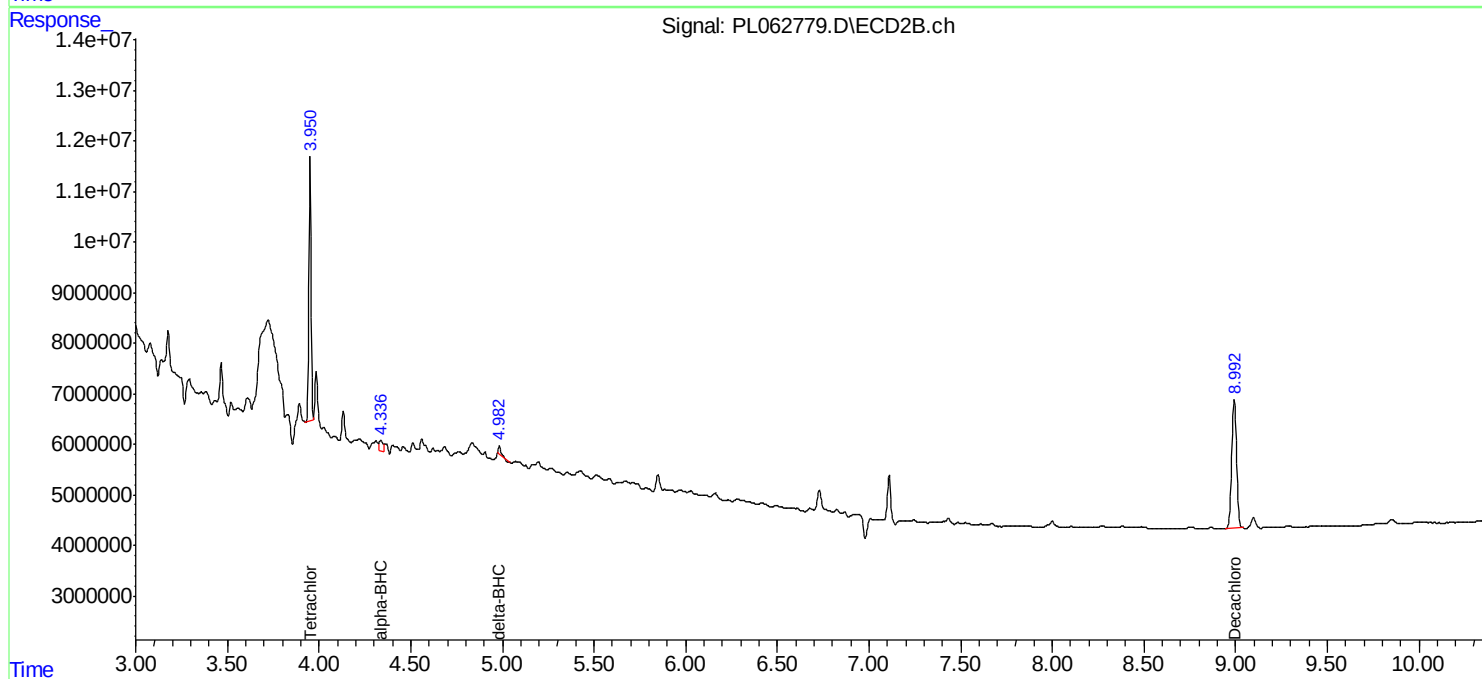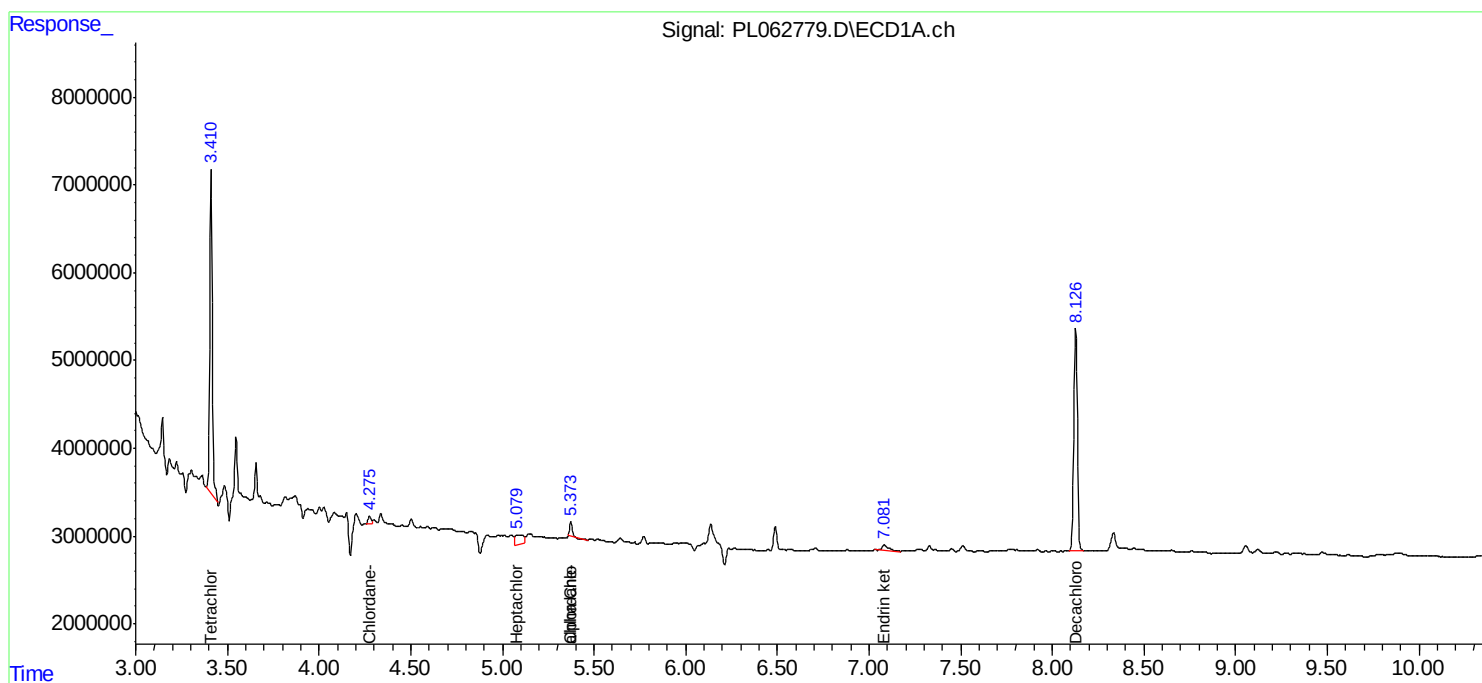


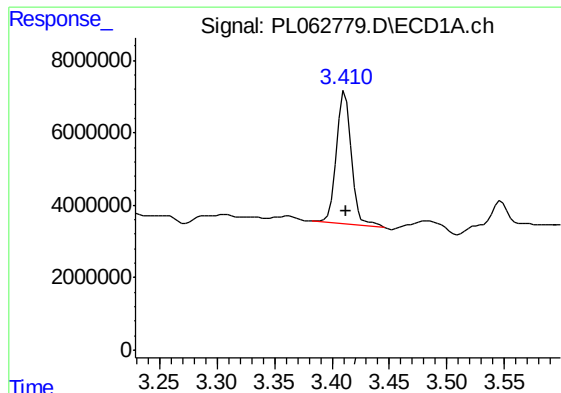

#1 Tetrachloro-m-xylene


R.T.: 3.411 min
Delta R.T.: 0.000 min
Response: 33550204
Conc: 19.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
BUS-WASH-RECLAMATION-PIT

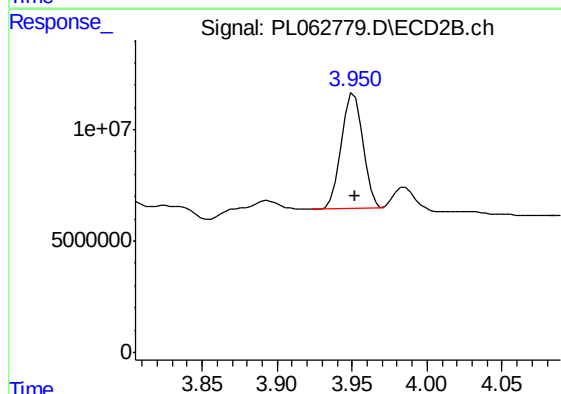


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 50505235
Conc: 17.19 ng/ml

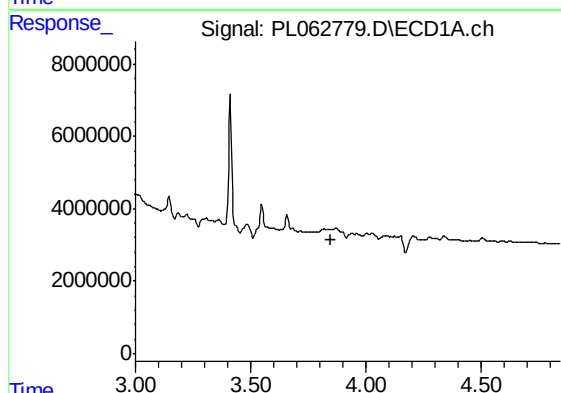


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.844 min
Response: 0
Conc: N.D.

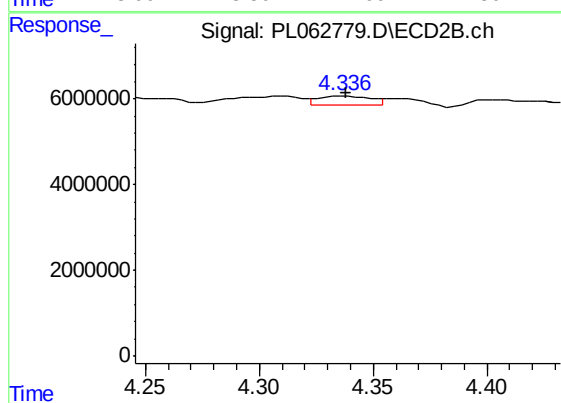

#2 alpha-BHC


R.T.: 4.338 min
Delta R.T.: 0.000 min
Response: 3481533
Conc: 0.78 ng/ml

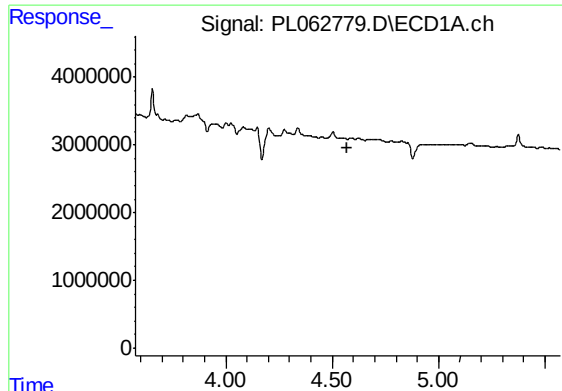

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.573 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
BUS-WASH-RECLAMATION-PIT

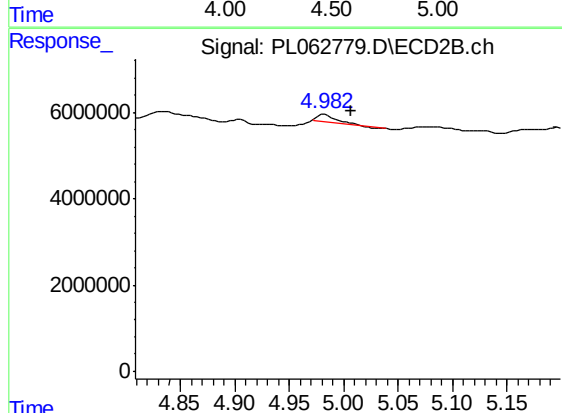


#7 delta-BHC

R.T.: 4.983 min
Delta R.T.: -0.023 min
Response: 1582379
Conc: 0.45 ng/ml

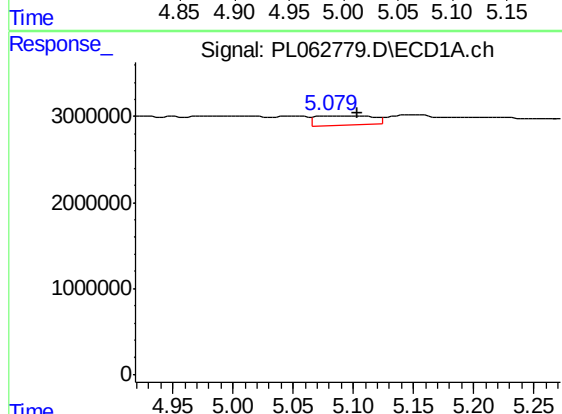


#8 Heptachlor epoxide

R.T.: 5.081 min
Delta R.T.: -0.022 min
Response: 3681795
Conc: 2.02 ng/ml

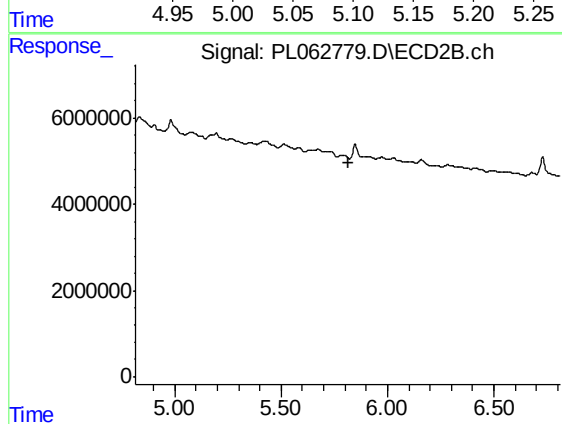

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.815 min
Response: 0
Conc: N.D.

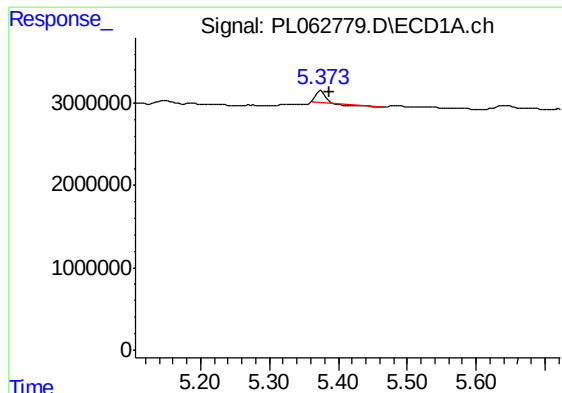

#11 alpha-Chlordane


R.T.: 5.375 min
Delta R.T.: -0.011 min
Response: 1107444
Conc: 0.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
BUS-WASH-RECLAMATION-PIT

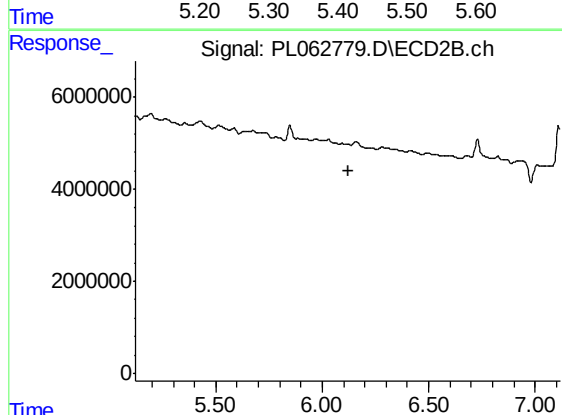


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.121 min
Response: 0
Conc: N.D.

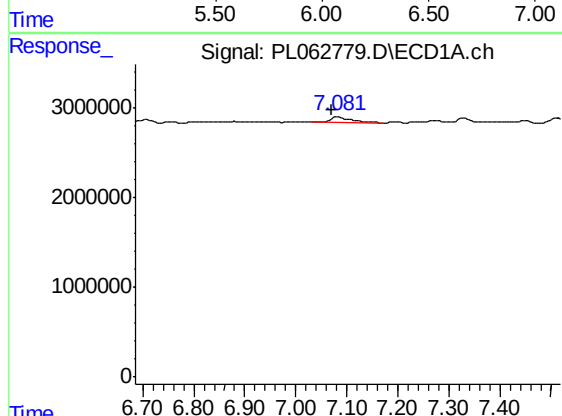


#21 Endrin ketone

R.T.: 7.083 min
Delta R.T.: 0.012 min
Response: 1507655
Conc: 0.84 ng/ml

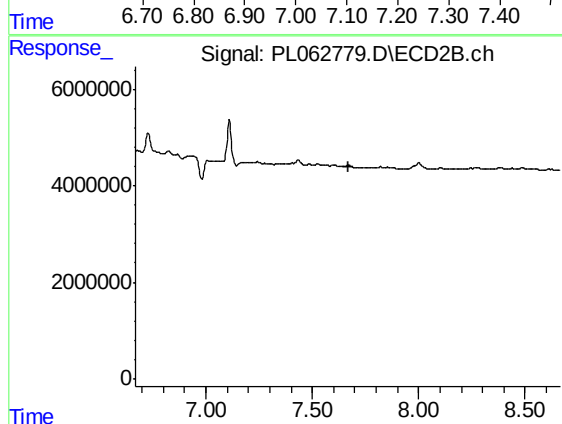

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.668 min
Response: 0
Conc: N.D.

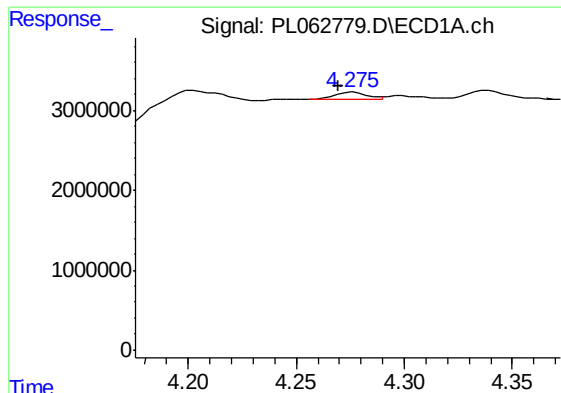

#23 Chlordane-1


R.T.: 4.276 min
Delta R.T.: 0.007 min
Response: 934486
Conc: 18.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
BUS-WASH-RECLAMATION-PIT

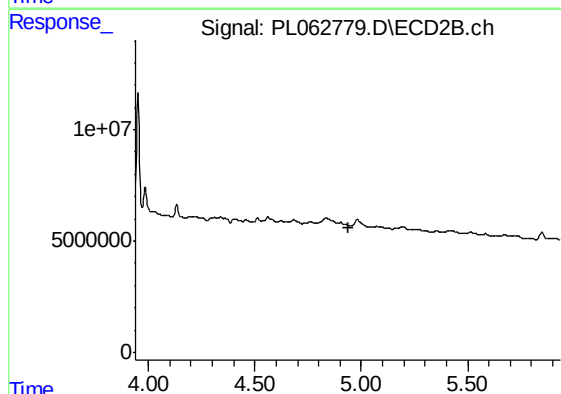


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.938 min
Response: 0
Conc: N.D.

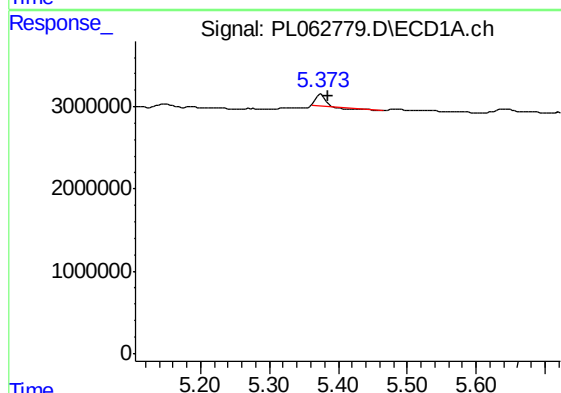


#26 Chlordane-4

R.T.: 5.375 min
Delta R.T.: -0.010 min
Response: 1107444
Conc: 8.50 ng/ml

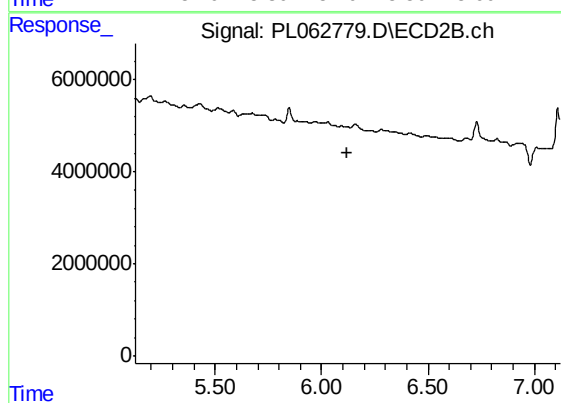

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.123 min
Response: 0
Conc: N.D.

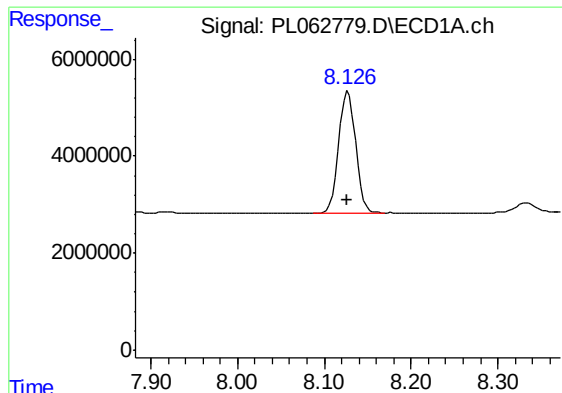

#28 Decachlorobiphenyl

R.T.: 8.127 min
Delta R.T.: 0.001 min
Response: 34423634
Conc: 21.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
BUS-WASH-RECLAMATION-PIT

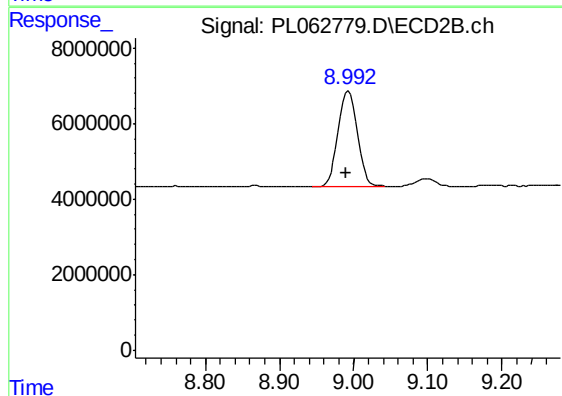

#28 Decachlorobiphenyl

R.T.: 8.993 min
Delta R.T.: 0.004 min
Response: 44968850
Conc: 21.49 ng/ml