

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110220\
 Data File : PL062762.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2020 13:22
 Operator : DD\AJ
 Sample : L4541-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 2015

Manual Integrations
 APPROVED

Ankita
 11/3/2020 3:32:34 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 03:02:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.411	3.951	21927071	36078069	12.748	12.277
28)	SA Decachlor...	8.127	8.991	9243457	10753608	5.762	5.138m
Target Compounds							
10)	B gamma-Chl...	5.328	6.037	1003228	6259664	0.557m	1.859 #
11)	B alpha-Chl...	5.380	6.121	2040163	2474113	1.129m	0.734m#
17)	MA 4,4'-DDT	6.300	7.067	597445	1070196	0.448m	0.477m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110220\
Data File : PL062762.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2020 13:22
Operator : DD\AJ
Sample : L4541-10
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
2015


Manual Integrations
APPROVED

Ankita
11/3/2020 3:32:34 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 03:02:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

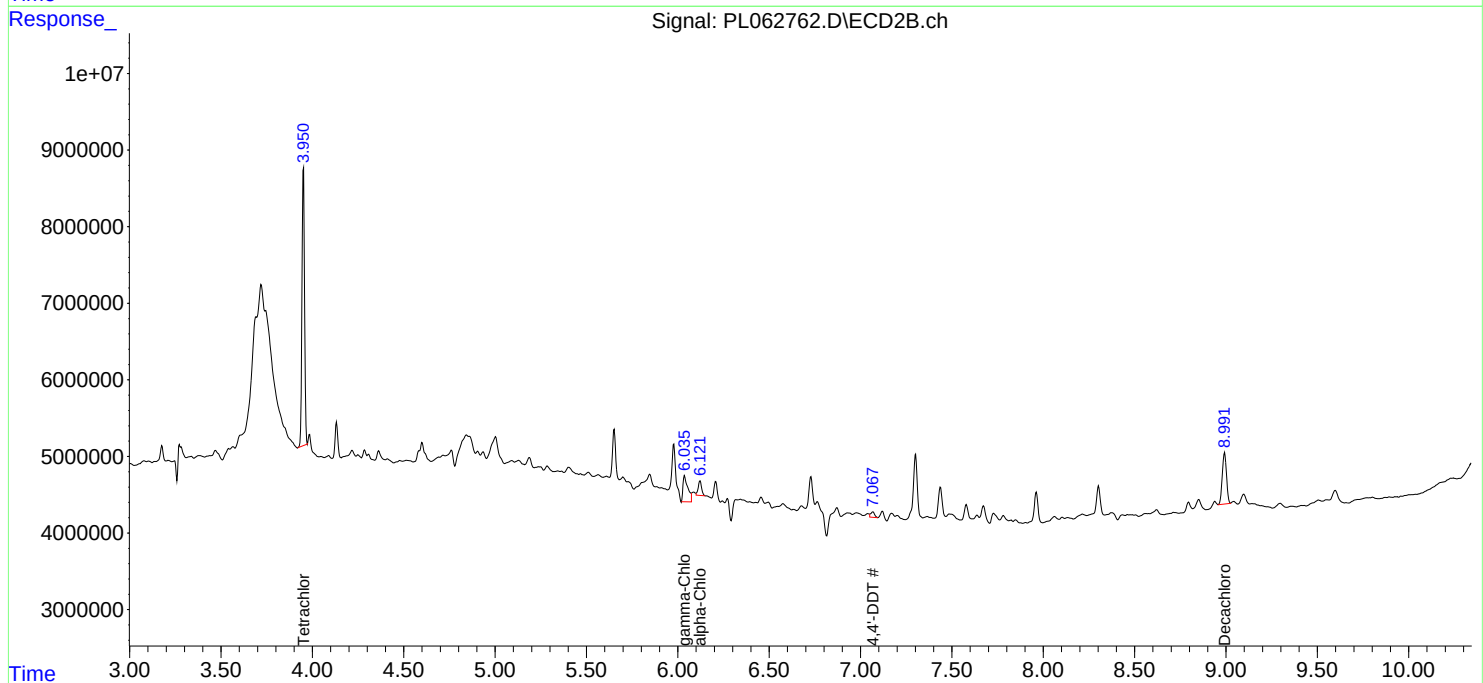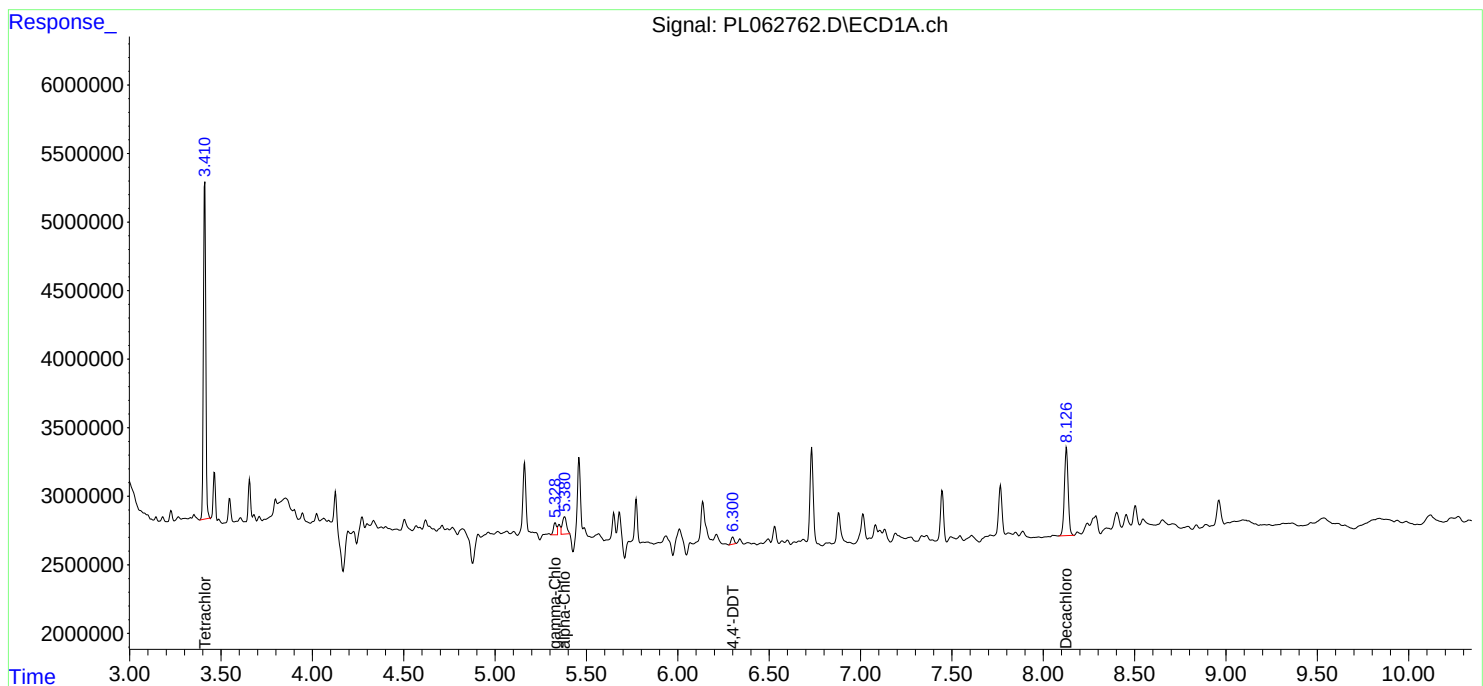

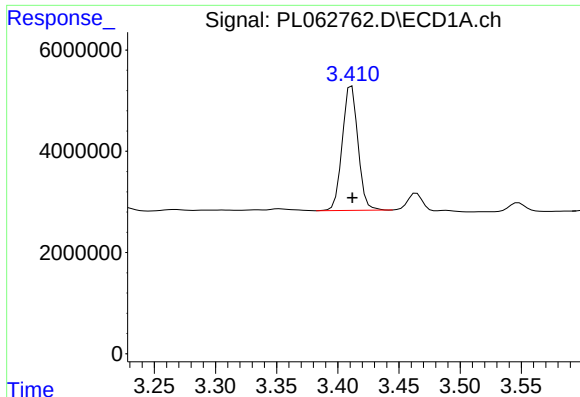


#1 Tetrachloro-m-xylene

R.T.: 3.411 min
Delta R.T.: 0.000 min
Response: 21927071
Conc: 12.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
2015


Manual Integrations
APPROVED

Ankita
11/3/2020 3:32:34 PM

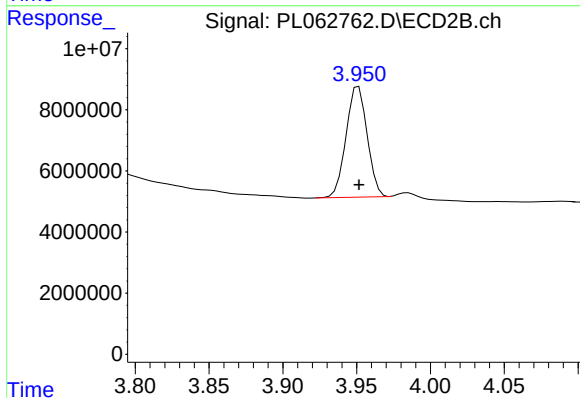


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 36078069
Conc: 12.28 ng/ml

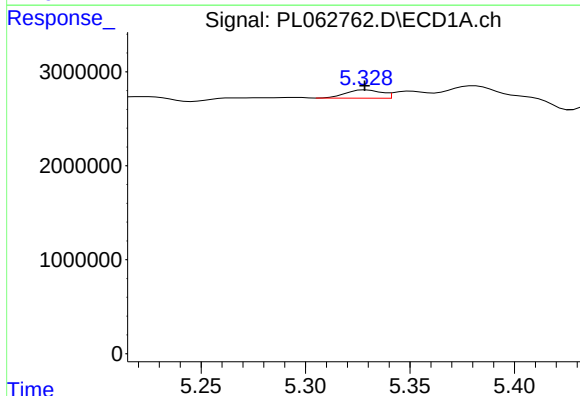


#10 gamma-Chlordane

R.T.: 5.328 min
Delta R.T.: 0.000 min
Response: 1003228
Conc: 0.56 ng/ml m

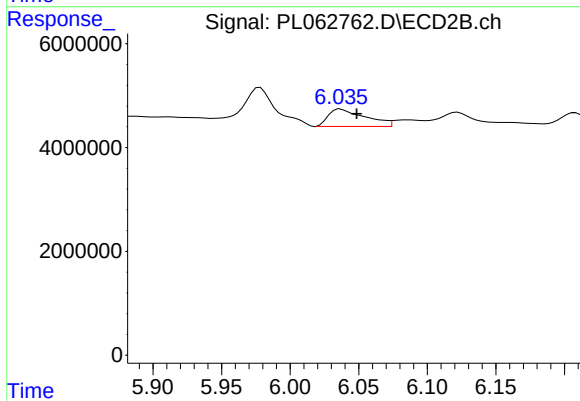

#10 gamma-Chlordane

R.T.: 6.037 min
Delta R.T.: -0.012 min
Response: 6259664
Conc: 1.86 ng/ml

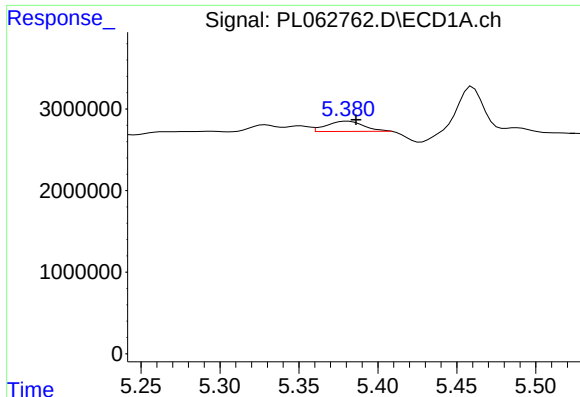


#11 alpha-Chlordane

R.T.: 5.380 min
Delta R.T.: -0.007 min
Response: 2040163
Conc: 1.13 ng/ml m

Instrument :
ECD_L
ClientSampleId :
2015


Manual Integrations
APPROVED

Ankita
11/3/2020 3:32:34 PM

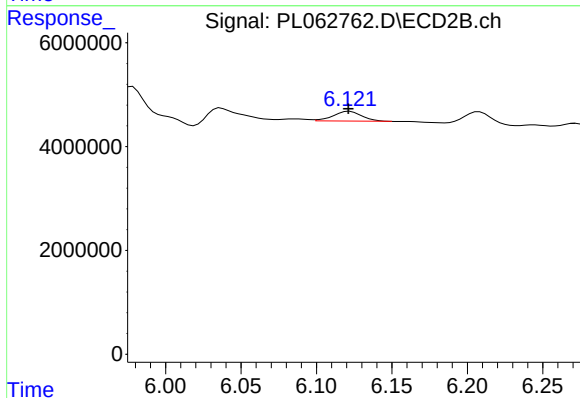


#11 alpha-Chlordane

R.T.: 6.121 min
Delta R.T.: 0.000 min
Response: 2474113
Conc: 0.73 ng/ml m

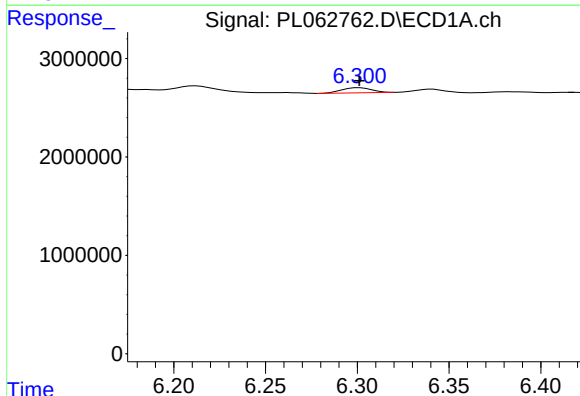


#17 4,4'-DDT

R.T.: 6.300 min
Delta R.T.: -0.001 min
Response: 597445
Conc: 0.45 ng/ml m

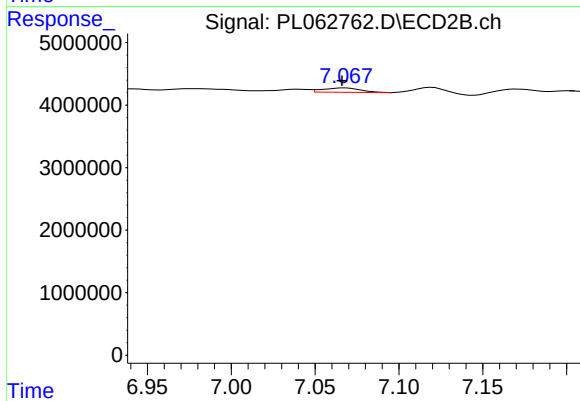

#17 4,4'-DDT

R.T.: 7.067 min
Delta R.T.: 0.000 min
Response: 1070196
Conc: 0.48 ng/ml m

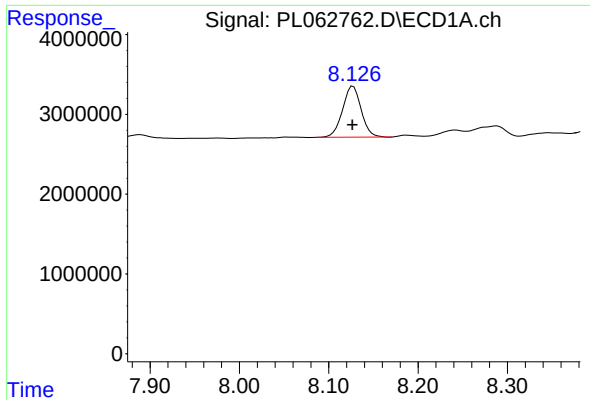


#28 Decachlorobiphenyl

R.T.: 8.127 min
Delta R.T.: 0.000 min
Response: 9243457
Conc: 5.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
2015

Manual Integrations
APPROVED

Ankita
11/3/2020 3:32:34 PM

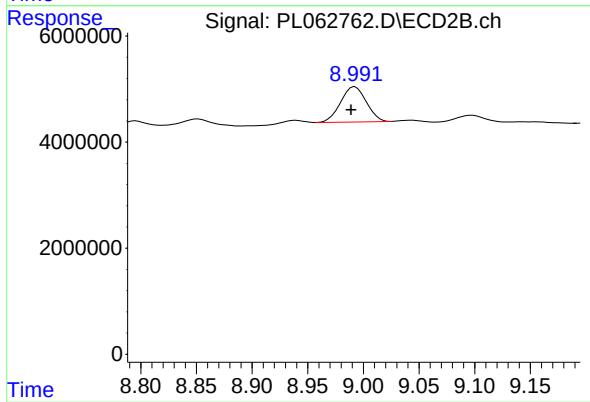

#28 Decachlorobiphenyl

R.T.: 8.991 min
Delta R.T.: 0.002 min
Response: 10753608
Conc: 5.14 ng/ml m