

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110221\
 Data File : PL070732.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2021 17:17
 Operator : AR\AJ
 Sample : M4411-01 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MH-HHS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/03/2021
 Supervised By : mohammad ahmed 11/03/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 22:45:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102921.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 29 09:09:01 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.587	5.516	1080239	2674684	2.396m	1.923m
28)	SA Decachlor...	10.349	11.422	1618106	3420835	2.710m	2.393

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110221\
Data File : PL070732.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2021 17:17
Operator : AR\AJ
Sample : M4411-01 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MH-HHS


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/03/2021
Supervised By : mohammad ahmed 11/03/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 22:45:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102921.M
Quant Title : GC Extractables
QLast Update : Fri Oct 29 09:09:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

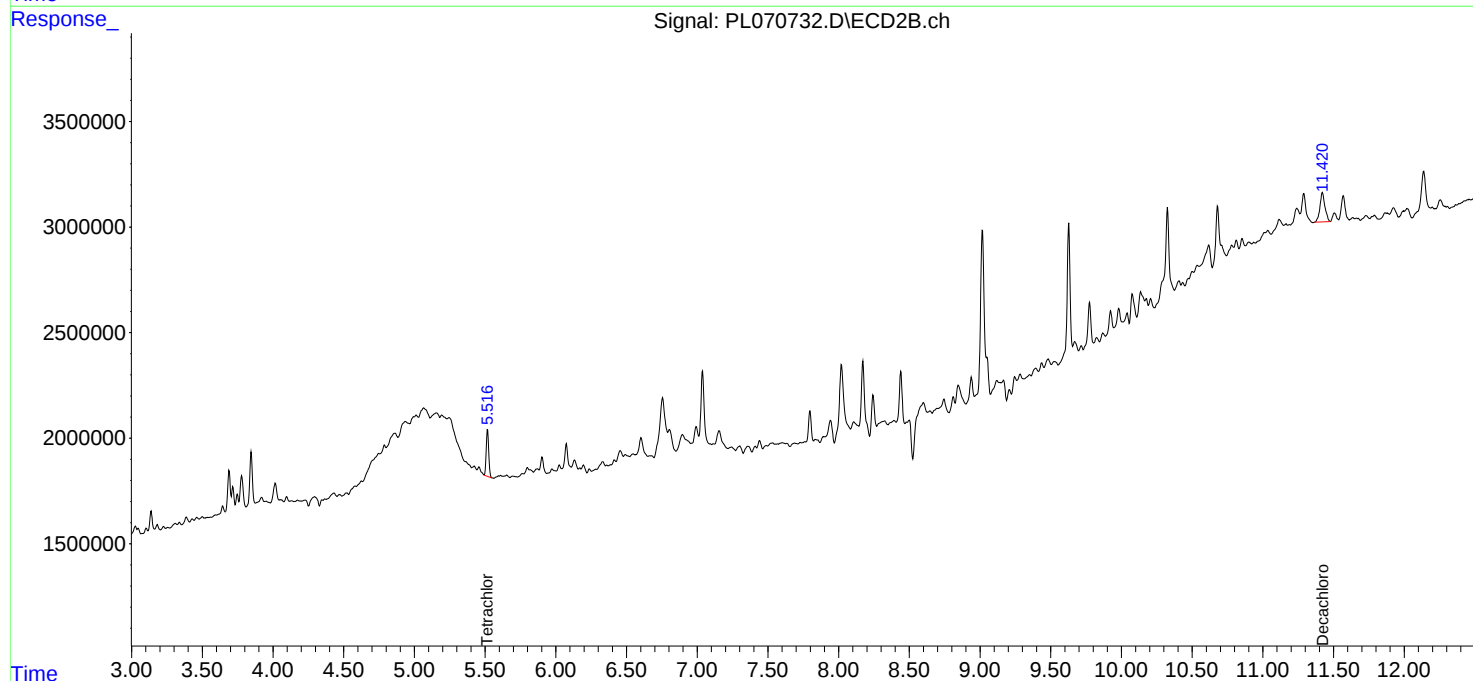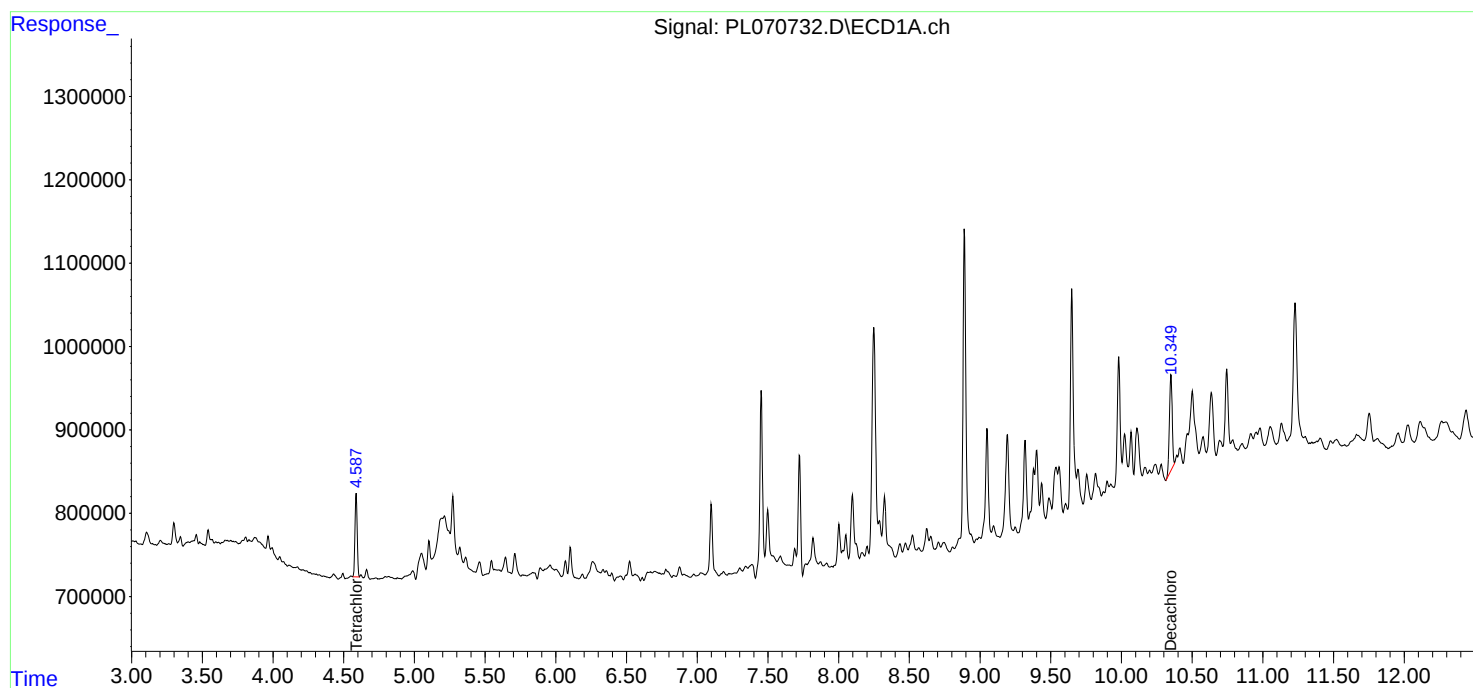

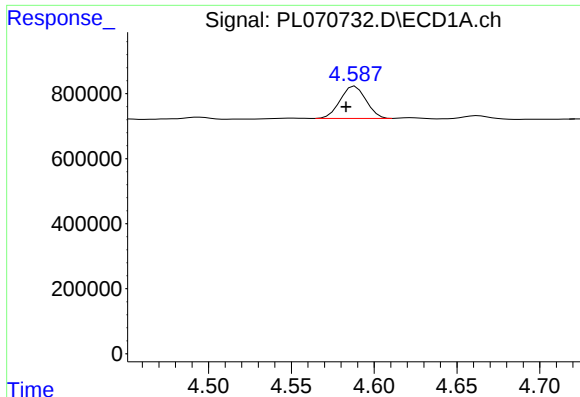


#1 Tetrachloro-m-xylene

R.T.: 4.587 min
Delta R.T.: 0.004 min
Response: 1080239
Conc: 2.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
MH-HHS


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/03/2021
Supervised By :mohammad ahmed 11/03/2021

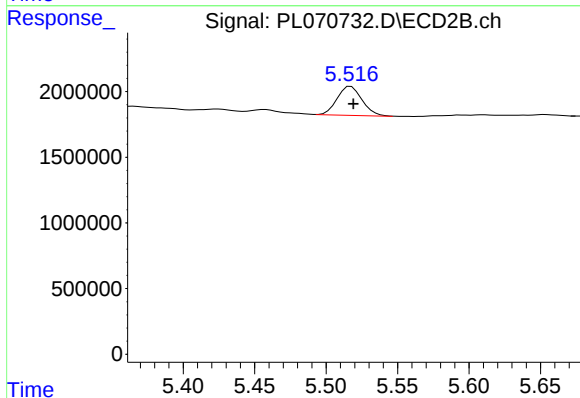


#1 Tetrachloro-m-xylene

R.T.: 5.516 min
Delta R.T.: -0.003 min
Response: 2674684
Conc: 1.92 ng/ml m

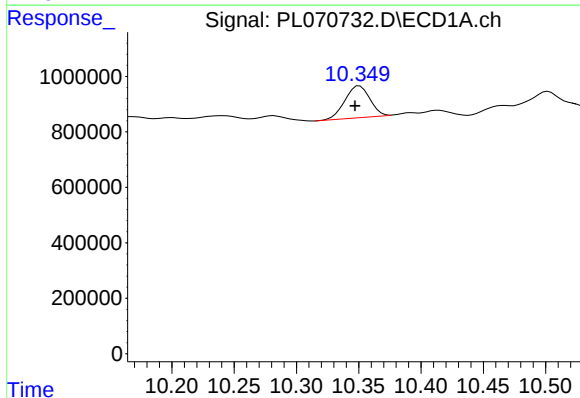

#28 Decachlorobiphenyl

R.T.: 10.349 min
Delta R.T.: 0.002 min
Response: 1618106
Conc: 2.71 ng/ml m

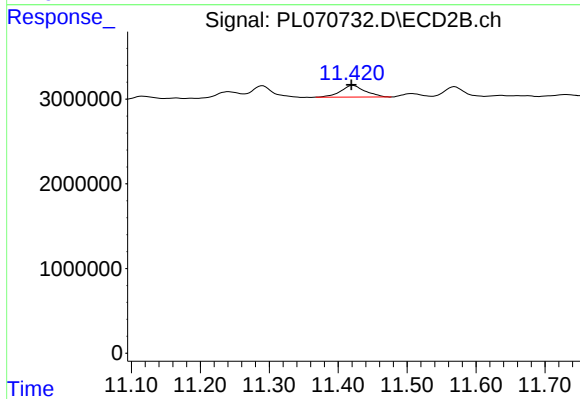

#28 Decachlorobiphenyl

R.T.: 11.422 min
Delta R.T.: 0.003 min
Response: 3420835
Conc: 2.39 ng/ml