

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110223\
 Data File : PL086385.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2023 09:08
 Operator : AR\AJ
 Sample : PIBLK216
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 21:27:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102623CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 27 01:35:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.354	2.618	60754859	17535015	21.316	19.333
27)	SA Decachlor...	8.854	7.768	106.7E6	44163881	42.832	38.473
Target Compounds							
3)	MA gamma-BHC...	4.132	0.000	387342	0	<MDL	N.D. #
4)	MA Heptachlor	4.734	0.000	43554	0	<MDL	N.D. #
7)	B delta-BHC	4.588	0.000	3073570	0	0.826	N.D. #
8)	B Heptachlo...	5.535f	0.000	405508	0	0.120	N.D. #
9)	A Endosulfan I	5.905	0.000	23595	0	<MDL	N.D. #
10)	B trans-Chl...	5.759	0.000	96395	0	<MDL	N.D. #
11)	B cis-Chlor...	5.821	0.000	1002285	0	0.285	N.D. #
12)	B 4,4'-DDE	6.010	0.000	587997	0	0.187	N.D. #
13)	MA Dieldrin	6.160	0.000	338747	0	<MDL	N.D. #
15)	B Endosulfa...	6.608	0.000	1190042	0	0.380	N.D. #
19)	B Endosulfa...	6.960	0.000	481557	0	0.169	N.D. #
20)	A Methoxychlor	7.341	0.000	282464	0	0.224	N.D. #
21)	B Endrin ke...	7.399f	0.000	2591242	0	0.899	N.D. #
22)	Toxaphene-1	6.010f	0.000	587997	0	26.075	N.D. #
24)	Toxaphene-3	6.960	0.000	481557	0	7.673	N.D. #
26)	Toxaphene-5	7.787f	0.000	567760	0	12.865	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110223\
Data File : PL086385.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2023 09:08
Operator : AR\AJ
Sample : PIBLK216
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 21:27:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102623CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 27 01:35:51 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

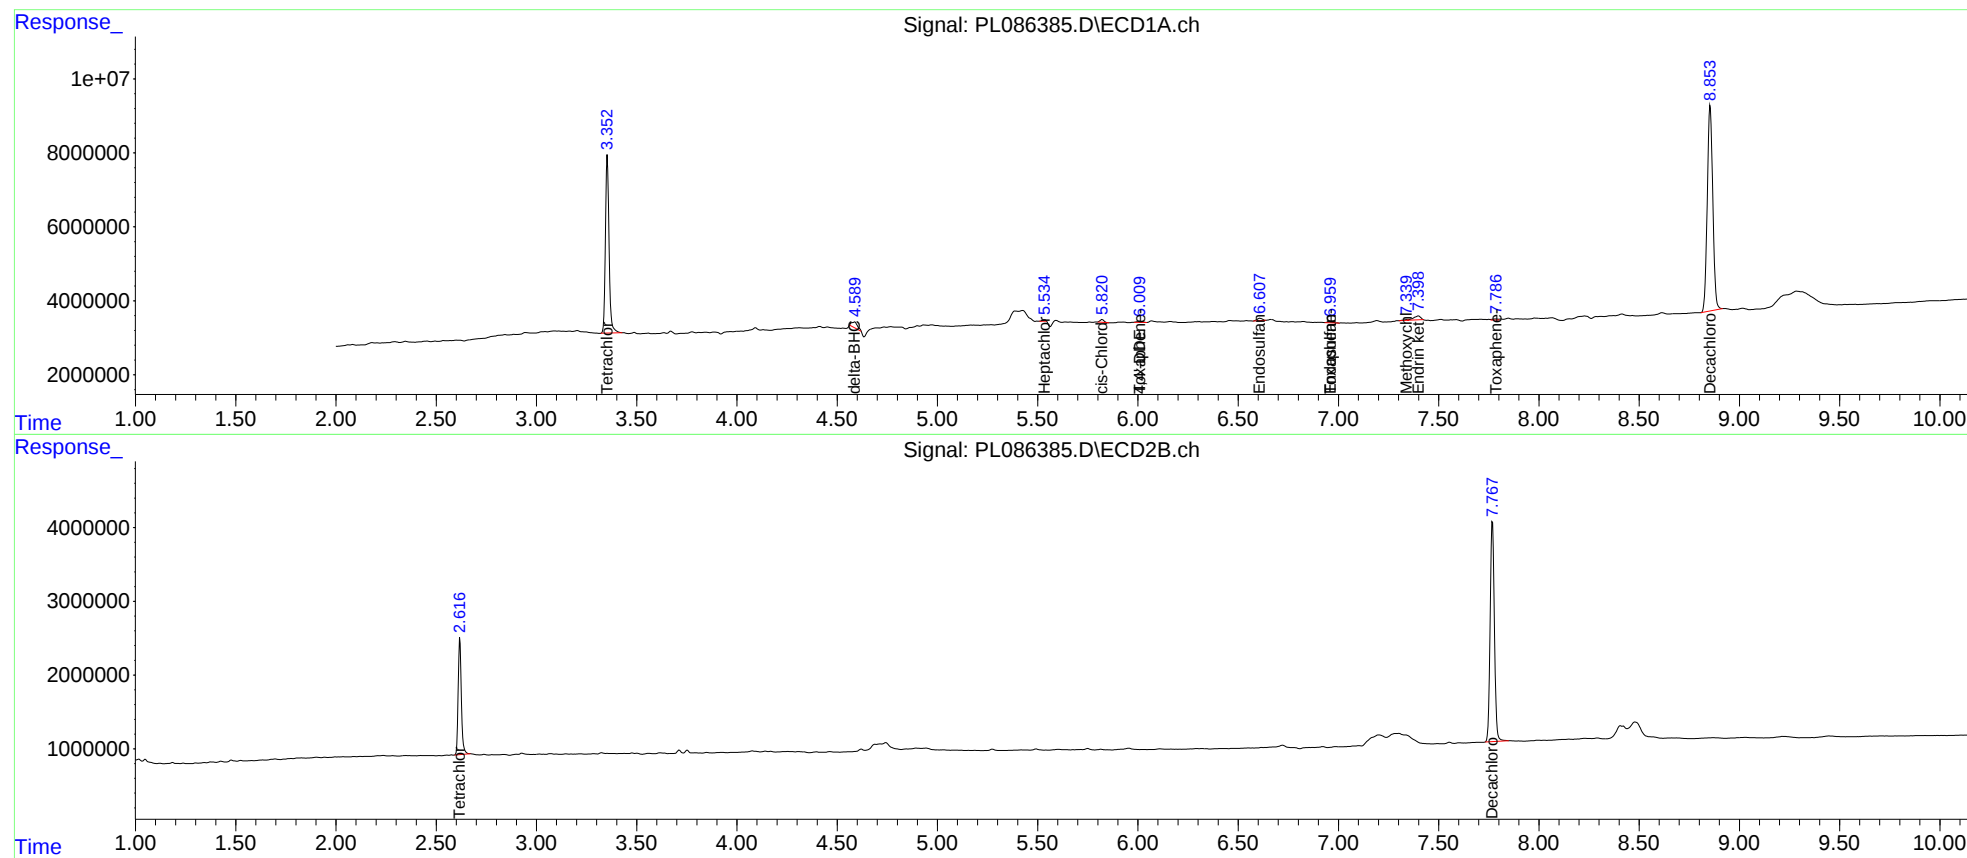

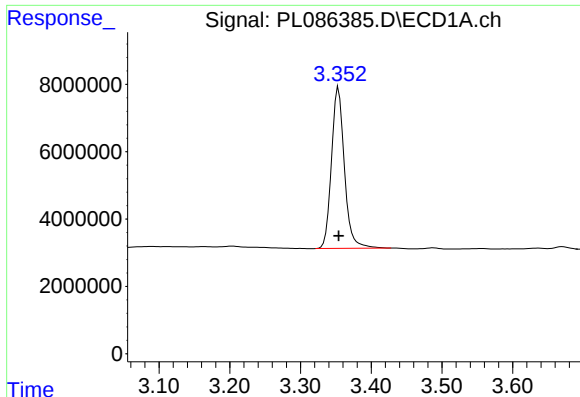


#1 Tetrachloro-m-xylene

R.T.: 3.354 min
Delta R.T.: 0.000 min
Response: 60754859
Conc: 21.32 ng/ml

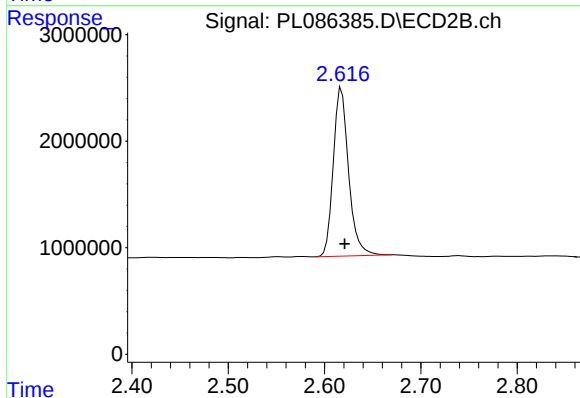


#1 Tetrachloro-m-xylene

R.T.: 2.618 min
Delta R.T.: -0.003 min
Response: 17535015
Conc: 19.33 ng/ml

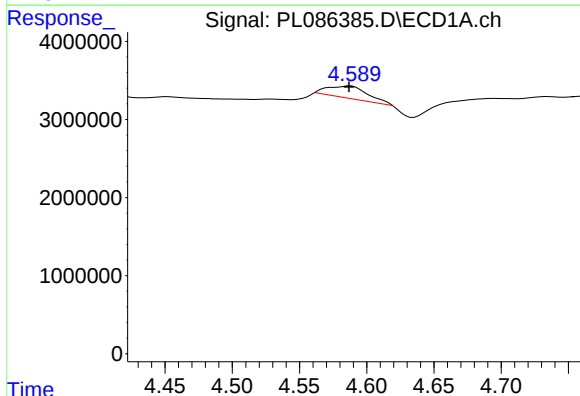


#7 delta-BHC

R.T.: 4.588 min
Delta R.T.: 0.000 min
Response: 3073570
Conc: 0.83 ng/ml

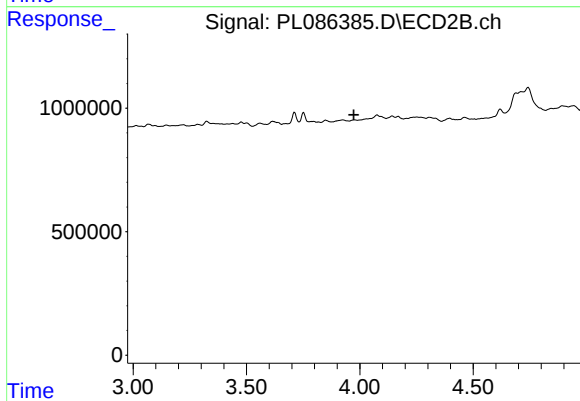


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 3.974 min
Response: 0
Conc: N.D.

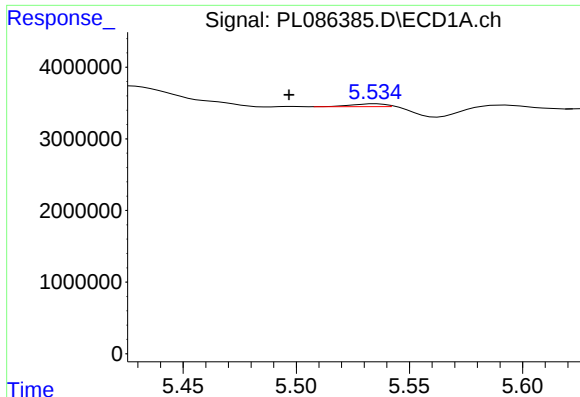


#8 Heptachlor epoxide

R.T.: 5.535 min
Delta R.T.: 0.038 min
Response: 405508
Conc: 0.12 ng/ml

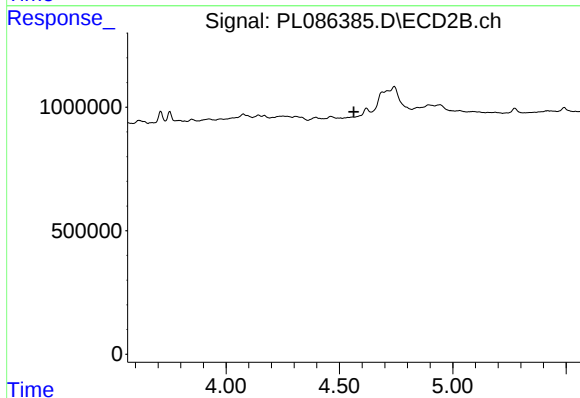


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.564 min
Response: 0
Conc: N.D.

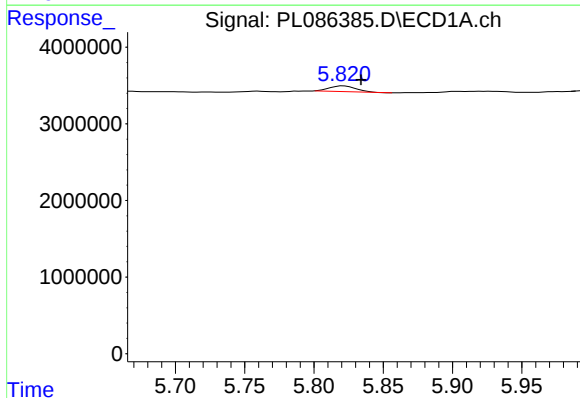


#11 cis-Chlordane

R.T.: 5.821 min
Delta R.T.: -0.013 min
Response: 1002285
Conc: 0.29 ng/ml

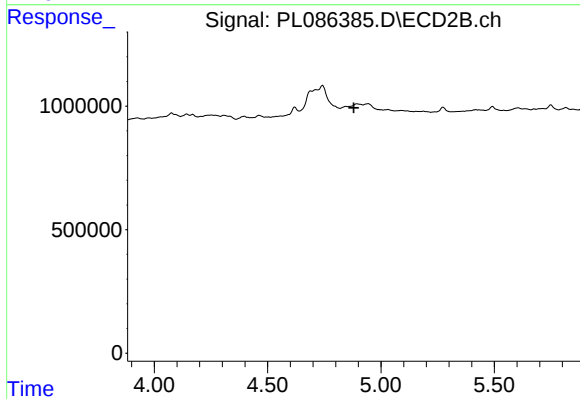


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 4.880 min
Response: 0
Conc: N.D.

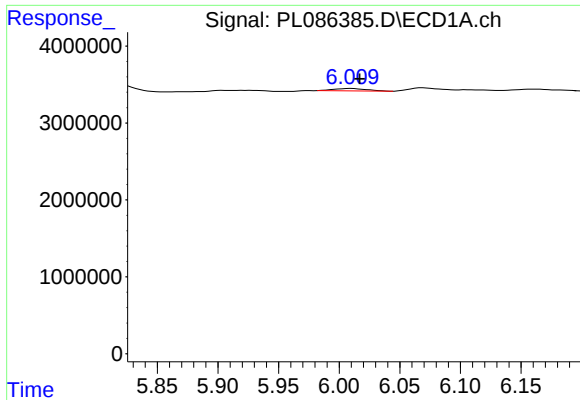


#12 4,4'-DDE

R.T.: 6.010 min
Delta R.T.: -0.007 min
Response: 587997
Conc: 0.19 ng/ml

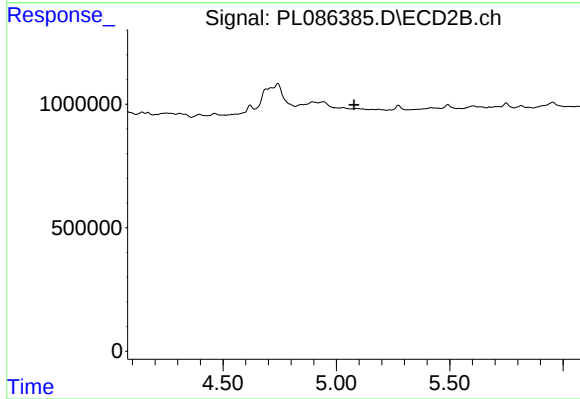


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.079 min
Response: 0
Conc: N.D.

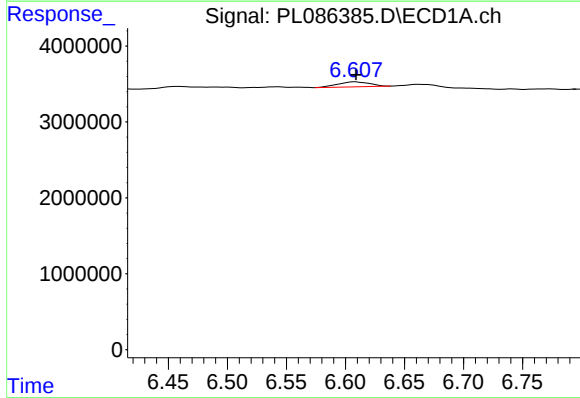


#15 Endosulfan II

R.T.: 6.608 min
Delta R.T.: 0.000 min
Response: 1190042
Conc: 0.38 ng/ml

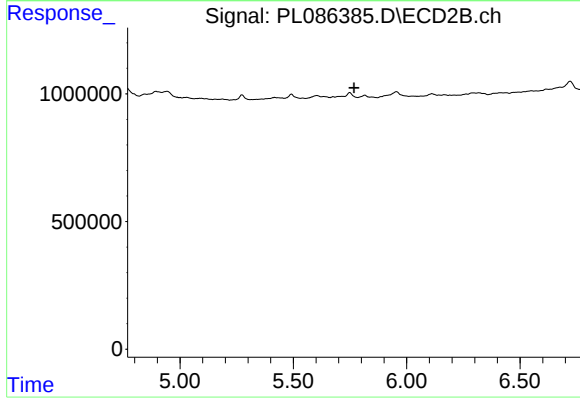


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 5.769 min
Response: 0
Conc: N.D.

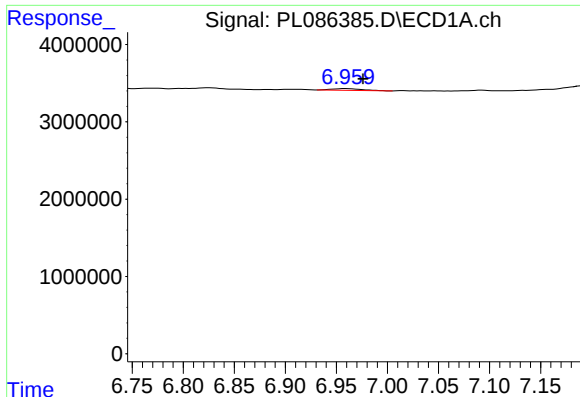


#19 Endosulfan Sulfate

R.T.: 6.960 min
Delta R.T.: -0.016 min
Response: 481557
Conc: 0.17 ng/ml

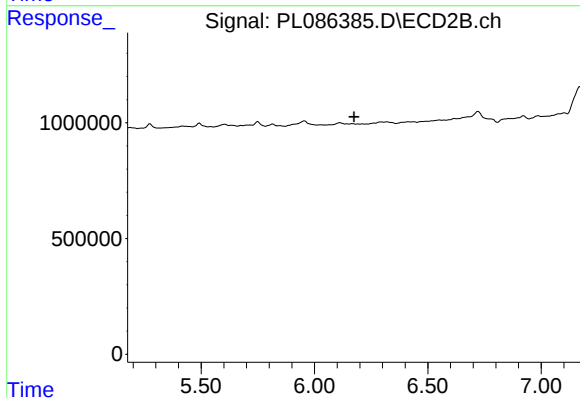


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 6.175 min
Response: 0
Conc: N.D.

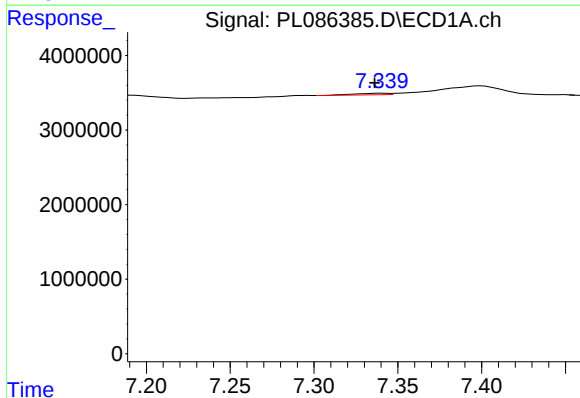


#20 Methoxychlor

R.T.: 7.341 min
Delta R.T.: 0.004 min
Response: 282464
Conc: 0.22 ng/ml

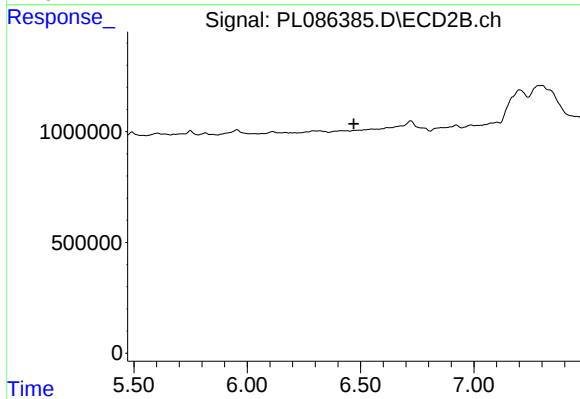


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.470 min
Response: 0
Conc: N.D.

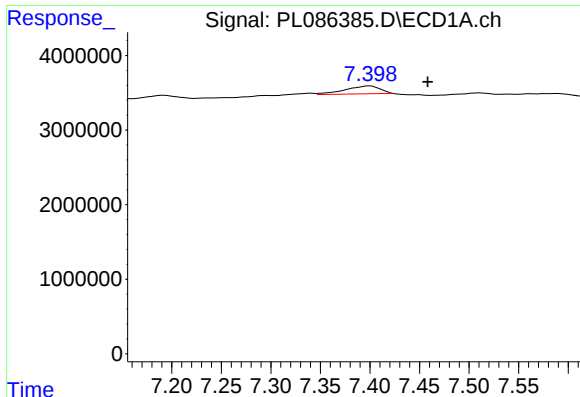


#21 Endrin ketone

R.T.: 7.399 min
Delta R.T.: -0.059 min
Response: 2591242
Conc: 0.90 ng/ml

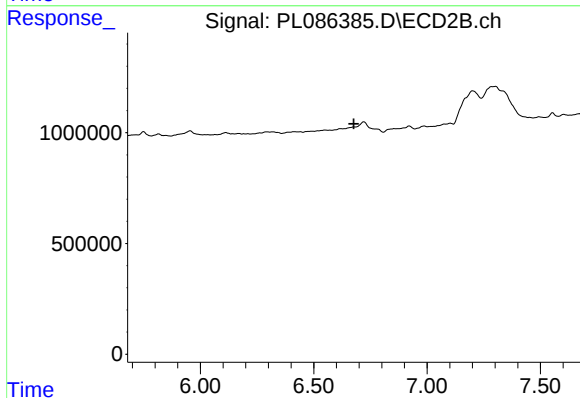


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 6.677 min
Response: 0
Conc: N.D.

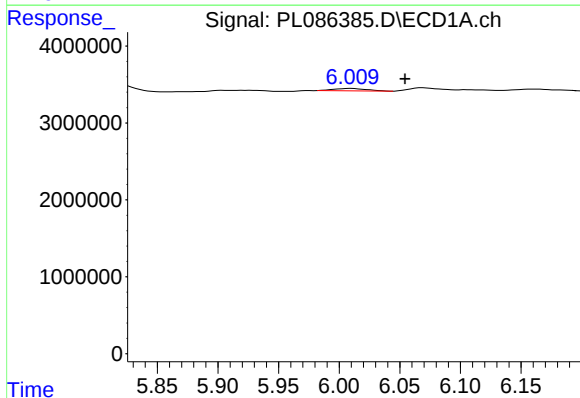


#22 Toxaphene-1

R.T.: 6.010 min
Delta R.T.: -0.045 min
Response: 587997
Conc: 26.08 ng/ml

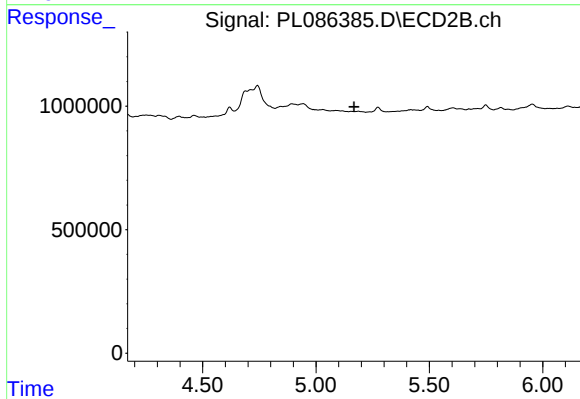


#22 Toxaphene-1

R.T.: 0.000 min
Exp R.T.: 5.168 min
Response: 0
Conc: N.D.

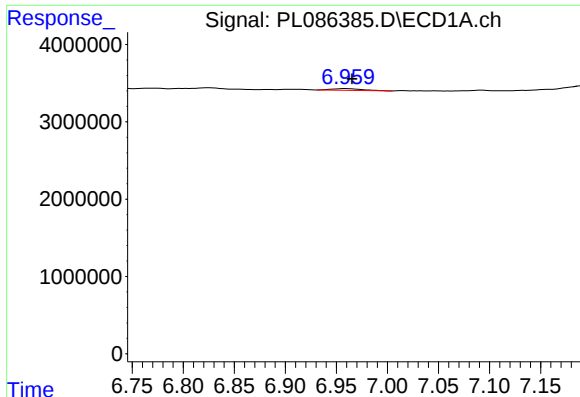


#24 Toxaphene-3

R.T.: 6.960 min
Delta R.T.: -0.005 min
Response: 481557
Conc: 7.67 ng/ml

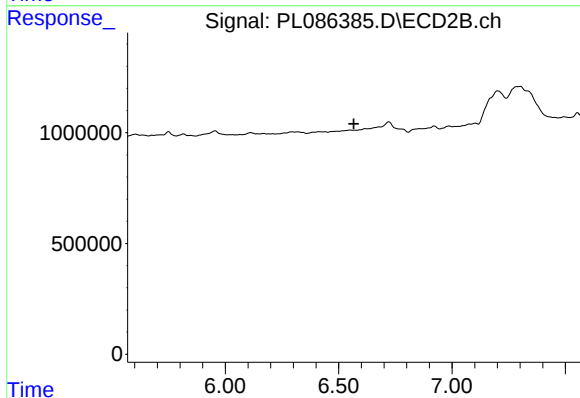


#24 Toxaphene-3

R.T.: 0.000 min
Exp R.T. : 6.567 min
Response: 0
Conc: N.D.

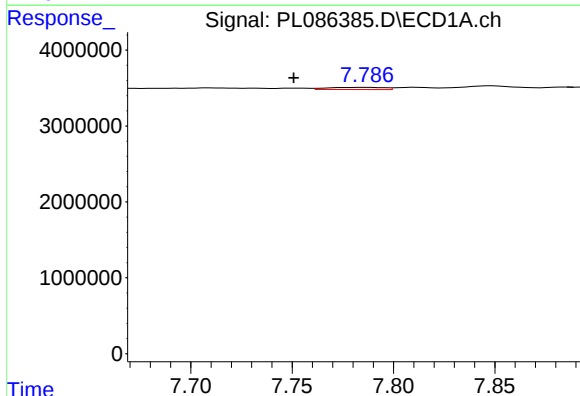


#26 Toxaphene-5

R.T.: 7.787 min
Delta R.T.: 0.036 min
Response: 567760
Conc: 12.86 ng/ml

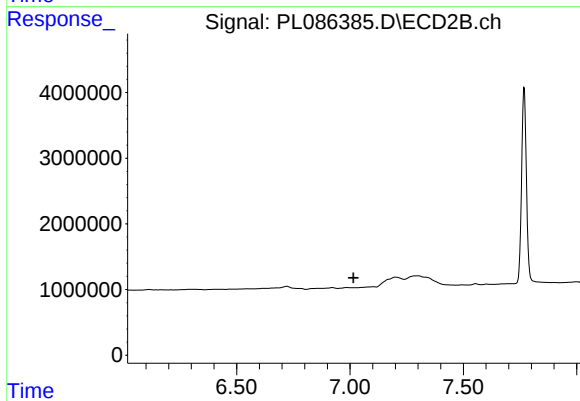


#26 Toxaphene-5

R.T.: 0.000 min
Exp R.T. : 7.016 min
Response: 0
Conc: N.D.

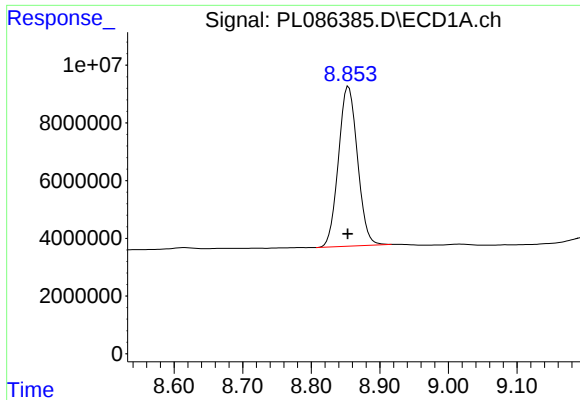

#27 Decachlorobiphenyl

R.T.: 8.854 min
Delta R.T.: 0.001 min
Response: 106743483
Conc: 42.83 ng/ml

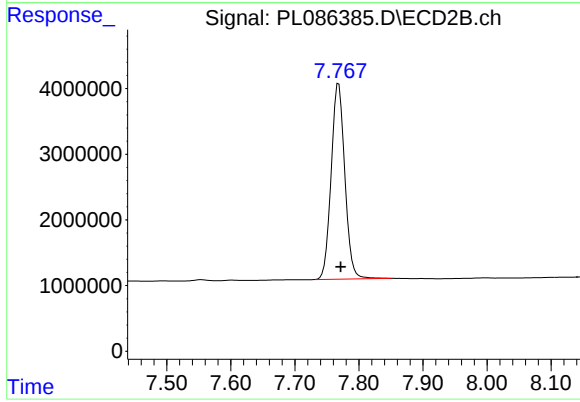

#27 Decachlorobiphenyl

R.T.: 7.768 min
Delta R.T.: -0.003 min
Response: 44163881
Conc: 38.47 ng/ml