

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110320\
 Data File : PL062792.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2020 08:13
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 17:00:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
5) MB	Aldrin	4.658	5.434	863788	2997680	0.453 0.828 #
7) B	delta-BHC	4.576	0.000	4061024	0	1.869 N.D. #
8) B	Heptachlo...	5.096	5.814	2198494	7550252	1.205 2.331 #
10) B	gamma-Chl...	0.000	6.032f	0	3813573	N.D. 1.133 #
17) MA	4,4'-DDT	6.306	7.079	3010110	3482691	2.255 1.551 #
18) B	Endrin al...	6.398f	6.971	2094446	2619469	1.442 1.149
20) A	Methoxychlor	6.852	0.000	1218720	0	1.415 N.D. #
23)	Chlordane-1	4.277	0.000	700121	0	13.581 N.D. #
24)	Chlordane-2	0.000	5.378f	0	15681459	N.D. 143.819 #
25)	Chlordane-3	0.000	6.032f	0	3813573	N.D. 9.441 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110320\
Data File : PL062792.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2020 08:13
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 17:00:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

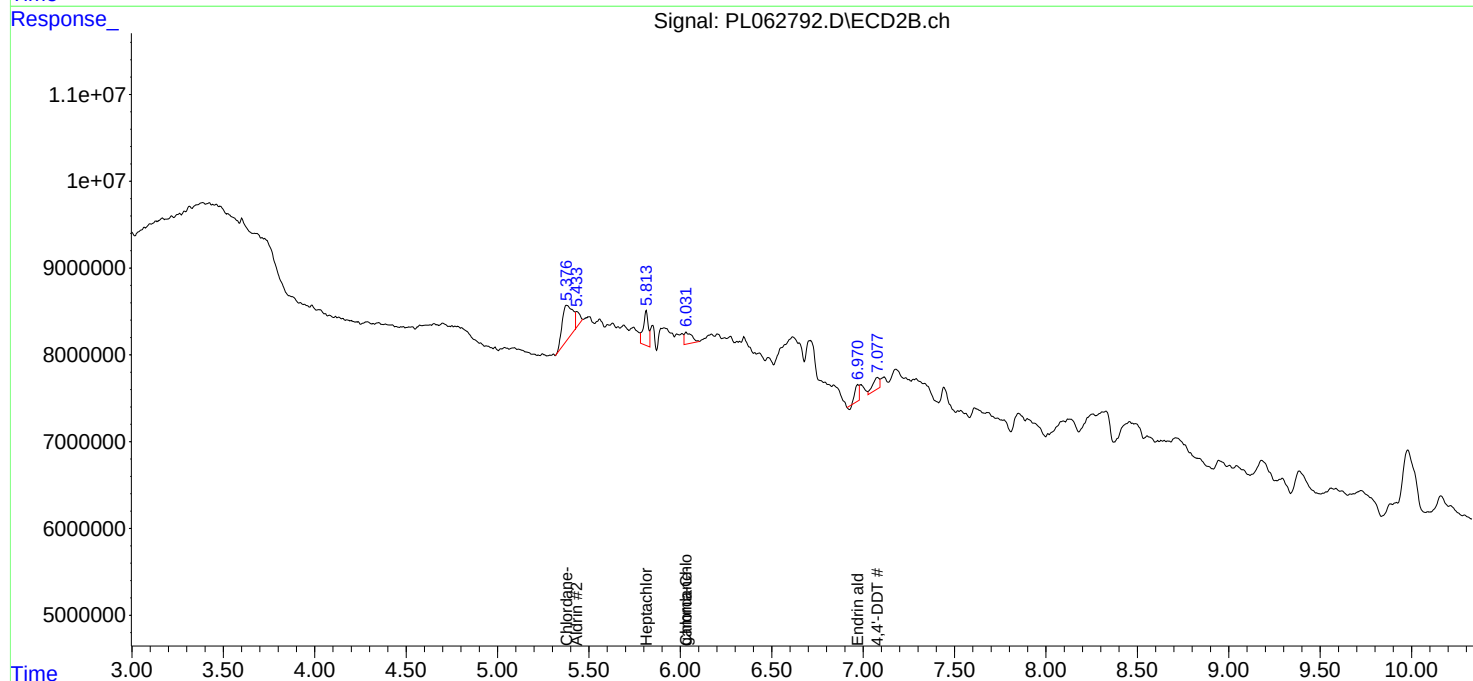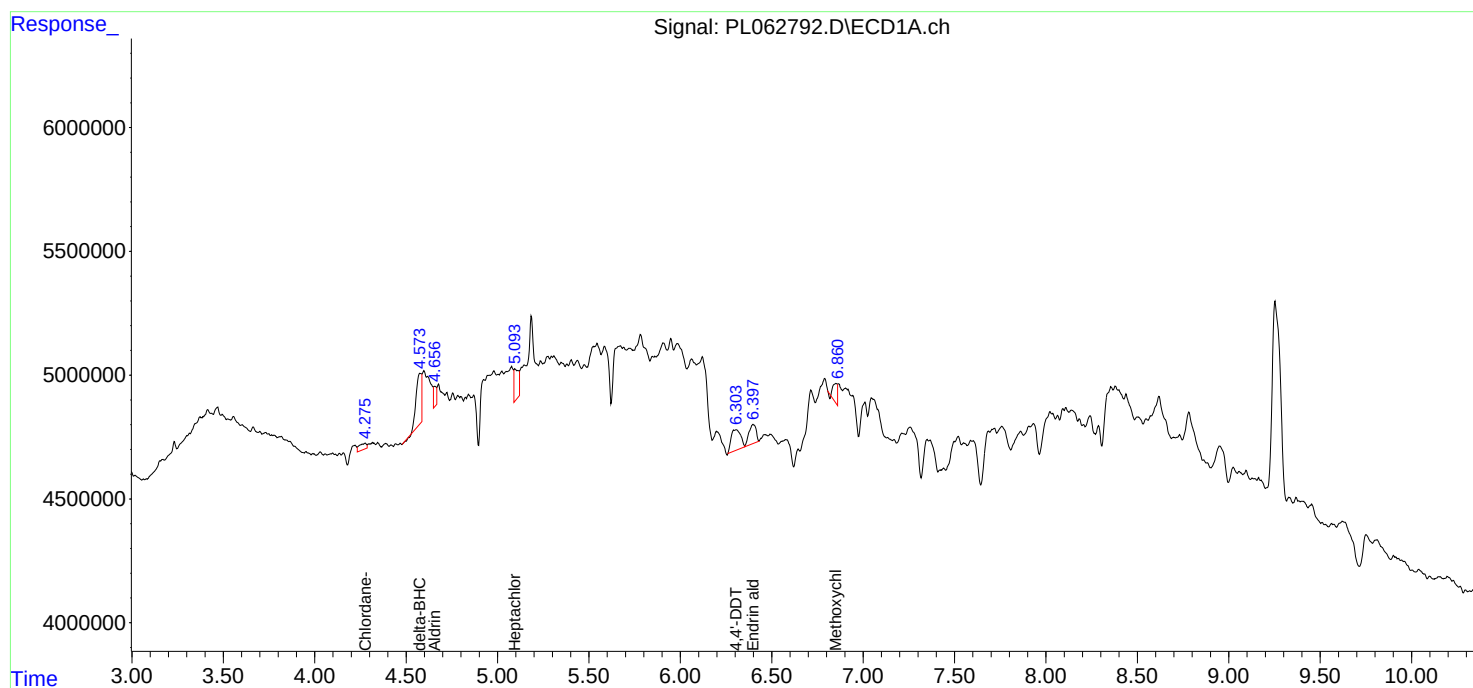


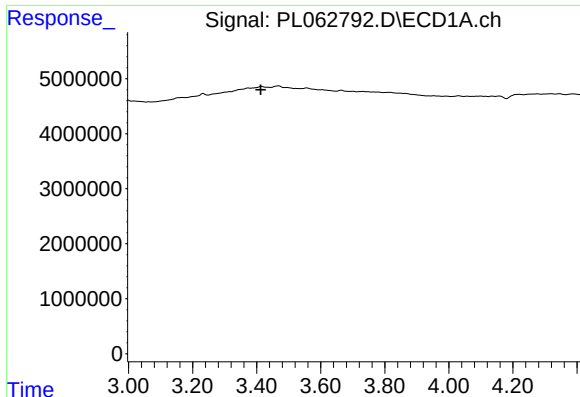

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.412 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

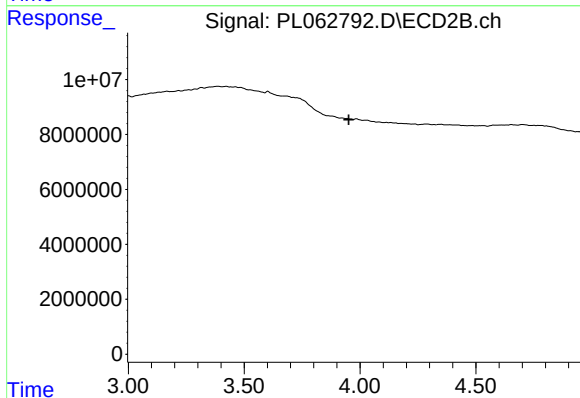


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.952 min
Response: 0
Conc: N.D.

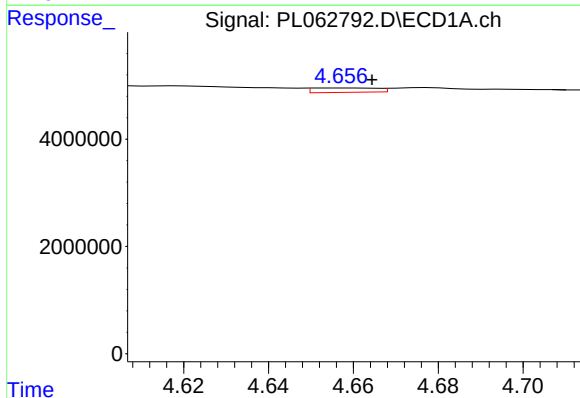


#5 Aldrin

R.T.: 4.658 min
Delta R.T.: -0.006 min
Response: 863788
Conc: 0.45 ng/ml

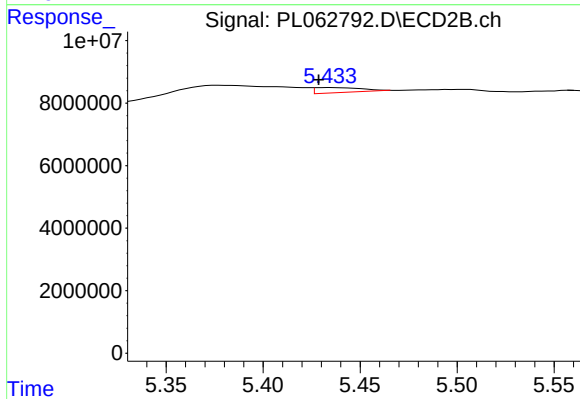

#5 Aldrin


R.T.: 5.434 min
Delta R.T.: 0.006 min
Response: 2997680
Conc: 0.83 ng/ml

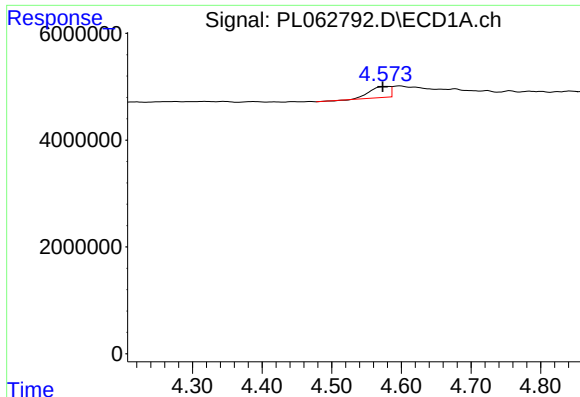

#7 delta-BHC


R.T.: 4.576 min
Delta R.T.: 0.003 min
Response: 4061024
Conc: 1.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

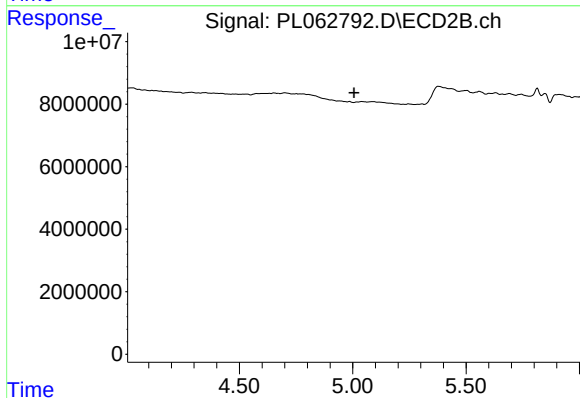


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 5.007 min
Response: 0
Conc: N.D.

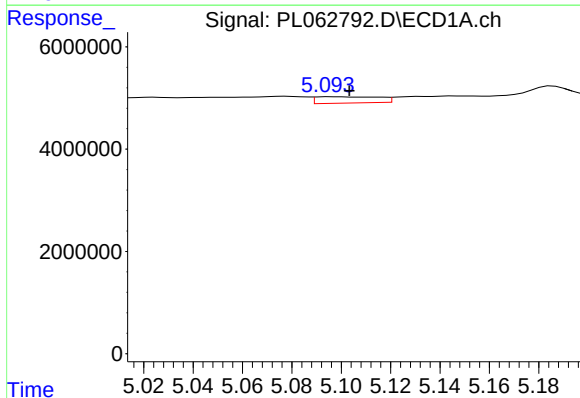


#8 Heptachlor epoxide

R.T.: 5.096 min
Delta R.T.: -0.008 min
Response: 2198494
Conc: 1.20 ng/ml

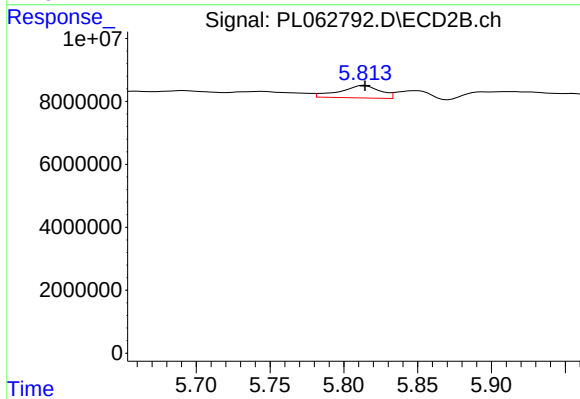

#8 Heptachlor epoxide


R.T.: 5.814 min
Delta R.T.: 0.000 min
Response: 7550252
Conc: 2.33 ng/ml

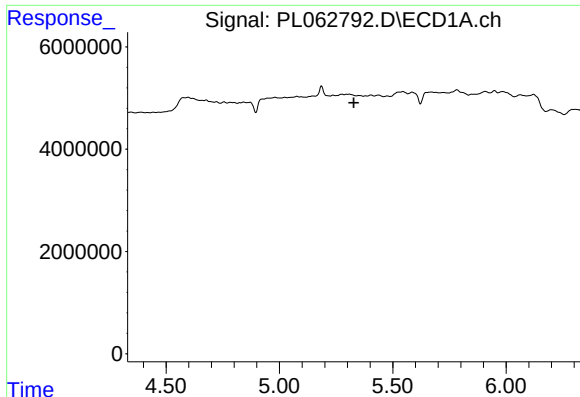

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

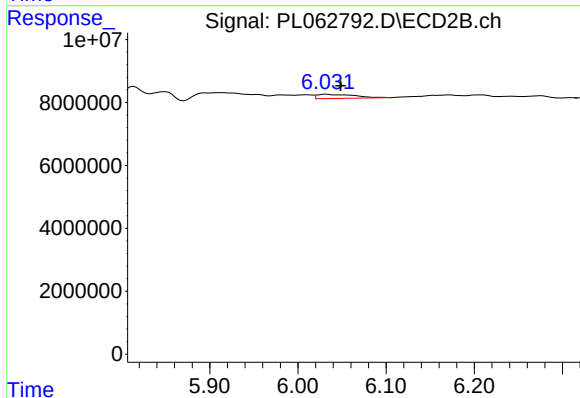


#10 gamma-Chlordane

R.T.: 6.032 min
Delta R.T.: -0.016 min
Response: 3813573
Conc: 1.13 ng/ml

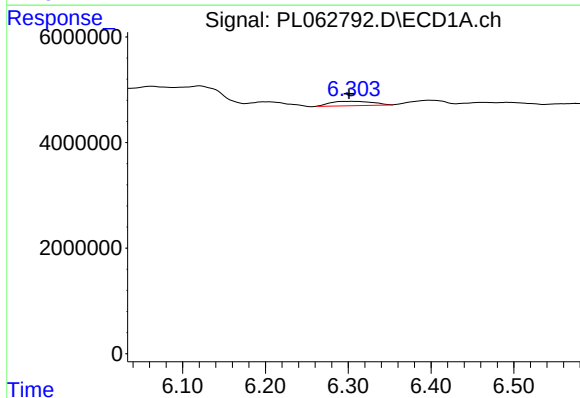


#17 4,4'-DDT

R.T.: 6.306 min
Delta R.T.: 0.005 min
Response: 3010110
Conc: 2.26 ng/ml

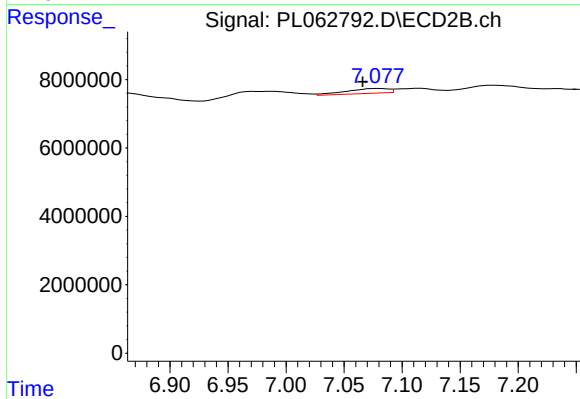

#17 4,4'-DDT


R.T.: 7.079 min
Delta R.T.: 0.013 min
Response: 3482691
Conc: 1.55 ng/ml

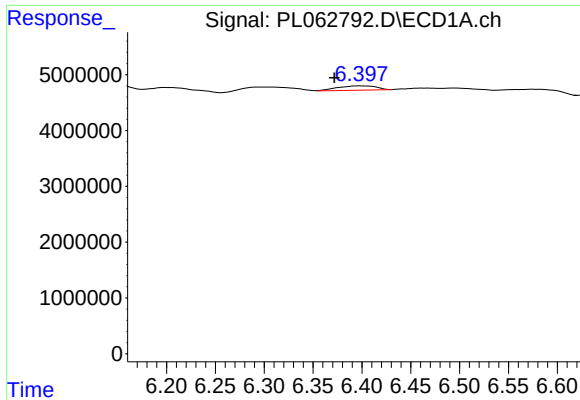

#18 Endrin aldehyde


R.T.: 6.398 min
Delta R.T.: 0.026 min
Response: 2094446
Conc: 1.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

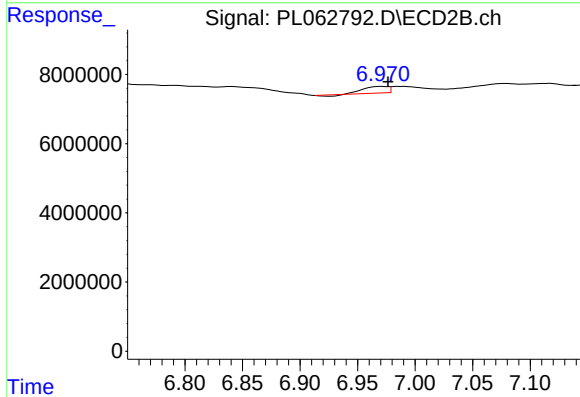


#18 Endrin aldehyde

R.T.: 6.971 min
Delta R.T.: -0.005 min
Response: 2619469
Conc: 1.15 ng/ml

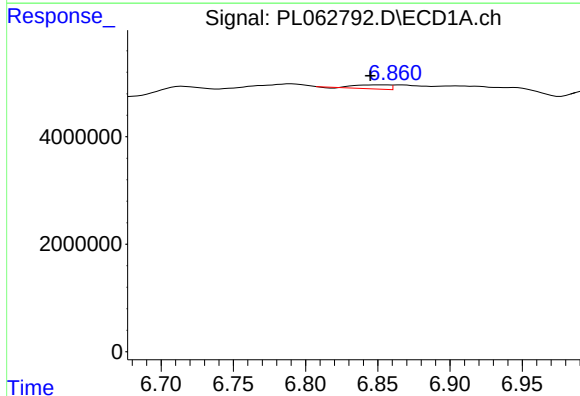


#20 Methoxychlor

R.T.: 6.852 min
Delta R.T.: 0.008 min
Response: 1218720
Conc: 1.41 ng/ml

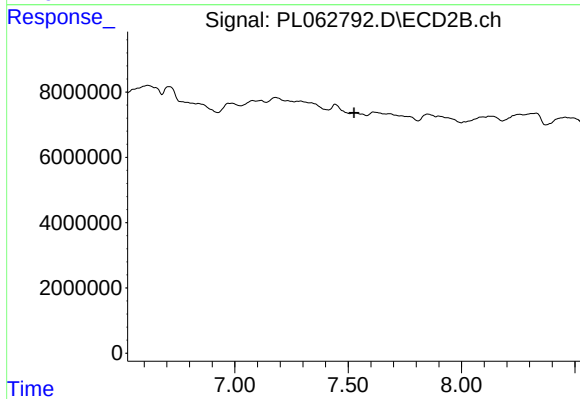

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.526 min
Response: 0
Conc: N.D.

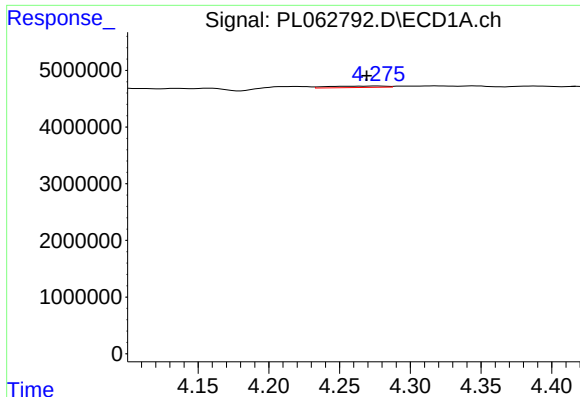

#23 Chlordane-1


R.T.: 4.277 min
Delta R.T.: 0.007 min
Response: 700121
Conc: 13.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

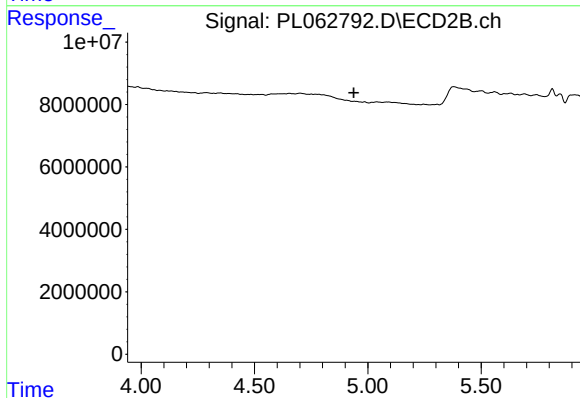


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.938 min
Response: 0
Conc: N.D.

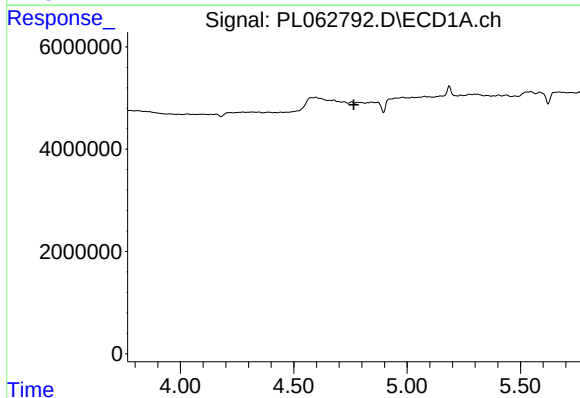


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.765 min
Response: 0
Conc: N.D.

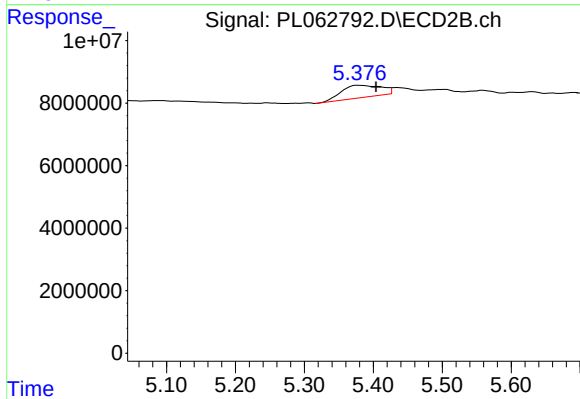

#24 Chlordane-2


R.T.: 5.378 min
Delta R.T.: -0.026 min
Response: 15681459
Conc: 143.82 ng/ml

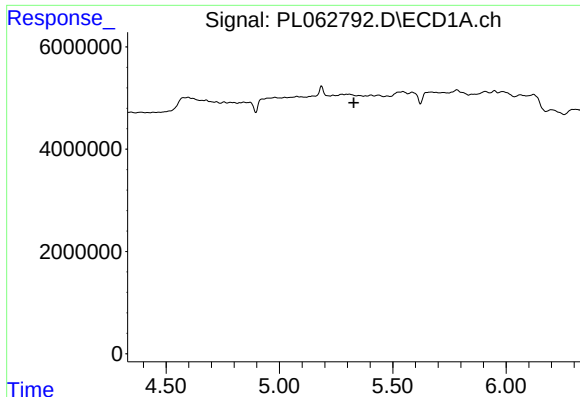

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

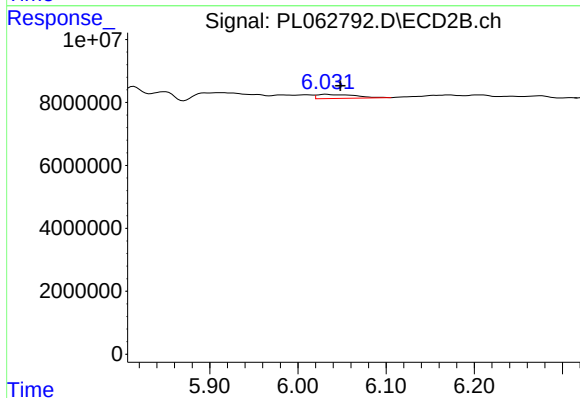


#25 Chlordane-3

R.T.: 6.032 min
Delta R.T.: -0.016 min
Response: 3813573
Conc: 9.44 ng/ml

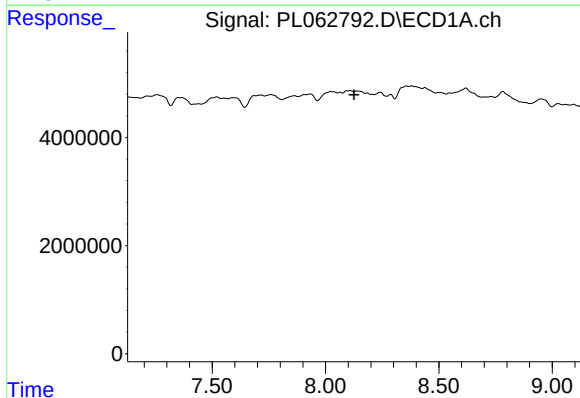

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.126 min
Response: 0
Conc: N.D.

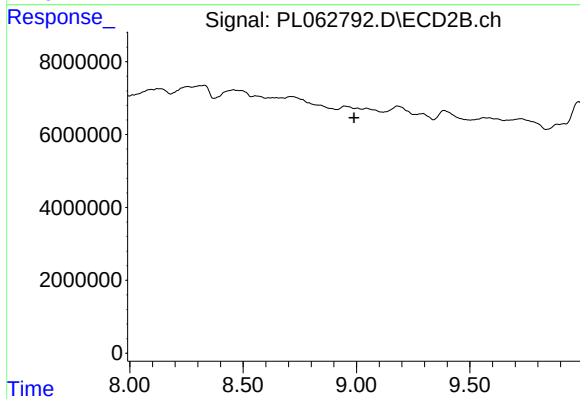

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.989 min
Response: 0
Conc: N.D.