

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110320\
 Data File : PL062797.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2020 12:20
 Operator : DD\AJ
 Sample : PB132788BS
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB132788BS

Manual Integrations
 APPROVED

Ankita
 11/4/2020 4:56:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 17:01:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.411	3.950	34166301	58033966	19.863	19.748
28)	SA Decachlor...	8.129	8.990	38017258	47380924	23.697	22.638
Target Compounds							
2)	A alpha-BHC	3.843	4.337	116.9E6	202.7E6	45.831	45.617
3)	MA gamma-BHC...	4.123	4.620	106.0E6	191.0E6	45.757	45.740
4)	MA Heptachlor	4.420	5.125	98868142	180.5E6	46.075	45.271
5)	MB Aldrin	4.664	5.428	88655722	170.5E6	46.447	47.110
6)	B beta-BHC	4.373	4.791	44053332	84750989	46.120	45.008
7)	B delta-BHC	4.573	5.006	101.8E6	171.8E6	46.839	49.089
8)	B Heptachlo...	5.104	5.813	88395761	155.8E6	48.447	48.106m
9)	A Endosulfan I	5.439	6.170	80650005	143.8E6	48.247	45.604
10)	B gamma-Chl...	5.329	6.048	84741463	154.9E6	47.037	46.005
11)	B alpha-Chl...	5.387	6.120	84559074	154.9E6	46.776	45.977
12)	B 4,4'-DDE	5.552	6.279	78930757	150.2E6	47.708	46.616
13)	MA Dieldrin	5.680	6.426	84353489	149.1E6	47.739	46.571
14)	MA Endrin	5.935	6.642	76151593	122.7E6	45.770	43.963m
15)	B Endosulfa...	6.207	6.853	79273109	127.6E6	48.084	44.634
16)	A 4,4'-DDD	6.064	6.768	70469153	124.4E6	49.819	48.605
17)	MA 4,4'-DDT	6.303	7.067	61923986	103.0E6	46.400	45.855
18)	B Endrin al...	6.374	6.977	69777045	108.5E6	48.053	47.576
19)	B Endosulfa...	6.586	7.200	78776234	118.0E6	47.736	49.186
20)	A Methoxychlor	6.847	7.526	39938011	59075600	46.370	47.815
21)	B Endrin ke...	7.073	7.669	91911865	122.6E6	50.977	51.722
22)	Mirex	7.259	8.122	70117615	84558858	49.459	49.621

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110320\
Data File : PL062797.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2020 12:20
Operator : DD\AJ
Sample : PB132788BS
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB132788BS


Manual Integrations
APPROVED

Ankita
11/4/2020 4:56:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 17:01:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

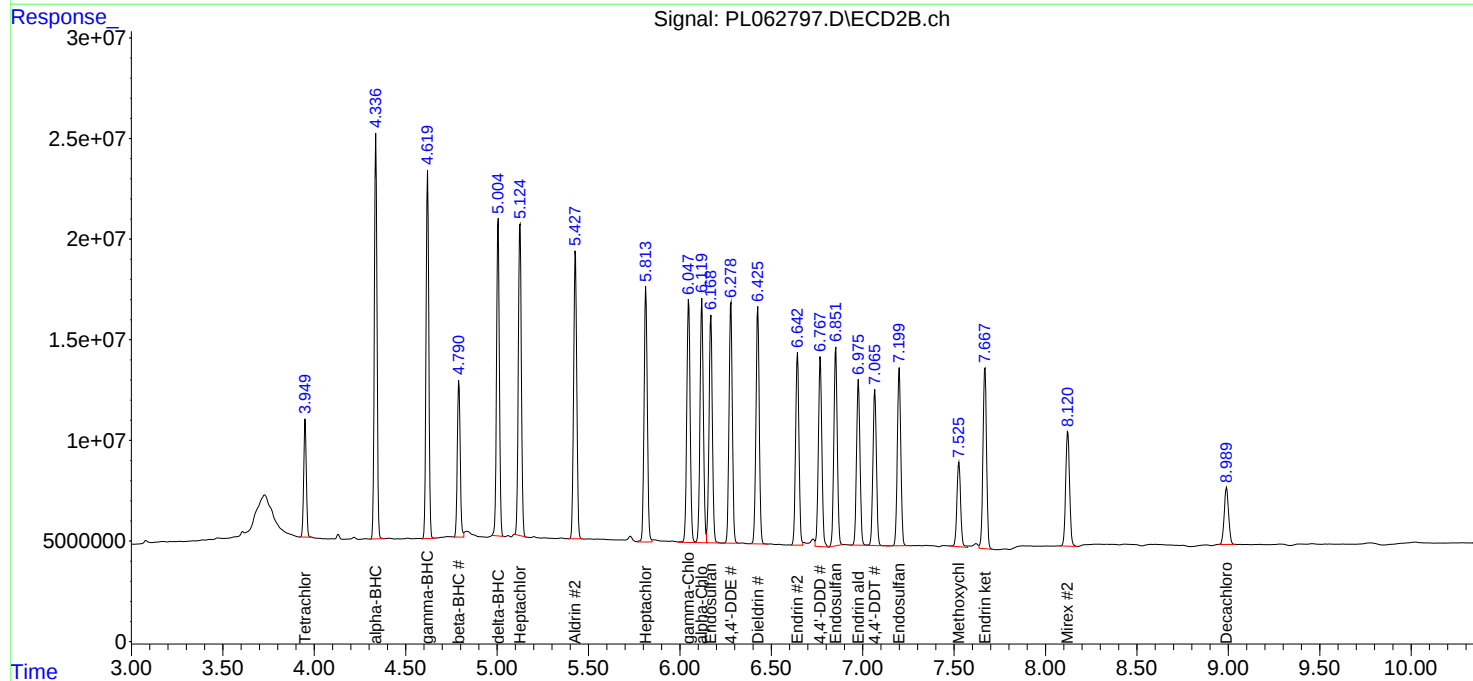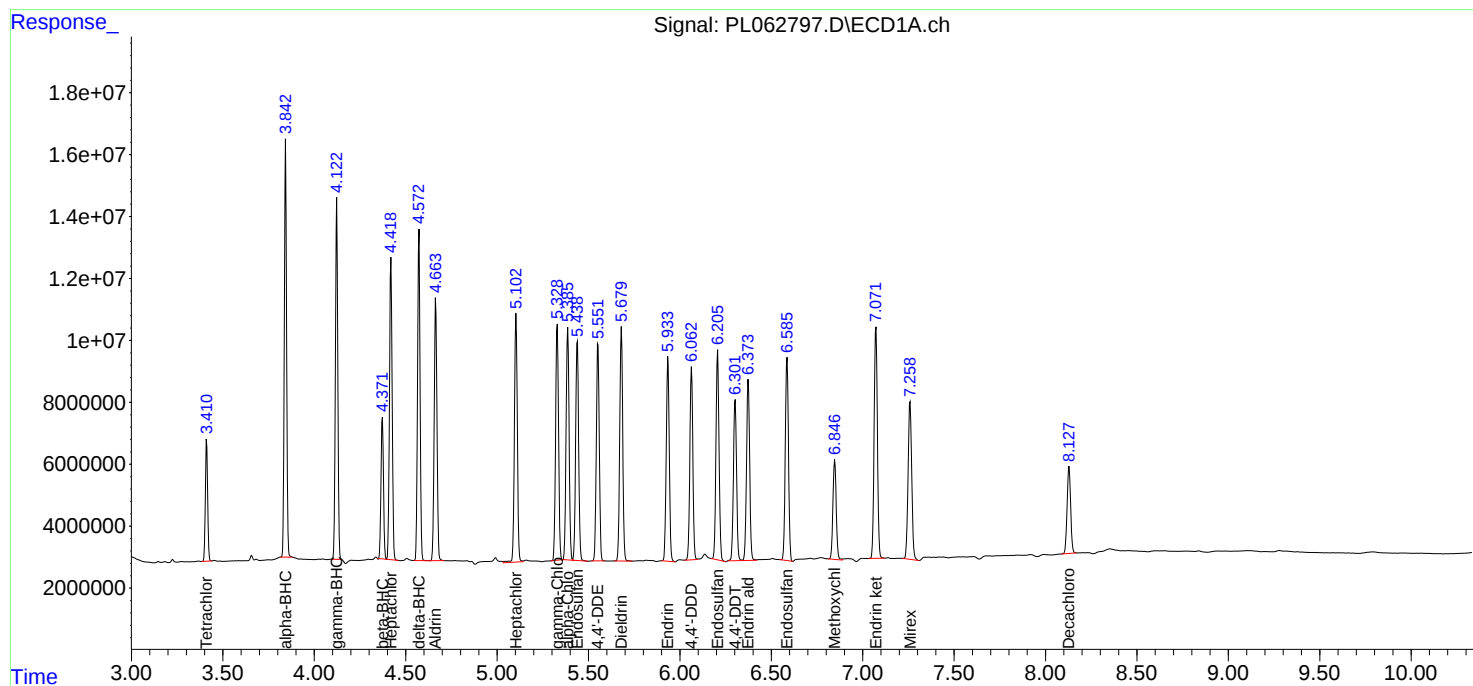

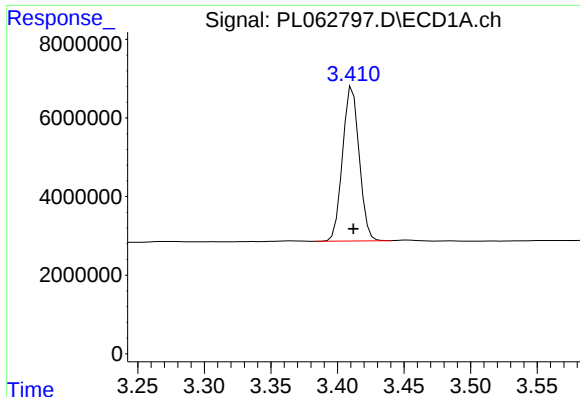


#1 Tetrachloro-m-xylene

R.T.: 3.411 min
Delta R.T.: 0.000 min
Response: 34166301
Conc: 19.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB132788BS


Manual Integrations
APPROVED

Ankita
11/4/2020 4:56:55 PM

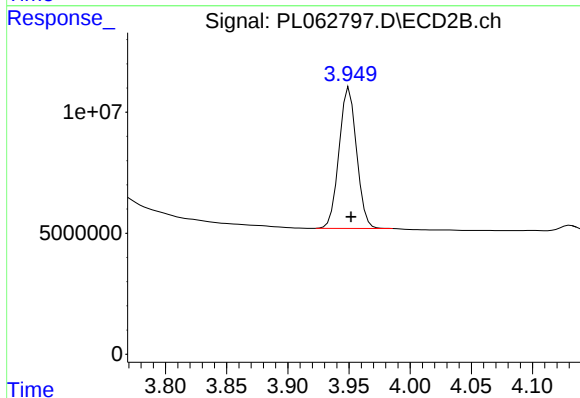


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: -0.001 min
Response: 58033966
Conc: 19.75 ng/ml

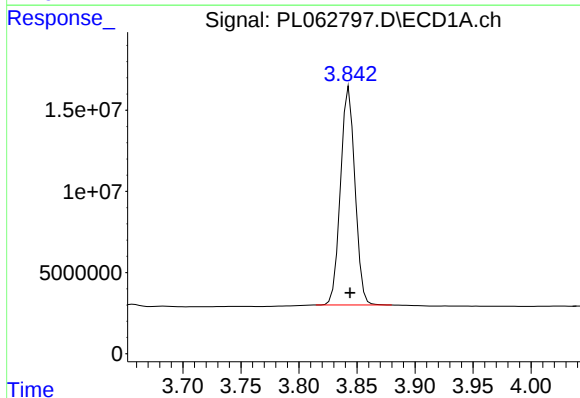


#2 alpha-BHC

R.T.: 3.843 min
Delta R.T.: 0.000 min
Response: 116854730
Conc: 45.83 ng/ml

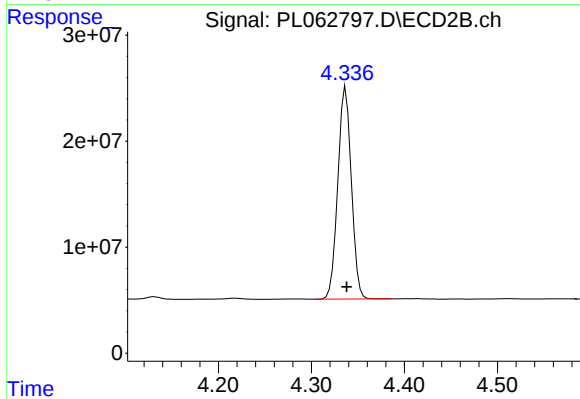

#2 alpha-BHC

R.T.: 4.337 min
Delta R.T.: -0.001 min
Response: 202687465
Conc: 45.62 ng/ml

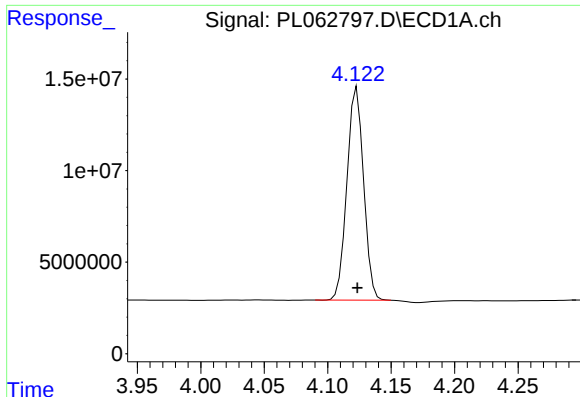


#3 gamma-BHC (Lindane)

R.T.: 4.123 min
Delta R.T.: 0.000 min
Response: 106004738
Conc: 45.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB132788BS


Manual Integrations
APPROVED

Ankita
11/4/2020 4:56:55 PM

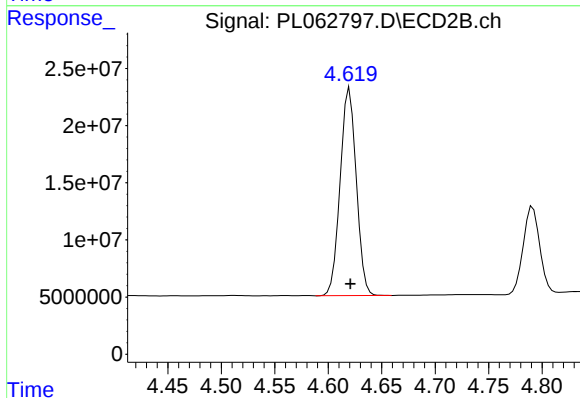


#3 gamma-BHC (Lindane)

R.T.: 4.620 min
Delta R.T.: 0.000 min
Response: 190995715
Conc: 45.74 ng/ml

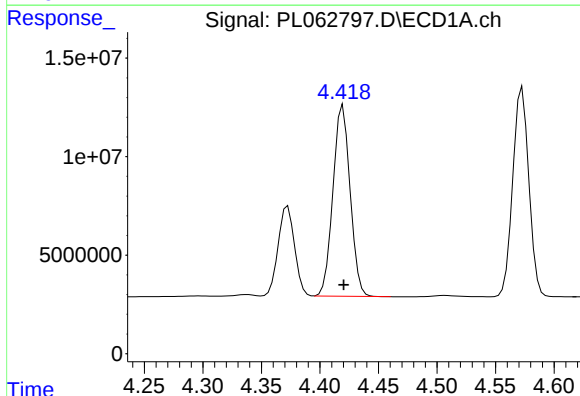


#4 Heptachlor

R.T.: 4.420 min
Delta R.T.: 0.000 min
Response: 98868142
Conc: 46.08 ng/ml

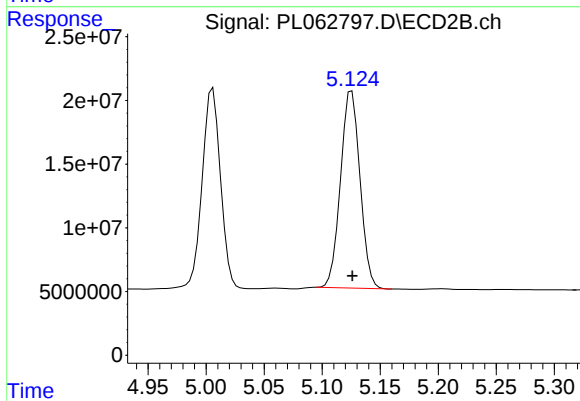

#4 Heptachlor

R.T.: 5.125 min
Delta R.T.: 0.000 min
Response: 180536299
Conc: 45.27 ng/ml

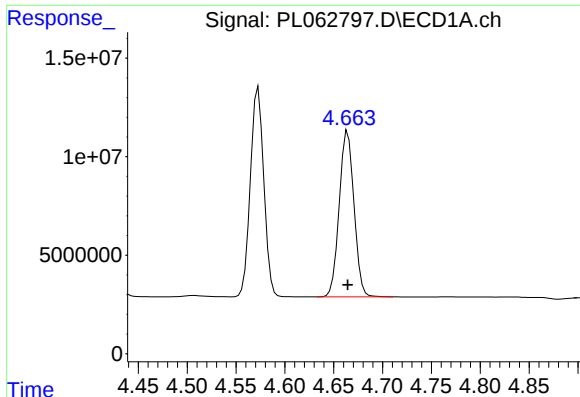

#5 Aldrin

R.T.: 4.664 min

Delta R.T.: 0.000 min


Response: 88655722

Conc: 46.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB132788BS

Manual Integrations
APPROVED

Ankita
11/4/2020 4:56:55 PM

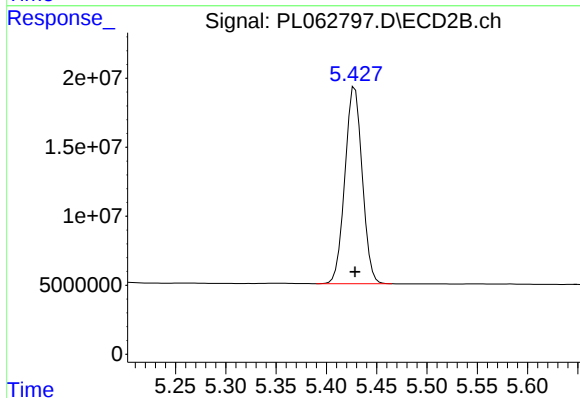


#5 Aldrin

R.T.: 5.428 min

Delta R.T.: 0.000 min

Response: 170513668

Conc: 47.11 ng/ml

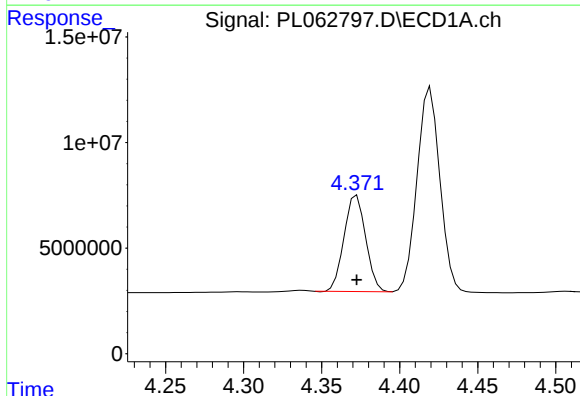


#6 beta-BHC

R.T.: 4.373 min

Delta R.T.: 0.000 min

Response: 44053332

Conc: 46.12 ng/ml

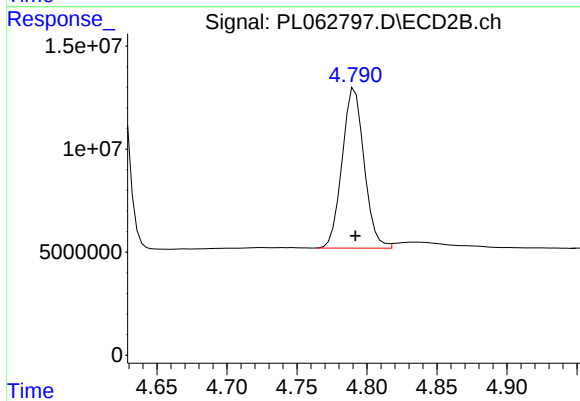


#6 beta-BHC

R.T.: 4.791 min

Delta R.T.: 0.000 min

Response: 84750989




Conc: 45.01 ng/ml

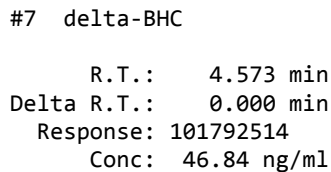


Instrument :
ECD_L
ClientSampleId :
PB132788BS

Manual Integrations
APPROVED

Ankita
11/4/2020 4:56:55 PM

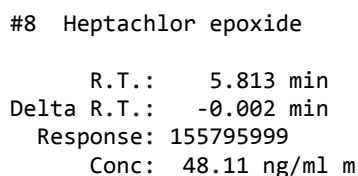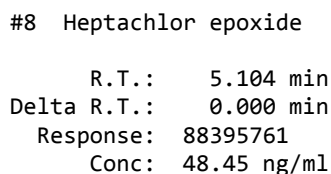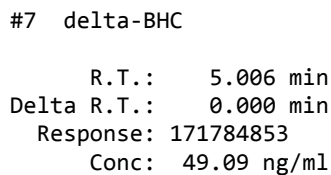

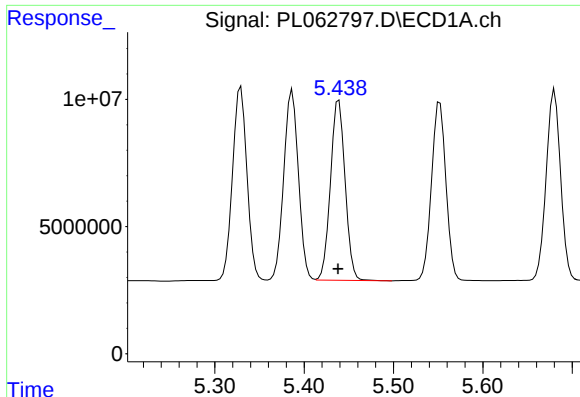


#9 Endosulfan I

R.T.: 5.439 min
Delta R.T.: 0.000 min
Response: 80650005
Conc: 48.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB132788BS


Manual Integrations
APPROVED

Ankita
11/4/2020 4:56:55 PM

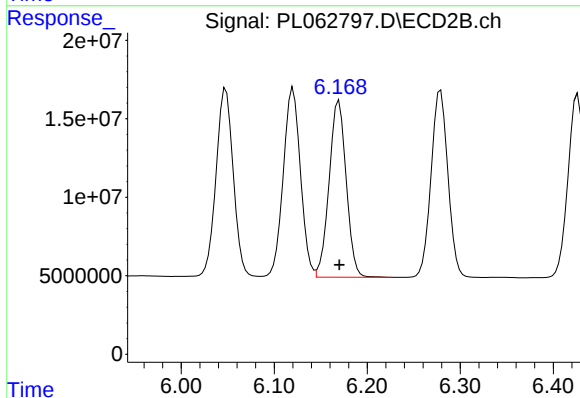


#9 Endosulfan I

R.T.: 6.170 min
Delta R.T.: 0.000 min
Response: 143827976
Conc: 45.60 ng/ml

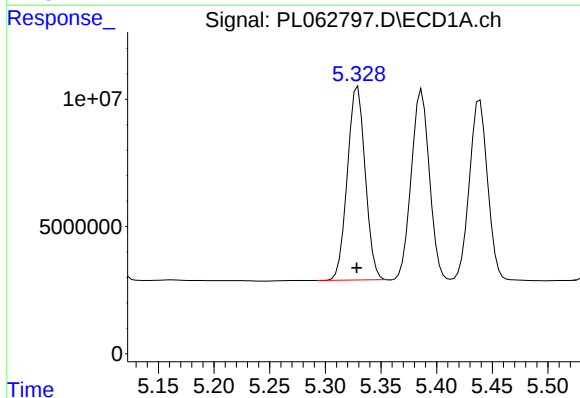


#10 gamma-Chlordane

R.T.: 5.329 min
Delta R.T.: 0.000 min
Response: 84741463
Conc: 47.04 ng/ml

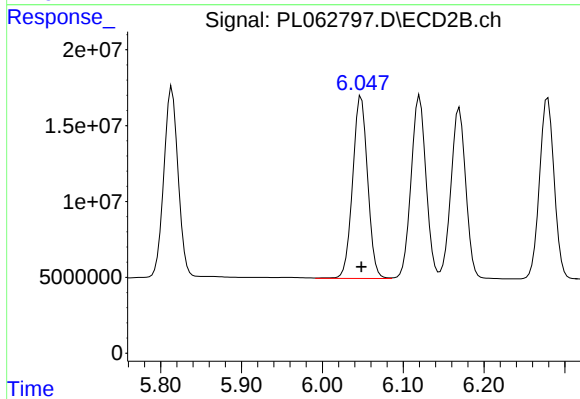

#10 gamma-Chlordane

R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 154868204
Conc: 46.00 ng/ml

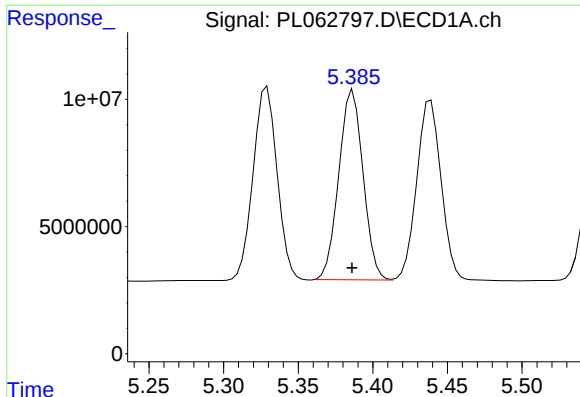


#11 alpha-Chlordane

R.T.: 5.387 min
Delta R.T.: 0.000 min
Response: 84559074
Conc: 46.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB132788BS


Manual Integrations
APPROVED

Ankita
11/4/2020 4:56:55 PM

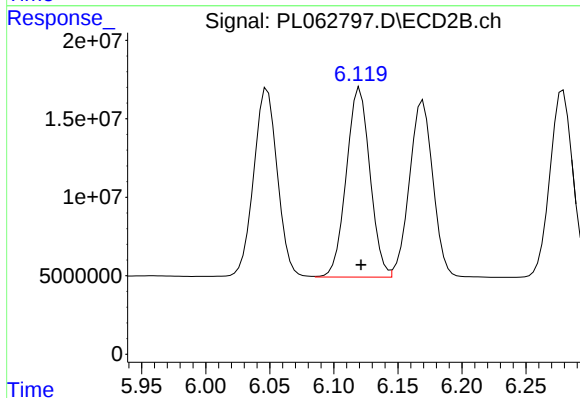


#11 alpha-Chlordane

R.T.: 6.120 min
Delta R.T.: 0.000 min
Response: 154893256
Conc: 45.98 ng/ml

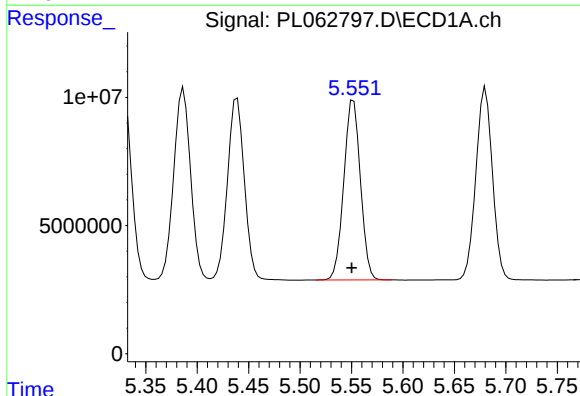


#12 4,4'-DDE

R.T.: 5.552 min
Delta R.T.: 0.002 min
Response: 78930757
Conc: 47.71 ng/ml

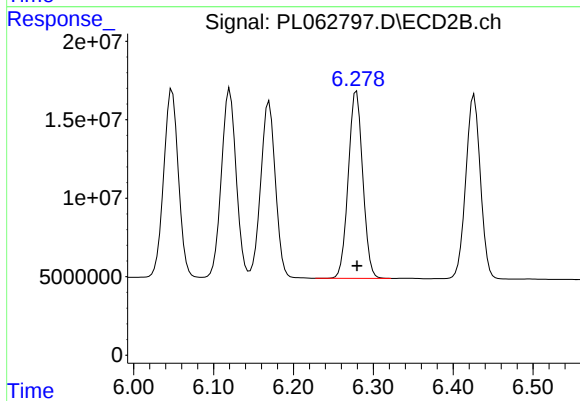

#12 4,4'-DDE

R.T.: 6.279 min
Delta R.T.: 0.000 min
Response: 150199289
Conc: 46.62 ng/ml

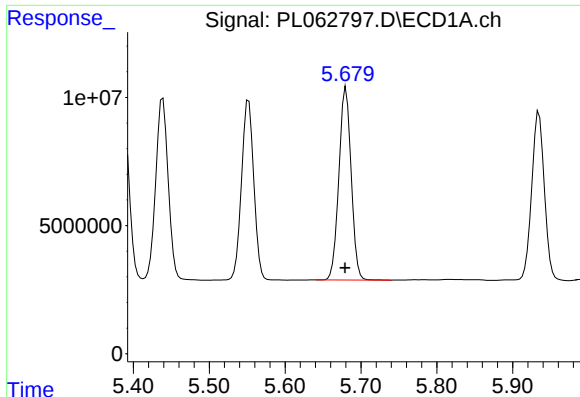


#13 Dieldrin

R.T.: 5.680 min
Delta R.T.: 0.001 min
Response: 84353489
Conc: 47.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB132788BS


Manual Integrations
APPROVED

Ankita
11/4/2020 4:56:55 PM

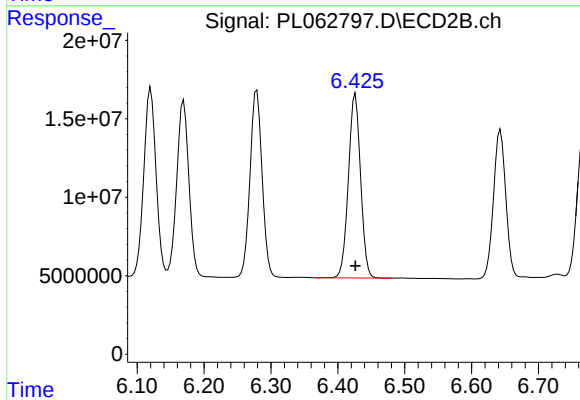


#13 Dieldrin

R.T.: 6.426 min
Delta R.T.: 0.000 min
Response: 149066047
Conc: 46.57 ng/ml

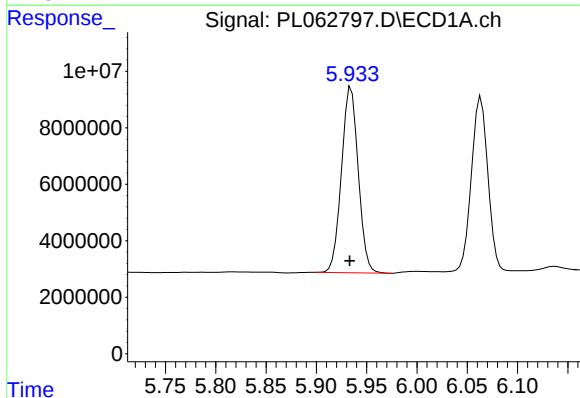


#14 Endrin

R.T.: 5.935 min
Delta R.T.: 0.002 min
Response: 76151593
Conc: 45.77 ng/ml

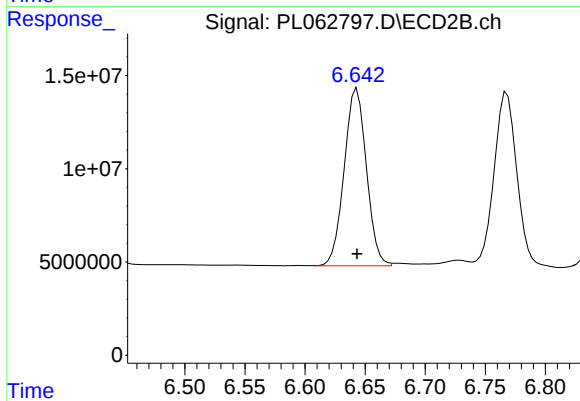

#14 Endrin

R.T.: 6.642 min
Delta R.T.: -0.001 min
Response: 122706331
Conc: 43.96 ng/ml m

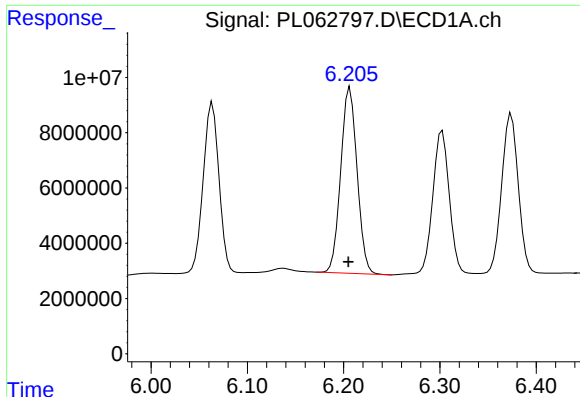


#15 Endosulfan II

R.T.: 6.207 min
Delta R.T.: 0.002 min
Response: 79273109
Conc: 48.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB132788BS


Manual Integrations
APPROVED

Ankita
11/4/2020 4:56:55 PM

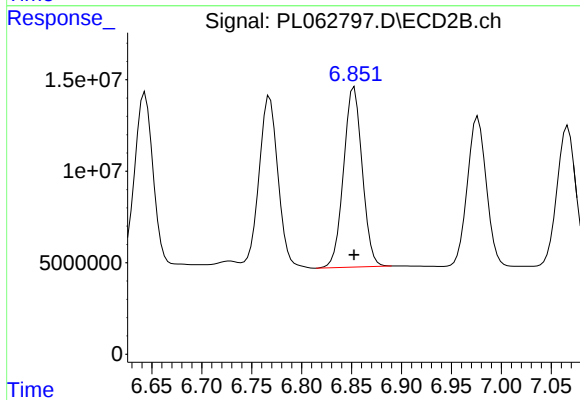


#15 Endosulfan II

R.T.: 6.853 min
Delta R.T.: 0.000 min
Response: 127594063
Conc: 44.63 ng/ml

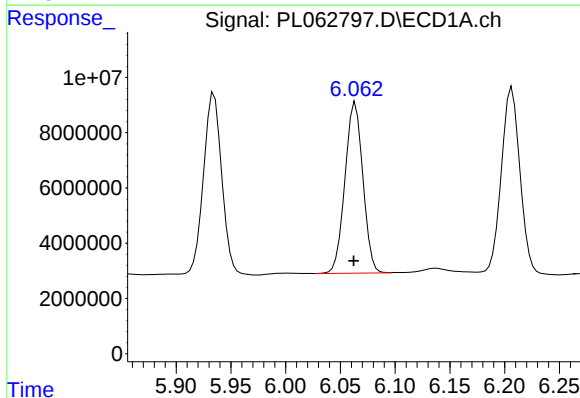


#16 4,4'-DDD

R.T.: 6.064 min
Delta R.T.: 0.002 min
Response: 70469153
Conc: 49.82 ng/ml

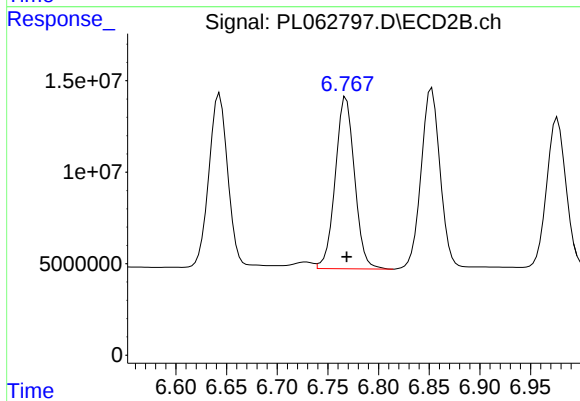

#16 4,4'-DDD

R.T.: 6.768 min
Delta R.T.: 0.000 min
Response: 124427006
Conc: 48.60 ng/ml

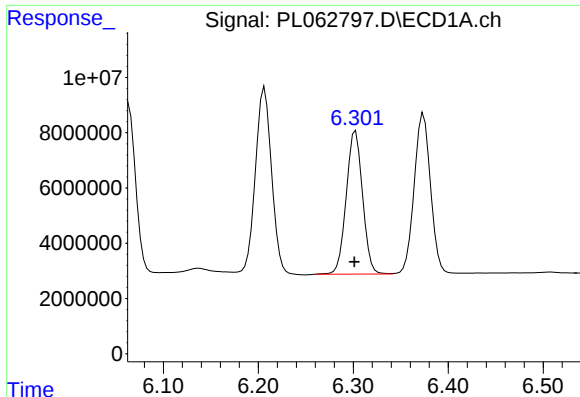


#17 4,4'-DDT

R.T.: 6.303 min
Delta R.T.: 0.001 min
Response: 61923986
Conc: 46.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB132788BS


Manual Integrations
APPROVED

Ankita
11/4/2020 4:56:55 PM

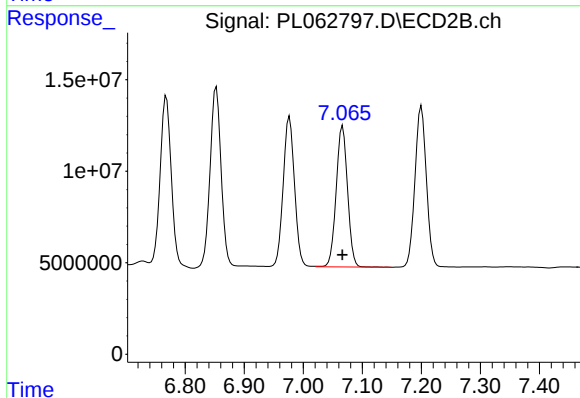


#17 4,4'-DDT

R.T.: 7.067 min
Delta R.T.: 0.000 min
Response: 102956204
Conc: 45.85 ng/ml

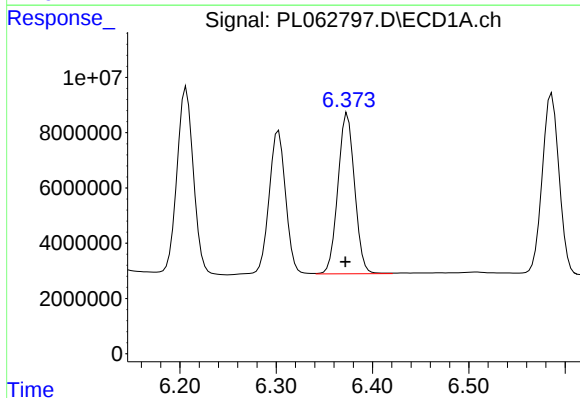


#18 Endrin aldehyde

R.T.: 6.374 min
Delta R.T.: 0.002 min
Response: 69777045
Conc: 48.05 ng/ml

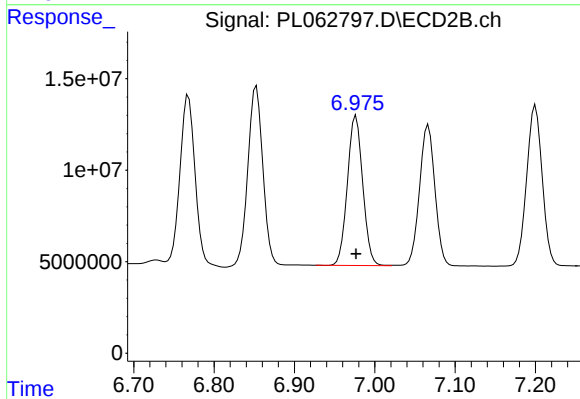

#18 Endrin aldehyde

R.T.: 6.977 min
Delta R.T.: 0.000 min
Response: 108501139
Conc: 47.58 ng/ml

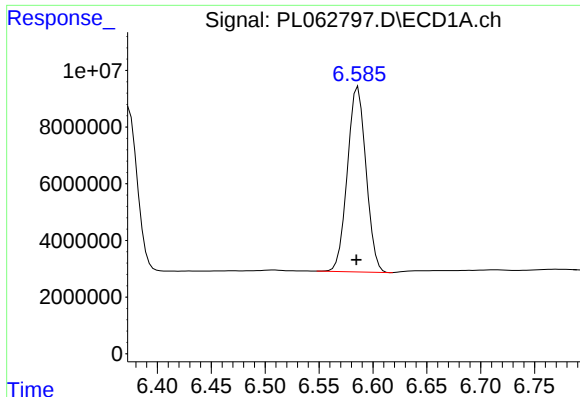


#19 Endosulfan Sulfate

R.T.: 6.586 min
Delta R.T.: 0.002 min
Response: 78776234
Conc: 47.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB132788BS


Manual Integrations
APPROVED

Ankita
11/4/2020 4:56:55 PM

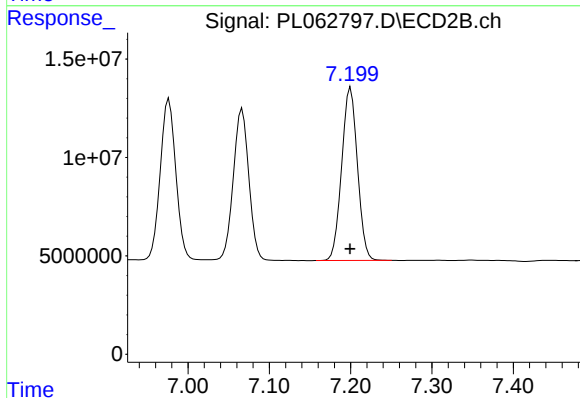


#19 Endosulfan Sulfate

R.T.: 7.200 min
Delta R.T.: 0.000 min
Response: 118008560
Conc: 49.19 ng/ml

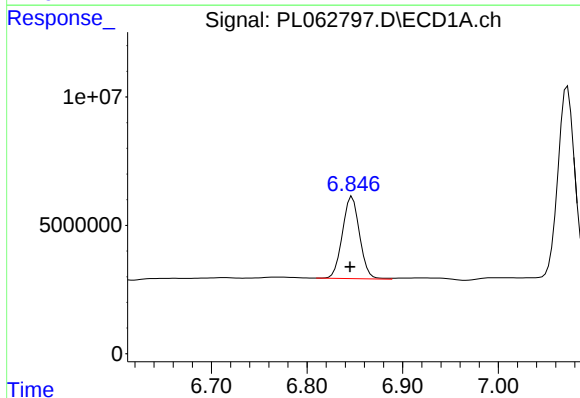


#20 Methoxychlor

R.T.: 6.847 min
Delta R.T.: 0.002 min
Response: 39938011
Conc: 46.37 ng/ml

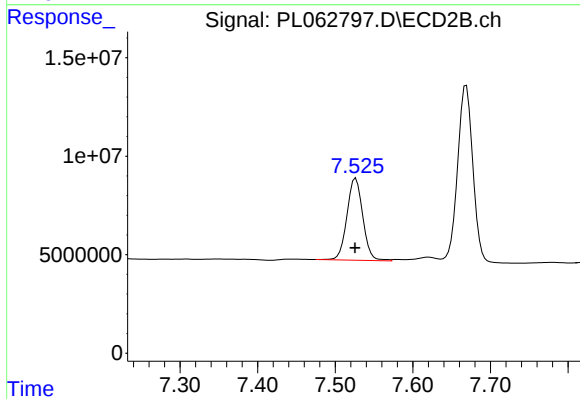

#20 Methoxychlor

R.T.: 7.526 min
Delta R.T.: 0.000 min
Response: 59075600
Conc: 47.81 ng/ml

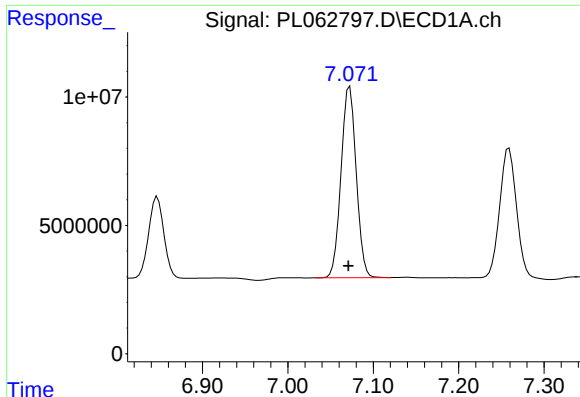


#21 Endrin ketone

R.T.: 7.073 min
Delta R.T.: 0.001 min
Response: 91911865
Conc: 50.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB132788BS


Manual Integrations
APPROVED

Ankita
11/4/2020 4:56:55 PM

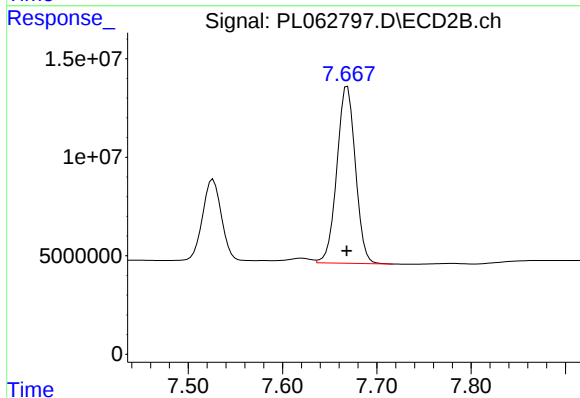


#21 Endrin ketone

R.T.: 7.669 min
Delta R.T.: 0.000 min
Response: 122571846
Conc: 51.72 ng/ml

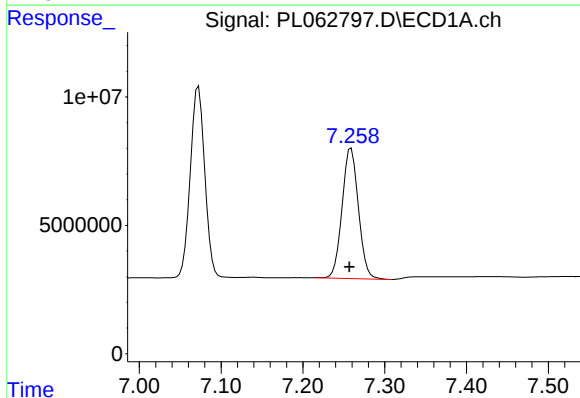


#22 Mirex

R.T.: 7.259 min
Delta R.T.: 0.002 min
Response: 70117615
Conc: 49.46 ng/ml

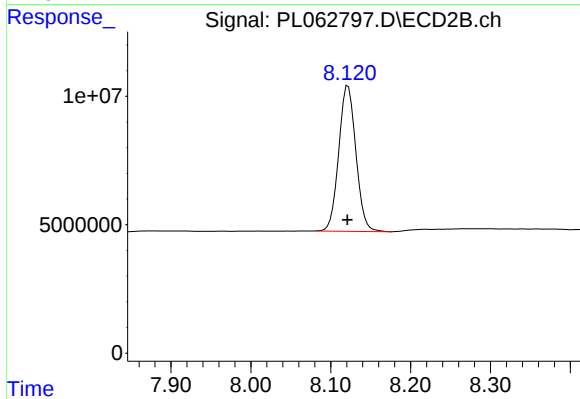

#22 Mirex

R.T.: 8.122 min
Delta R.T.: 0.000 min
Response: 84558858
Conc: 49.62 ng/ml

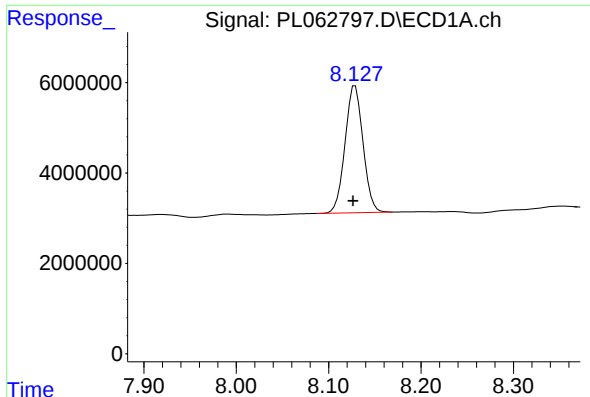


#28 Decachlorobiphenyl

R.T.: 8.129 min
Delta R.T.: 0.002 min
Response: 38017258
Conc: 23.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB132788BS

Manual Integrations
APPROVED

Ankita
11/4/2020 4:56:55 PM

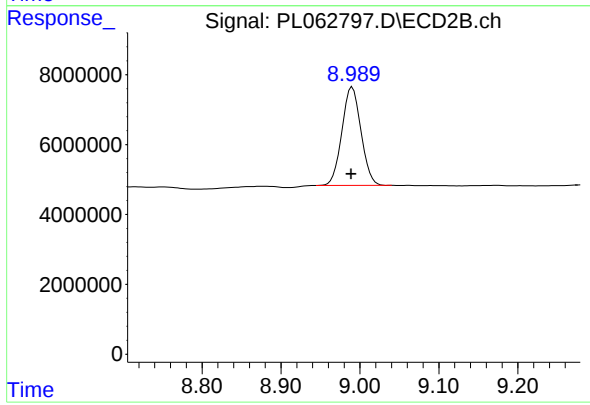

#28 Decachlorobiphenyl

R.T.: 8.990 min
Delta R.T.: 0.001 min
Response: 47380924
Conc: 22.64 ng/ml