

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110320\
 Data File : PL062800.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2020 13:02
 Operator : DD\AJ
 Sample : L4600-09
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CRT-19

Manual Integrations
 APPROVED

Ankita
 11/4/2020 3:53:03 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 17:02:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.411	3.951	26029534	40724495	15.133	13.858
28)	SA Decachlor...	8.126	8.989	32063281	36922277	19.986	17.641m
Target Compounds							
17)	MA 4,4'-DDT	6.300	7.065	1574489	2588319	1.180	1.153m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110320\
Data File : PL062800.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2020 13:02
Operator : DD\AJ
Sample : L4600-09
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CRT-19


Manual Integrations
APPROVED

Ankita
11/4/2020 3:53:03 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 17:02:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

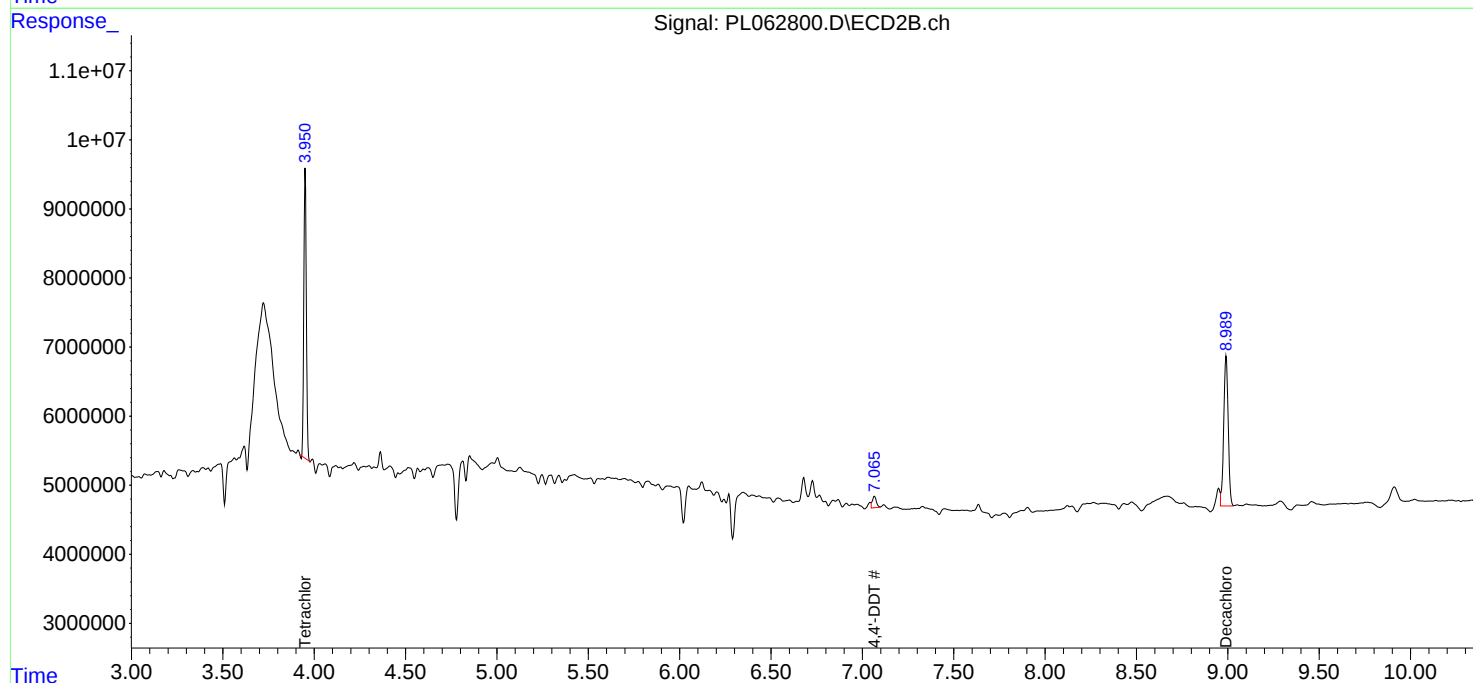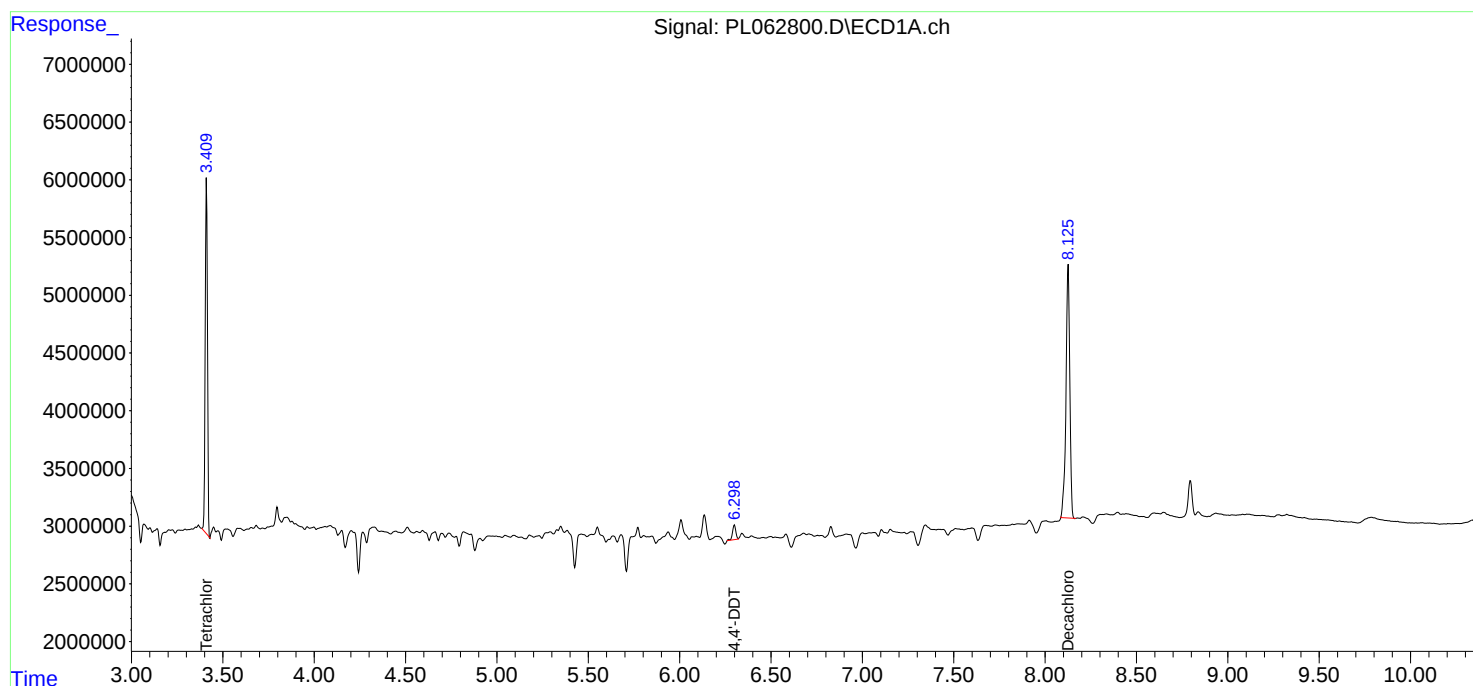

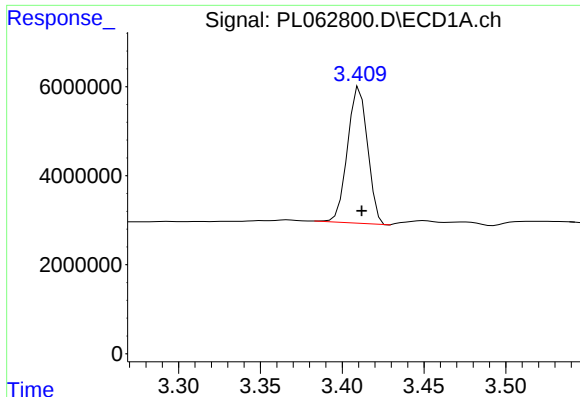


#1 Tetrachloro-m-xylene

R.T.: 3.411 min
Delta R.T.: -0.001 min
Response: 26029534
Conc: 15.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
CRT-19


Manual Integrations
APPROVED

Ankita
11/4/2020 3:53:03 PM

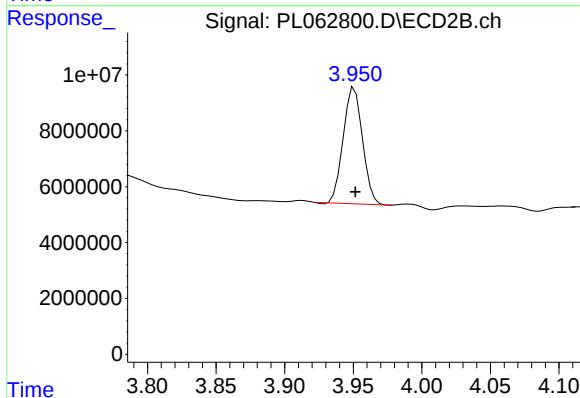


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 40724495
Conc: 13.86 ng/ml

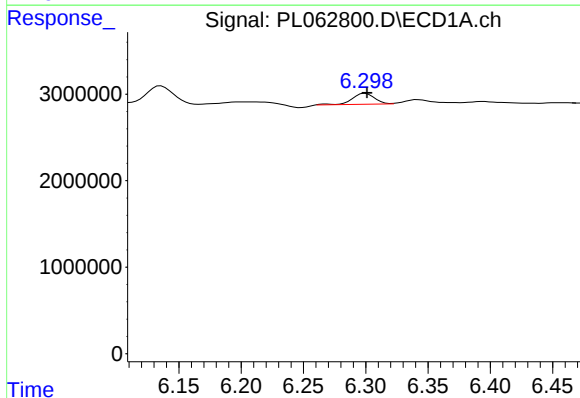


#17 4,4'-DDT

R.T.: 6.300 min
Delta R.T.: -0.001 min
Response: 1574489
Conc: 1.18 ng/ml

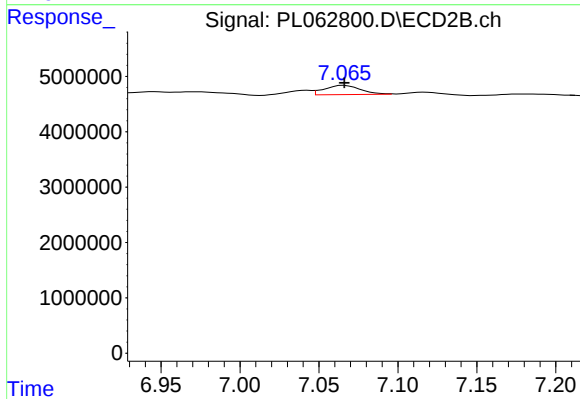

#17 4,4'-DDT

R.T.: 7.065 min
Delta R.T.: -0.002 min
Response: 2588319
Conc: 1.15 ng/ml m

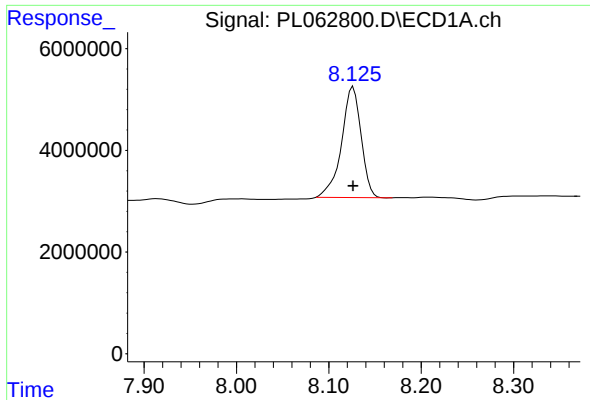


#28 Decachlorobiphenyl

R.T.: 8.126 min
Delta R.T.: 0.000 min
Response: 32063281
Conc: 19.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
CRT-19

Manual Integrations
APPROVED

Ankita
11/4/2020 3:53:03 PM

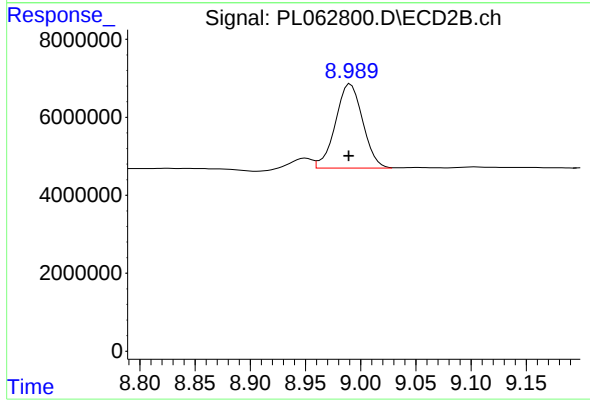

#28 Decachlorobiphenyl

R.T.: 8.989 min
Delta R.T.: 0.000 min
Response: 36922277
Conc: 17.64 ng/ml m