

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110320\
 Data File : PL062801.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2020 13:17
 Operator : DD\AJ
 Sample : L4600-13
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CRT-6

Manual Integrations
 APPROVED

Ankita
 11/4/2020 3:53:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 17:02:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.411	3.951	28334994	48414646	16.473	16.475
28) SA Decachlor...	8.127	8.990	32628795	37526724	20.339	17.930m
Target Compounds						
11) B alpha-Chl...	5.384	6.119	1053929	2610452	0.583m	0.775m#
17) MA 4,4'-DDT	6.299	7.065	1048405	1697632	0.786m	0.756m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110320\
Data File : PL062801.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2020 13:17
Operator : DD\AJ
Sample : L4600-13
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
CRT-6


Manual Integrations
APPROVED

Ankita
11/4/2020 3:53:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 17:02:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

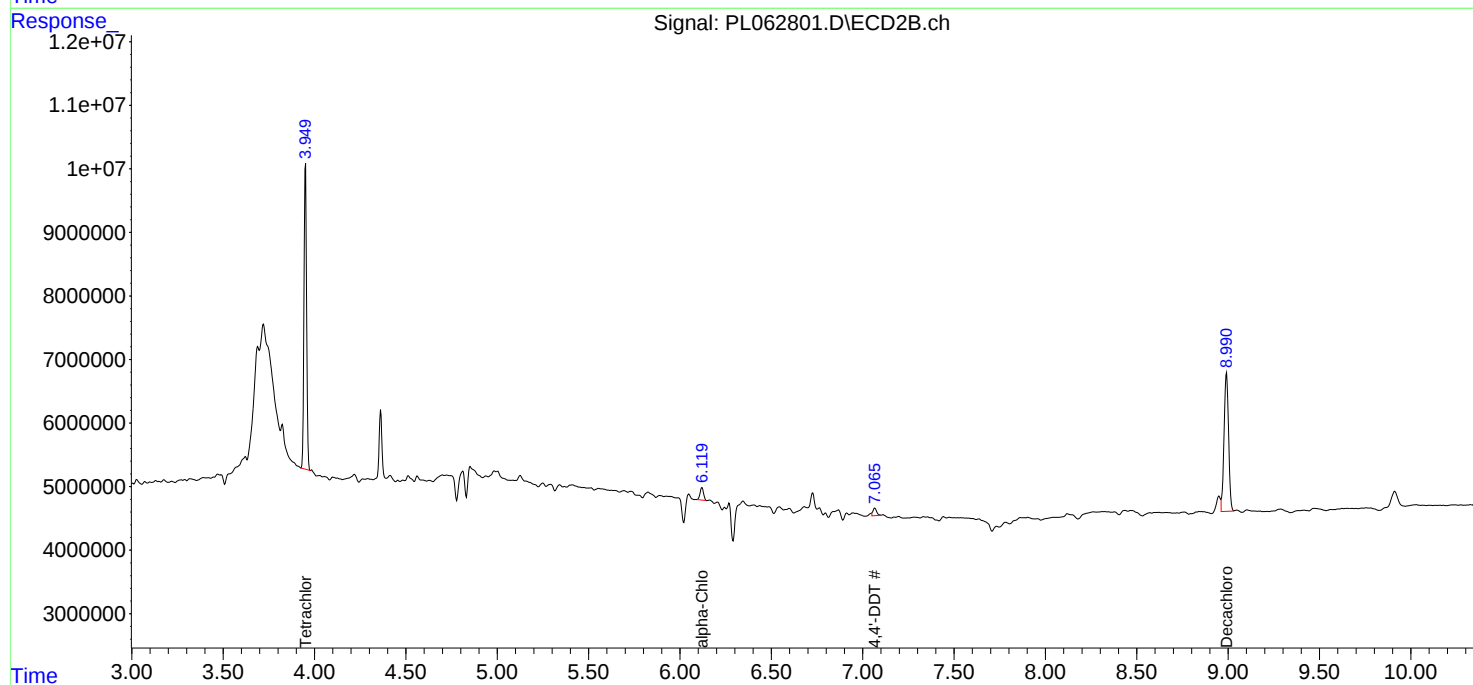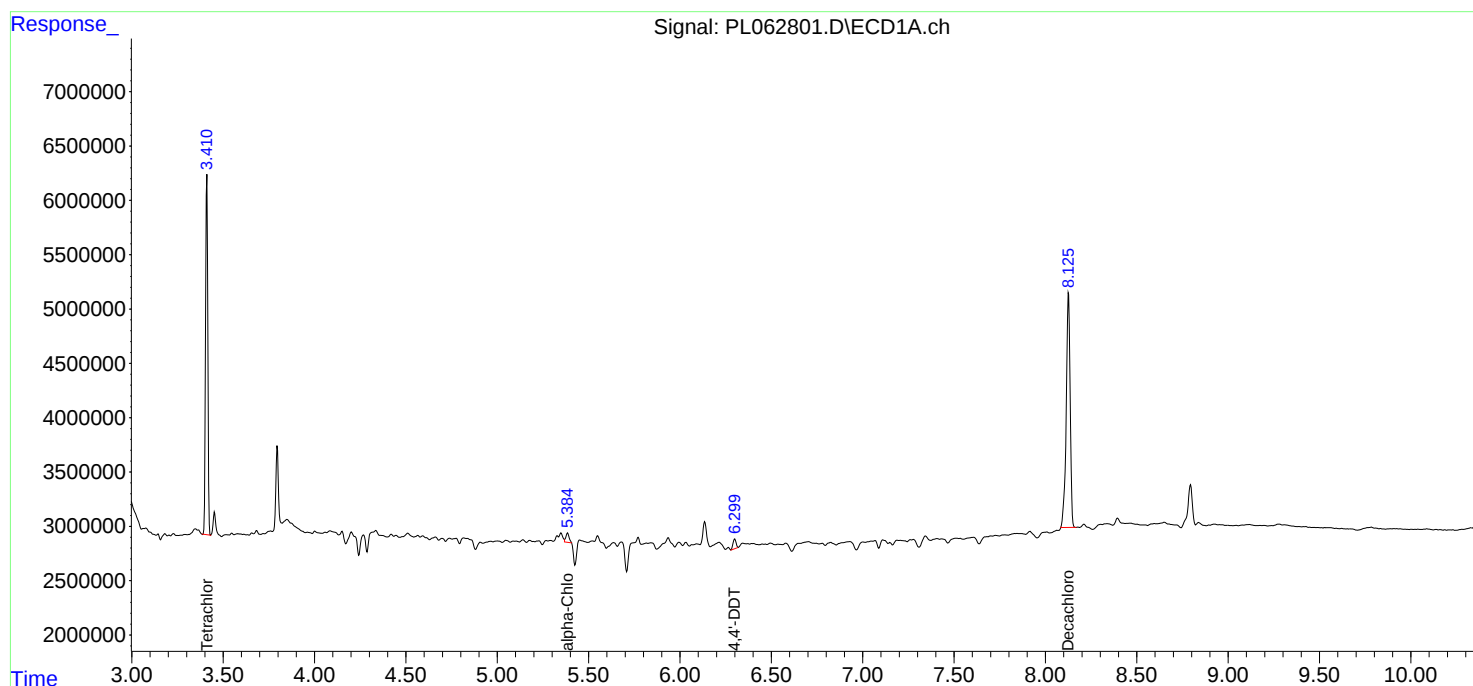

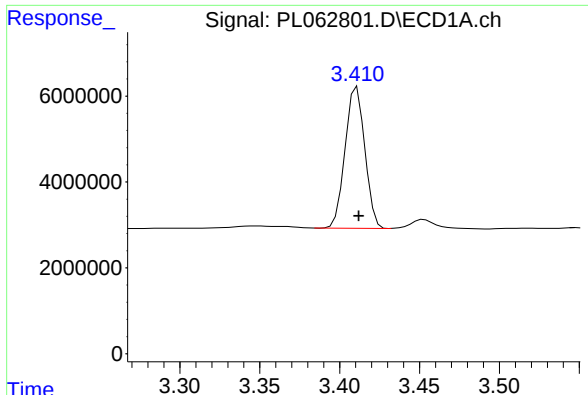


#1 Tetrachloro-m-xylene

R.T.: 3.411 min
Delta R.T.: -0.001 min
Response: 28334994
Conc: 16.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
CRT-6


Manual Integrations
APPROVED

Ankita
11/4/2020 3:53:05 PM

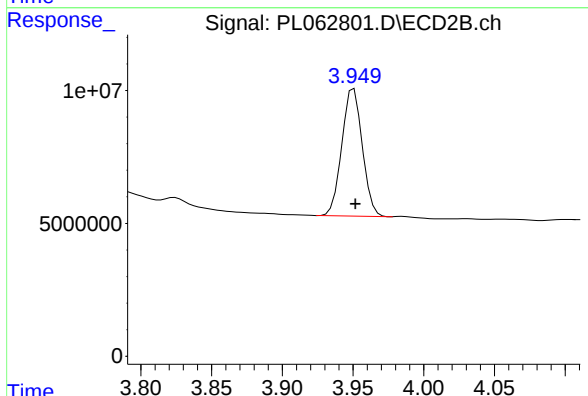


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: -0.001 min
Response: 48414646
Conc: 16.47 ng/ml

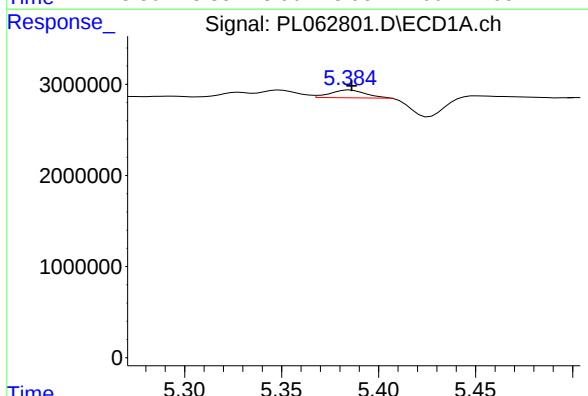


#11 alpha-Chlordane

R.T.: 5.384 min
Delta R.T.: -0.002 min
Response: 1053929
Conc: 0.58 ng/ml m

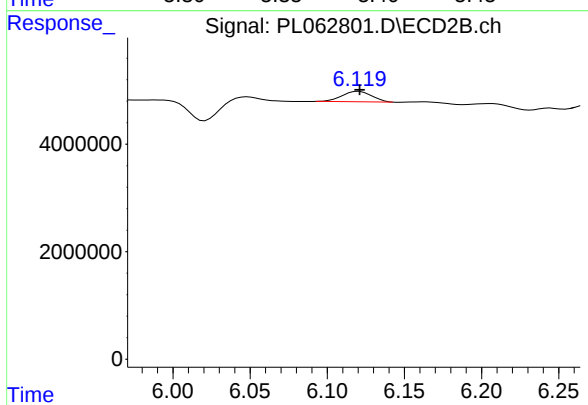

#11 alpha-Chlordane

R.T.: 6.119 min
Delta R.T.: -0.002 min
Response: 2610452
Conc: 0.77 ng/ml m

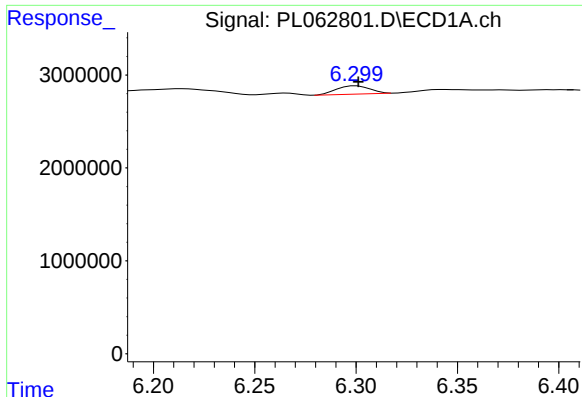


#17 4,4'-DDT

R.T.: 6.299 min
Delta R.T.: -0.002 min
Response: 1048405
Conc: 0.79 ng/ml m

Instrument :
ECD_L
ClientSampleId :
CRT-6


Manual Integrations
APPROVED

Ankita
11/4/2020 3:53:05 PM

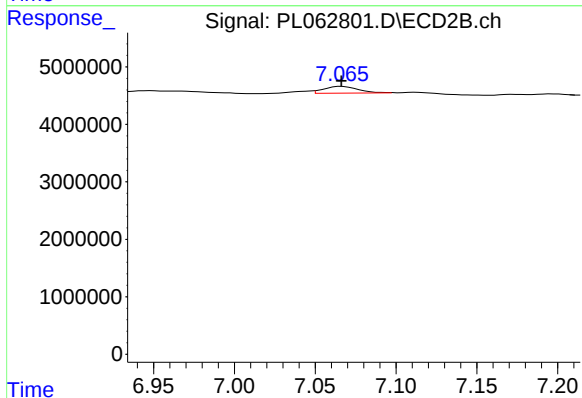


#17 4,4'-DDT

R.T.: 7.065 min
Delta R.T.: -0.001 min
Response: 1697632
Conc: 0.76 ng/ml m

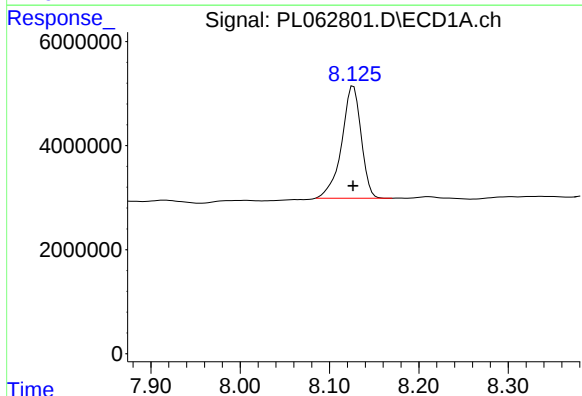

#28 Decachlorobiphenyl

R.T.: 8.127 min
Delta R.T.: 0.000 min
Response: 32628795
Conc: 20.34 ng/ml

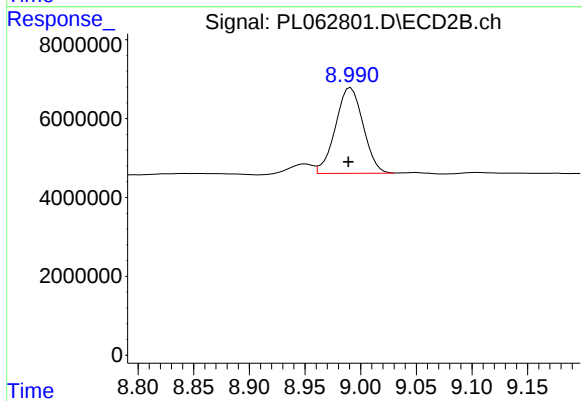

#28 Decachlorobiphenyl

R.T.: 8.990 min
Delta R.T.: 0.000 min
Response: 37526724
Conc: 17.93 ng/ml m