

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110321\
 Data File : PL070737.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2021 18:22
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 19:29:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 04 19:28:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
2) A	alpha-BHC	0.000	6.059f	0	849526	N.D. 0.461 #
5) MB	Aldrin	0.000	7.499	0	631593	N.D. 0.389 #
7) B	delta-BHC	6.366f	7.025f	-217667	1819476	N.D. 1.088
8) B	Heptachlo...	0.000	7.969	0	6720180	N.D. 4.409 #
9) A	Endosulfan I	7.385f	0.000	3581569	0	5.847 N.D. #
13) MA	Dieldrin	7.695	0.000	590793	0	0.946 N.D. #
15) B	Endosulfa...	8.269f	9.099f	2825348	746281	4.667 0.611 #
24)	Chlordane-2	0.000	7.499f	0	631593	N.D. 12.041 #
27)	Chlordane-5	8.269f	0.000	2825348	0	126.369 N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110321\
Data File : PL070737.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2021 18:22
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 19:29:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
Quant Title : GC Extractables
QLast Update : Thu Nov 04 19:28:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

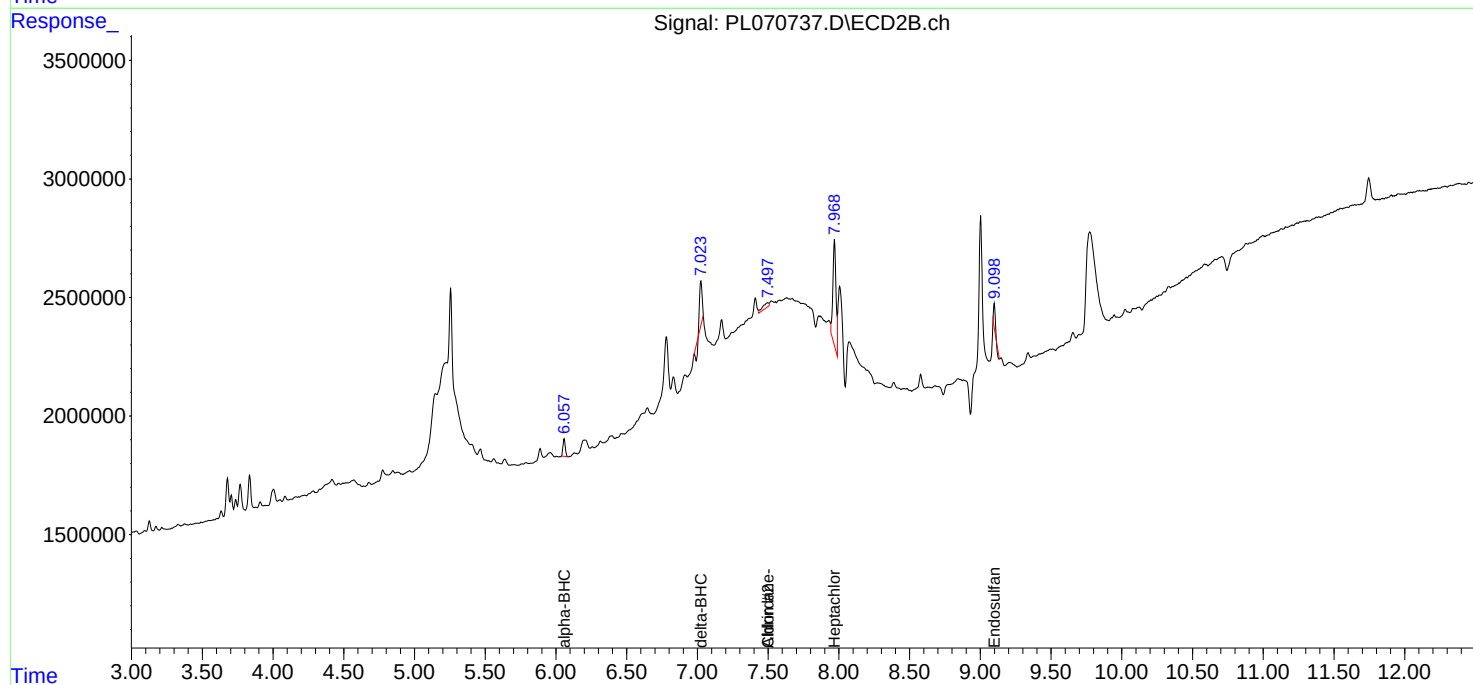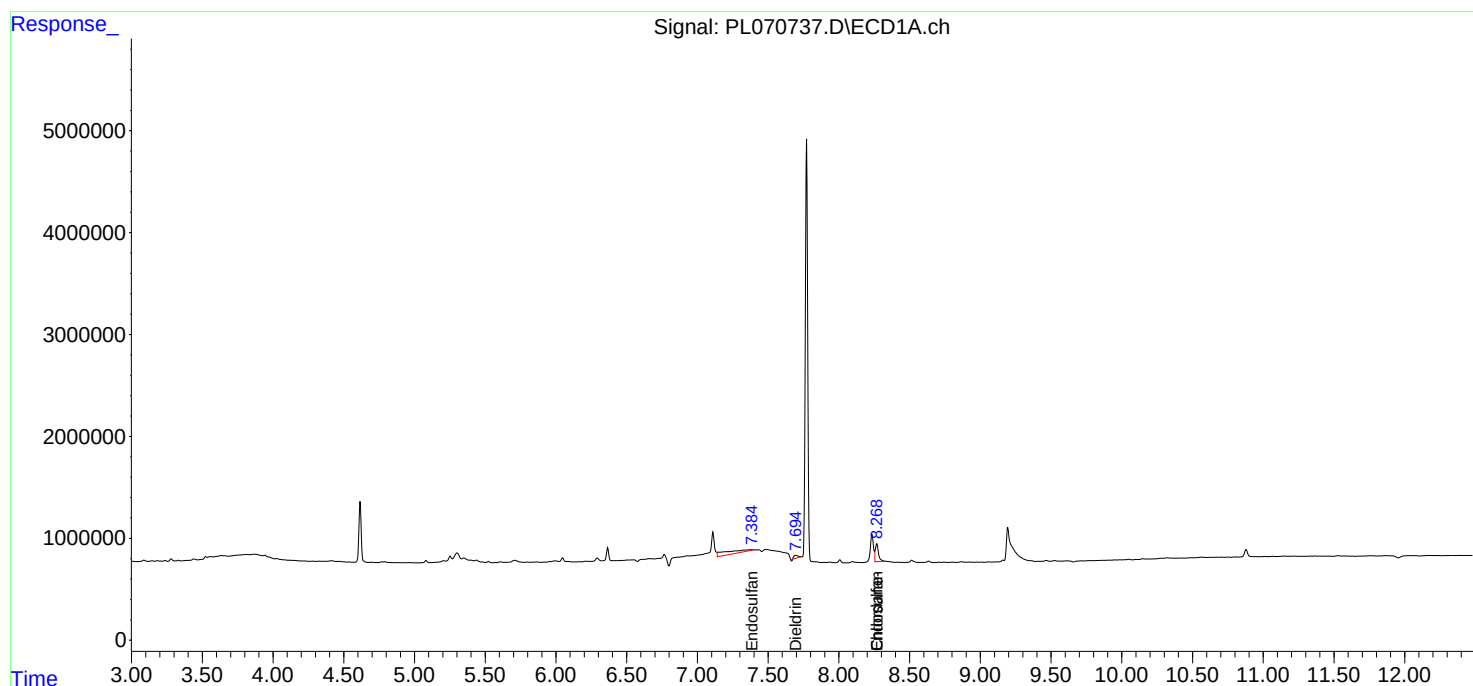


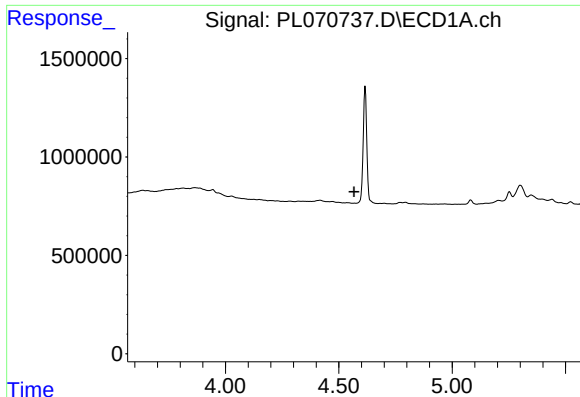

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.568 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

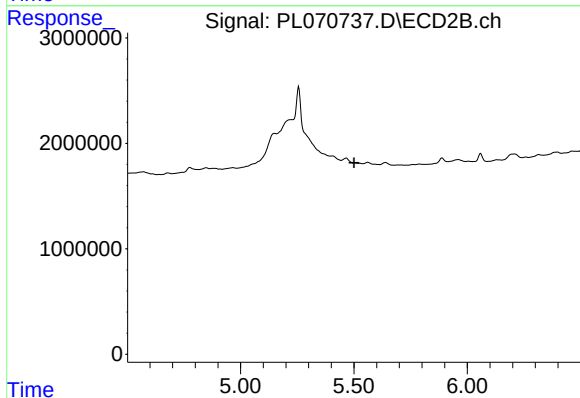


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

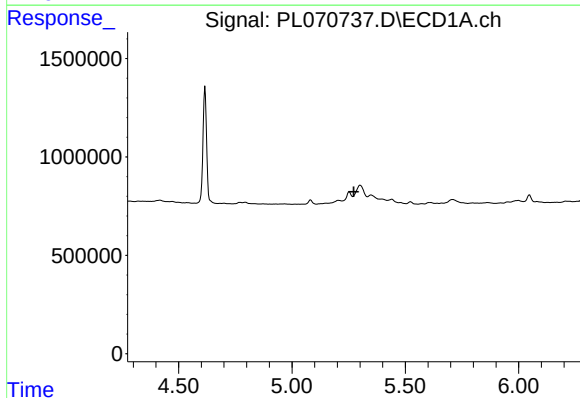


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.273 min
Response: 0
Conc: N.D.

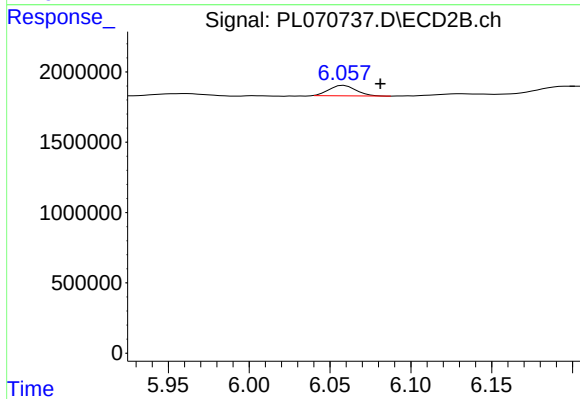

#2 alpha-BHC


R.T.: 6.059 min
Delta R.T.: -0.022 min
Response: 849526
Conc: 0.46 ng/ml

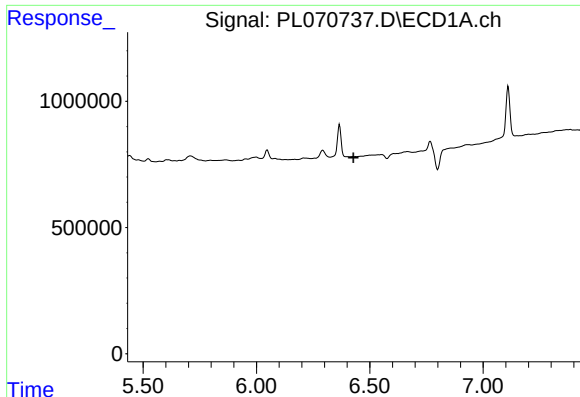

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 6.428 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

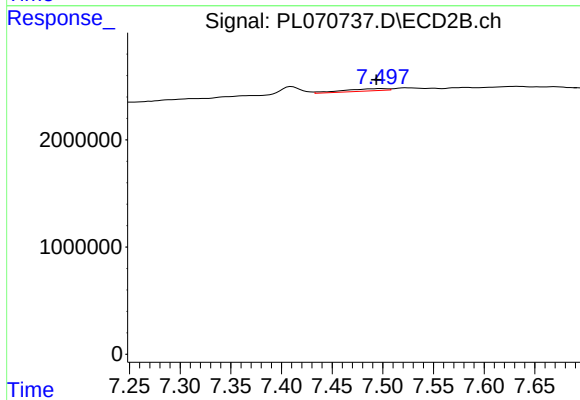


#5 Aldrin

R.T.: 7.499 min
Delta R.T.: 0.005 min
Response: 631593
Conc: 0.39 ng/ml

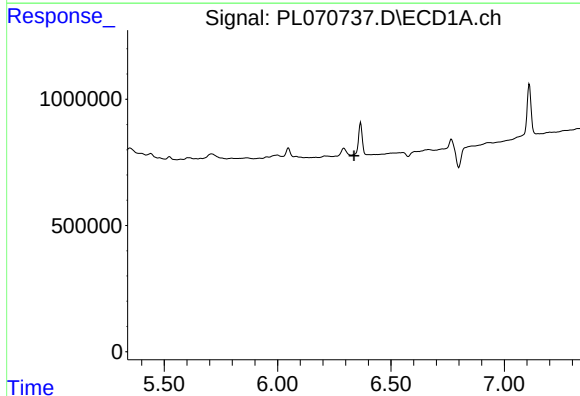


#7 delta-BHC

R.T.: 6.366 min
Delta R.T.: 0.028 min
Response: -217667
Conc: N.D.

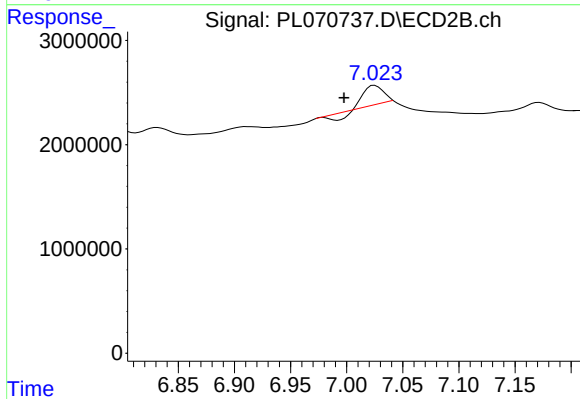

#7 delta-BHC


R.T.: 7.025 min
Delta R.T.: 0.027 min
Response: 1819476
Conc: 1.09 ng/ml

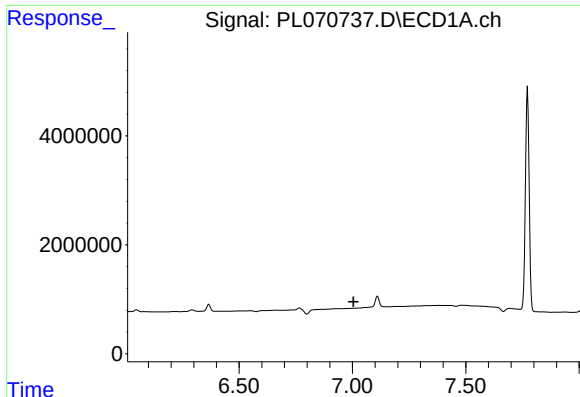

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 7.005 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

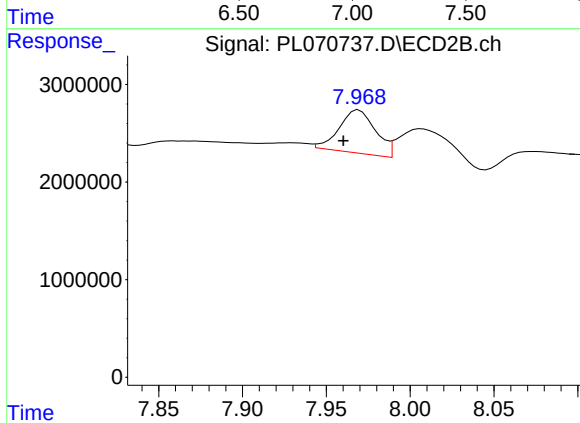


#8 Heptachlor epoxide

R.T.: 7.969 min
Delta R.T.: 0.009 min
Response: 6720180
Conc: 4.41 ng/ml

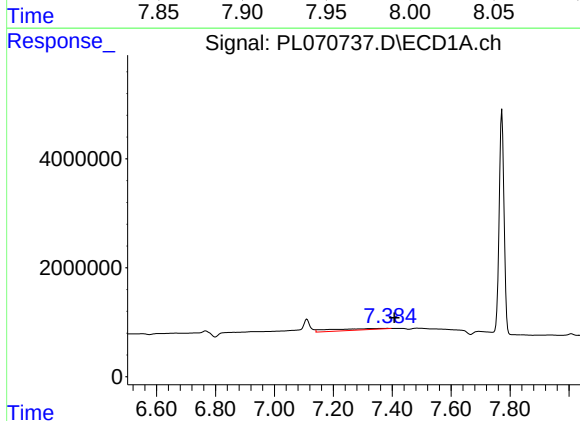


#9 Endosulfan I

R.T.: 7.385 min
Delta R.T.: -0.023 min
Response: 3581569
Conc: 5.85 ng/ml

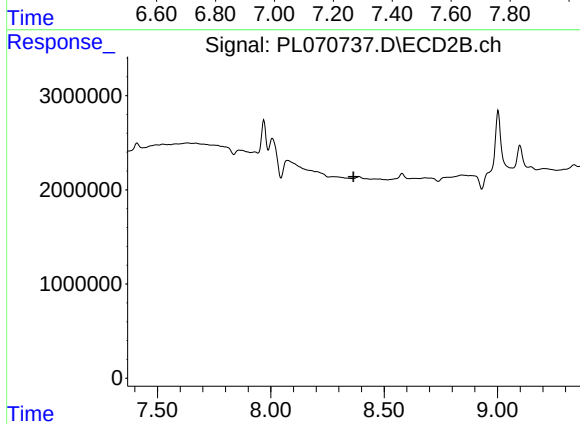

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 8.365 min
Response: 0
Conc: N.D.

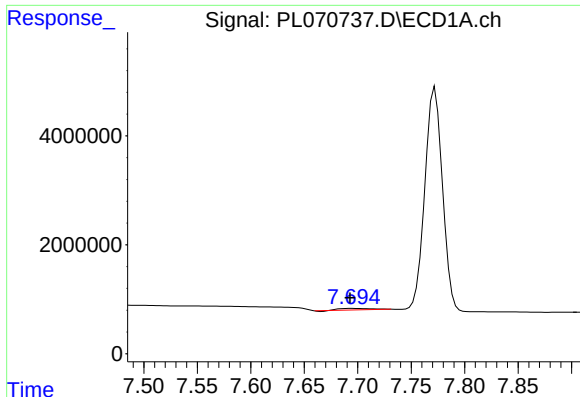

#13 Dieldrin


R.T.: 7.695 min
Delta R.T.: 0.002 min
Response: 590793
Conc: 0.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

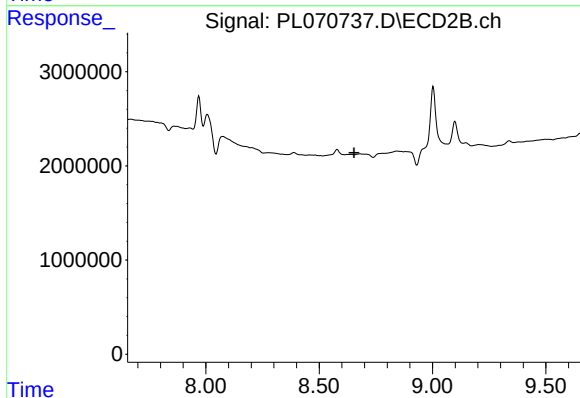


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.654 min
Response: 0
Conc: N.D.

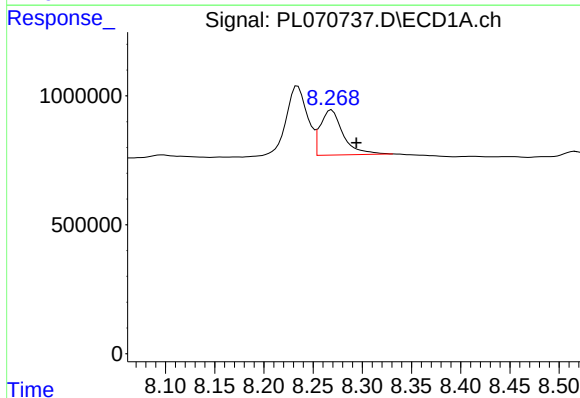


#15 Endosulfan II

R.T.: 8.269 min
Delta R.T.: -0.025 min
Response: 2825348
Conc: 4.67 ng/ml

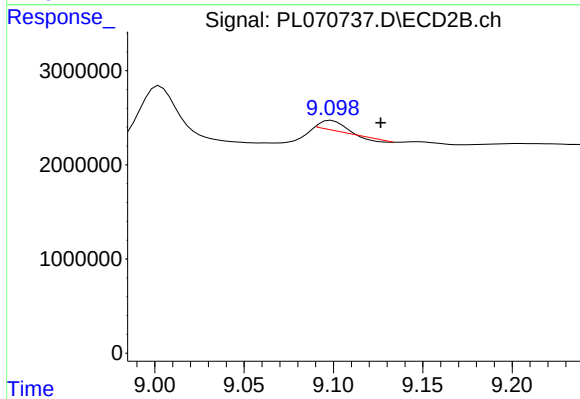

#15 Endosulfan II

R.T.: 9.099 min
Delta R.T.: -0.027 min
Response: 746281
Conc: 0.61 ng/ml

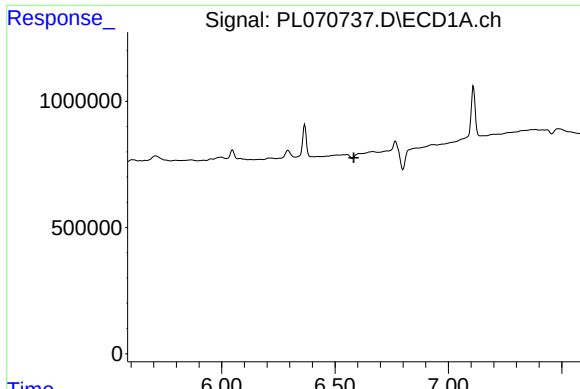

#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 6.582 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

#24 Chlordane-2


R.T.: 7.499 min
Delta R.T.: 0.025 min
Response: 631593
Conc: 12.04 ng/ml

#27 Chlordane-5

R.T.: 8.269 min
Delta R.T.: -0.029 min
Response: 2825348
Conc: 126.37 ng/ml

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 9.197 min
Response: 0
Conc: N.D.

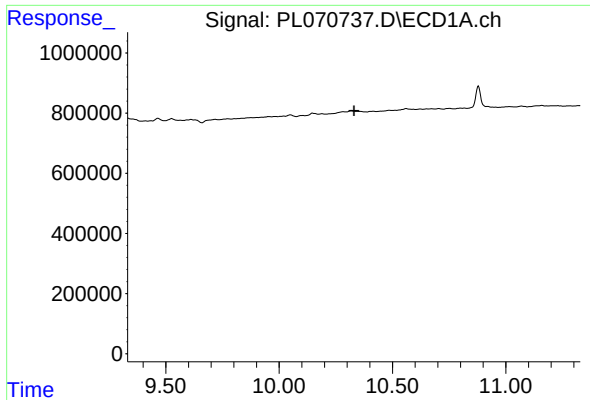

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.330 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

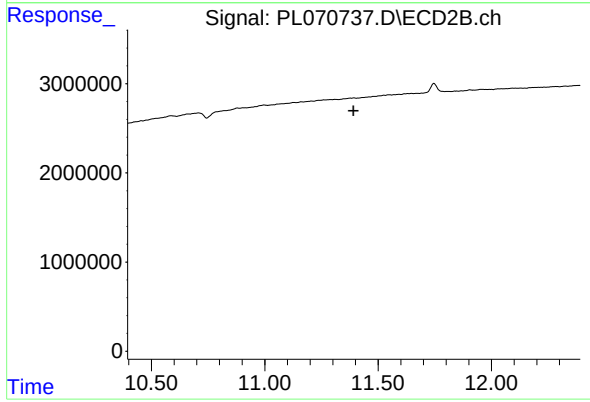

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 11.392 min
Response: 0
Conc: N.D.