

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110321\
 Data File : PL070747.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2021 21:08
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 18:40:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 04 18:39:10 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.568	5.501	38430888	95829620	75.417	75.692
28)	SA Decachlor...	10.330	11.392	48159450	99277045	71.369	72.158
Target Compounds							
23)	Chlordane-1	5.894	6.883	12930065	36934182	746.977	748.284
24)	Chlordane-2	6.583	7.474	16738368	39246862	730.341	735.033
25)	Chlordane-3	7.283	8.231	46323344	156.5E6	741.697	744.025
26)	Chlordane-4	7.351	8.313	49737842	187.0E6	741.030	736.649
27)	Chlordane-5	8.300	9.198	15804123	31697016	718.282	731.852



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110321\
Data File : PL070747.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2021 21:08
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 18:40:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
Quant Title : GC Extractables
QLast Update : Thu Nov 04 18:39:10 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

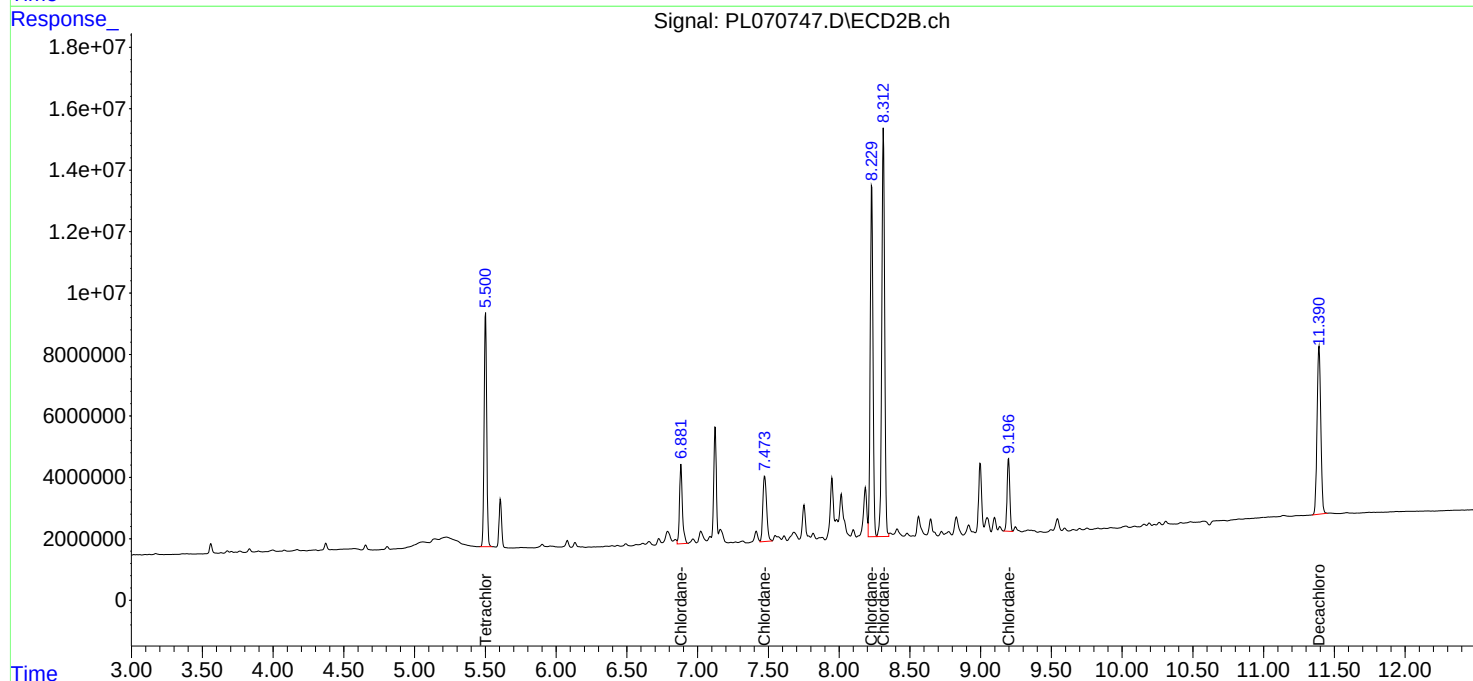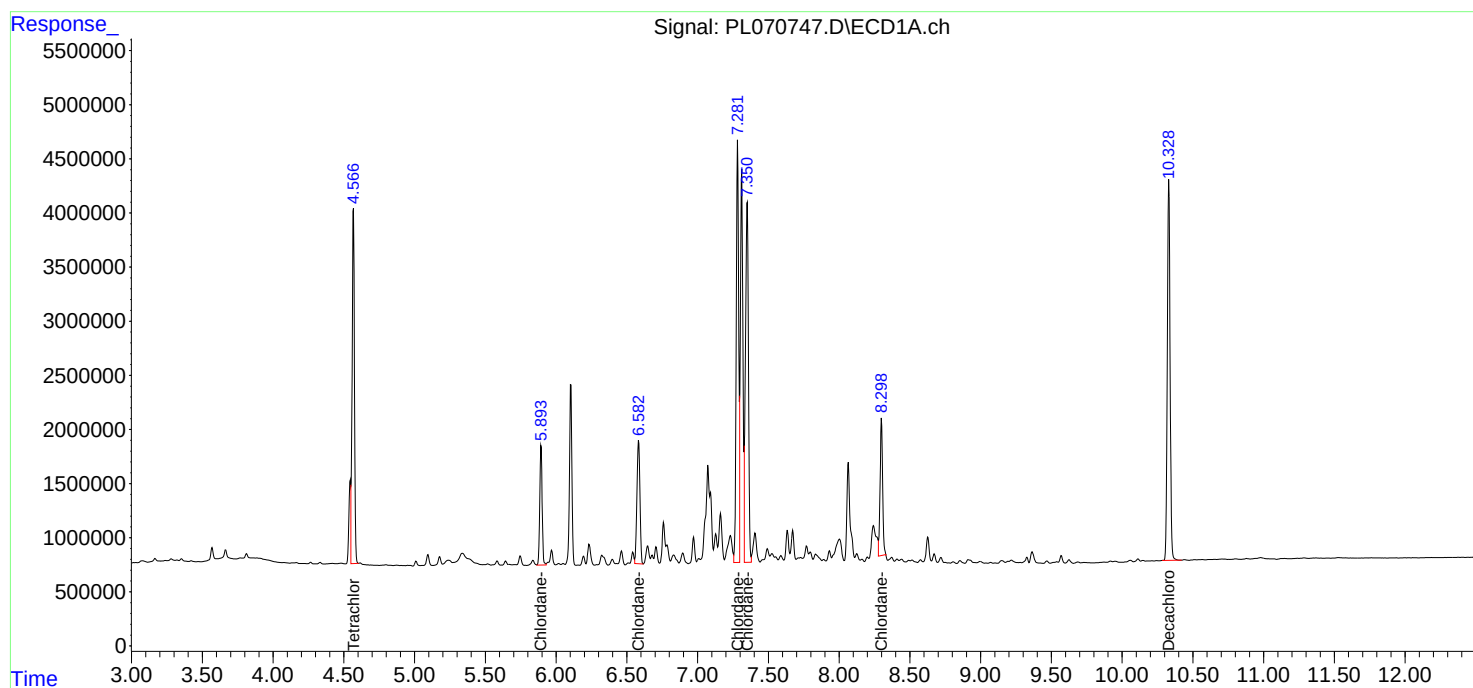


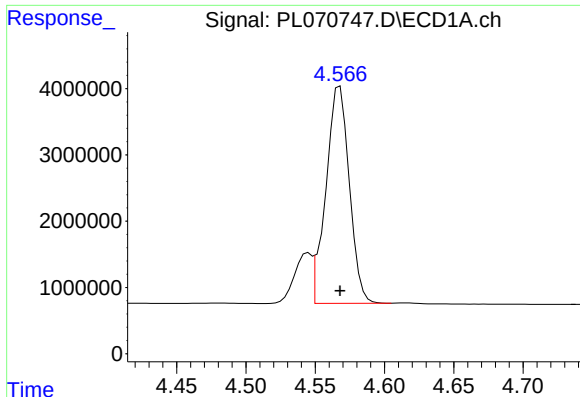

#1 Tetrachloro-m-xylene


R.T.: 4.568 min
Delta R.T.: 0.000 min
Response: 38430888
Conc: 75.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

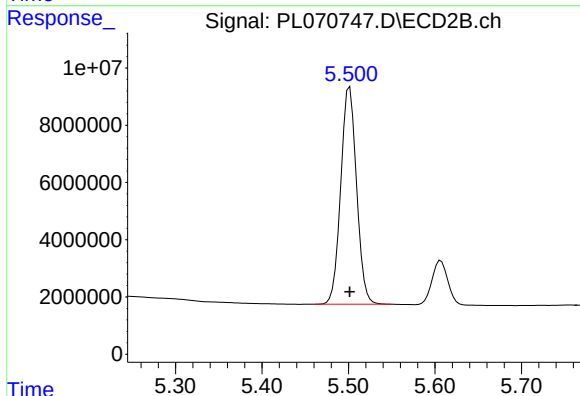


#1 Tetrachloro-m-xylene

R.T.: 5.501 min
Delta R.T.: 0.000 min
Response: 95829620
Conc: 75.69 ng/ml

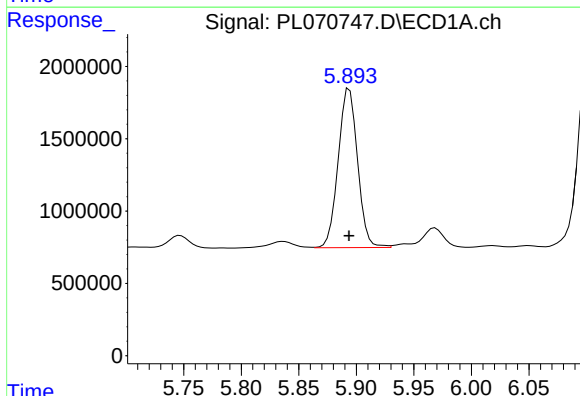


#23 Chlordane-1

R.T.: 5.894 min
Delta R.T.: 0.000 min
Response: 12930065
Conc: 746.98 ng/ml

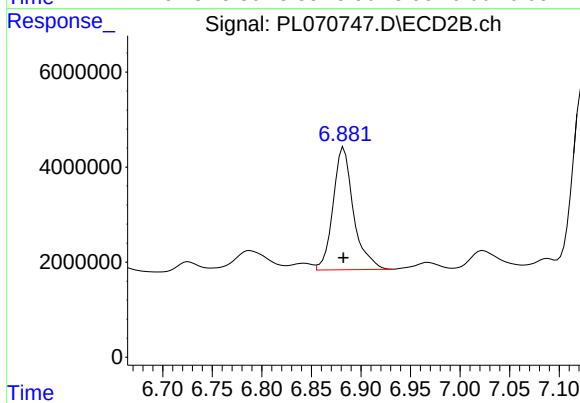

#23 Chlordane-1


R.T.: 6.883 min
Delta R.T.: 0.000 min
Response: 36934182
Conc: 748.28 ng/ml

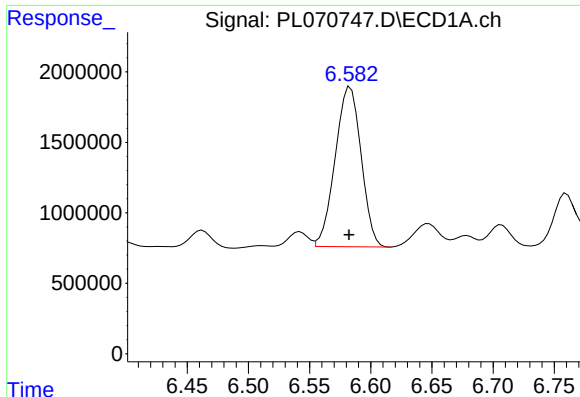

#24 Chlordane-2


R.T.: 6.583 min
Delta R.T.: 0.001 min
Response: 16738368
Conc: 730.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

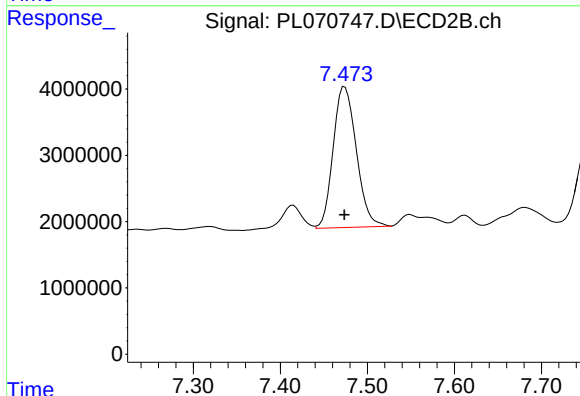


#24 Chlordane-2

R.T.: 7.474 min
Delta R.T.: 0.000 min
Response: 39246862
Conc: 735.03 ng/ml

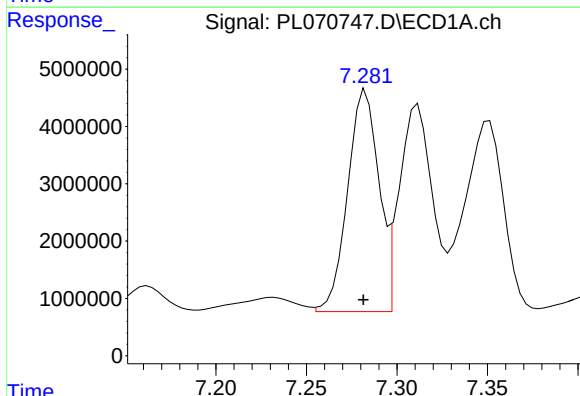


#25 Chlordane-3

R.T.: 7.283 min
Delta R.T.: 0.001 min
Response: 46323344
Conc: 741.70 ng/ml

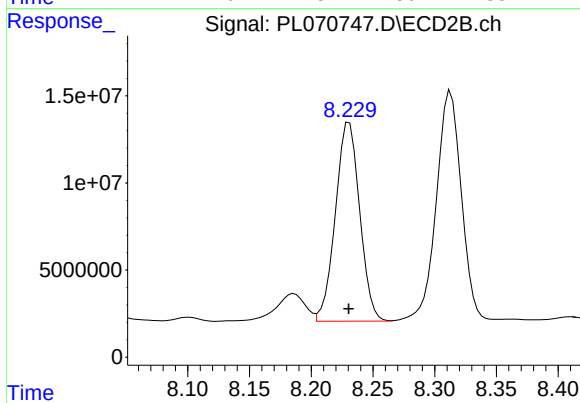

#25 Chlordane-3


R.T.: 8.231 min
Delta R.T.: 0.000 min
Response: 156456445
Conc: 744.03 ng/ml

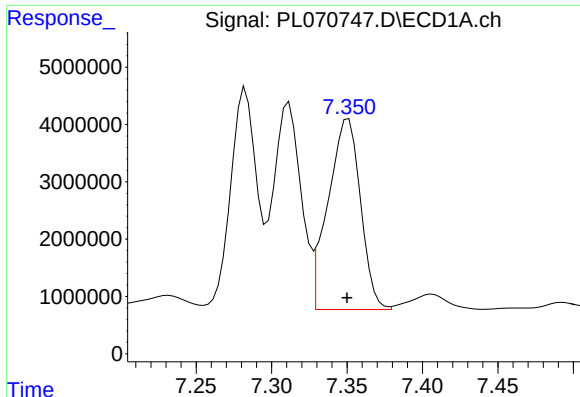

#26 Chlordane-4


R.T.: 7.351 min
Delta R.T.: 0.000 min
Response: 49737842
Conc: 741.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

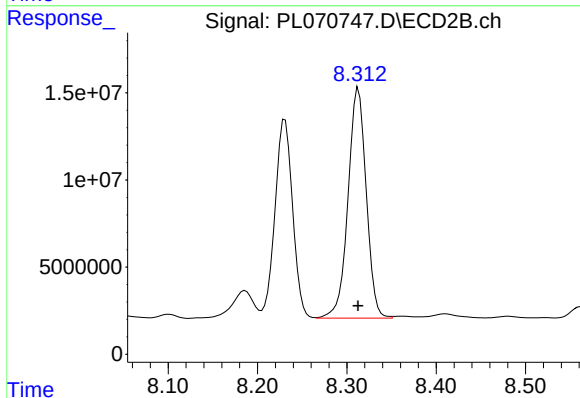


#26 Chlordane-4

R.T.: 8.313 min
Delta R.T.: 0.000 min
Response: 186993554
Conc: 736.65 ng/ml

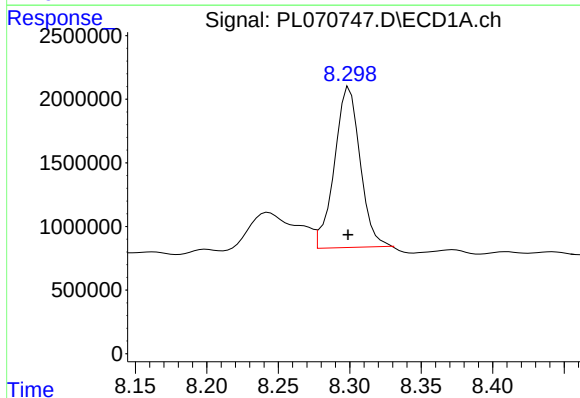


#27 Chlordane-5

R.T.: 8.300 min
Delta R.T.: 0.000 min
Response: 15804123
Conc: 718.28 ng/ml

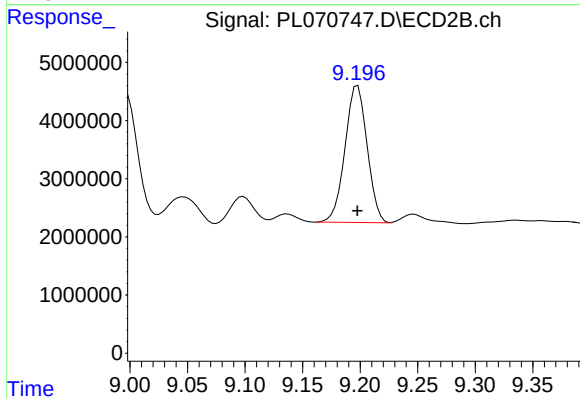

#27 Chlordane-5


R.T.: 9.198 min
Delta R.T.: 0.000 min
Response: 31697016
Conc: 731.85 ng/ml

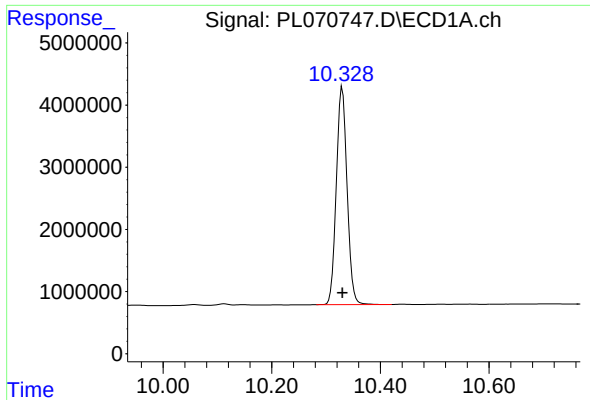

#28 Decachlorobiphenyl

R.T.: 10.330 min
Delta R.T.: 0.000 min
Response: 48159450
Conc: 71.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

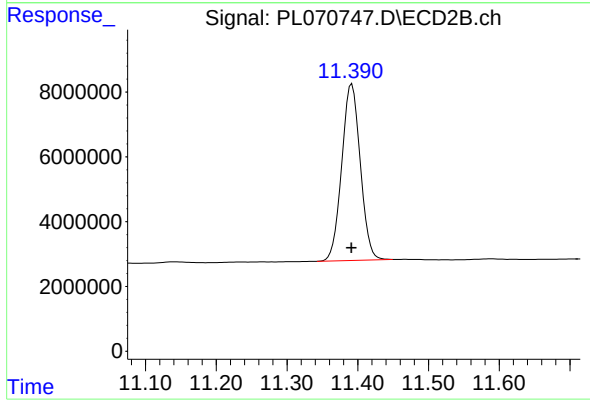

#28 Decachlorobiphenyl

R.T.: 11.392 min
Delta R.T.: 0.000 min
Response: 99277045
Conc: 72.16 ng/ml