

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110321\
 Data File : PL070746.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2021 20:51
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 18:39:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 04 18:39:10 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.568	5.501	49000973	123.3E6	96.160	97.364
28)	SA Decachlor...	10.330	11.391	62430518	130.5E6	92.518	94.815
Target Compounds							
23)	Chlordane-1	5.894	6.882	16818369	48144830	971.606	975.411
24)	Chlordane-2	6.582	7.474	21547617	50860690	940.182	952.542
25)	Chlordane-3	7.282	8.230	61402367	207.2E6	983.131	985.332
26)	Chlordane-4	7.350	8.312	65678946	246.9E6	978.533	972.667
27)	Chlordane-5	8.299	9.198	20954518	42115428	952.362	972.403



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110321\
Data File : PL070746.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2021 20:51
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 18:39:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
Quant Title : GC Extractables
QLast Update : Thu Nov 04 18:39:10 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

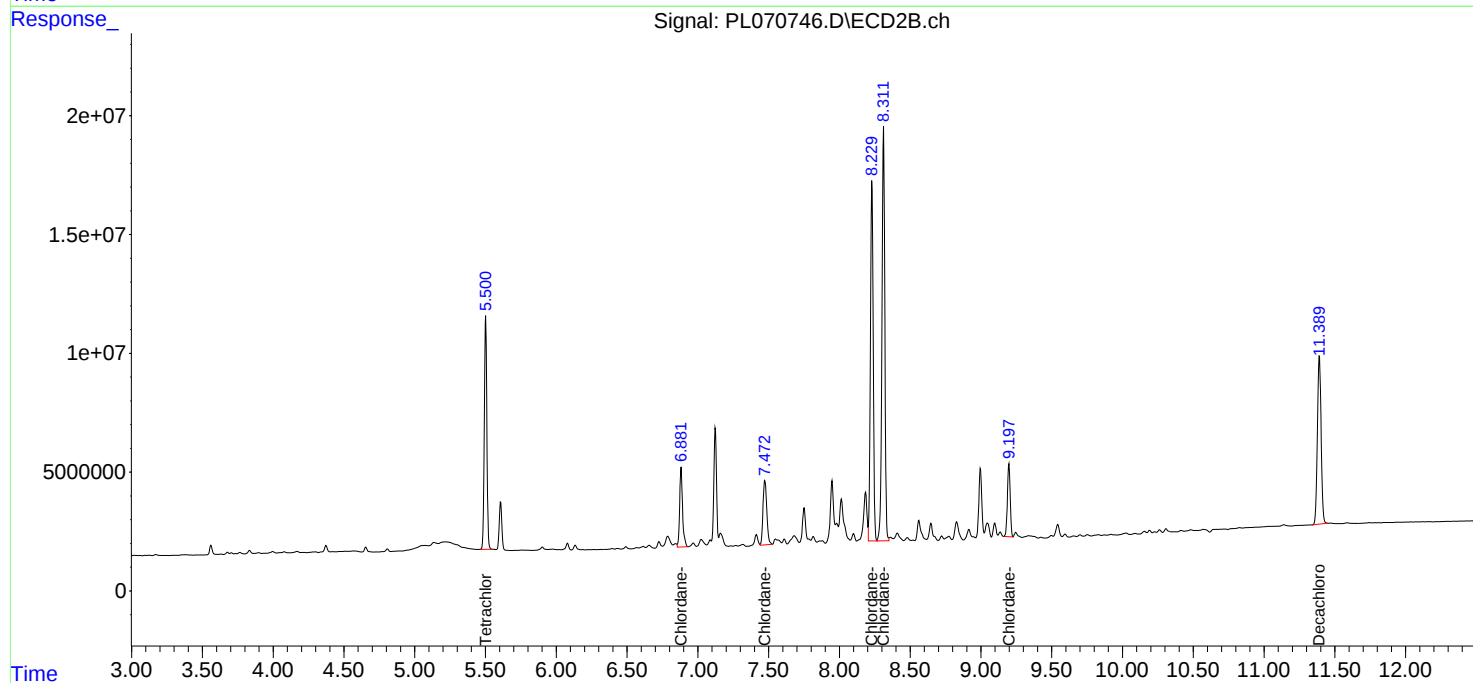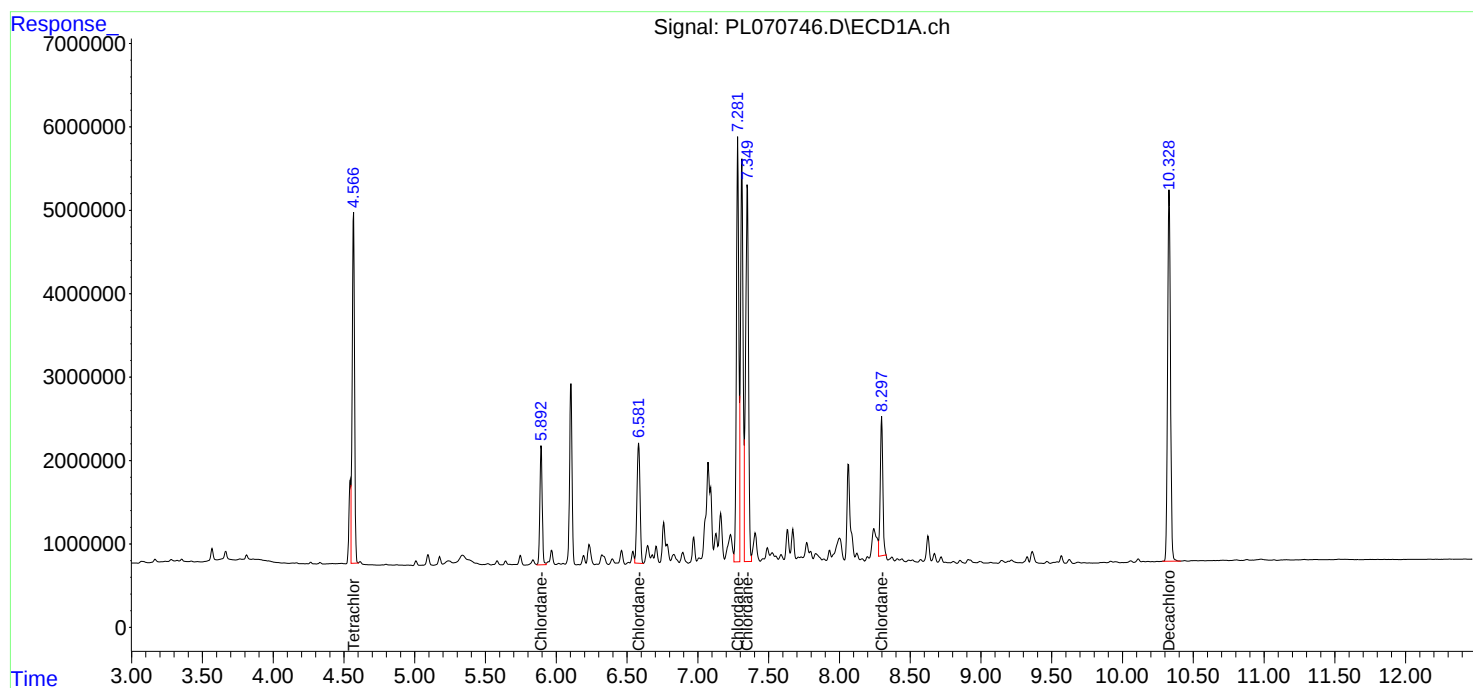


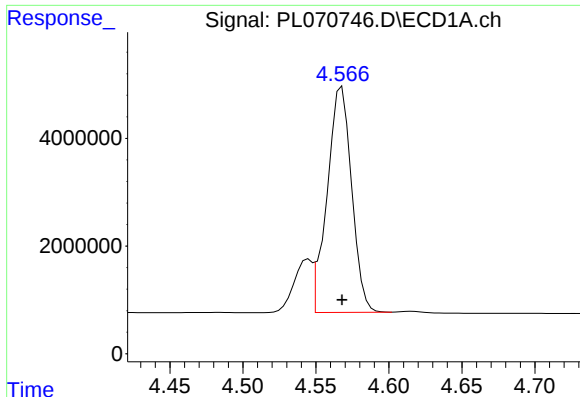

#1 Tetrachloro-m-xylene


R.T.: 4.568 min
Delta R.T.: 0.000 min
Response: 49000973
Conc: 96.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

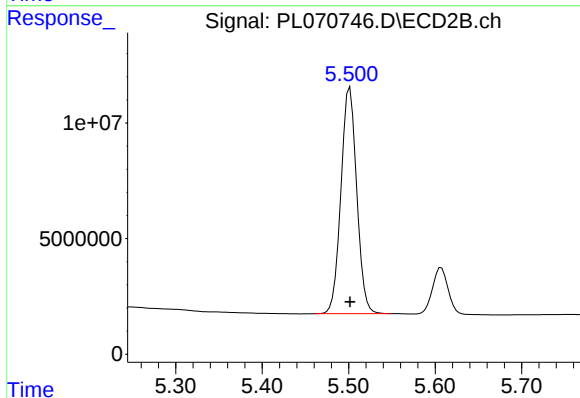


#1 Tetrachloro-m-xylene

R.T.: 5.501 min
Delta R.T.: 0.000 min
Response: 123267208
Conc: 97.36 ng/ml

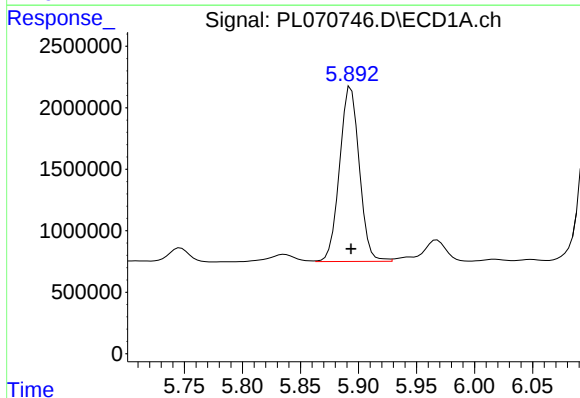


#23 Chlordane-1

R.T.: 5.894 min
Delta R.T.: 0.000 min
Response: 16818369
Conc: 971.61 ng/ml

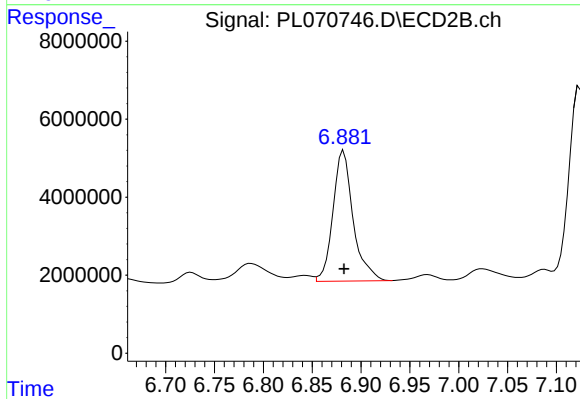

#23 Chlordane-1


R.T.: 6.882 min
Delta R.T.: 0.000 min
Response: 48144830
Conc: 975.41 ng/ml

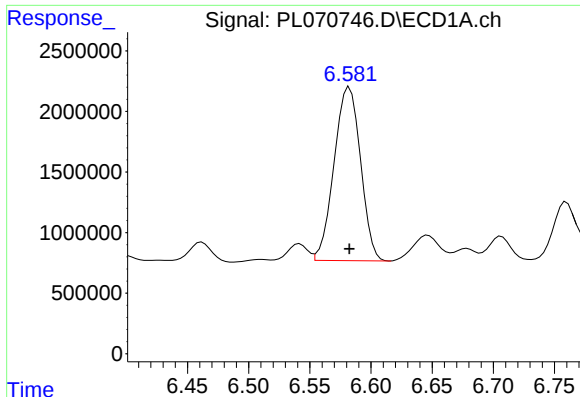

#24 Chlordane-2


R.T.: 6.582 min
Delta R.T.: 0.000 min
Response: 21547617
Conc: 940.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

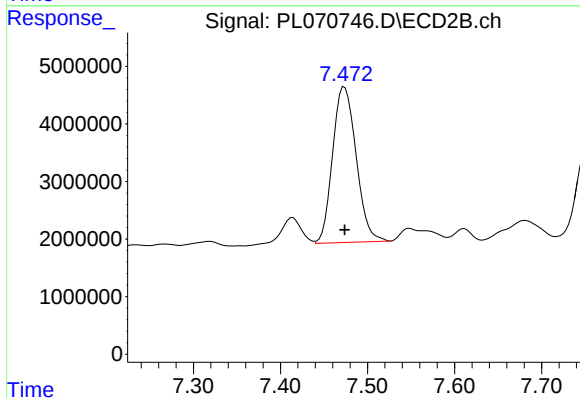


#24 Chlordane-2

R.T.: 7.474 min
Delta R.T.: 0.000 min
Response: 50860690
Conc: 952.54 ng/ml

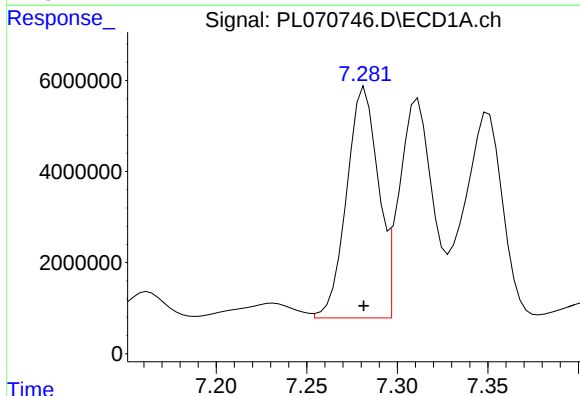


#25 Chlordane-3

R.T.: 7.282 min
Delta R.T.: 0.000 min
Response: 61402367
Conc: 983.13 ng/ml

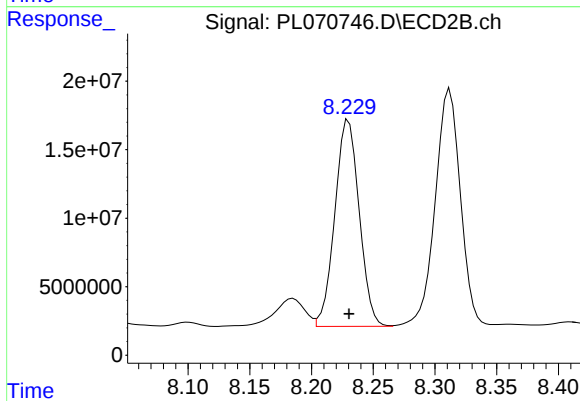

#25 Chlordane-3


R.T.: 8.230 min
Delta R.T.: 0.000 min
Response: 207199439
Conc: 985.33 ng/ml

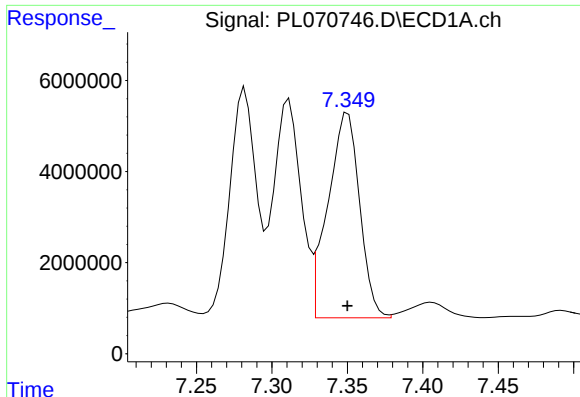

#26 Chlordane-4


R.T.: 7.350 min
Delta R.T.: 0.000 min
Response: 65678946
Conc: 978.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

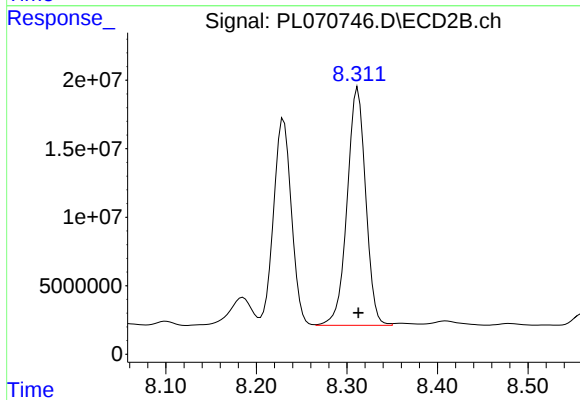


#26 Chlordane-4

R.T.: 8.312 min
Delta R.T.: 0.000 min
Response: 246905044
Conc: 972.67 ng/ml

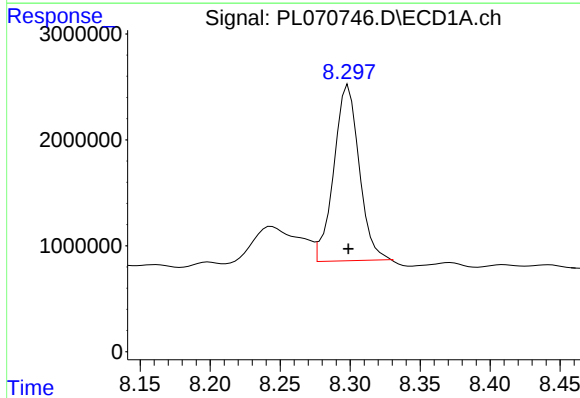


#27 Chlordane-5

R.T.: 8.299 min
Delta R.T.: 0.000 min
Response: 20954518
Conc: 952.36 ng/ml

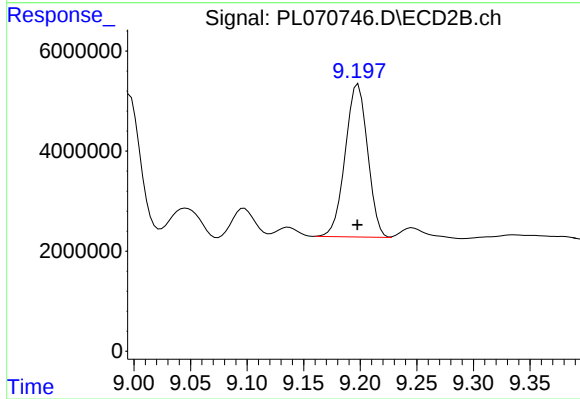

#27 Chlordane-5


R.T.: 9.198 min
Delta R.T.: 0.000 min
Response: 42115428
Conc: 972.40 ng/ml

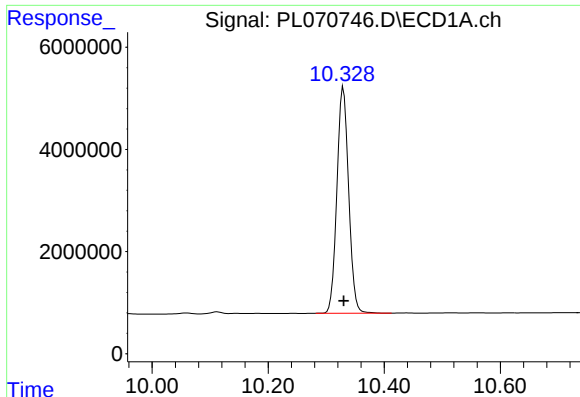

#28 Decachlorobiphenyl

R.T.: 10.330 min
Delta R.T.: 0.000 min
Response: 62430518
Conc: 92.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

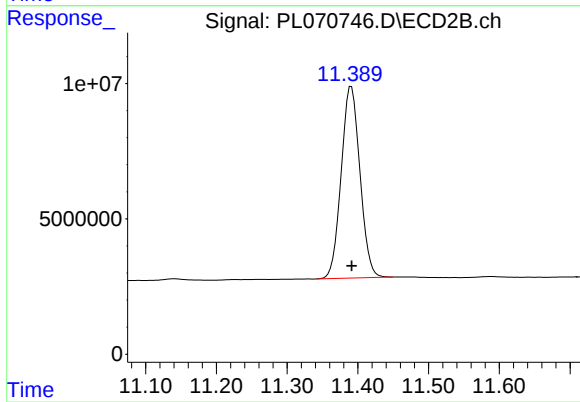

#28 Decachlorobiphenyl

R.T.: 11.391 min
Delta R.T.: 0.000 min
Response: 130450050
Conc: 94.82 ng/ml