

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110323\
 Data File : PL086409.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2023 18:26
 Operator : AR\AJ
 Sample : 05220-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 L-2(125FT)(0-5)

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/04/2023
 Supervised By : mohammad ahmed 11/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 21:43:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110123.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 02 05:32:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.351	2.619	20037802	7689116	6.314m	8.077 #
2) SA Decachlor...	8.851	7.768	31046512	11472045	11.739	10.001

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110323\
Data File : PL086409.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2023 18:26
Operator : AR\AJ
Sample : 05220-07
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
L-2(125FT)(0-5)


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/04/2023
Supervised By : mohammad ahmed 11/06/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 21:43:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110123.M
Quant Title : GC Extractables
QLast Update : Thu Nov 02 05:32:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

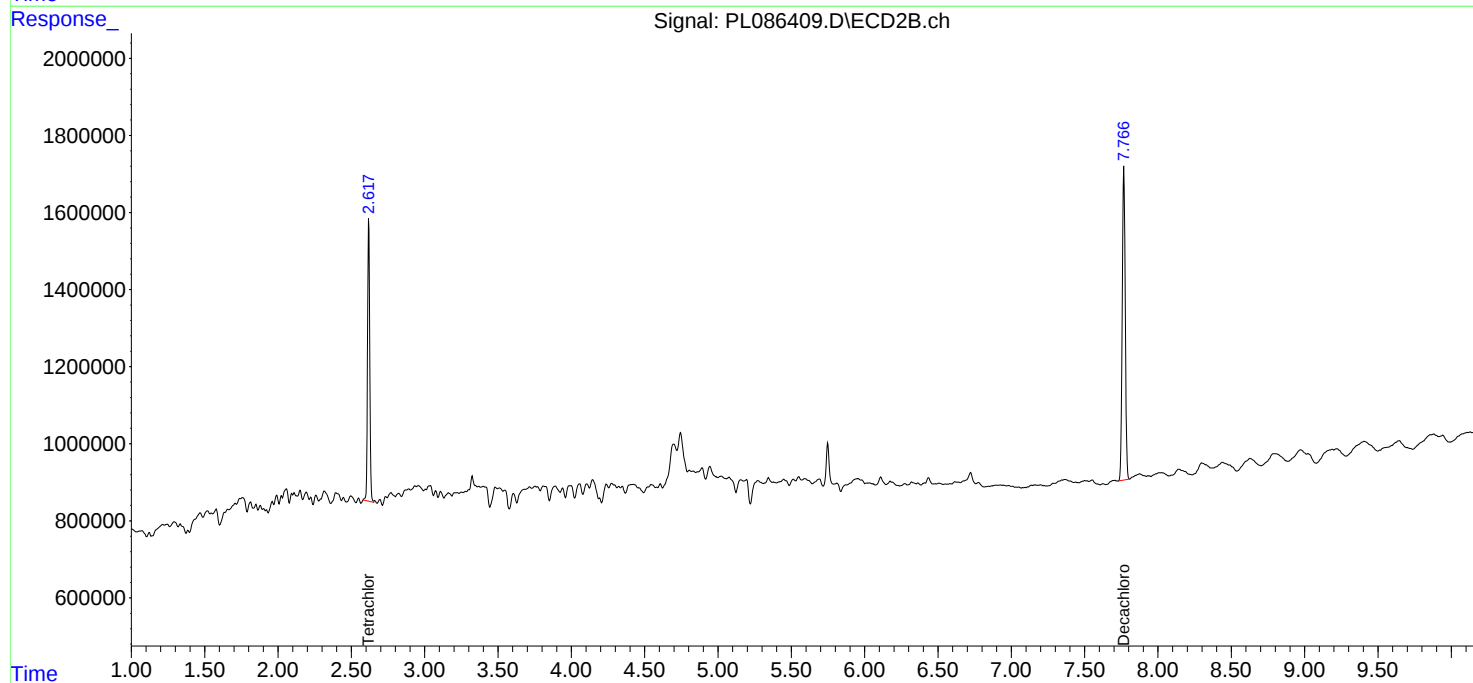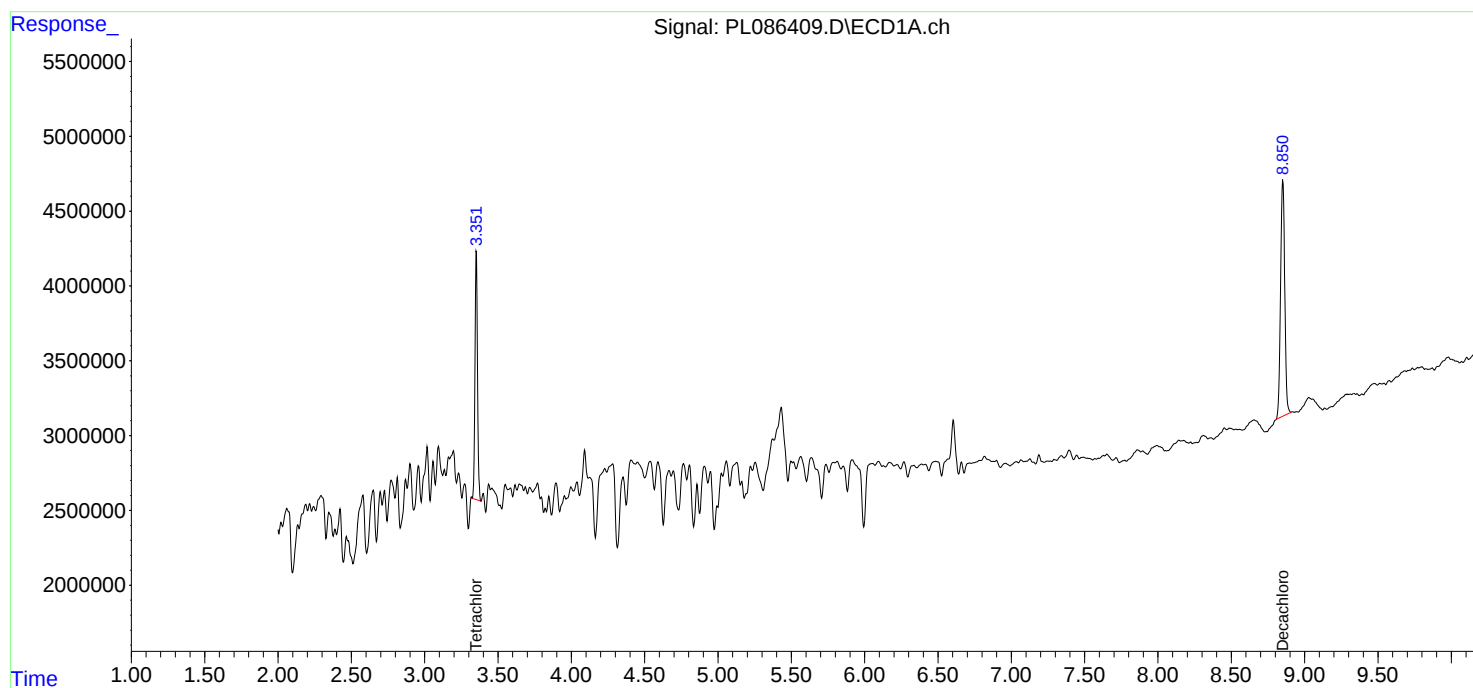

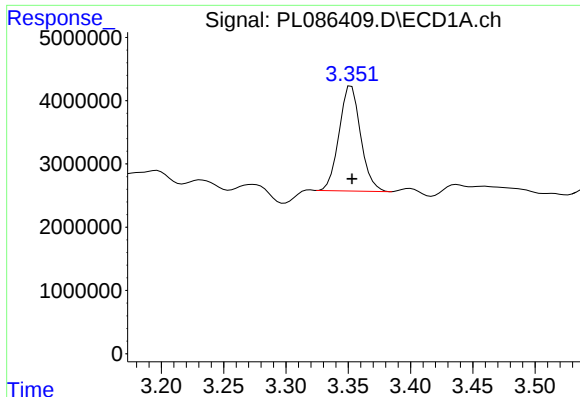


#1 Tetrachloro-m-xylene

R.T.: 3.351 min
Delta R.T.: -0.002 min
Response: 20037802
Conc: 6.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
L-2(125FT)(0-5)


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/04/2023
Supervised By :mohammad ahmed 11/06/2023

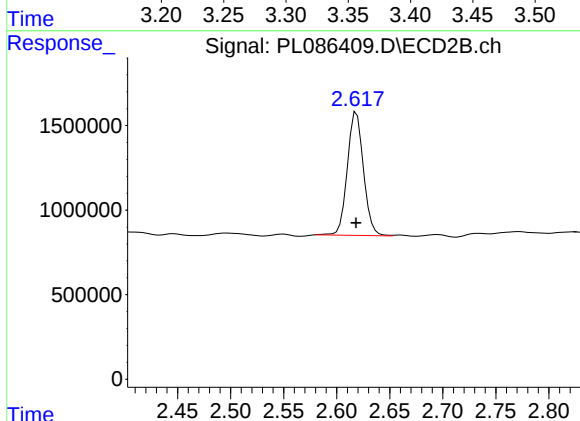


#1 Tetrachloro-m-xylene

R.T.: 2.619 min
Delta R.T.: 0.000 min
Response: 7689116
Conc: 8.08 ng/ml

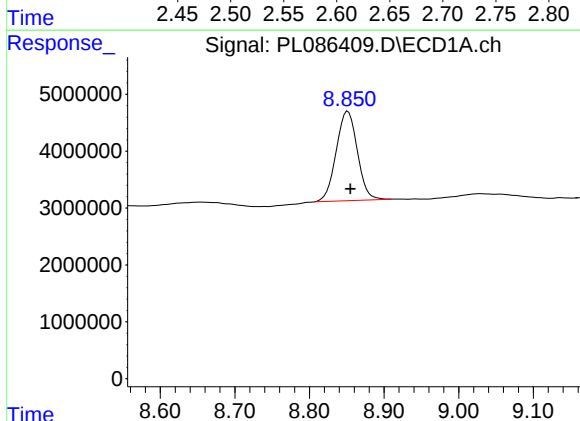

#28 Decachlorobiphenyl

R.T.: 8.851 min
Delta R.T.: -0.004 min
Response: 31046512
Conc: 11.74 ng/ml

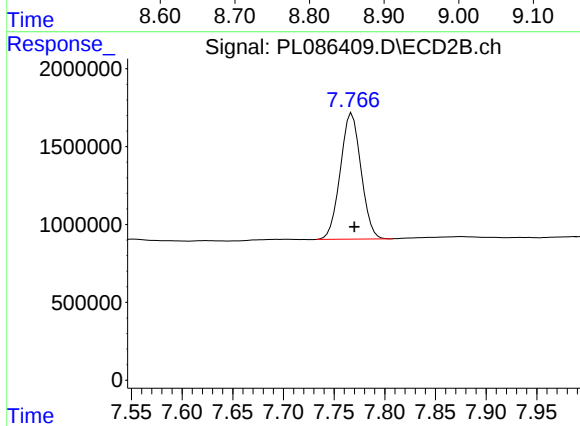

#28 Decachlorobiphenyl

R.T.: 7.768 min
Delta R.T.: -0.002 min
Response: 11472045
Conc: 10.00 ng/ml