

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110419\
 Data File : PL054009.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Nov 2019 09:07
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 00:09:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	4.043	264.1E6	58297506	24.361	23.297
28)	SA Decachlor...	8.326	9.121	206.1E6	60214376	21.001	21.383
Target Compounds							
18)	B Endrin al...	0.000	7.061f	0	1044917	N.D.	0.476 #
27)	Chlordane-5	0.000	7.061f	0	1044917	N.D.	13.668 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110419\
Data File : PL054009.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Nov 2019 09:07
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 00:09:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

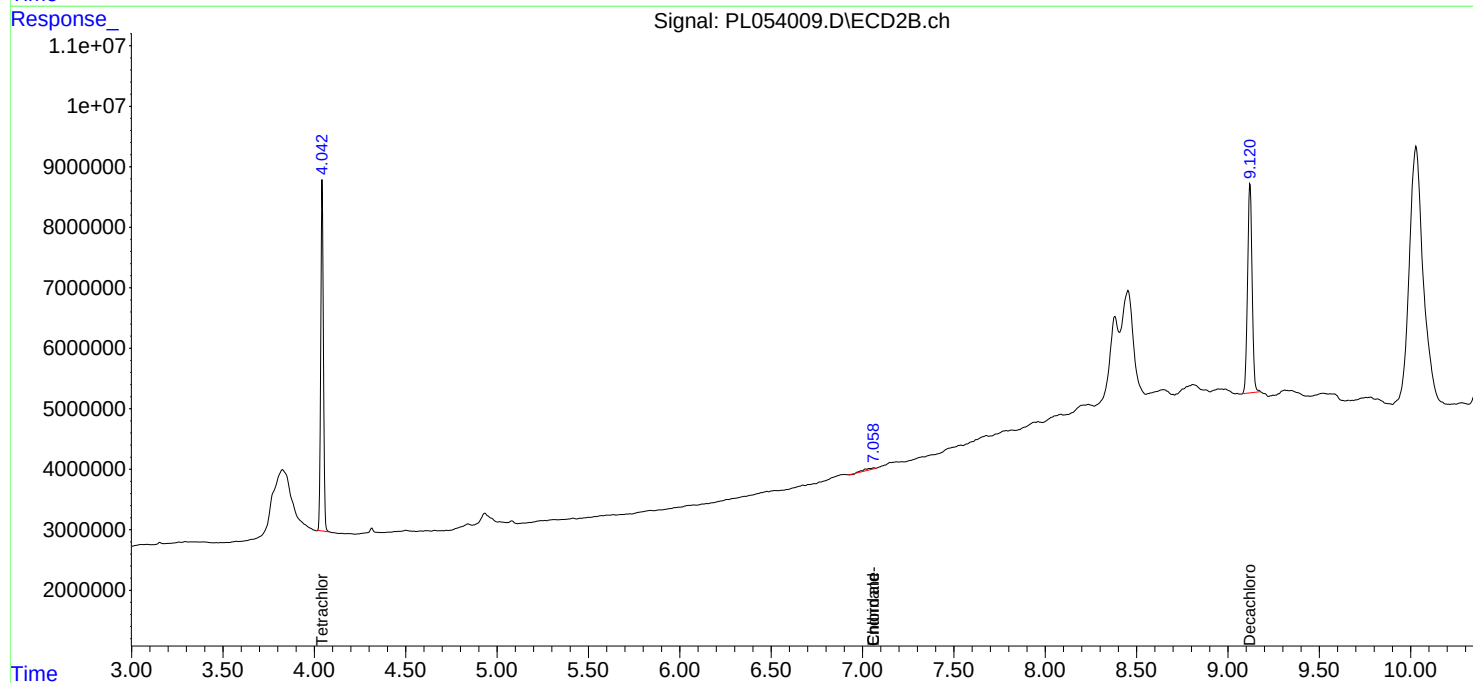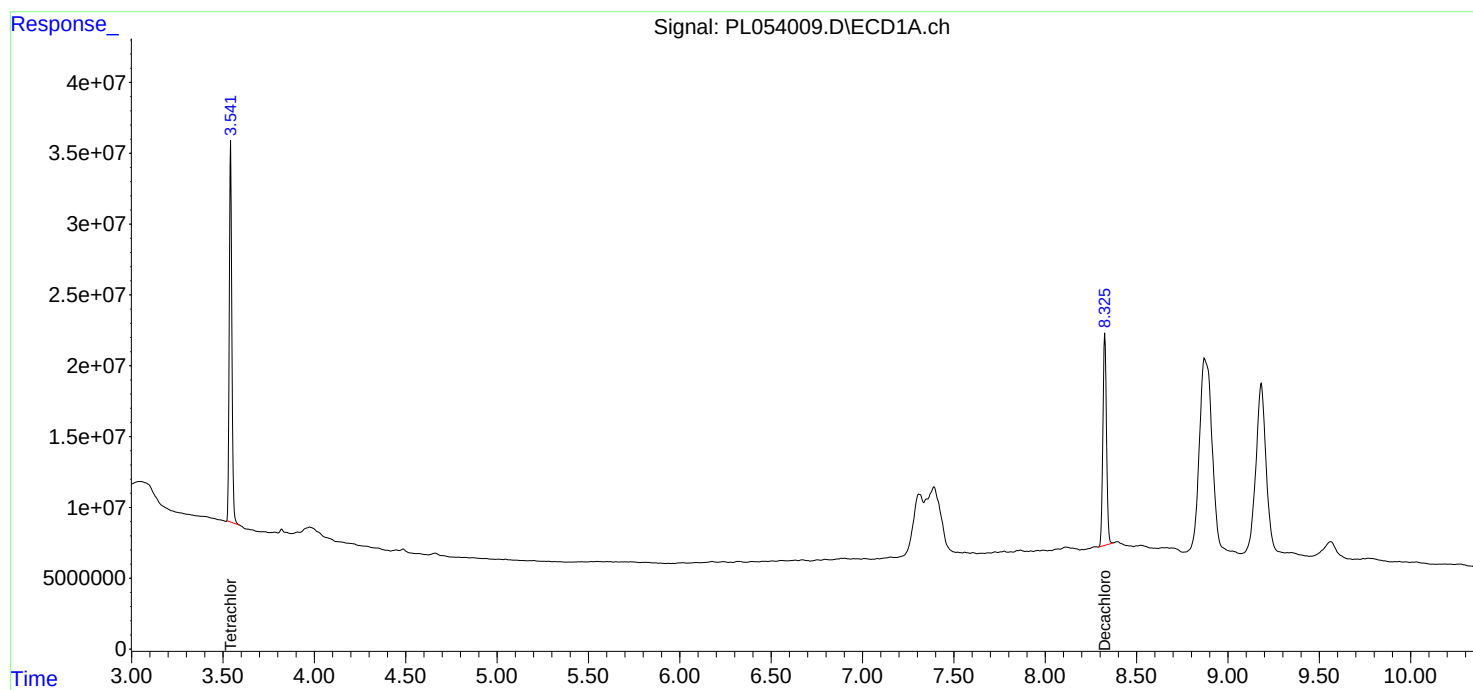


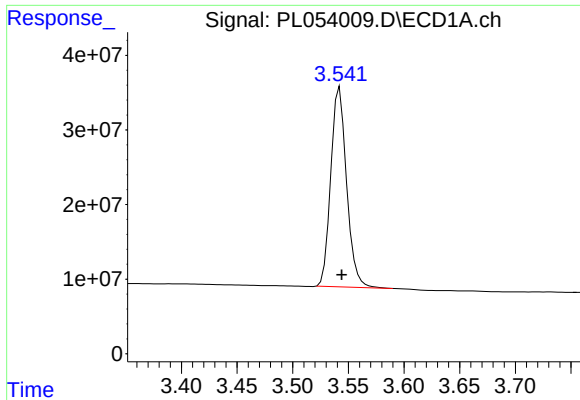

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: -0.002 min
Response: 264060626
Conc: 24.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

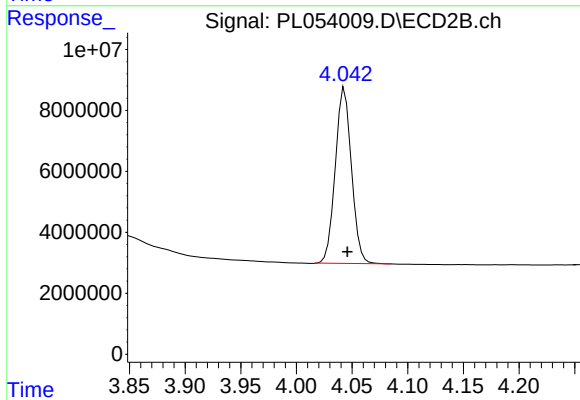


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: -0.003 min
Response: 58297506
Conc: 23.30 ng/ml

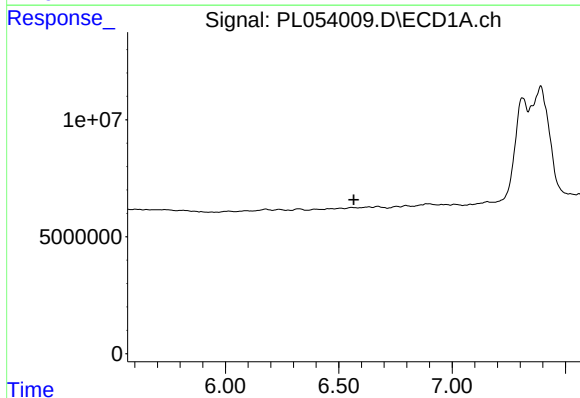


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.567 min
Response: 0
Conc: N.D.

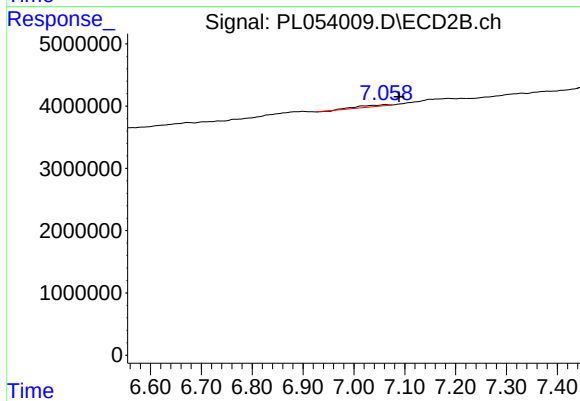

#18 Endrin aldehyde


R.T.: 7.061 min
Delta R.T.: -0.028 min
Response: 1044917
Conc: 0.48 ng/ml

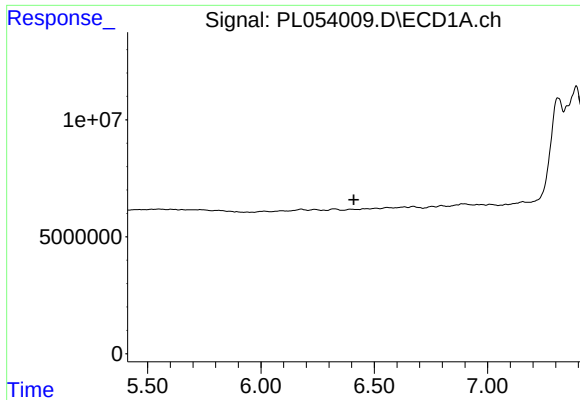

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.409 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

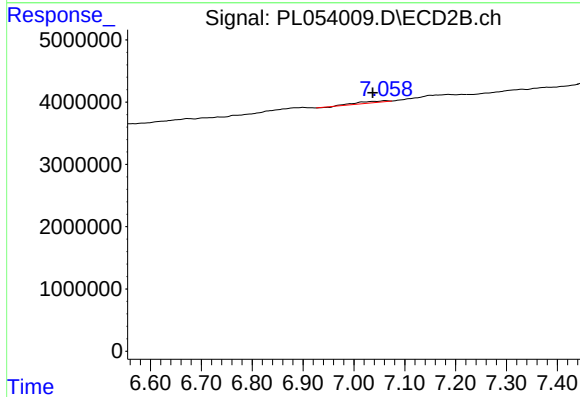


#27 Chlordane-5

R.T.: 7.061 min
Delta R.T.: 0.024 min
Response: 1044917
Conc: 13.67 ng/ml

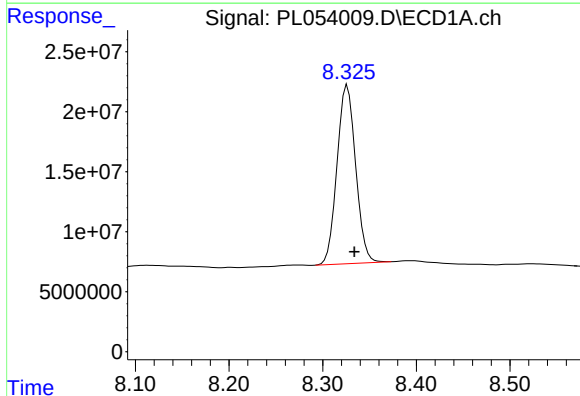

#28 Decachlorobiphenyl

R.T.: 8.326 min
Delta R.T.: -0.008 min
Response: 206055086
Conc: 21.00 ng/ml

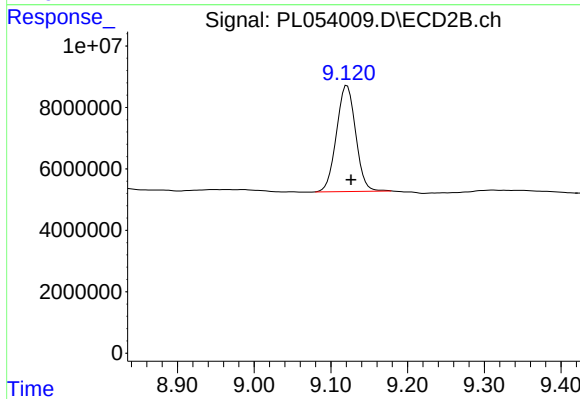

#28 Decachlorobiphenyl

R.T.: 9.121 min
Delta R.T.: -0.005 min
Response: 60214376
Conc: 21.38 ng/ml