

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110419\
 Data File : PL054016.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Nov 2019 14:05
 Operator : SG\AJ
 Sample : K5658-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-30-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 00:10:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	4.043	228.9E6	52134917	21.117	20.834
28)	SA Decachlor...	8.325	9.120	194.0E6	54055934	19.771	19.196
Target Compounds							
15)	B Endosulfa...	0.000	6.973	0	3434308	N.D.	1.344 #
16)	A 4,4'-DDD	6.243	0.000	3205081	0	0.360	N.D. #
17)	MA 4,4'-DDT	0.000	7.146f	0	5467323	N.D.	2.364 #
23)	Chlordane-1	4.444f	0.000	9487475	0	26.750	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110419\
Data File : PL054016.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Nov 2019 14:05
Operator : SG\AJ
Sample : K5658-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-30-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 00:10:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

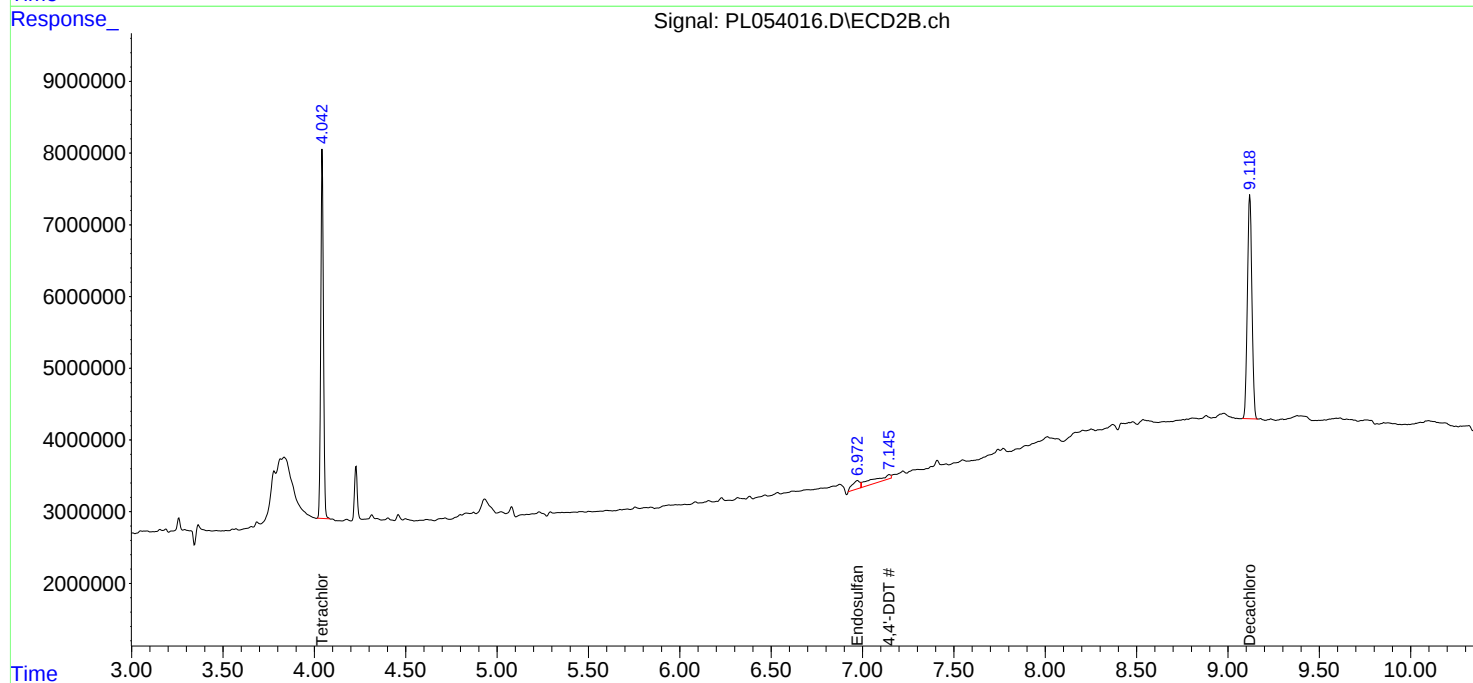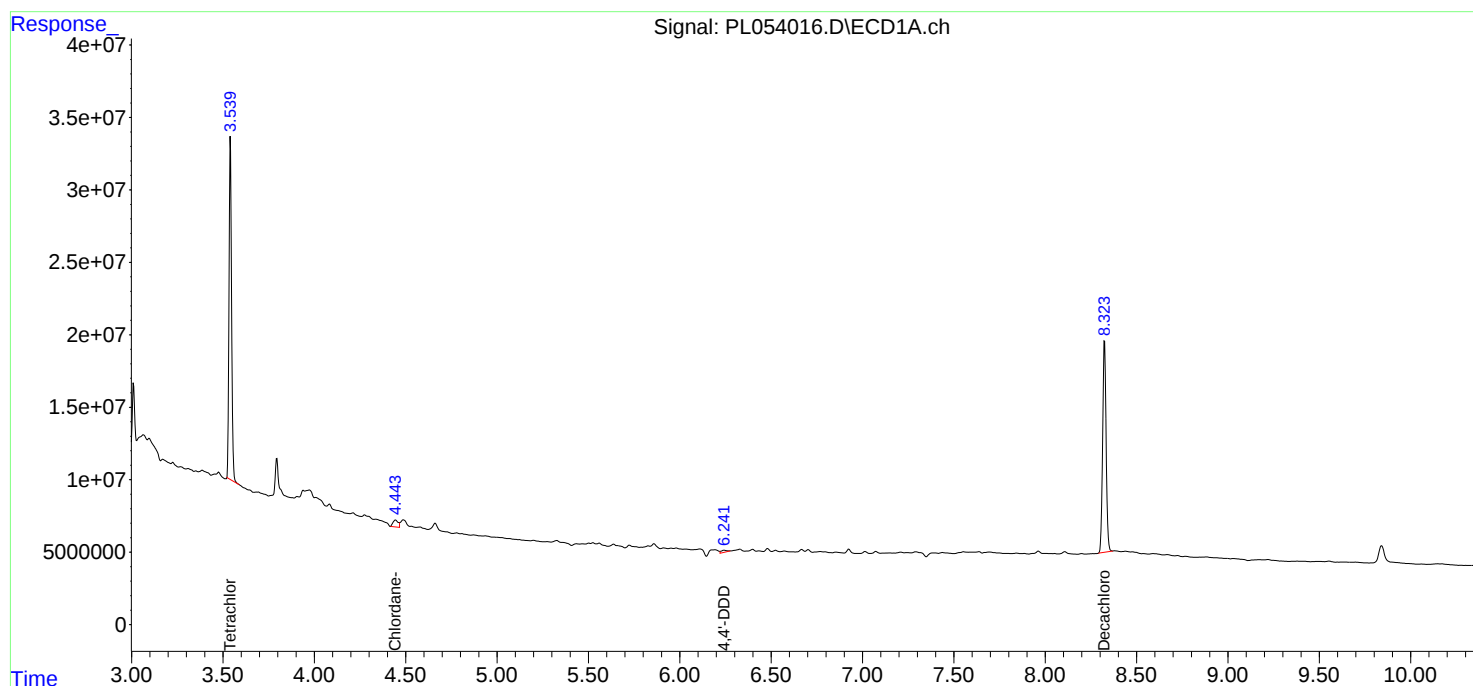


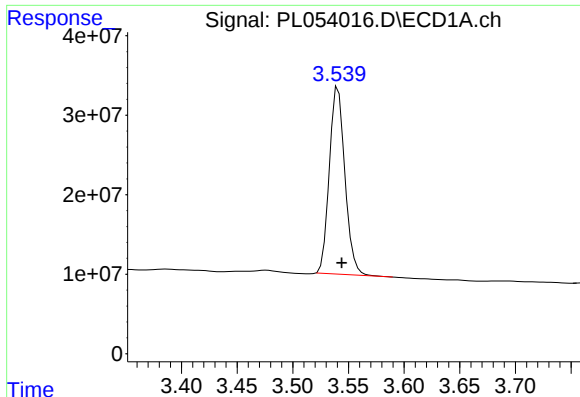

#1 Tetrachloro-m-xylene


R.T.: 3.541 min
Delta R.T.: -0.003 min
Response: 228895906
Conc: 21.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-30-S

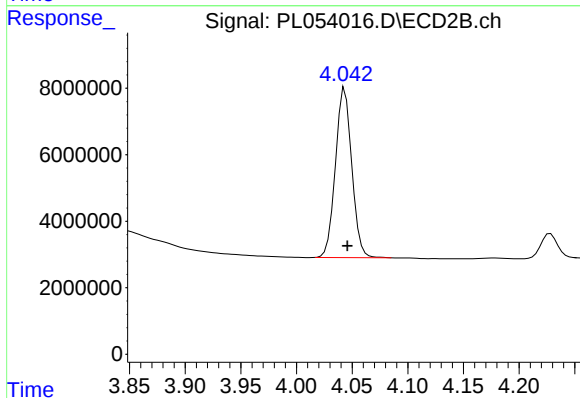


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: -0.002 min
Response: 52134917
Conc: 20.83 ng/ml

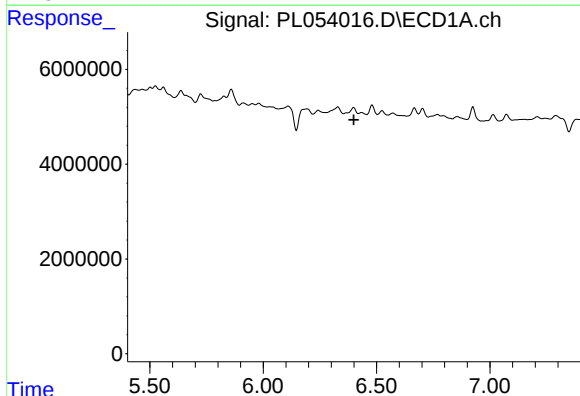


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.399 min
Response: 0
Conc: N.D.

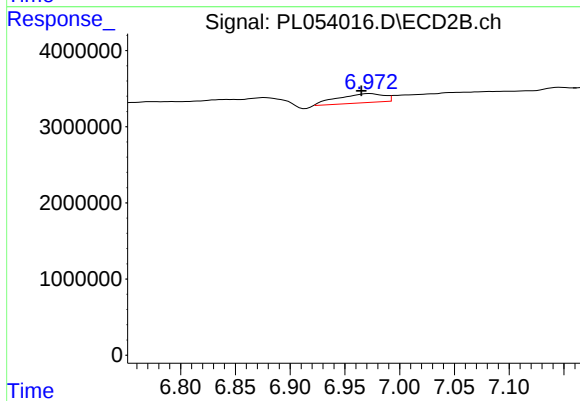

#15 Endosulfan II


R.T.: 6.973 min
Delta R.T.: 0.008 min
Response: 3434308
Conc: 1.34 ng/ml

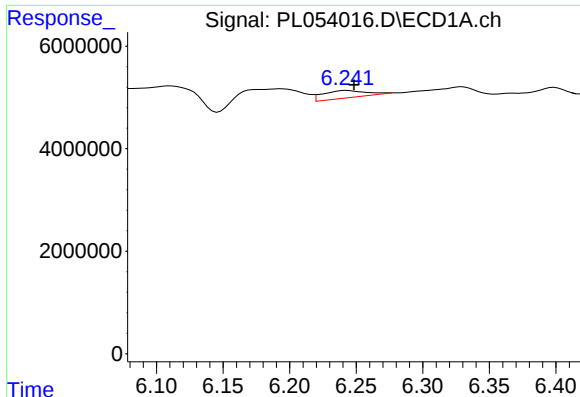

#16 4,4'-DDD


R.T.: 6.243 min
Delta R.T.: -0.006 min
Response: 3205081
Conc: 0.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-30-S

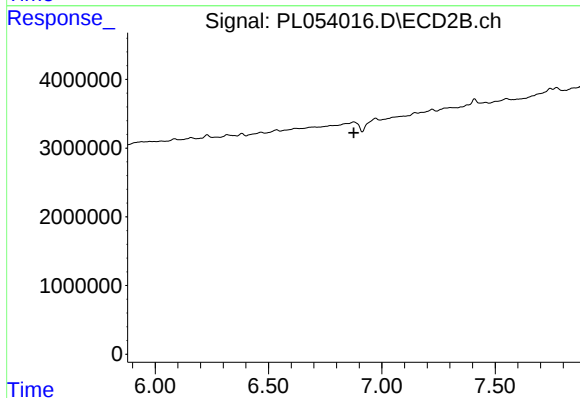


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.877 min
Response: 0
Conc: N.D.

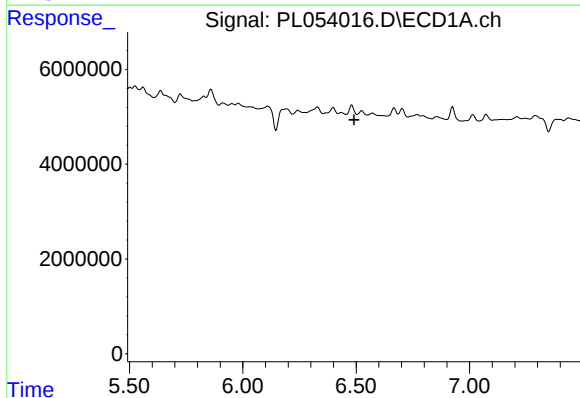


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.491 min
Response: 0
Conc: N.D.

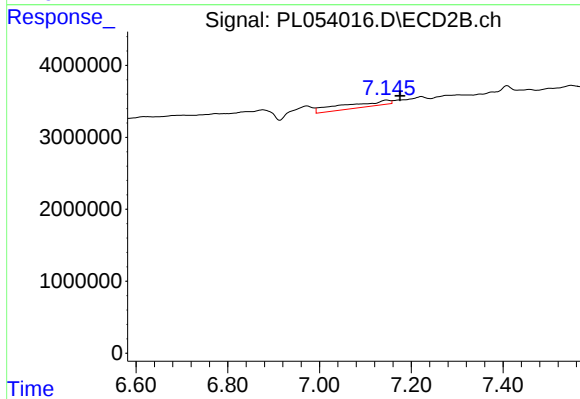

#17 4,4'-DDT


R.T.: 7.146 min
Delta R.T.: -0.029 min
Response: 5467323
Conc: 2.36 ng/ml

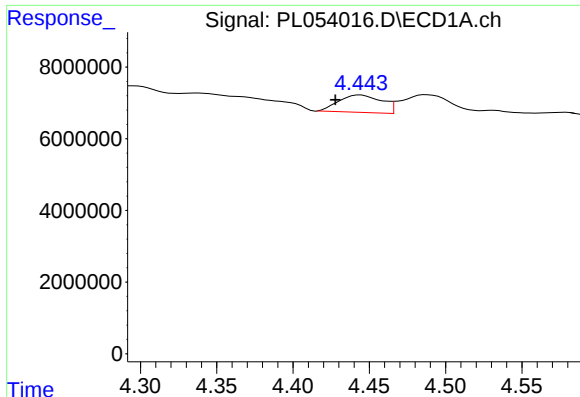

#23 Chlordane-1


R.T.: 4.444 min
Delta R.T.: 0.016 min
Response: 9487475
Conc: 26.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-30-S

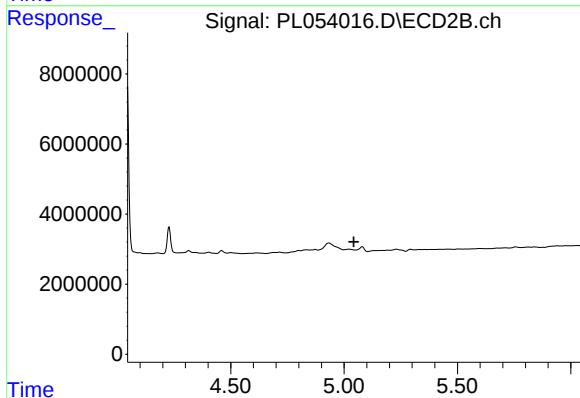


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.043 min
Response: 0
Conc: N.D.

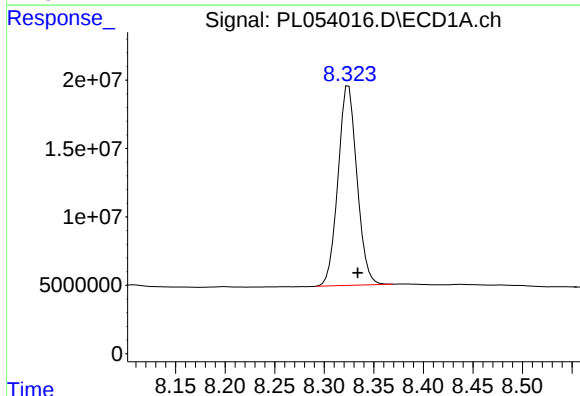

#28 Decachlorobiphenyl

R.T.: 8.325 min
Delta R.T.: -0.009 min
Response: 193987861
Conc: 19.77 ng/ml

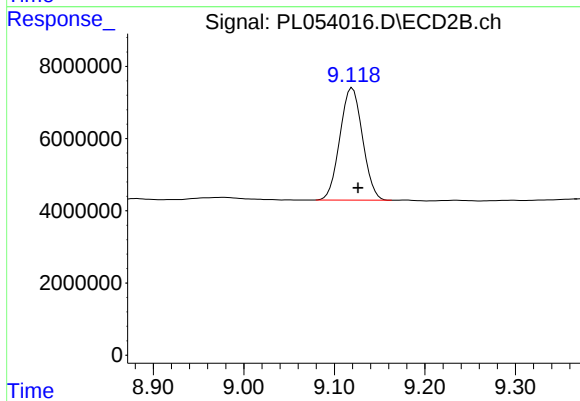

#28 Decachlorobiphenyl

R.T.: 9.120 min
Delta R.T.: -0.006 min
Response: 54055934
Conc: 19.20 ng/ml