

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110420\
 Data File : PL062826.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Nov 2020 16:19
 Operator : DD\AJ
 Sample : L4621-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 00:21:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.410	3.949	21332132	36949484	12.402	12.573
28)	SA Decachlor...	8.123	8.986	21638425	27731737	13.488	13.250
Target Compounds							
5)	MB Aldrin	4.653	5.416	1427136	1641401	0.748	0.453 #
6)	B beta-BHC	0.000	4.814f	0	3575878	N.D.	1.899 #
8)	B Heptachlo...	0.000	5.823	0	7855894	N.D.	2.426 #
9)	A Endosulfan I	5.450	6.162	2620030	3433863	1.567	1.089 #
10)	B gamma-Chl...	0.000	6.057	0	16074393	N.D.	4.775 #
23)	Chlordane-1	4.268	4.916f	3013687	564247	58.462	5.621 #
24)	Chlordane-2	0.000	5.416	0	1641401	N.D.	15.054 #
25)	Chlordane-3	0.000	6.057	0	16074393	N.D.	39.794 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110420\
Data File : PL062826.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Nov 2020 16:19
Operator : DD\AJ
Sample : L4621-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 00:21:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

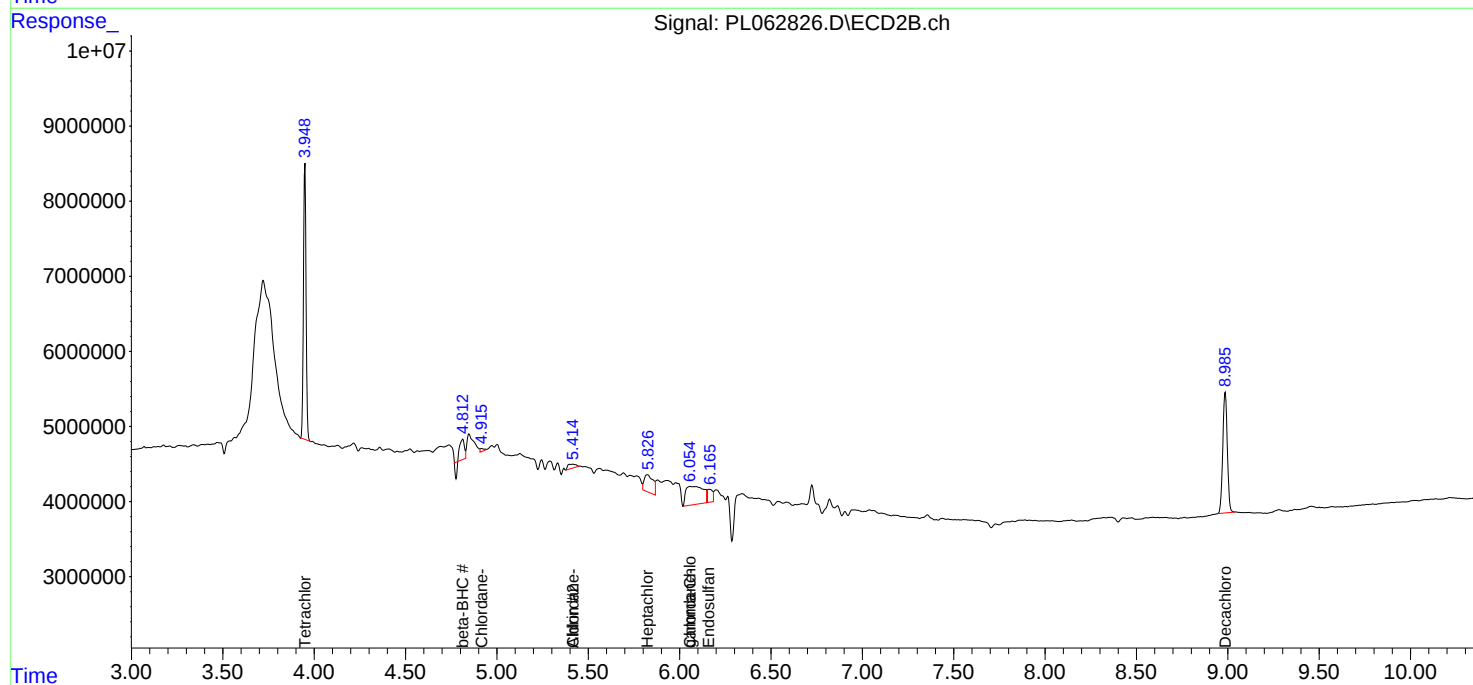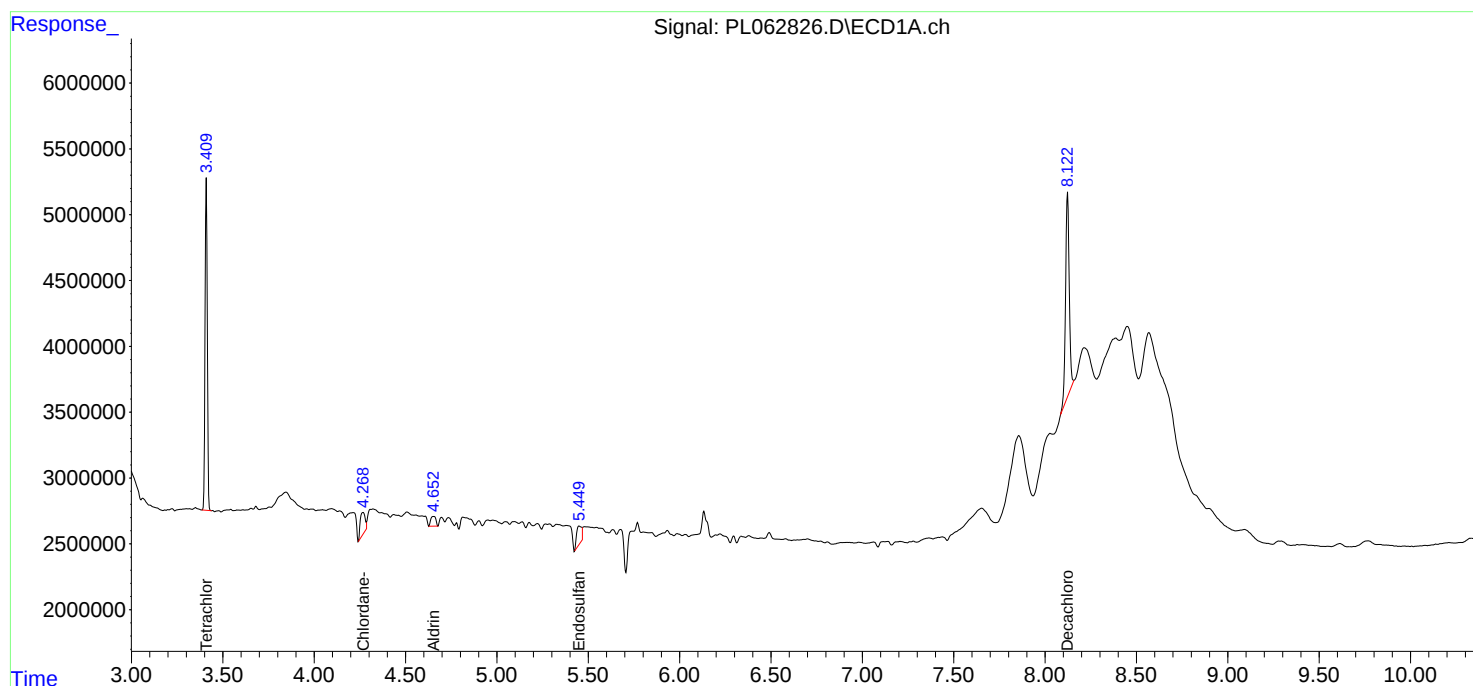


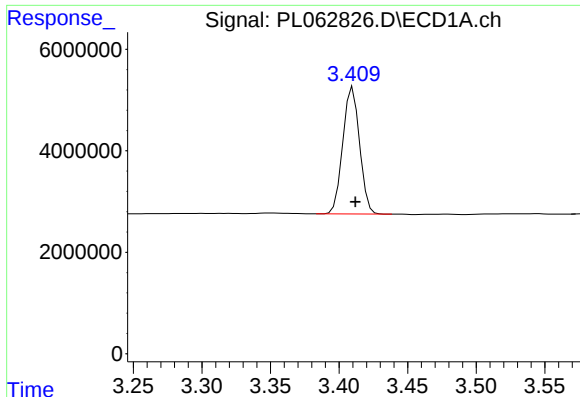

#1 Tetrachloro-m-xylene


R.T.: 3.410 min
Delta R.T.: -0.002 min
Response: 21332132
Conc: 12.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

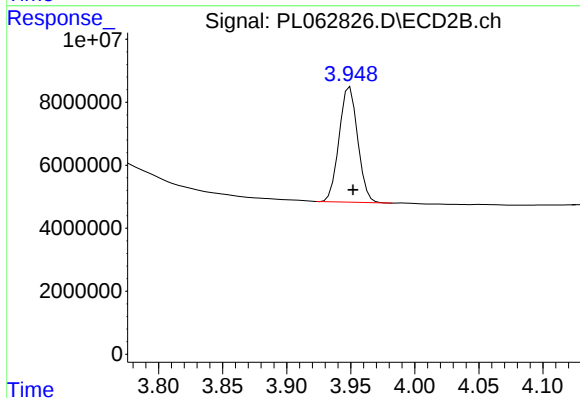


#1 Tetrachloro-m-xylene

R.T.: 3.949 min
Delta R.T.: -0.002 min
Response: 36949484
Conc: 12.57 ng/ml

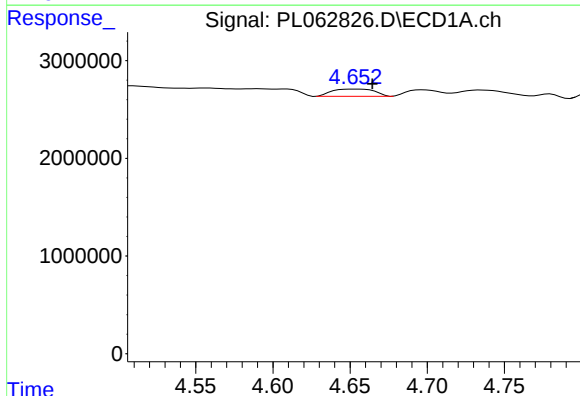


#5 Aldrin

R.T.: 4.653 min
Delta R.T.: -0.011 min
Response: 1427136
Conc: 0.75 ng/ml

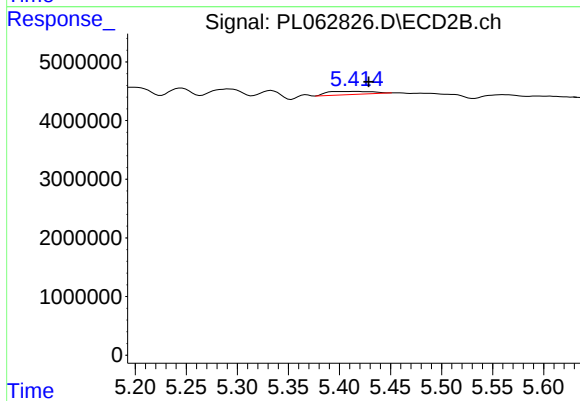

#5 Aldrin


R.T.: 5.416 min
Delta R.T.: -0.013 min
Response: 1641401
Conc: 0.45 ng/ml

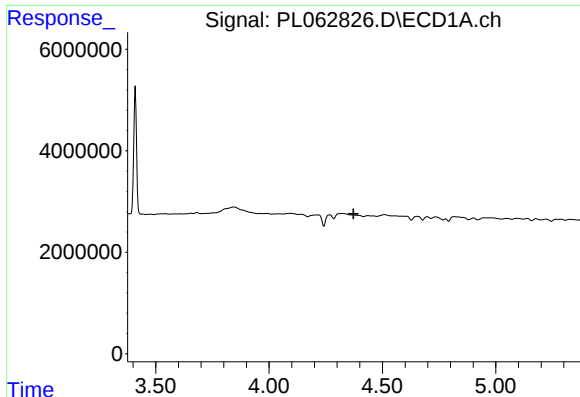

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

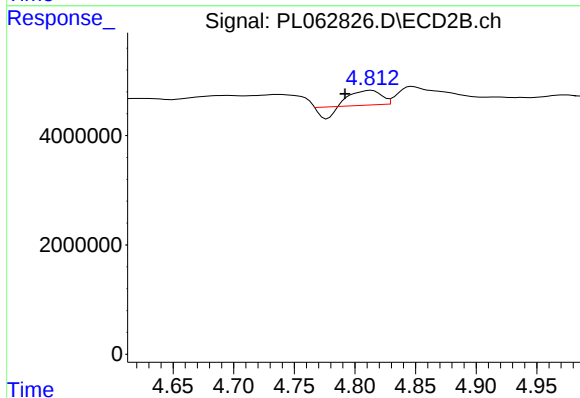


#6 beta-BHC

R.T.: 4.814 min
Delta R.T.: 0.022 min
Response: 3575878
Conc: 1.90 ng/ml

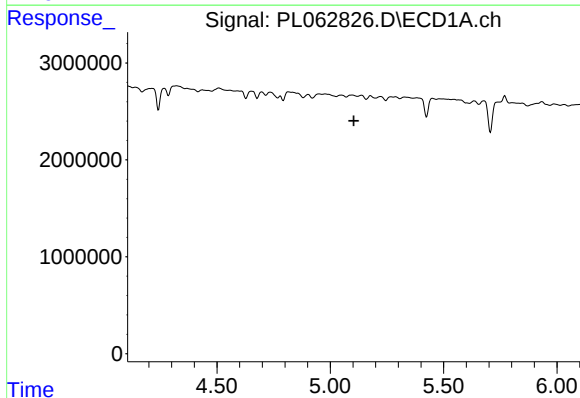


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.103 min
Response: 0
Conc: N.D.

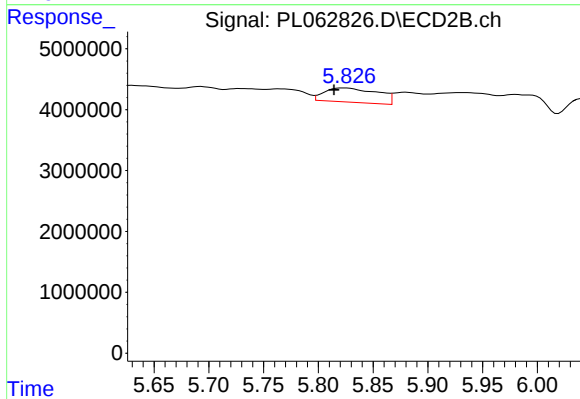

#8 Heptachlor epoxide


R.T.: 5.823 min
Delta R.T.: 0.009 min
Response: 7855894
Conc: 2.43 ng/ml

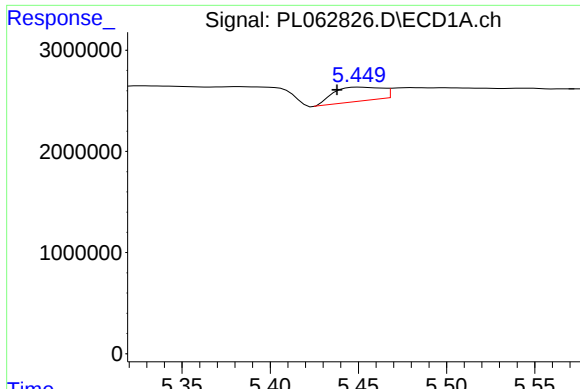

#9 Endosulfan I


R.T.: 5.450 min
Delta R.T.: 0.012 min
Response: 2620030
Conc: 1.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

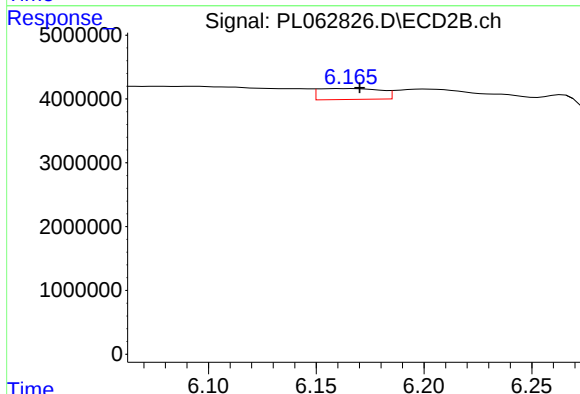


#9 Endosulfan I

R.T.: 6.162 min
Delta R.T.: -0.008 min
Response: 3433863
Conc: 1.09 ng/ml

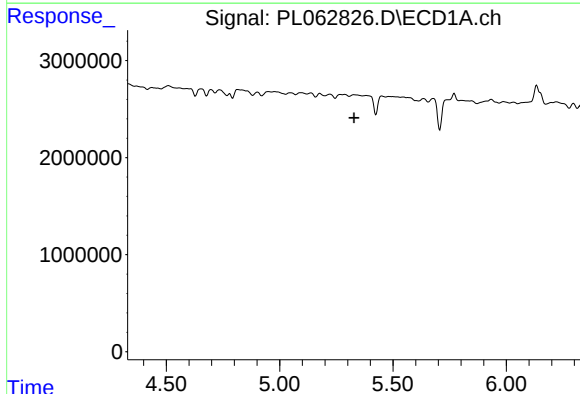


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.328 min
Response: 0
Conc: N.D.

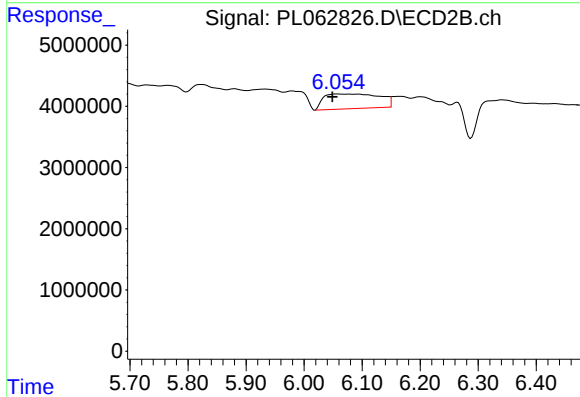

#10 gamma-Chlordane


R.T.: 6.057 min
Delta R.T.: 0.008 min
Response: 16074393
Conc: 4.78 ng/ml

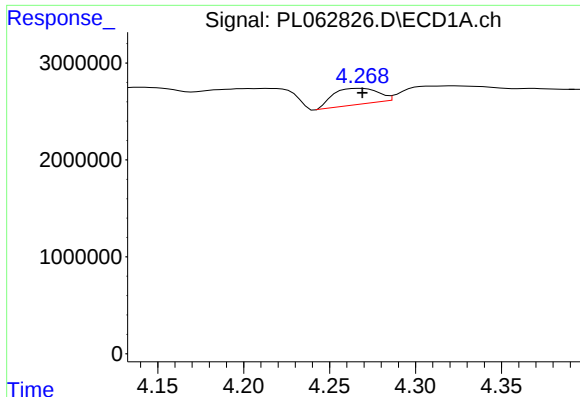

#23 Chlordane-1


R.T.: 4.268 min
Delta R.T.: -0.001 min
Response: 3013687
Conc: 58.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

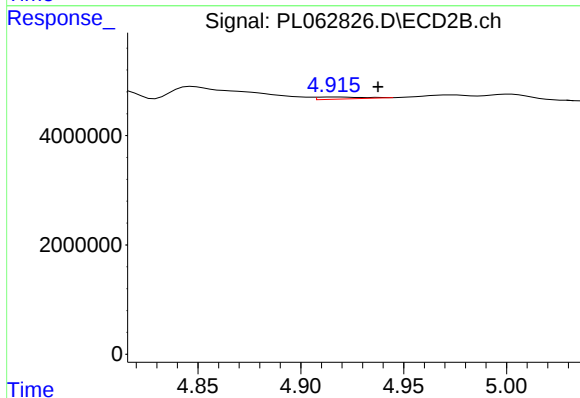


#23 Chlordane-1

R.T.: 4.916 min
Delta R.T.: -0.021 min
Response: 564247
Conc: 5.62 ng/ml

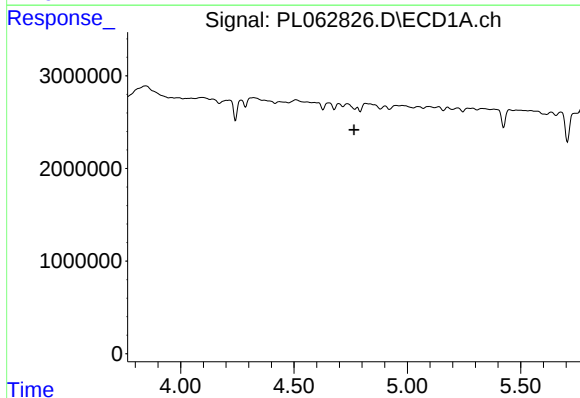


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.765 min
Response: 0
Conc: N.D.

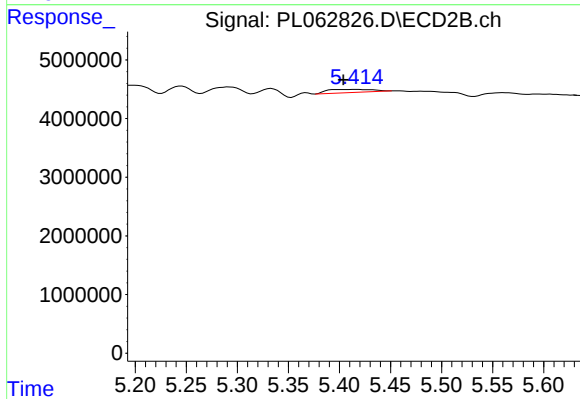

#24 Chlordane-2


R.T.: 5.416 min
Delta R.T.: 0.012 min
Response: 1641401
Conc: 15.05 ng/ml

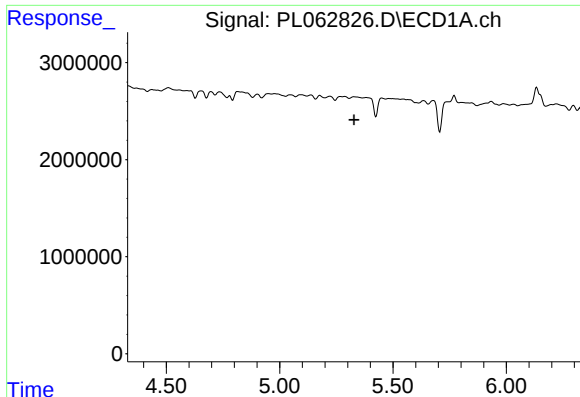

#25 Chloroform-3


R.T.: 0.000 min
Exp R.T.: 5.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

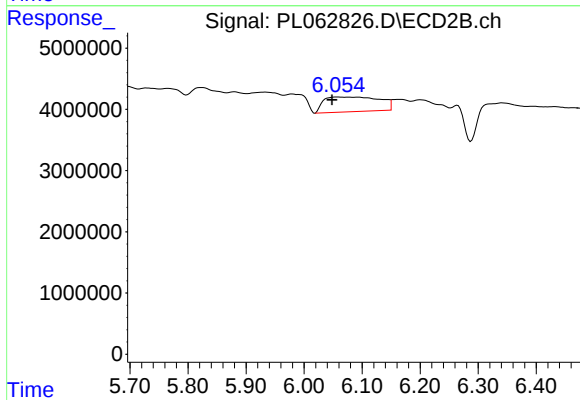


#25 Chloroform-3

R.T.: 6.057 min
Delta R.T.: 0.008 min
Response: 16074393
Conc: 39.79 ng/ml

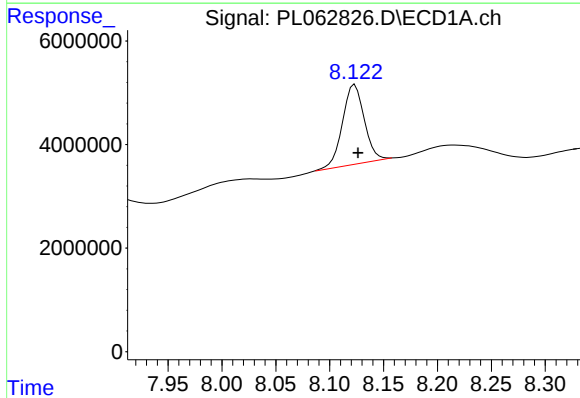

#28 Decachlorobiphenyl

R.T.: 8.123 min
Delta R.T.: -0.003 min
Response: 21638425
Conc: 13.49 ng/ml

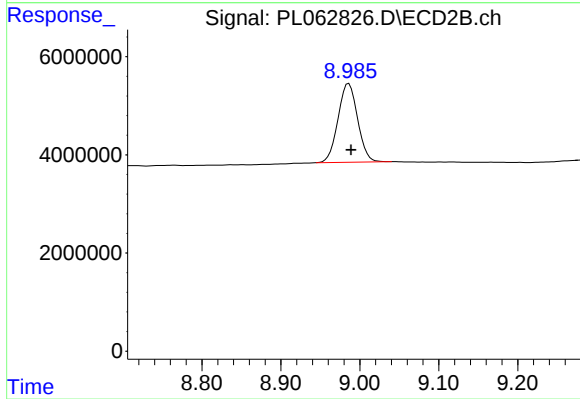

#28 Decachlorobiphenyl

R.T.: 8.986 min
Delta R.T.: -0.003 min
Response: 27731737
Conc: 13.25 ng/ml