

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110420\
 Data File : PL062817.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Nov 2020 13:57
 Operator : DD\AJ
 Sample : L4596-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-05-110320

Manual Integrations
 APPROVED

Ankita
 11/5/2020 1:25:10 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 00:19:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.411	3.949	25600842	40703717	14.884	13.851
2) SA Decachlor...	8.124	8.987	21807440	27650971	13.593	13.211
Target Compounds						
10) B gamma-Chl...	5.326	6.044	4070737	6952893	2.260m	2.065m
11) B alpha-Chl...	5.382	6.119	6829262	16871127	3.778m	5.008 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110420\
Data File : PL062817.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Nov 2020 13:57
Operator : DD\AJ
Sample : L4596-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TR-05-110320


Manual Integrations
APPROVED

Ankita
11/5/2020 1:25:10 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 00:19:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

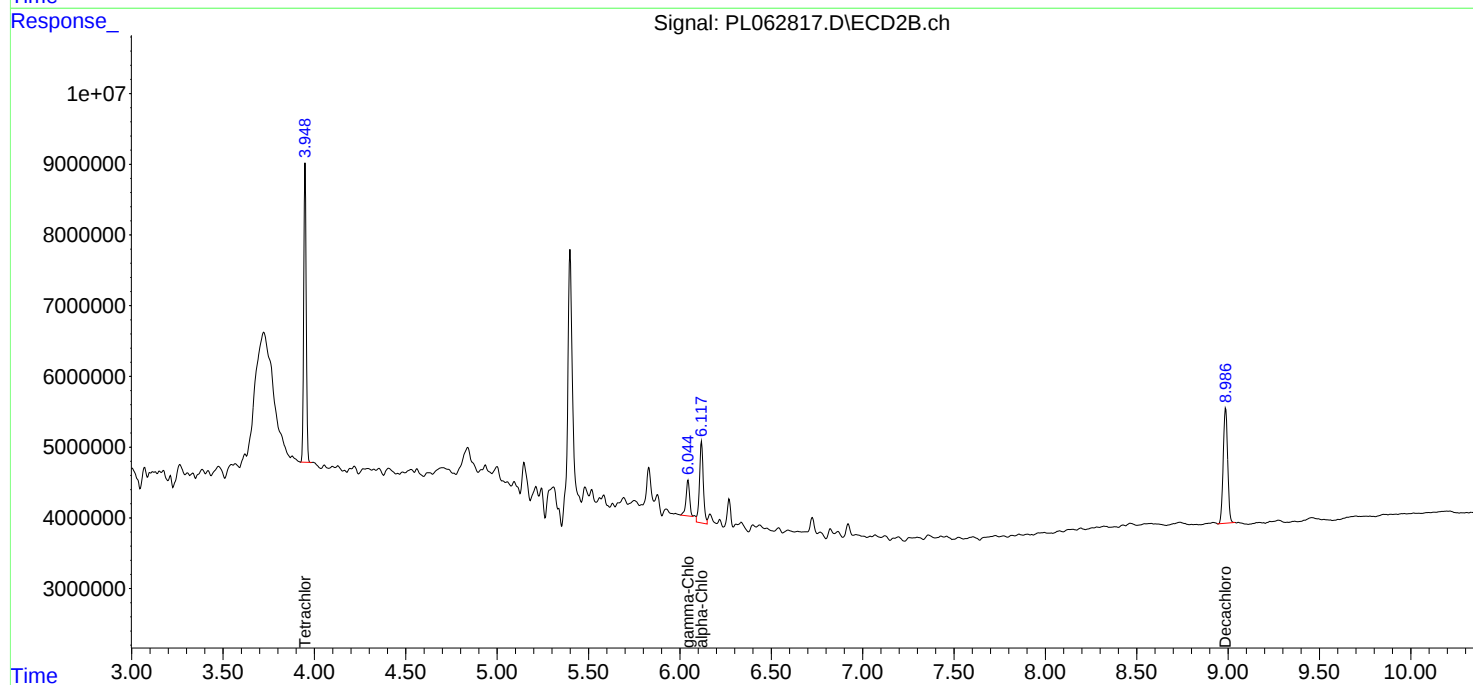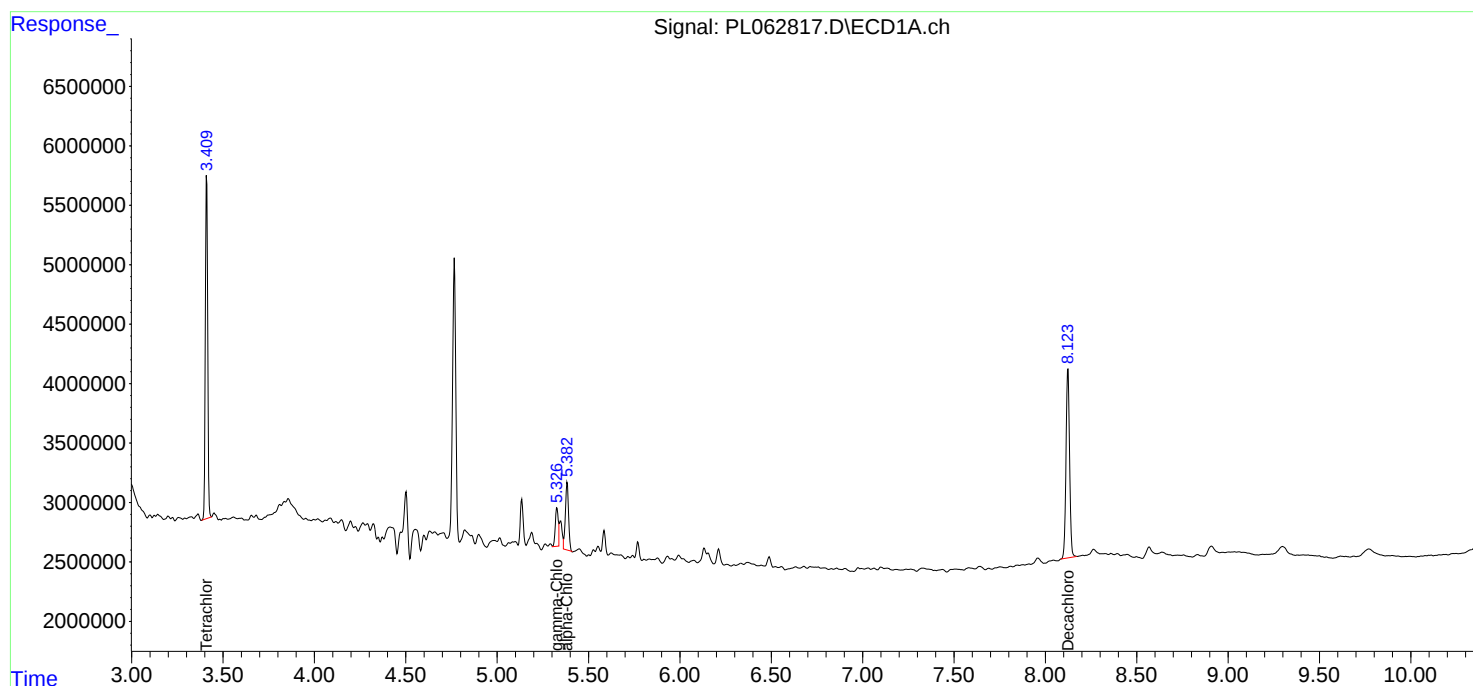

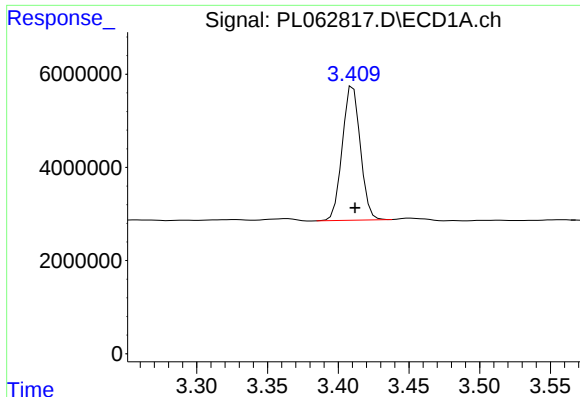


#1 Tetrachloro-m-xylene

R.T.: 3.411 min
Delta R.T.: -0.001 min
Response: 25600842
Conc: 14.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-110320


Manual Integrations
APPROVED

Ankita
11/5/2020 1:25:10 PM

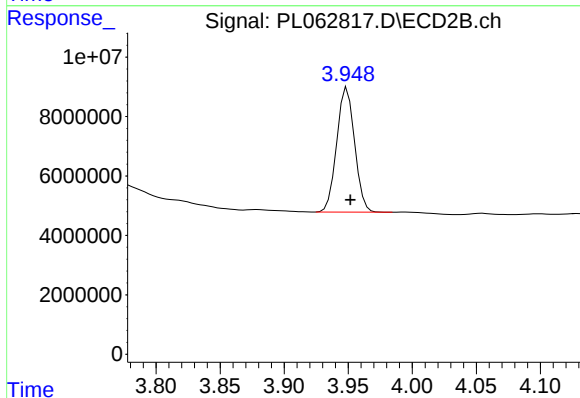


#1 Tetrachloro-m-xylene

R.T.: 3.949 min
Delta R.T.: -0.002 min
Response: 40703717
Conc: 13.85 ng/ml

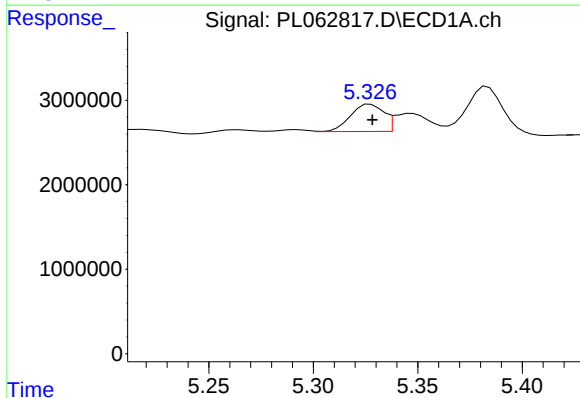


#10 gamma-Chlordane

R.T.: 5.326 min
Delta R.T.: -0.002 min
Response: 4070737
Conc: 2.26 ng/ml m

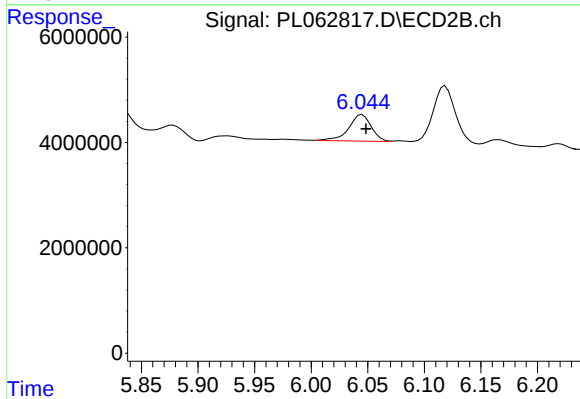

#10 gamma-Chlordane

R.T.: 6.044 min
Delta R.T.: -0.005 min
Response: 6952893
Conc: 2.07 ng/ml m

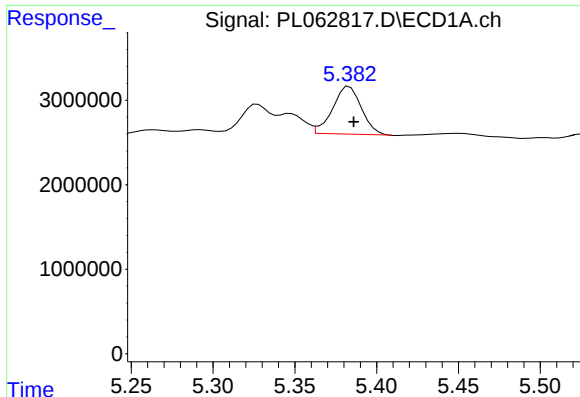


#11 alpha-Chlordane

R.T.: 5.382 min
Delta R.T.: -0.004 min
Response: 6829262
Conc: 3.78 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TR-05-110320


Manual Integrations
APPROVED

Ankita
11/5/2020 1:25:10 PM

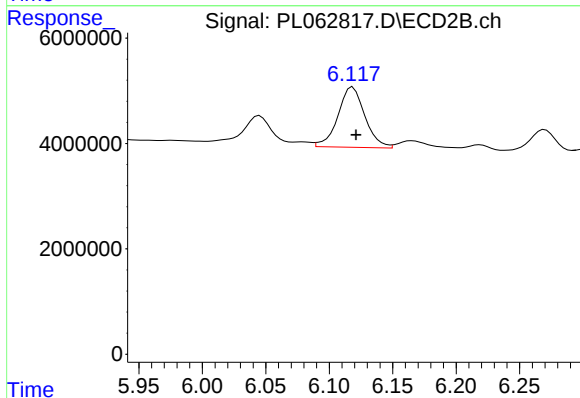


#11 alpha-Chlordane

R.T.: 6.119 min
Delta R.T.: -0.003 min
Response: 16871127
Conc: 5.01 ng/ml

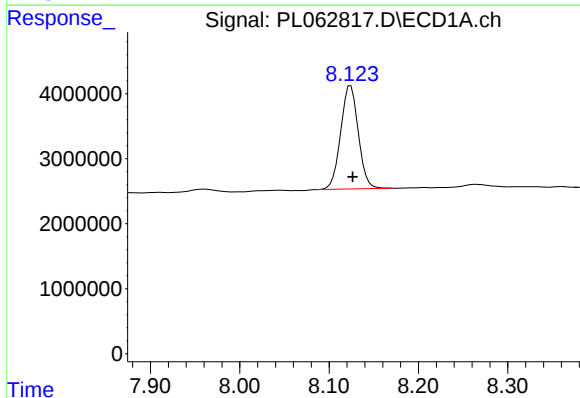

#28 Decachlorobiphenyl

R.T.: 8.124 min
Delta R.T.: -0.002 min
Response: 21807440
Conc: 13.59 ng/ml

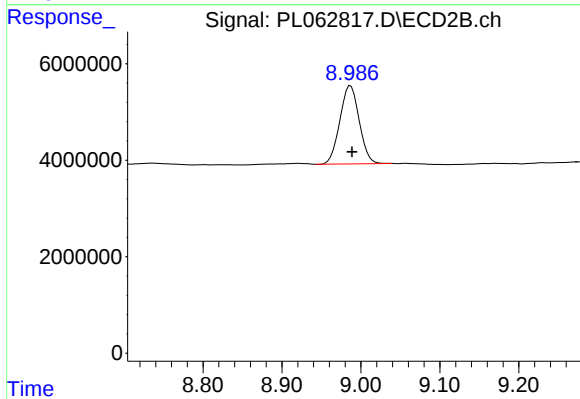

#28 Decachlorobiphenyl

R.T.: 8.987 min
Delta R.T.: -0.002 min
Response: 27650971
Conc: 13.21 ng/ml