

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110421\
 Data File : PL070766.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Nov 2021 12:18
 Operator : AR\AJ
 Sample : M4470-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 14:25:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 04 19:28:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.568	5.501	6188330	15858143	12.634	12.577
28)	SA Decachlor...	10.330	11.392	9822524	19460251	14.375	14.551
Target Compounds							
6)	B beta-BHC	0.000	6.730	0	1634409	N.D.	1.908 #
7)	B delta-BHC	0.000	7.025f	0	210611	N.D.	0.126 #
10)	B gamma-Chl...	0.000	8.258f	0	1250071	N.D.	0.807 #
14)	MA Endrin	0.000	8.893	0	457975	N.D.	0.395 #
16)	A 4,4'-DDD	0.000	9.035	0	776024	N.D.	0.645 #
17)	MA 4,4'-DDT	8.407	0.000	816905	0	1.485	N.D. #
21)	B Endrin ke...	0.000	10.018f	0	750157	N.D.	0.523 #
25)	Chlordane-3	0.000	8.258f	0	1250071	N.D.	6.185 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110421\
Data File : PL070766.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Nov 2021 12:18
Operator : AR\AJ
Sample : M4470-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 14:25:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
Quant Title : GC Extractables
QLast Update : Thu Nov 04 19:28:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

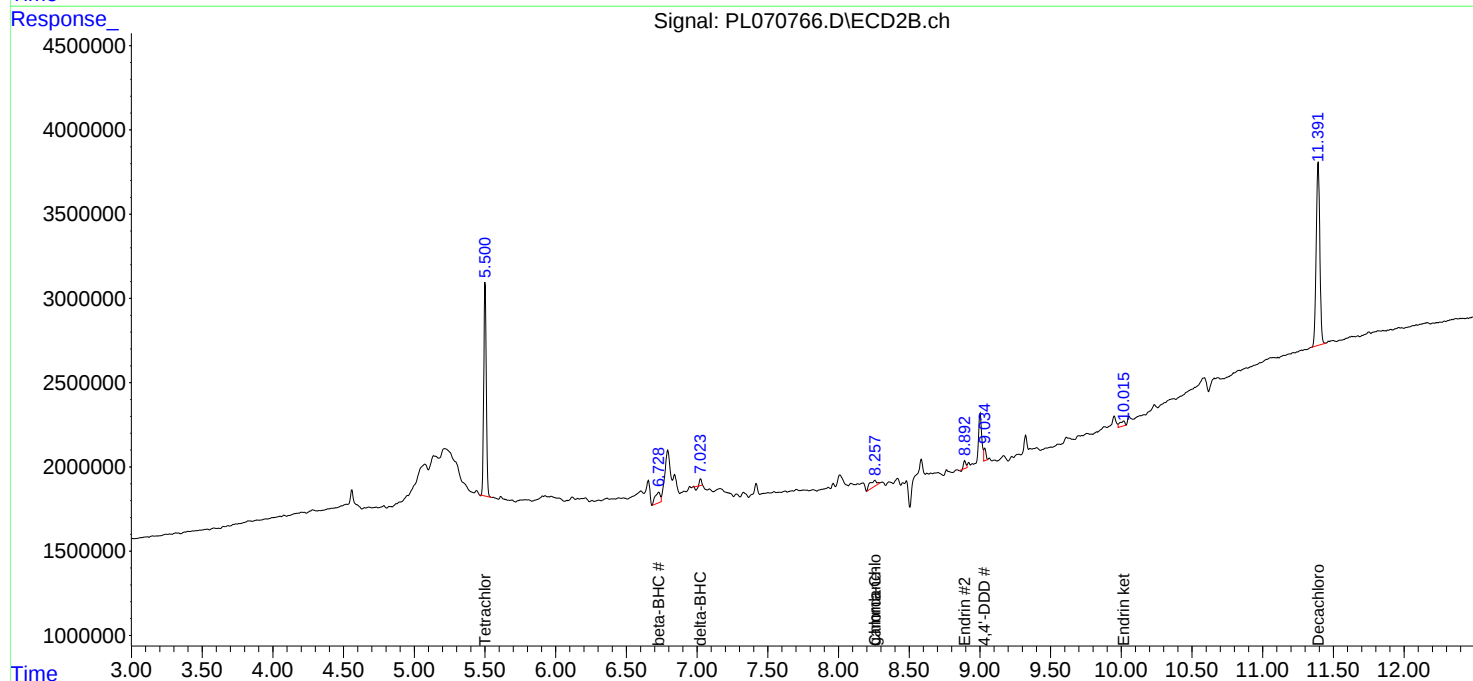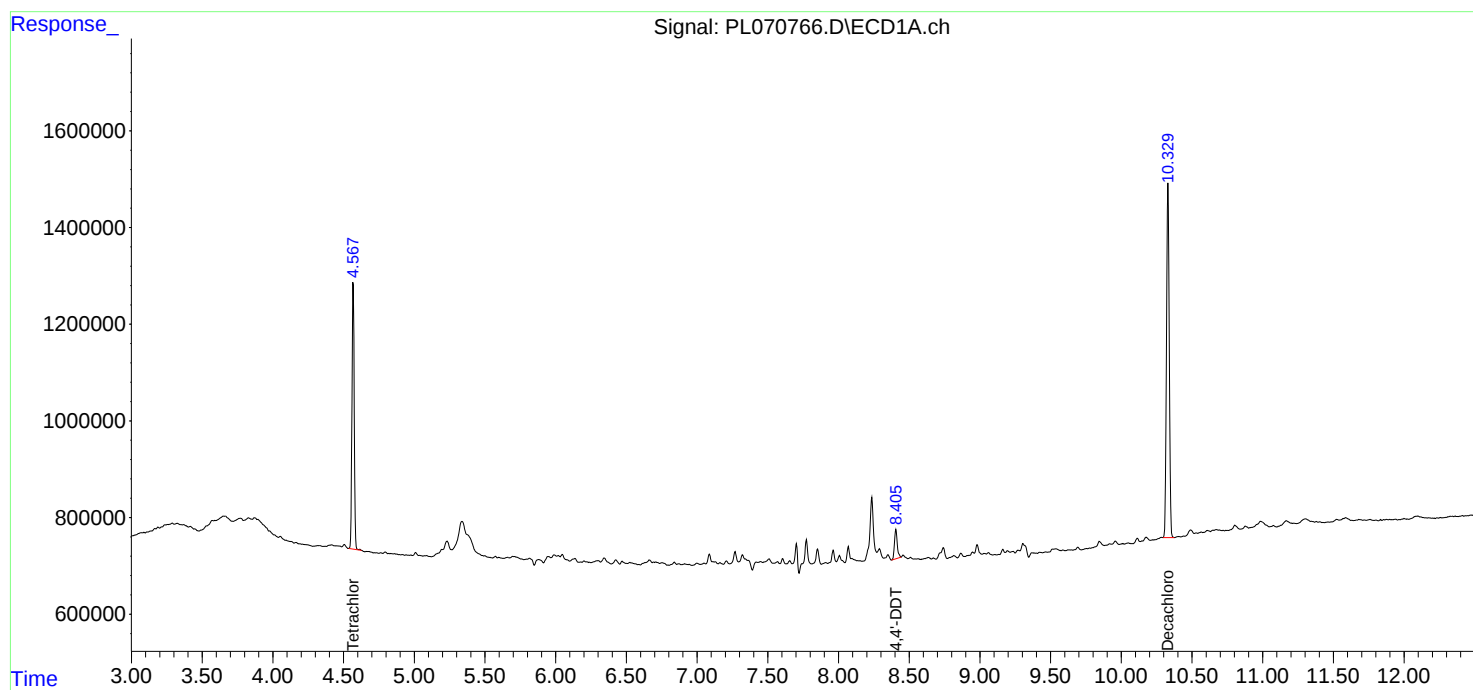


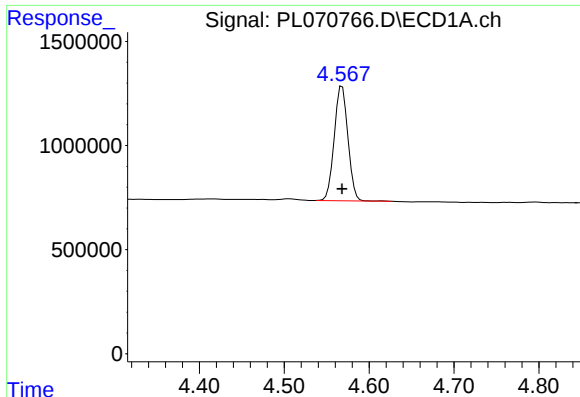

#1 Tetrachloro-m-xylene


R.T.: 4.568 min
Delta R.T.: 0.000 min
Response: 6188330
Conc: 12.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

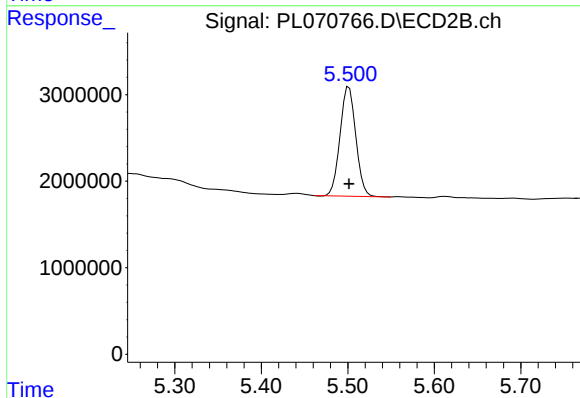


#1 Tetrachloro-m-xylene

R.T.: 5.501 min
Delta R.T.: 0.000 min
Response: 15858143
Conc: 12.58 ng/ml

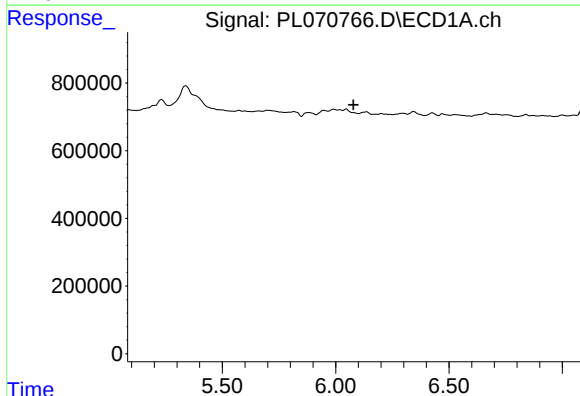


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.079 min
Response: 0
Conc: N.D.

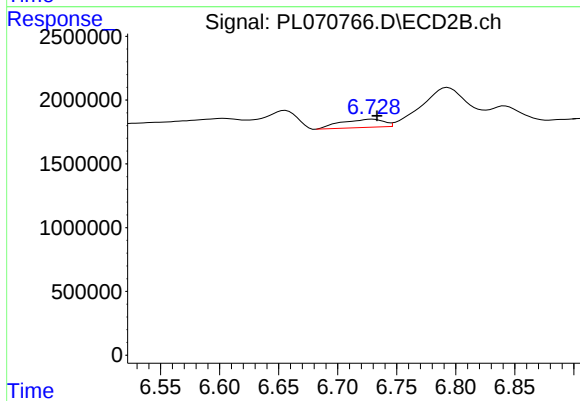

#6 beta-BHC


R.T.: 6.730 min
Delta R.T.: -0.004 min
Response: 1634409
Conc: 1.91 ng/ml

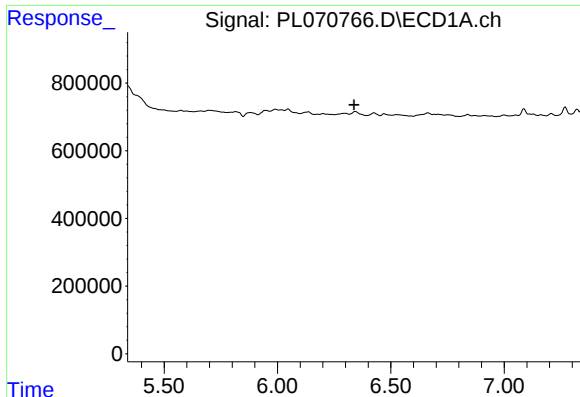

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.338 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

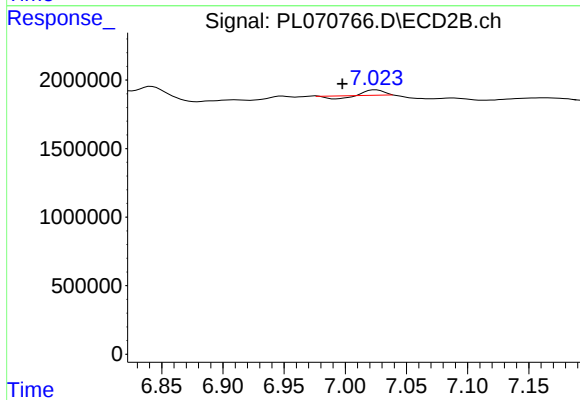


#7 delta-BHC

R.T.: 7.025 min
Delta R.T.: 0.027 min
Response: 210611
Conc: 0.13 ng/ml

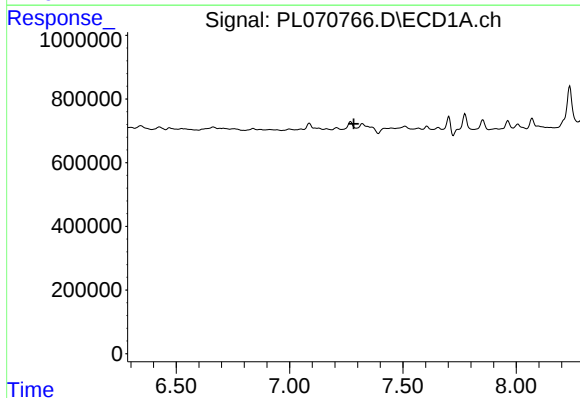


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.283 min
Response: 0
Conc: N.D.

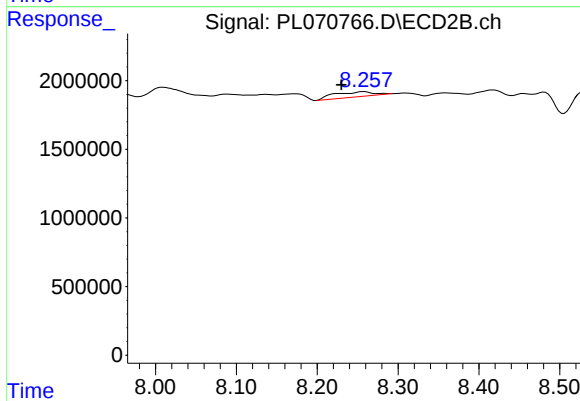

#10 gamma-Chlordane


R.T.: 8.258 min
Delta R.T.: 0.028 min
Response: 1250071
Conc: 0.81 ng/ml

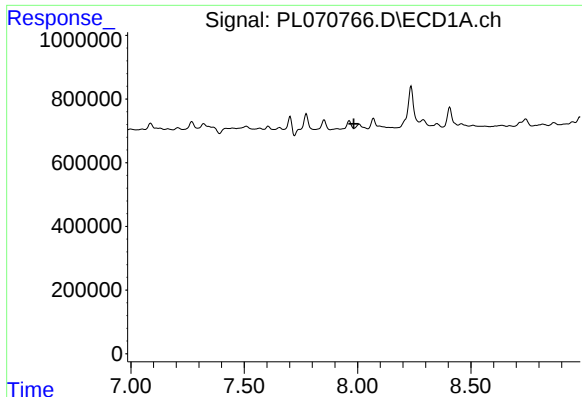

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 7.984 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

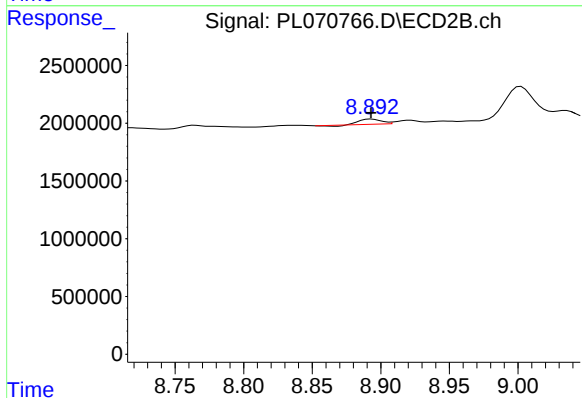


#14 Endrin

R.T.: 8.893 min
Delta R.T.: 0.000 min
Response: 457975
Conc: 0.40 ng/ml

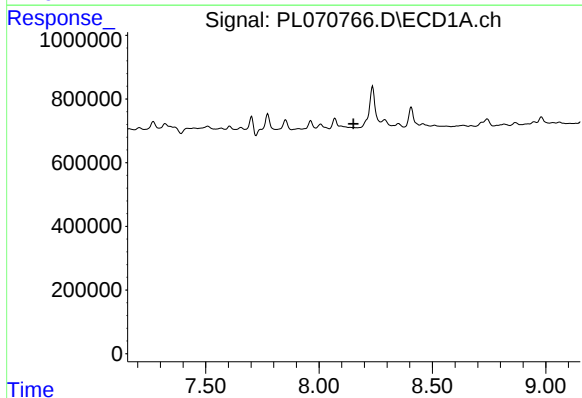


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.152 min
Response: 0
Conc: N.D.

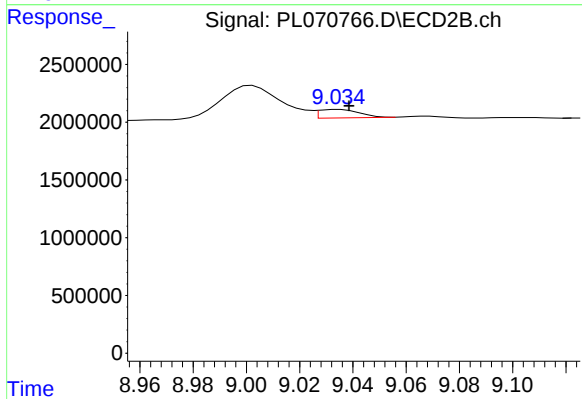

#16 4,4'-DDD


R.T.: 9.035 min
Delta R.T.: -0.004 min
Response: 776024
Conc: 0.64 ng/ml

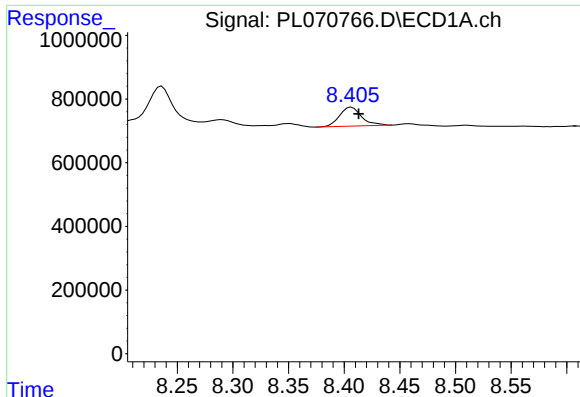

#17 4,4'-DDT


R.T.: 8.407 min
Delta R.T.: -0.006 min
Response: 816905
Conc: 1.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

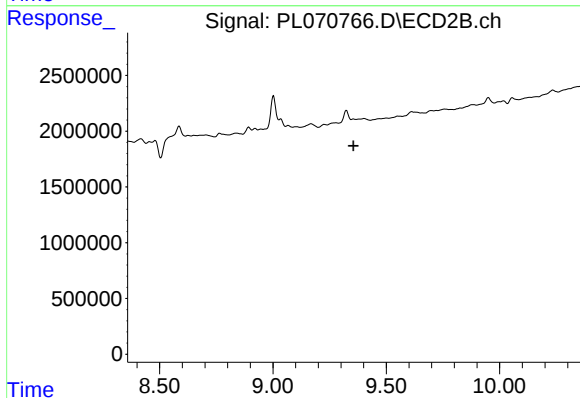


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.356 min
Response: 0
Conc: N.D.

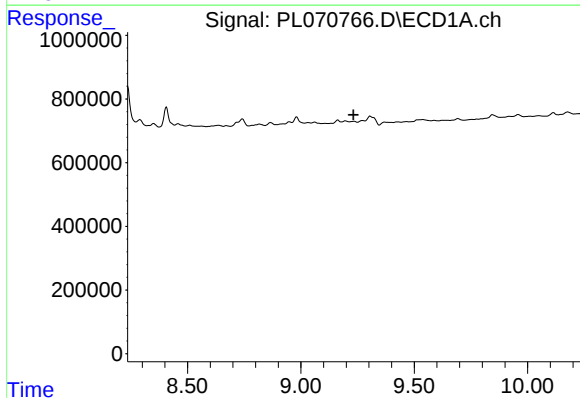


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.232 min
Response: 0
Conc: N.D.

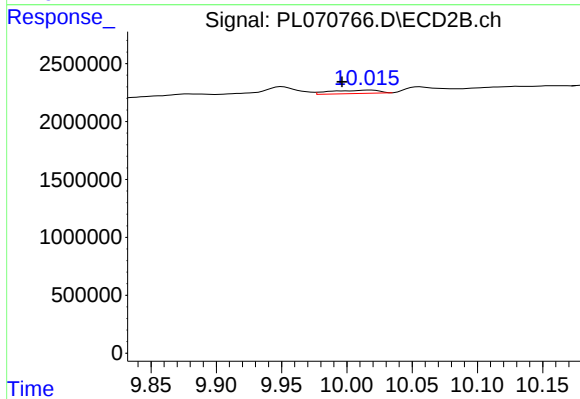

#21 Endrin ketone


R.T.: 10.018 min
Delta R.T.: 0.021 min
Response: 750157
Conc: 0.52 ng/ml

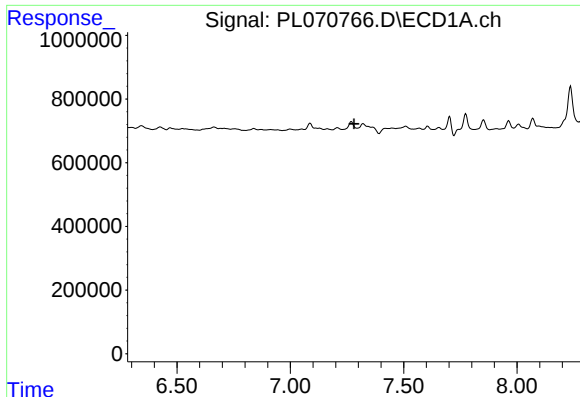

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.281 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

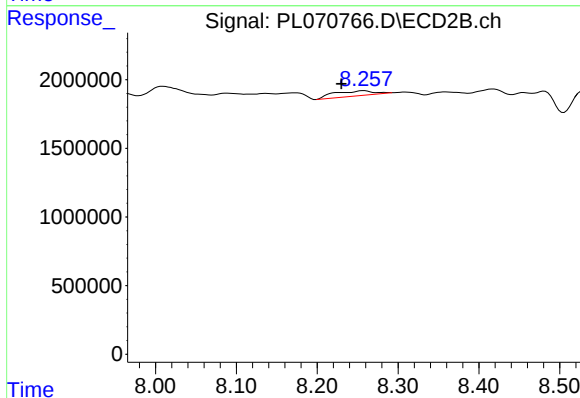


#25 Chlordane-3

R.T.: 8.258 min
Delta R.T.: 0.028 min
Response: 1250071
Conc: 6.18 ng/ml

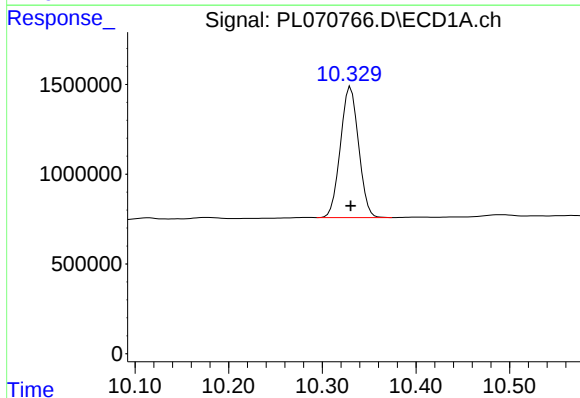

#28 Decachlorobiphenyl

R.T.: 10.330 min
Delta R.T.: 0.000 min
Response: 9822524
Conc: 14.38 ng/ml

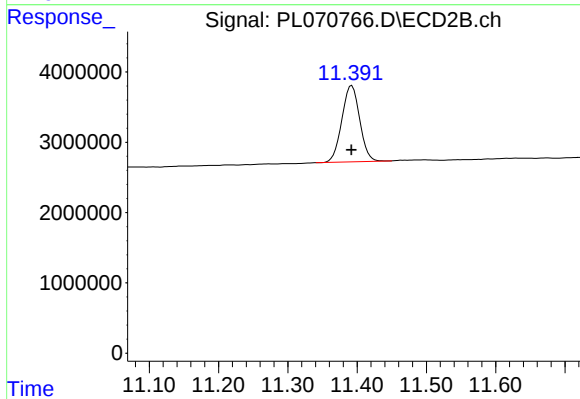

#28 Decachlorobiphenyl

R.T.: 11.392 min
Delta R.T.: 0.000 min
Response: 19460251
Conc: 14.55 ng/ml