

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110422\
 Data File : PL078825.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Nov 2022 15:25
 Operator : AR\AJ
 Sample : PB148802BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 03:16:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:08:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.330	2.569	31684456	43108096	16.615	16.884
28)	SA Decachlor...	8.780	7.641	27751572	38070487	18.447	20.099
Target Compounds							
7)	B delta-BHC	4.551f	0.000	1381026	0	0.607	N.D. #
11)	B alpha-Chl...	5.793	0.000	157900	0	0.068	N.D. #
12)	B 4,4'-DDE	5.981	0.000	30911	0	0.015	N.D. #
14)	MA Endrin	6.356	0.000	421240	0	0.222	N.D. #
15)	B Endosulfa...	6.594	0.000	712703	0	0.380	N.D. #
16)	A 4,4'-DDD	6.525f	0.000	192259	0	0.115	N.D. #
21)	B Endrin ke...	7.458f	6.591f	102377	1004424	0.054	0.389 #
26)	Chlordane-4	5.793	0.000	157900	0	0.385	N.D. #
27)	Chlordane-5	0.000	5.465f	0	3199467	N.D.	39.230 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110422\
Data File : PL078825.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Nov 2022 15:25
Operator : AR\AJ
Sample : PB148802BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 03:16:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:08:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

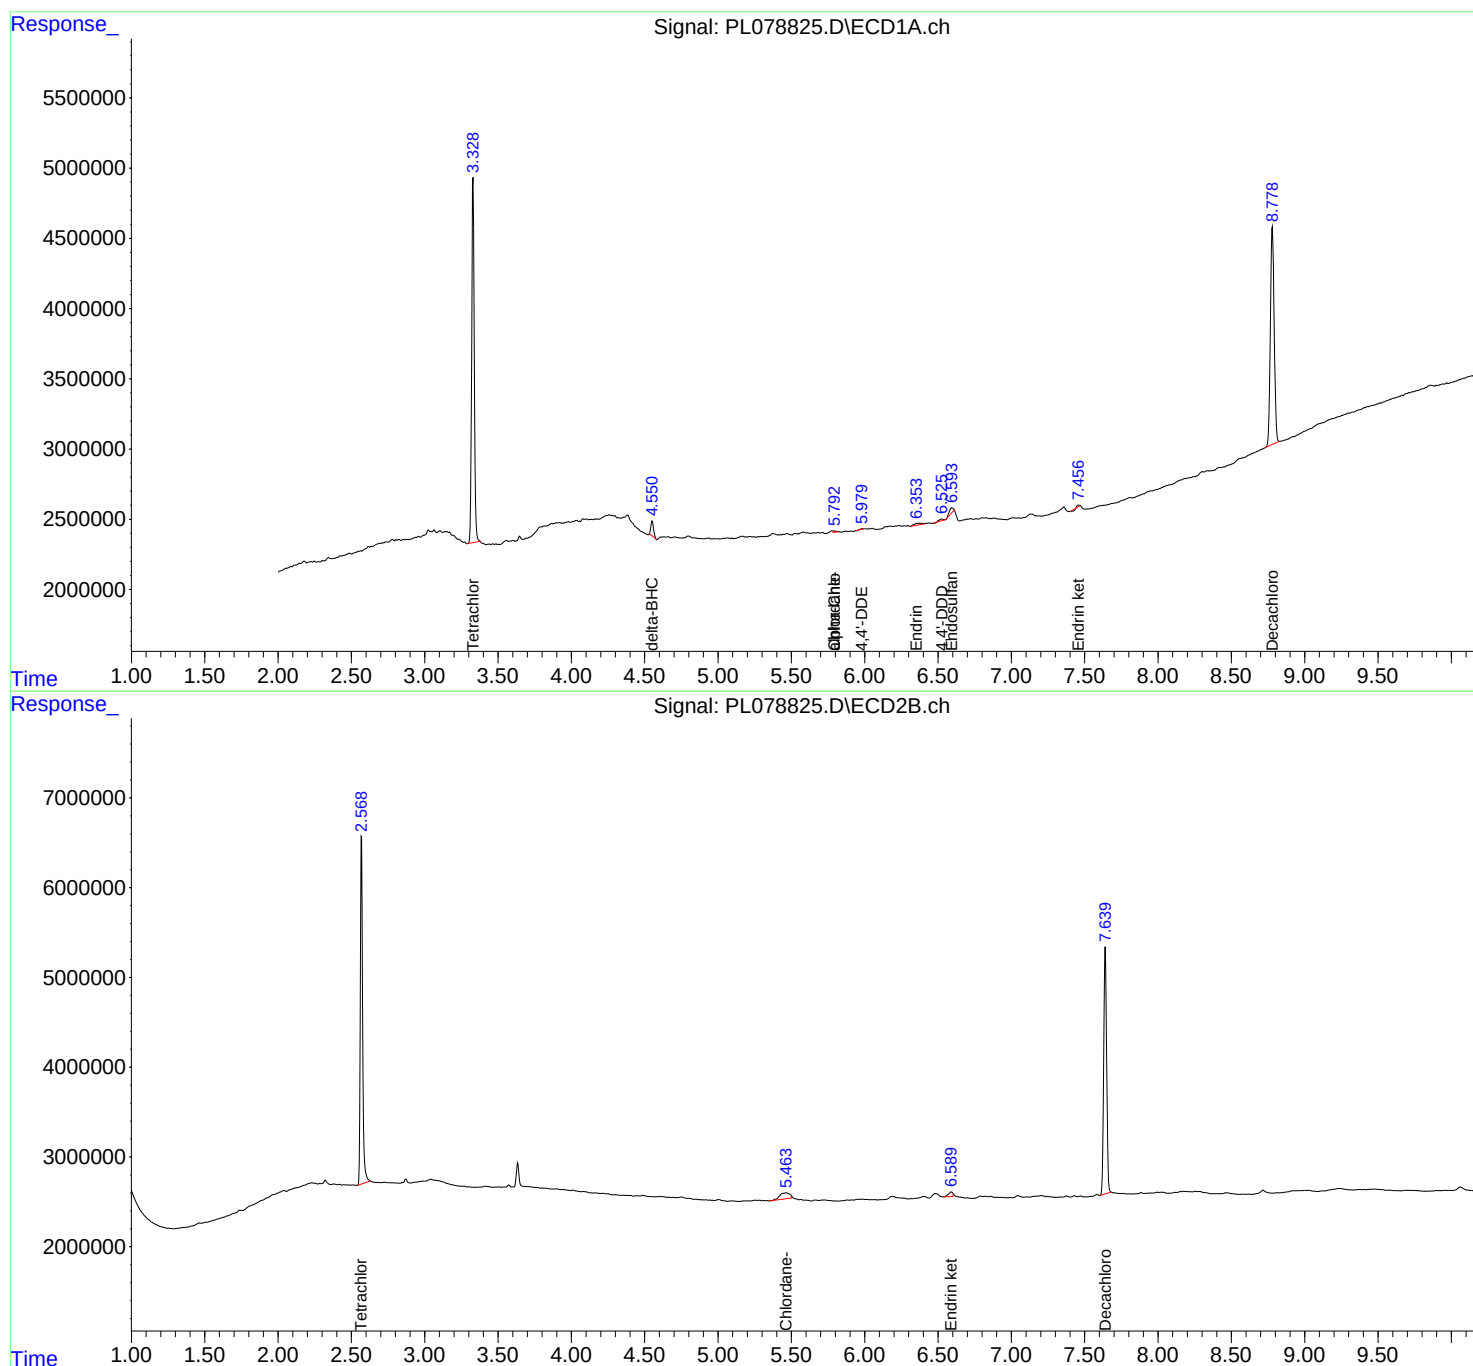


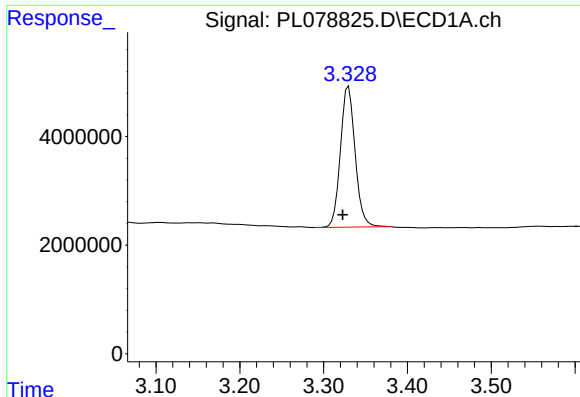

#1 Tetrachloro-m-xylene


R.T.: 3.330 min
Delta R.T.: 0.007 min
Response: 31684456
Conc: 16.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

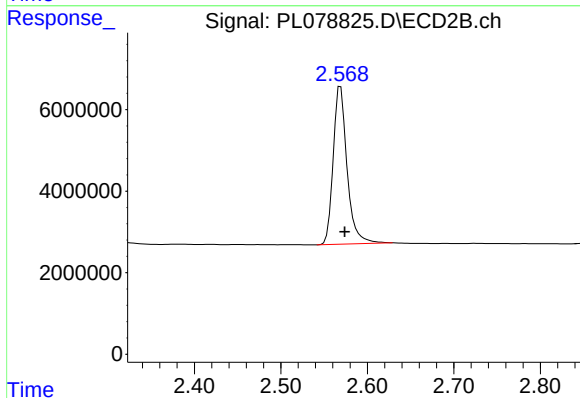


#1 Tetrachloro-m-xylene

R.T.: 2.569 min
Delta R.T.: -0.005 min
Response: 43108096
Conc: 16.88 ng/ml

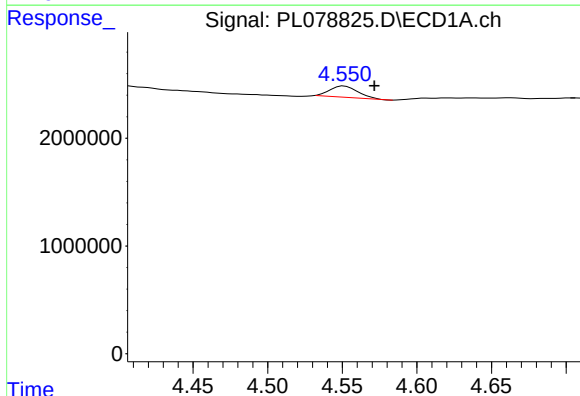


#7 delta-BHC

R.T.: 4.551 min
Delta R.T.: -0.020 min
Response: 1381026
Conc: 0.61 ng/ml

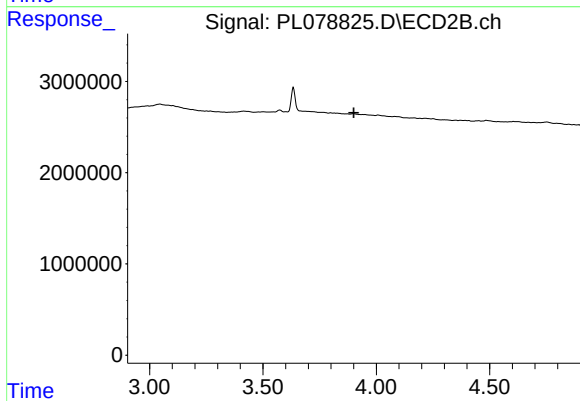

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 3.901 min
Response: 0
Conc: N.D.

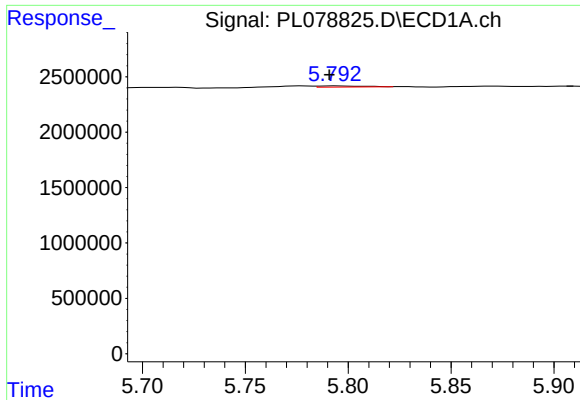

#11 alpha-Chlordane


R.T.: 5.793 min
Delta R.T.: 0.002 min
Response: 157900
Conc: 0.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

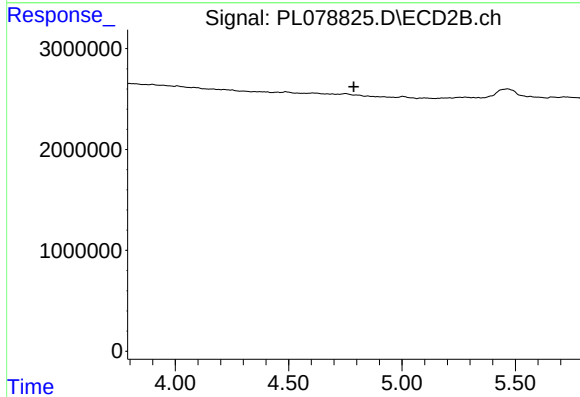


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.787 min
Response: 0
Conc: N.D.

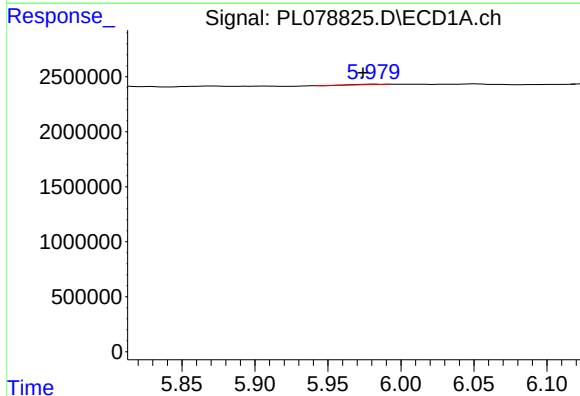


#12 4,4'-DDE

R.T.: 5.981 min
Delta R.T.: 0.007 min
Response: 30911
Conc: 0.02 ng/ml

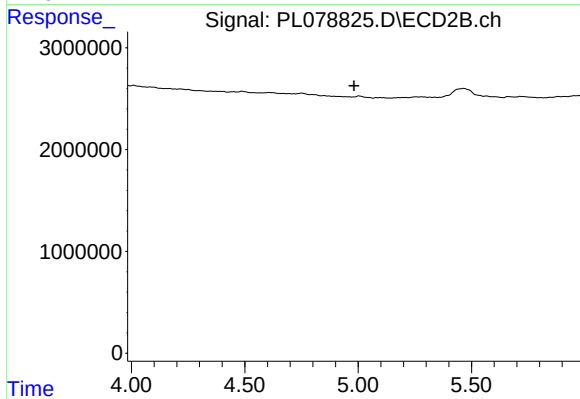

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 4.982 min
Response: 0
Conc: N.D.

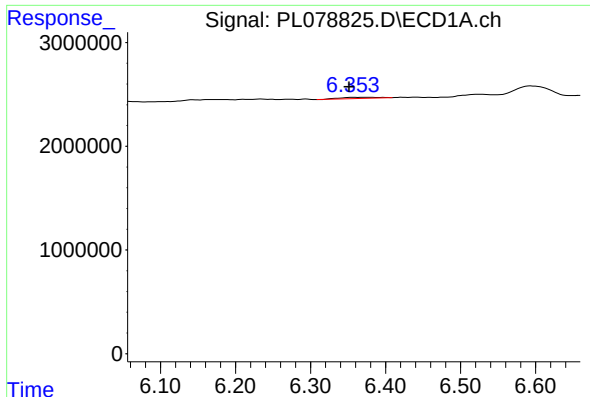

#14 Endrin


R.T.: 6.356 min
Delta R.T.: 0.004 min
Response: 421240
Conc: 0.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

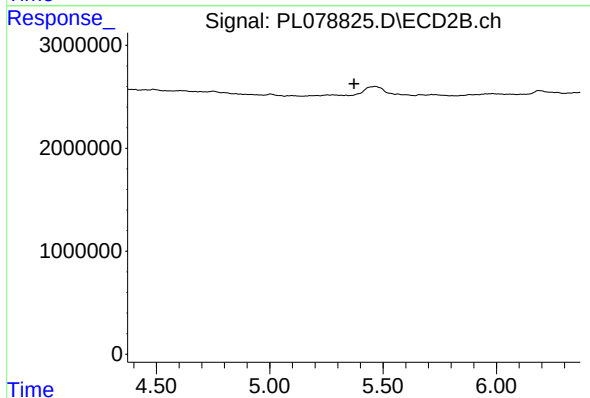


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 5.373 min
Response: 0
Conc: N.D.

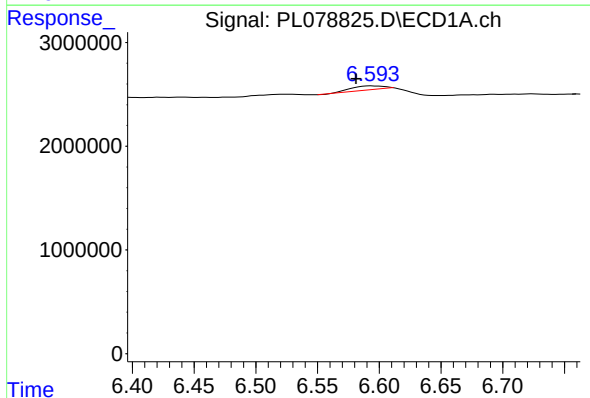


#15 Endosulfan II

R.T.: 6.594 min
Delta R.T.: 0.013 min
Response: 712703
Conc: 0.38 ng/ml

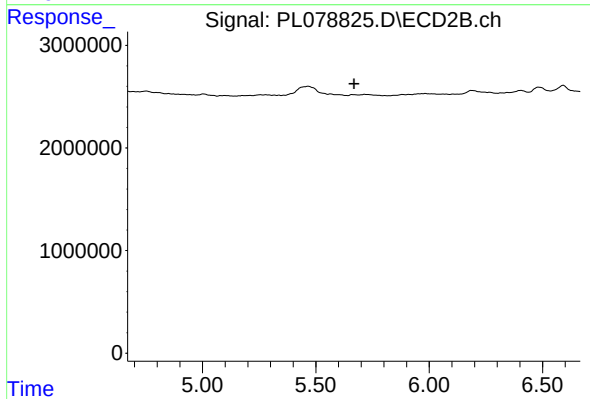

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 5.669 min
Response: 0
Conc: N.D.

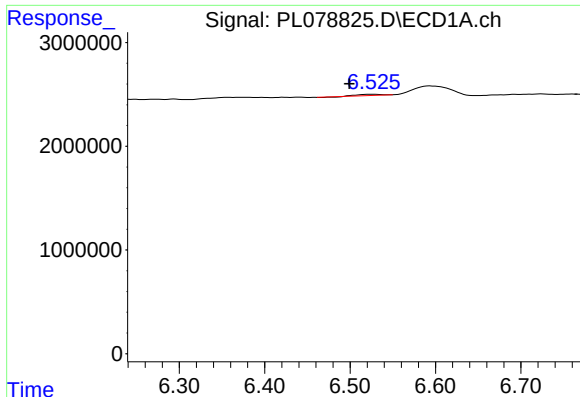

#16 4,4'-DDD


R.T.: 6.525 min
Delta R.T.: 0.026 min
Response: 192259
Conc: 0.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

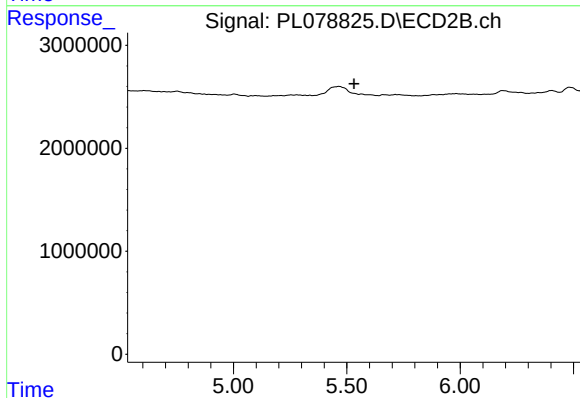


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.532 min
Response: 0
Conc: N.D.

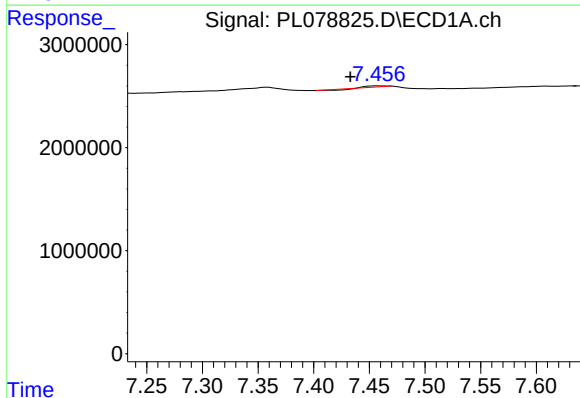


#21 Endrin ketone

R.T.: 7.458 min
Delta R.T.: 0.025 min
Response: 102377
Conc: 0.05 ng/ml

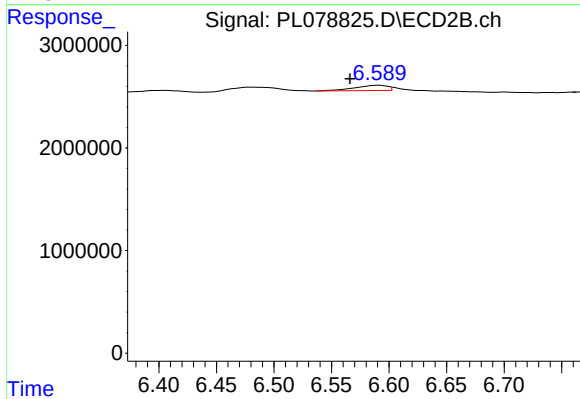

#21 Endrin ketone


R.T.: 6.591 min
Delta R.T.: 0.025 min
Response: 1004424
Conc: 0.39 ng/ml

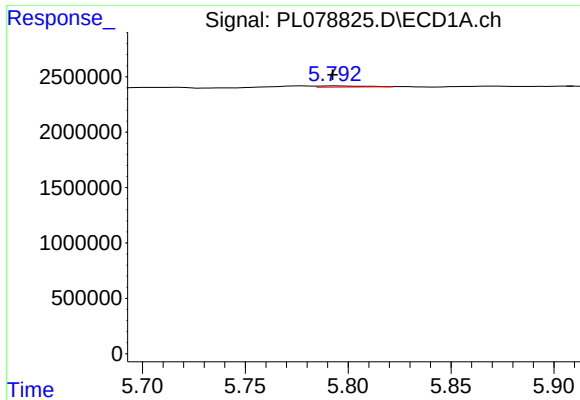

#26 Chlordane-4


R.T.: 5.793 min
Delta R.T.: 0.000 min
Response: 157900
Conc: 0.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

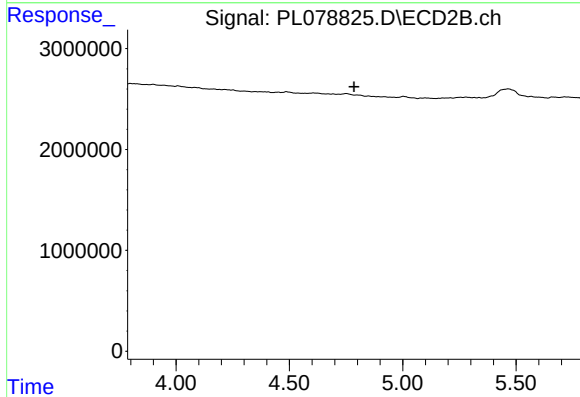


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 4.785 min
Response: 0
Conc: N.D.

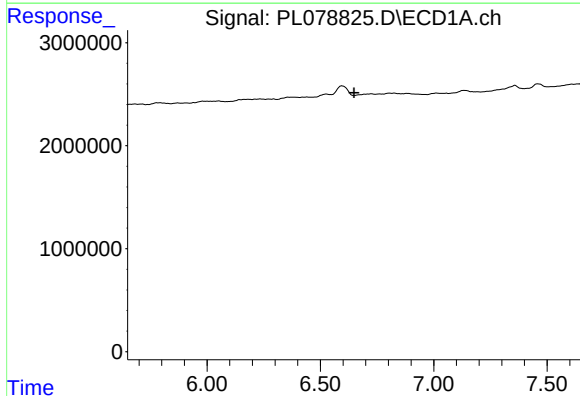


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.649 min
Response: 0
Conc: N.D.

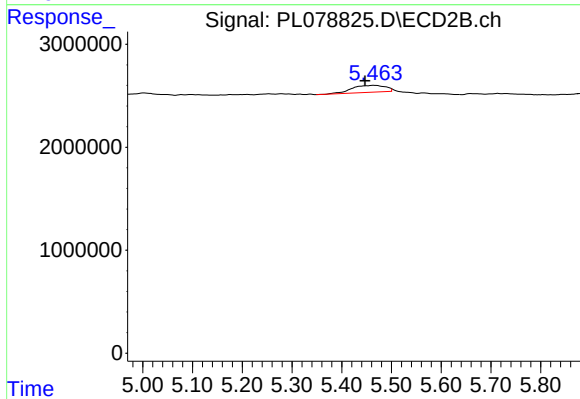

#27 Chlordane-5


R.T.: 5.465 min
Delta R.T.: 0.018 min
Response: 3199467
Conc: 39.23 ng/ml

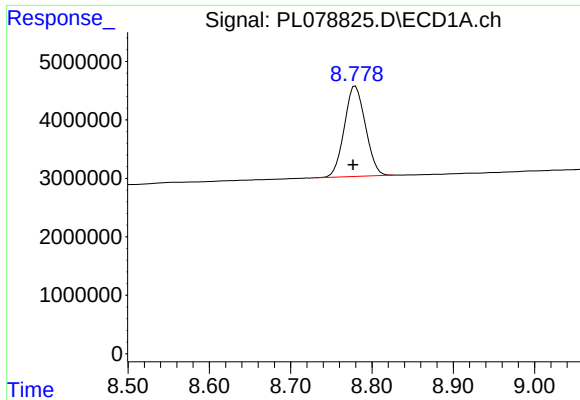

#28 Decachlorobiphenyl

R.T.: 8.780 min
Delta R.T.: 0.003 min
Response: 27751572
Conc: 18.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

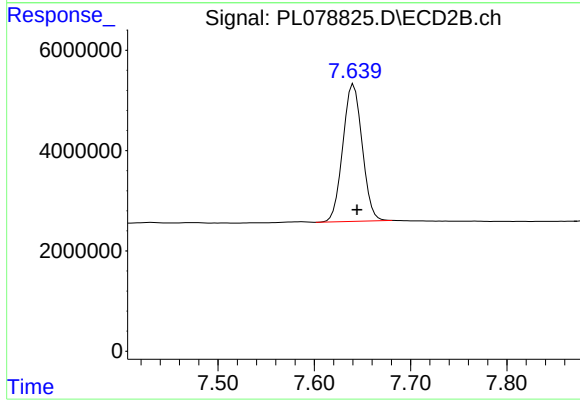

#28 Decachlorobiphenyl

R.T.: 7.641 min
Delta R.T.: -0.004 min
Response: 38070487
Conc: 20.10 ng/ml