

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110422\
 Data File : PL078826.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Nov 2022 16:07
 Operator : AR\AJ
 Sample : N5428-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MONTHLY-OUTFALL-002

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/07/2022
 Supervised By :Ankita Jodhani 11/07/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 03:16:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:08:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.327	2.569	24488327	35966951	12.841	14.087
2) SA Decachlor...	8.776	7.638	19045501	24433563	12.660m	12.900m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110422\
Data File : PL078826.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Nov 2022 16:07
Operator : AR\AJ
Sample : N5428-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MONTHLY-OUTFALL-002


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/07/2022
Supervised By : Ankita Jodhani 11/07/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 03:16:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:08:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

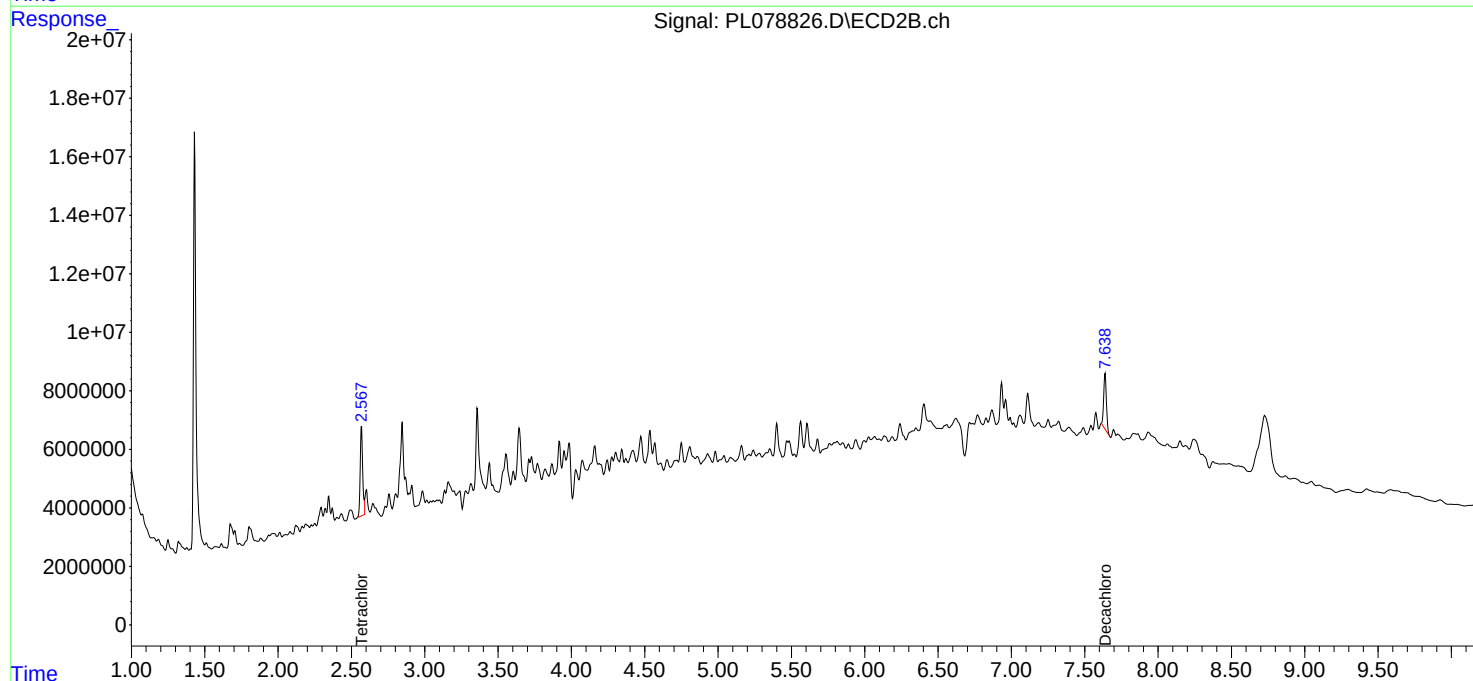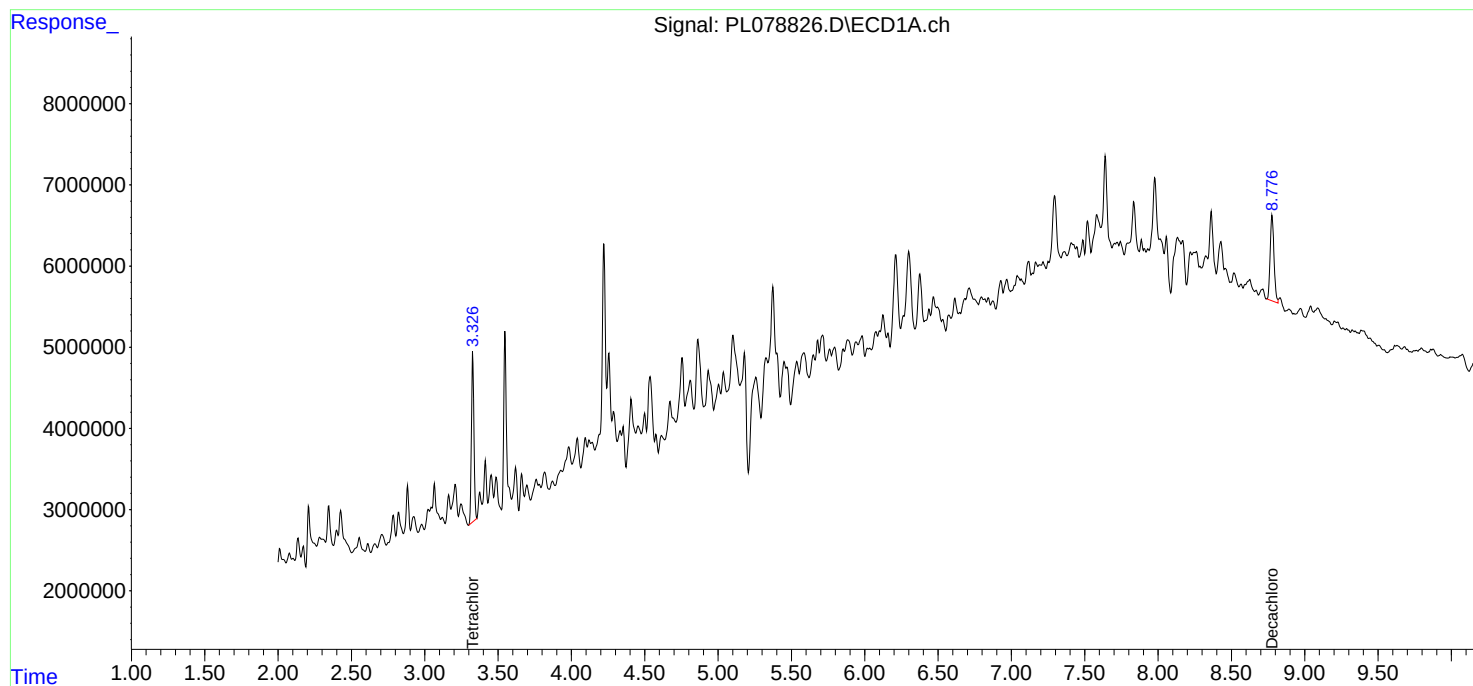

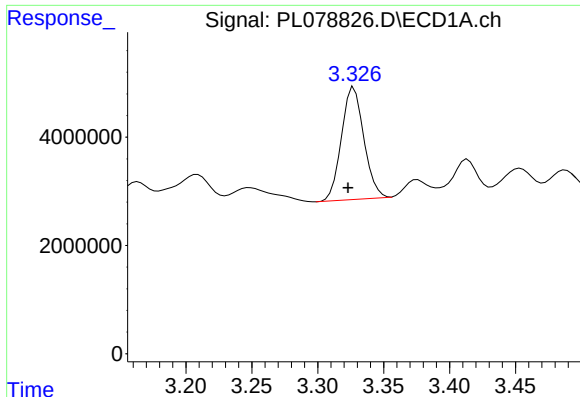


#1 Tetrachloro-m-xylene

R.T.: 3.327 min
Delta R.T.: 0.004 min
Response: 24488327
Conc: 12.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
MONTHLY-OUTFALL-002


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/07/2022
Supervised By :Ankita Jodhani 11/07/2022

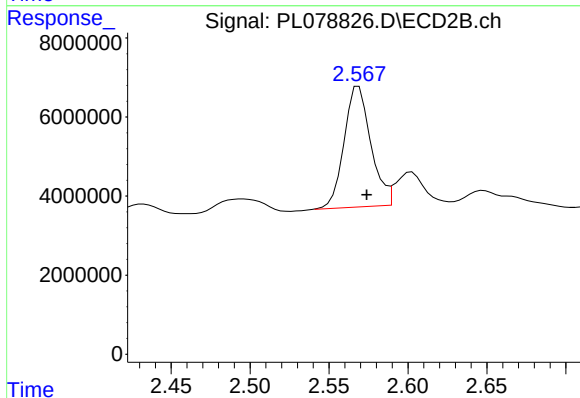


#1 Tetrachloro-m-xylene

R.T.: 2.569 min
Delta R.T.: -0.005 min
Response: 35966951
Conc: 14.09 ng/ml

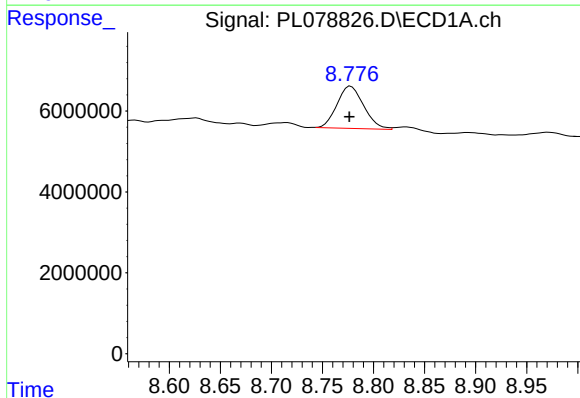

#28 Decachlorobiphenyl

R.T.: 8.776 min
Delta R.T.: 0.000 min
Response: 19045501
Conc: 12.66 ng/ml m

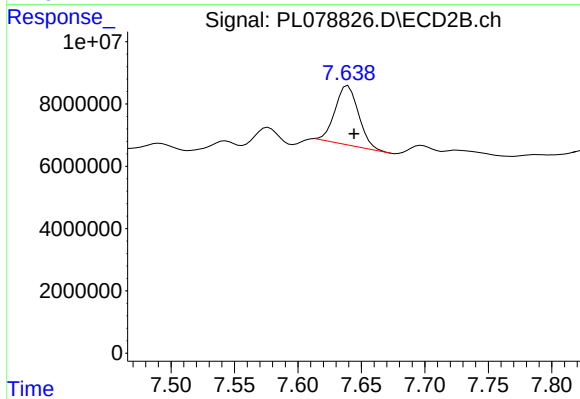

#28 Decachlorobiphenyl

R.T.: 7.638 min
Delta R.T.: -0.006 min
Response: 24433563
Conc: 12.90 ng/ml m