

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110423\
 Data File : PL086431.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2023 15:22
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 INDA4312

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 16:39:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 03 16:33:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.353	2.618	106.6E6	32347931	40.663	40.051
27)	SA Decachlor...	8.851	7.767	183.9E6	80957603	80.265	80.334
Target Compounds							
2)	A alpha-BHC	3.806	3.117	163.1E6	46898999	40.041	40.032
3)	MA gamma-BHC...	4.138	3.443	152.2E6	45426814	39.895	40.156
4)	MA Heptachlor	4.724	3.779	156.7E6	47221986	39.769	40.121
9)	A Endosulfan I	5.877	4.927	122.0E6	39357549	39.941	40.223
13)	MA Dieldrin	6.154	5.193	273.8E6	91333611	79.883	80.807
14)	MA Endrin	6.383	5.467	234.9E6	81208097	80.207	80.656
16)	A 4,4'-DDD	6.533	5.630	185.5E6	65659055	81.332	80.916
17)	MA 4,4'-DDT	6.849	5.881	194.4E6	74885485	79.651	80.660
20)	A Methoxychlor	7.334	6.465	505.1E6	217.9E6	401.608	407.114

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110423\
Data File : PL086431.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2023 15:22
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 16:39:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Nov 03 16:33:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

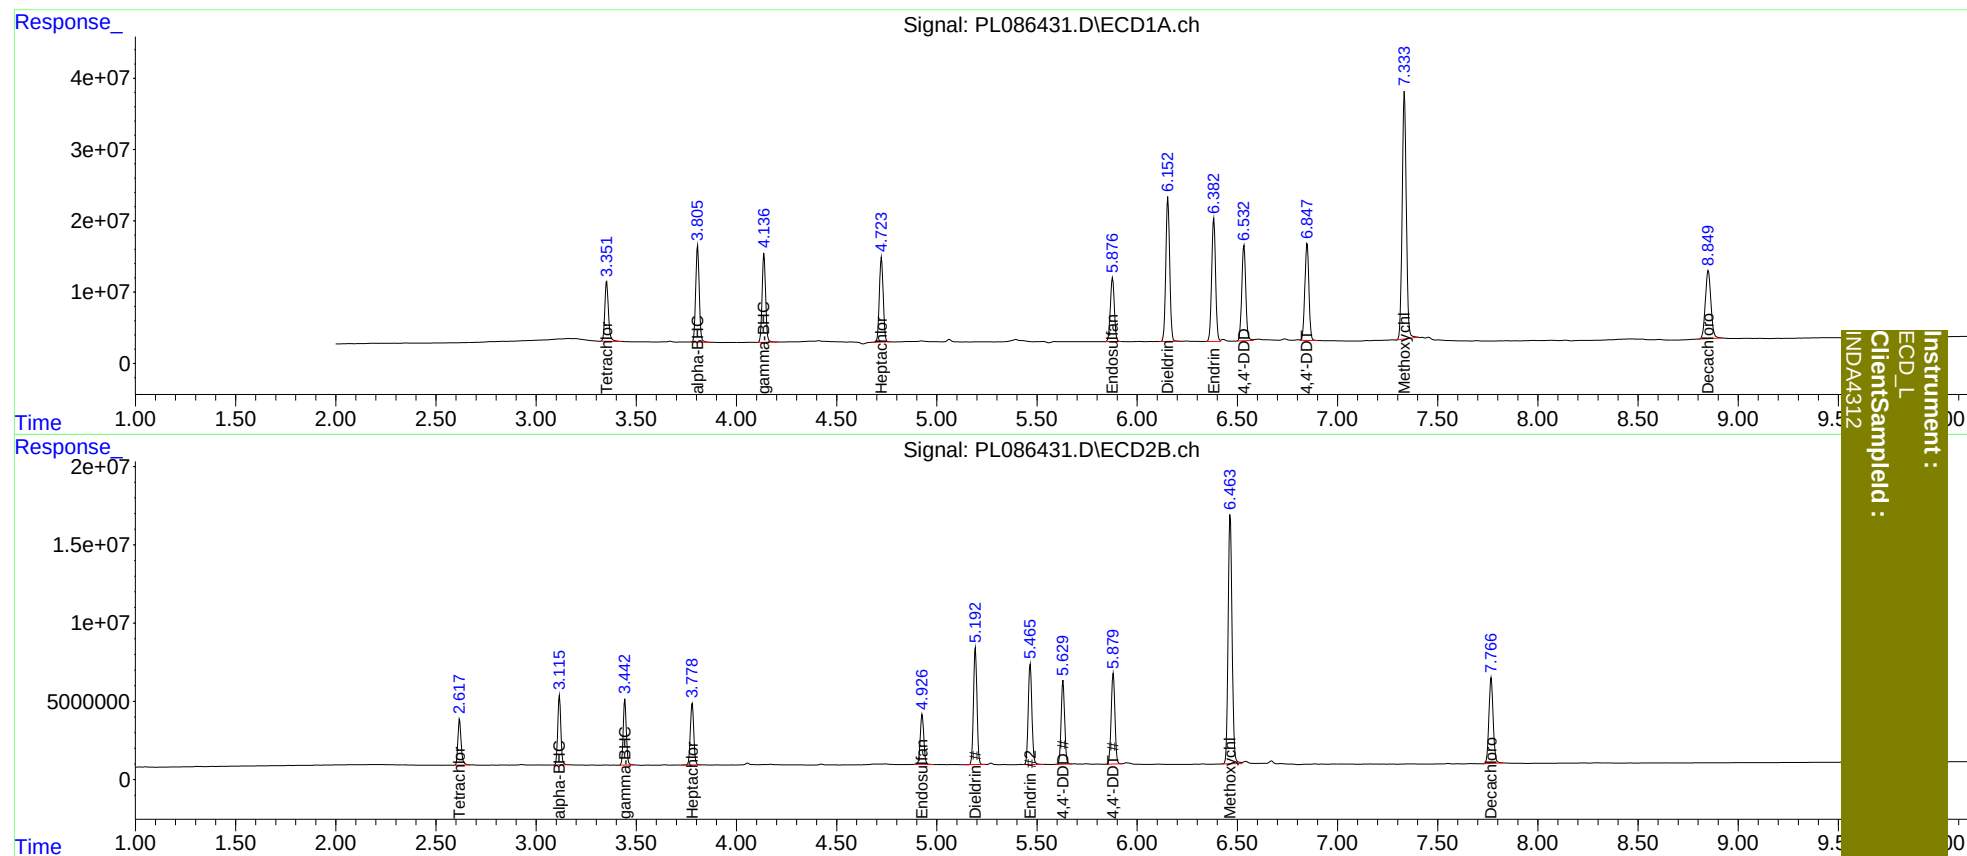

Instrument :
ECD_L
ClientSampled :
INDA4312