

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110423\
 Data File : PL086446.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2023 20:00
 Operator : AR\AJ
 Sample : 04953-05DL 2X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EOAS7DL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/04/2023
 Supervised By : mohammad ahmed 11/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 00:38:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 03 17:13:37 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.353	2.619	17097194	5070006	6.463	6.313
27)	SA Decachlor...	8.851	7.767	16711289	7209407	7.042	6.826
Target Compounds							
15)	B Endosulfa...	6.606	5.757	871787	362755	0.306m	0.373m
16)	A 4,4'-DDD	6.533	5.630	6230173	1696724	2.796	2.223
17)	MA 4,4'-DDT	6.848	5.881	238.7E6	89009383	100.312	100.975

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110423\
Data File : PL086446.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2023 20:00
Operator : AR\AJ
Sample : 04953-05DL 2X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 00:38:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Nov 03 17:13:37 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

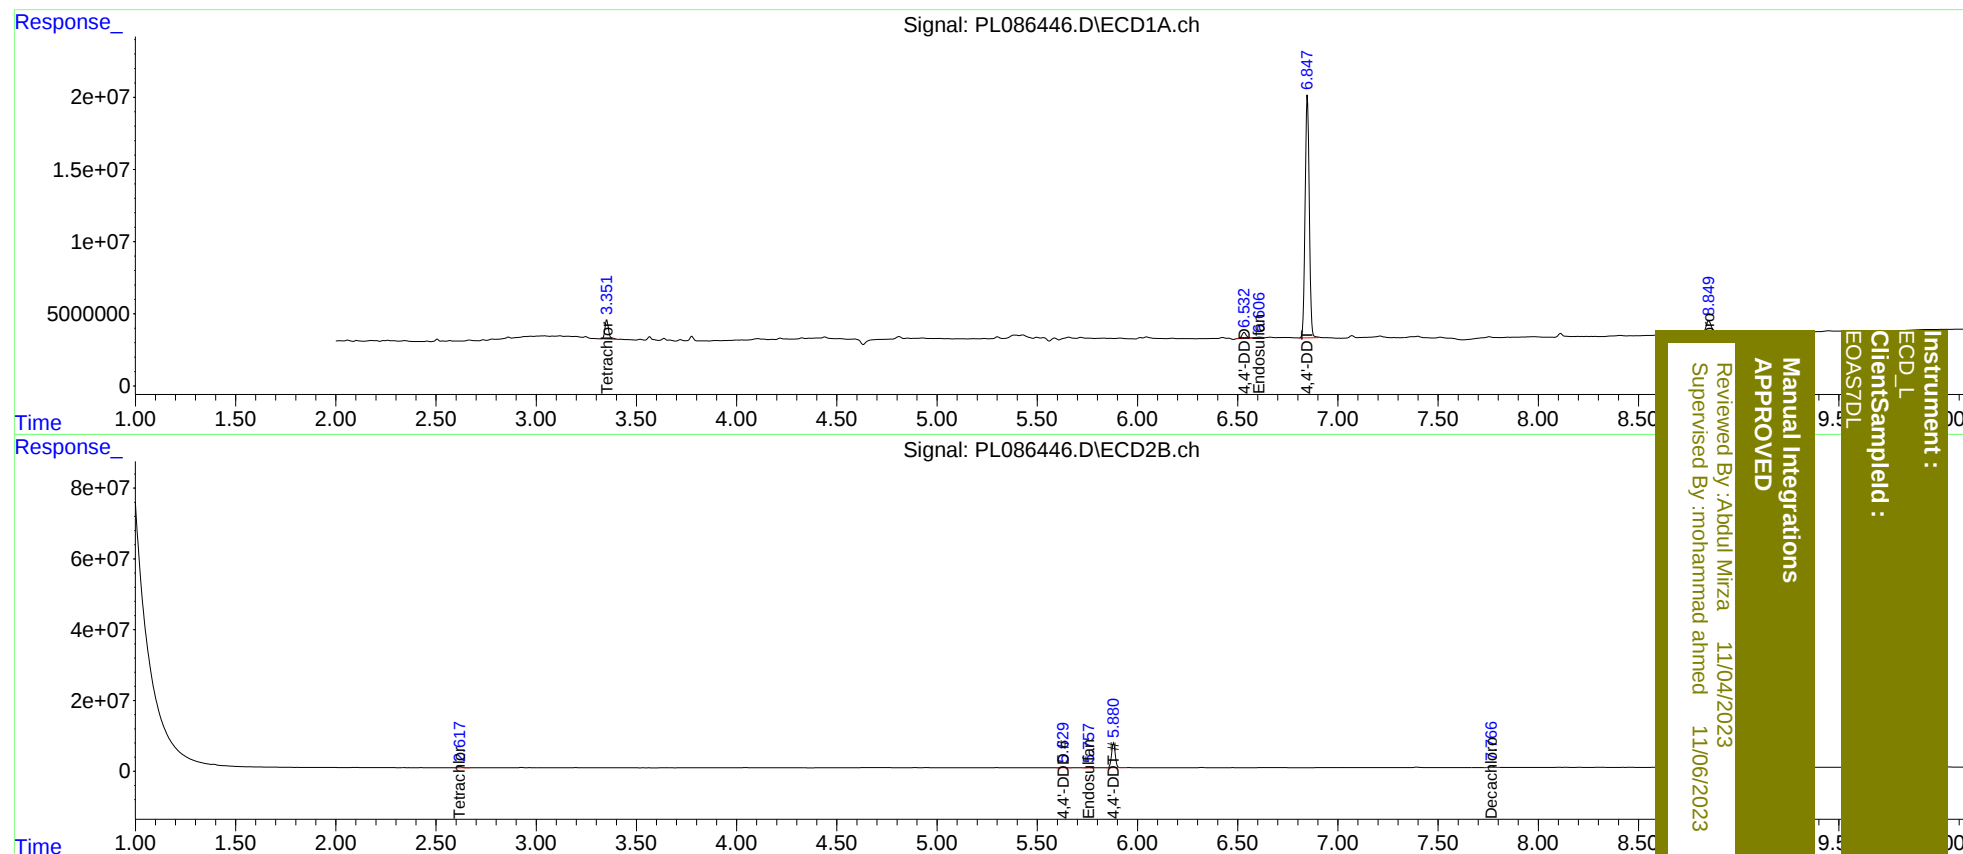

Instrument :
ECD_L
ClientSampled :
EOASTDL

Manual Integrations
APPROVED

Reviewed By: Abdul Miza 11/04/2023
Supervised By: mohammad ahmed 11/06/2023