

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110424\
 Data File : PL092834.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Nov 2024 17:02
 Operator : AR\AJ
 Sample : P4675-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 03:16:51 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.779	35013053	38791171	14.290	14.255
28)	SA Decachlor...	9.056	7.916	29717616	40974872	15.441	15.013
Target Compounds							
2)	A alpha-BHC	0.000	3.292	0	13425	N.D.	0.003 #
3)	MA gamma-BHC...	0.000	3.611	0	24207	N.D.	0.006 #
4)	MA Heptachlor	0.000	3.957	0	50468	N.D.	0.013 #
5)	MB Aldrin	0.000	4.219	0	64439	N.D.	0.018 #
6)	B beta-BHC	0.000	3.912	0	82074	N.D.	0.050 #
7)	B delta-BHC	0.000	4.136	0	259606	N.D.	0.068 #
12)	B 4,4'-DDE	0.000	5.230	0	70920	N.D.	0.022 #
13)	MA Dieldrin	0.000	5.369	0	133531	N.D.	0.040 #
14)	MA Endrin	0.000	5.658f	0	249696	N.D.	0.086 #
17)	MA 4,4'-DDT	0.000	6.036	0	421825	N.D.	0.157 #
23)	Chlordane-1	0.000	3.774	0	43131	N.D.	0.406 #
24)	Chlordane-2	0.000	4.365	0	104888	N.D.	0.847 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110424\
Data File : PL092834.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Nov 2024 17:02
Operator : AR\AJ
Sample : P4675-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
COMP-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 03:16:51 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

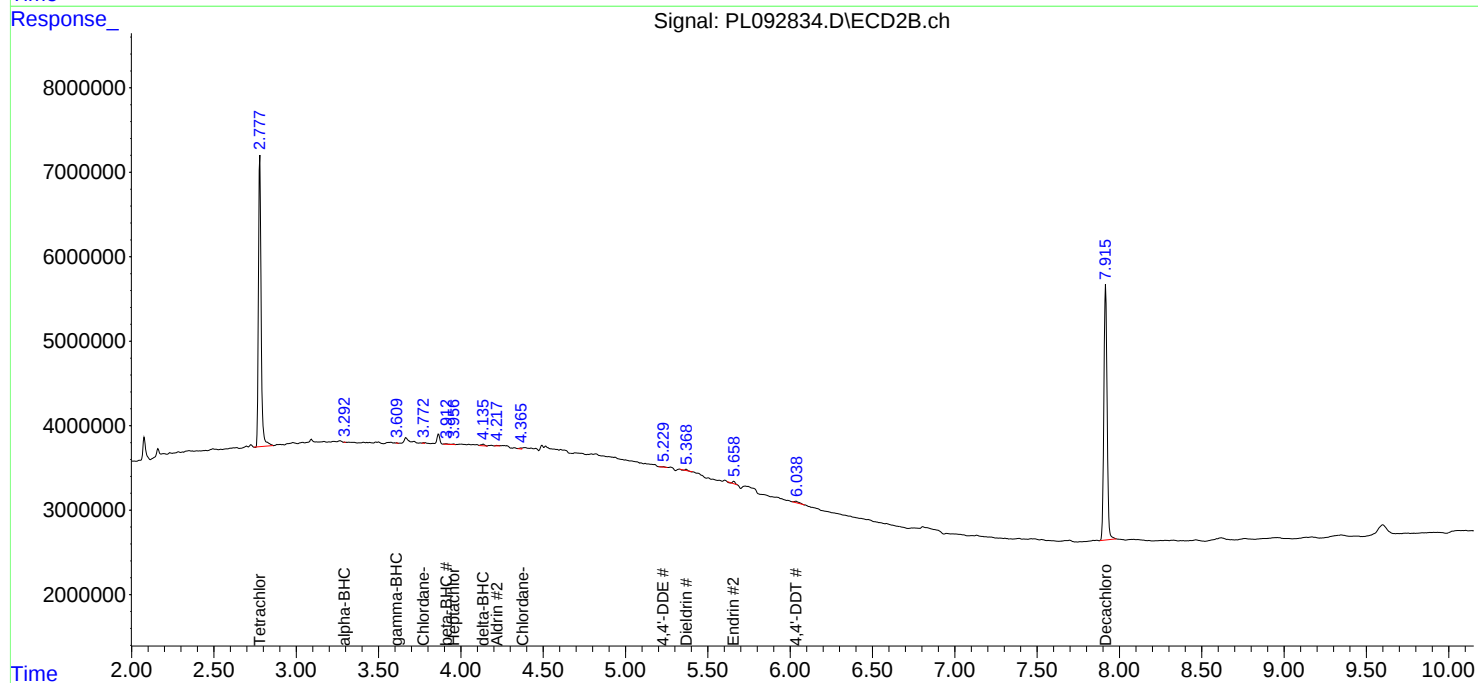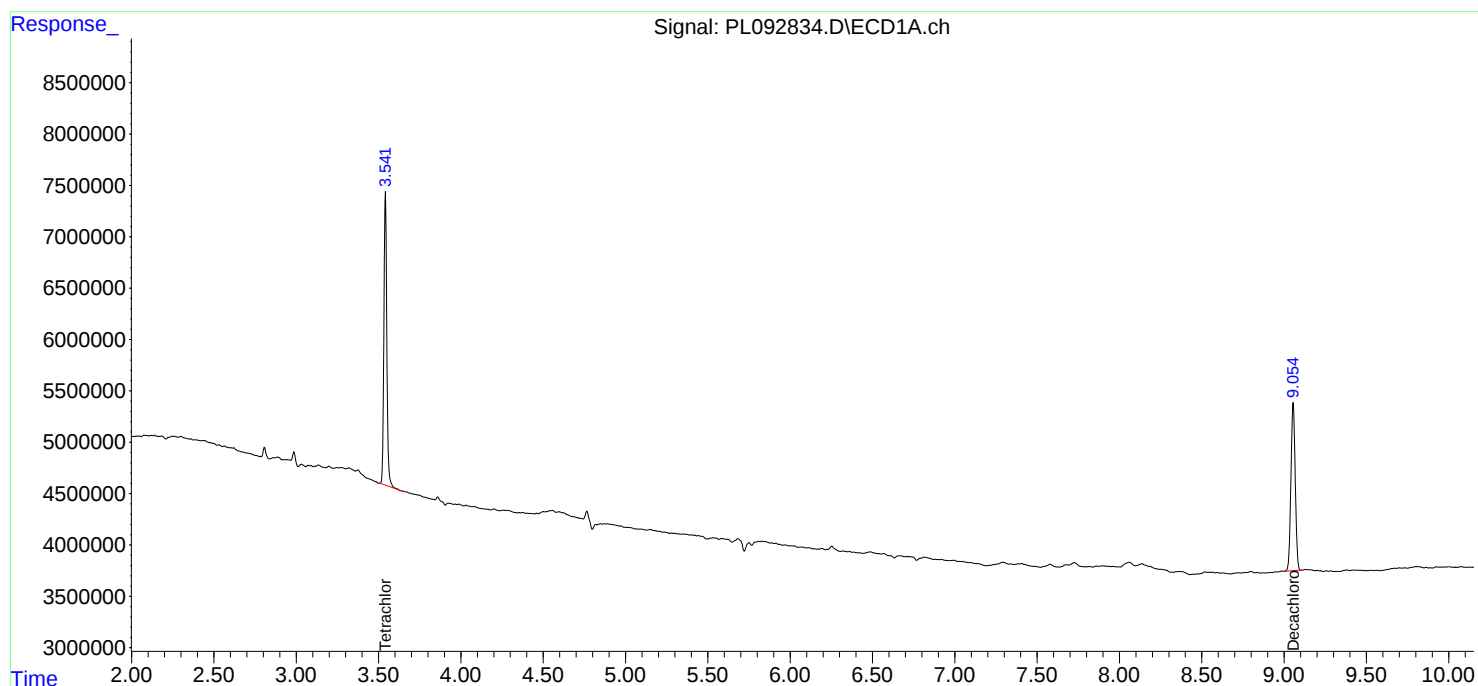


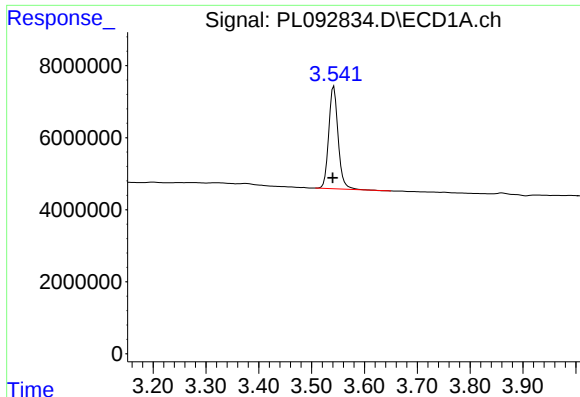

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: 0.002 min
Response: 35013053
Conc: 14.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-6

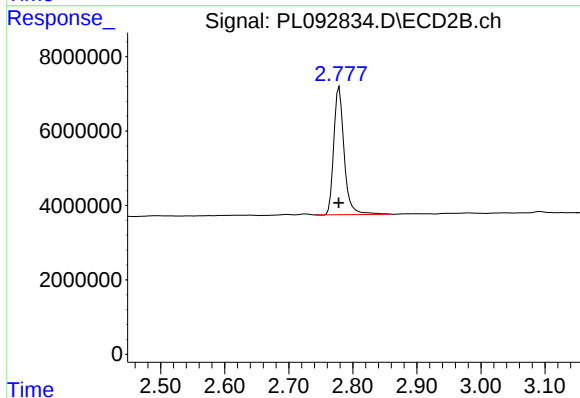


#1 Tetrachloro-m-xylene

R.T.: 2.779 min
Delta R.T.: 0.000 min
Response: 38791171
Conc: 14.26 ng/ml

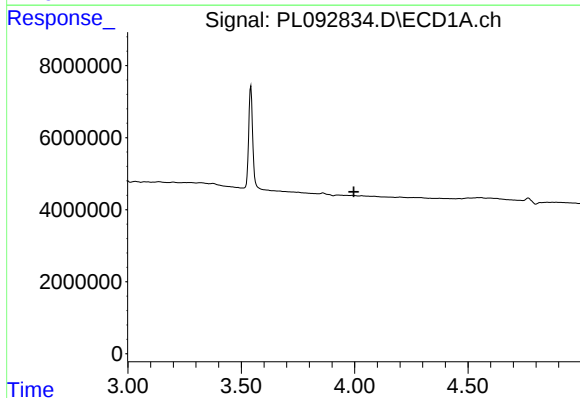


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.996 min
Response: 0
Conc: N.D.

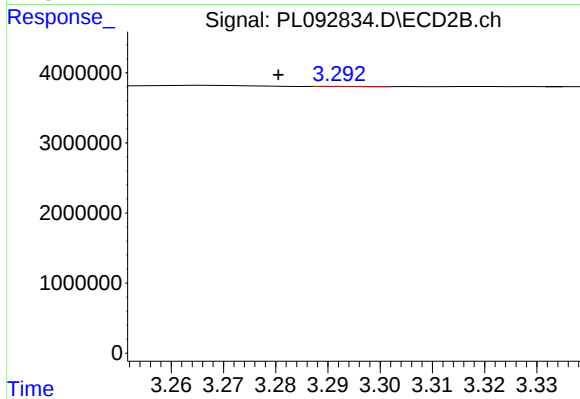

#2 alpha-BHC


R.T.: 3.292 min
Delta R.T.: 0.012 min
Response: 13425
Conc: 0.00 ng/ml

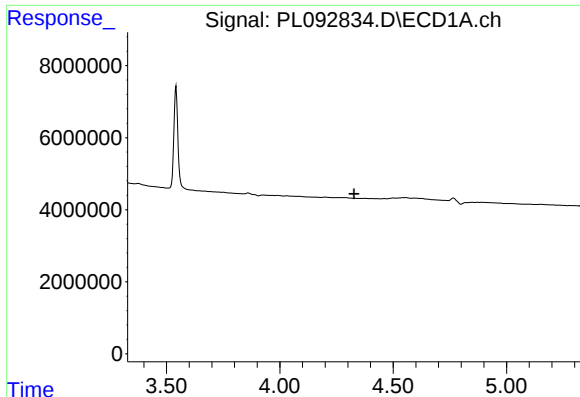

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-6

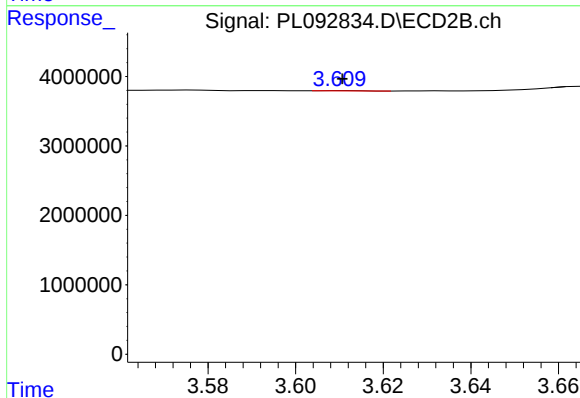


#3 gamma-BHC (Lindane)

R.T.: 3.611 min
Delta R.T.: 0.000 min
Response: 24207
Conc: 0.01 ng/ml

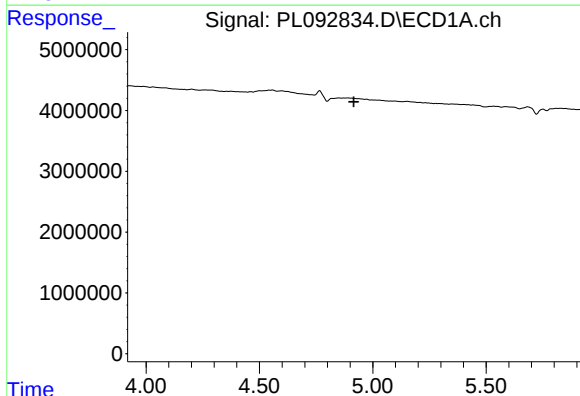


#4 Heptachlor

R.T.: 0.000 min
Exp R.T.: 4.917 min
Response: 0
Conc: N.D.

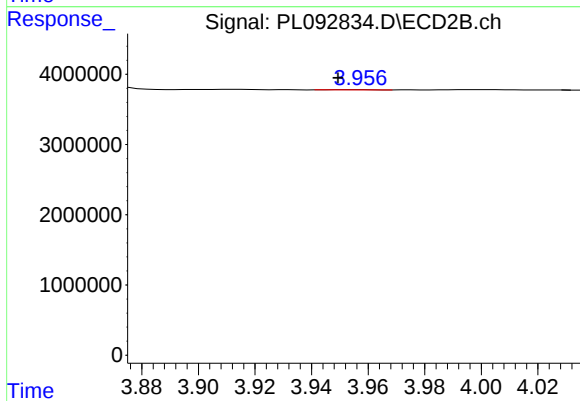

#4 Heptachlor


R.T.: 3.957 min
Delta R.T.: 0.008 min
Response: 50468
Conc: 0.01 ng/ml

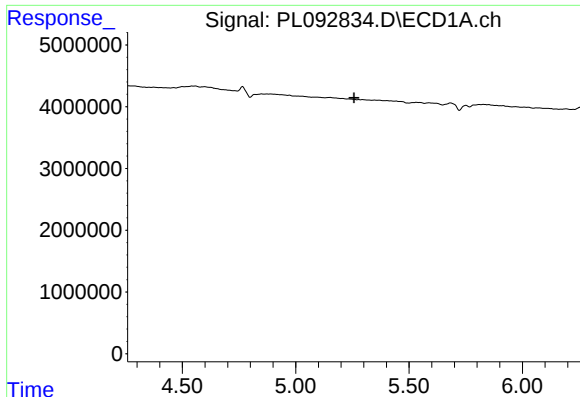

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.258 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-6

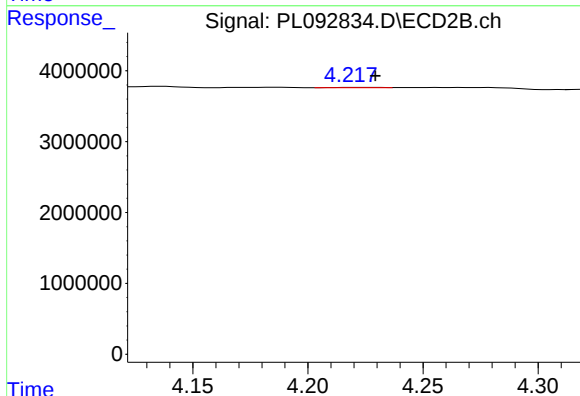


#5 Aldrin

R.T.: 4.219 min
Delta R.T.: -0.010 min
Response: 64439
Conc: 0.02 ng/ml

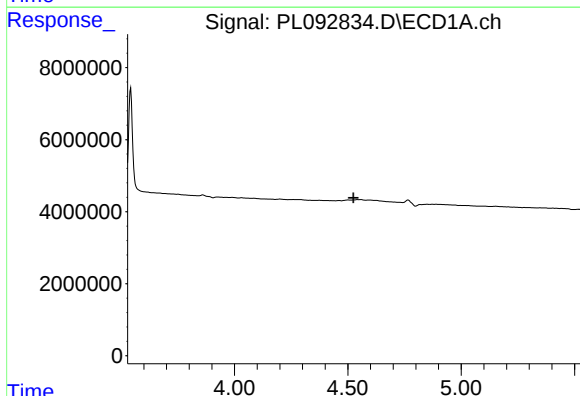


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.525 min
Response: 0
Conc: N.D.

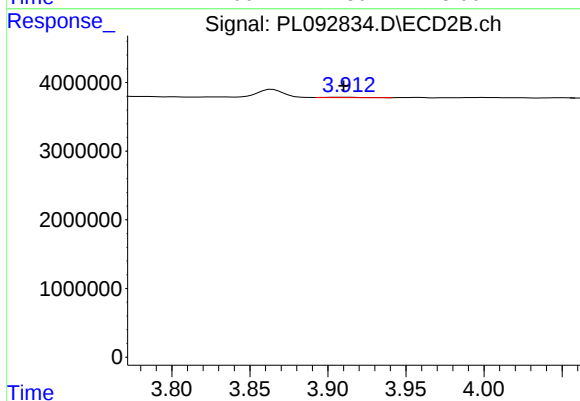

#6 beta-BHC


R.T.: 3.912 min
Delta R.T.: 0.002 min
Response: 82074
Conc: 0.05 ng/ml

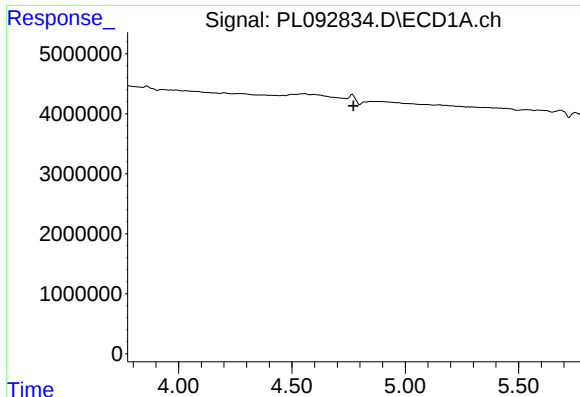

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.772 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-6

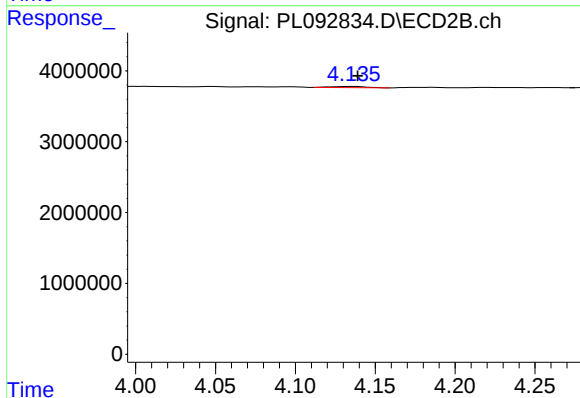


#7 delta-BHC

R.T.: 4.136 min
Delta R.T.: -0.003 min
Response: 259606
Conc: 0.07 ng/ml

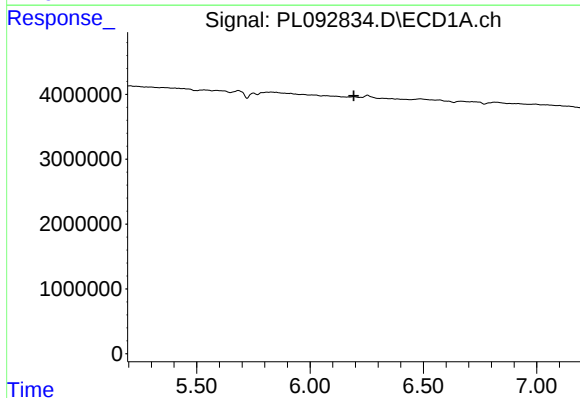


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 6.193 min
Response: 0
Conc: N.D.

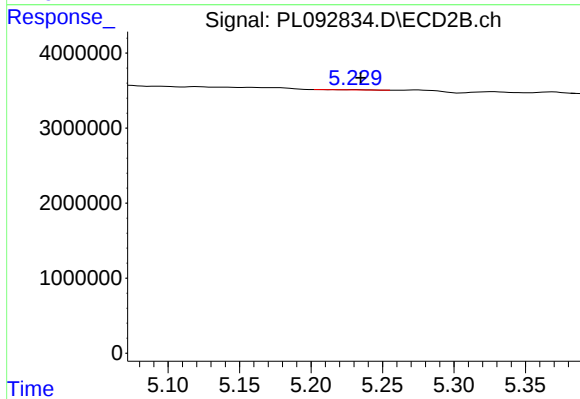

#12 4,4'-DDE


R.T.: 5.230 min
Delta R.T.: -0.004 min
Response: 70920
Conc: 0.02 ng/ml

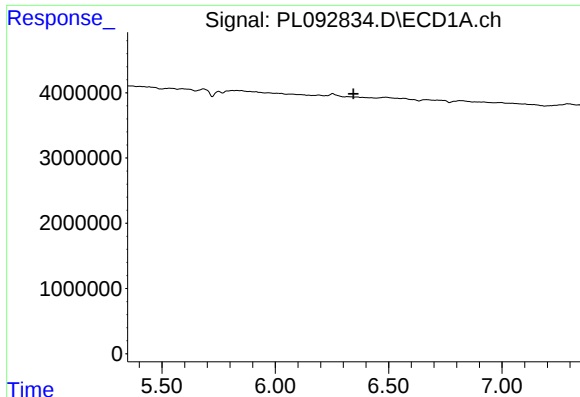

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.345 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-6

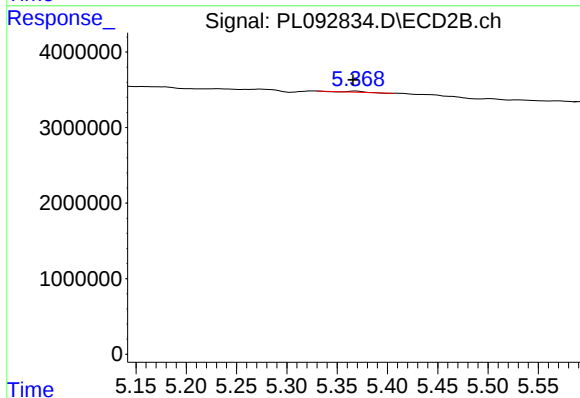


#13 Dieldrin

R.T.: 5.369 min
Delta R.T.: 0.003 min
Response: 133531
Conc: 0.04 ng/ml

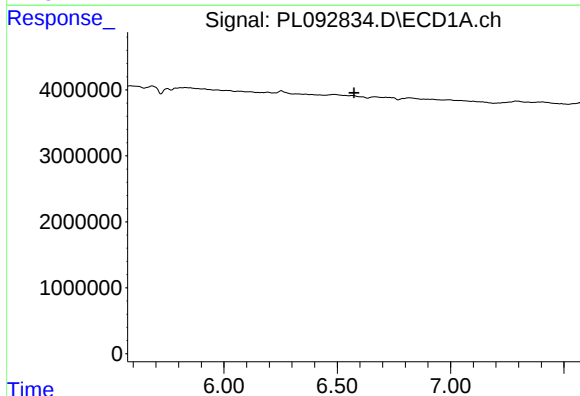


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.574 min
Response: 0
Conc: N.D.

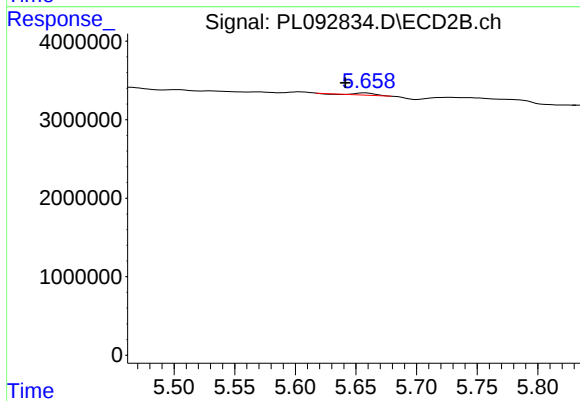

#14 Endrin


R.T.: 5.658 min
Delta R.T.: 0.016 min
Response: 249696
Conc: 0.09 ng/ml

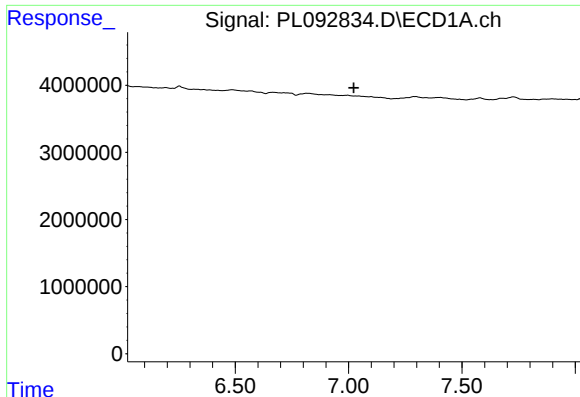

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.023 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-6

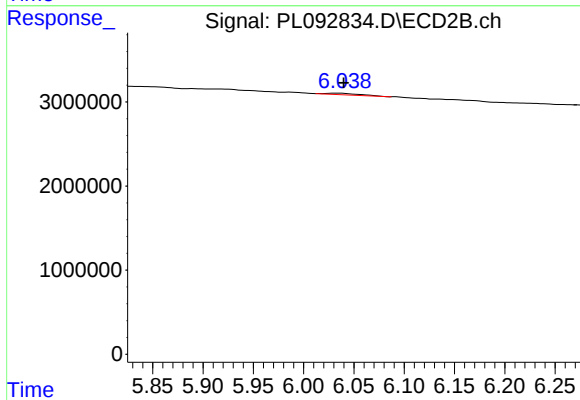


#17 4,4'-DDT

R.T.: 6.036 min
Delta R.T.: -0.004 min
Response: 421825
Conc: 0.16 ng/ml

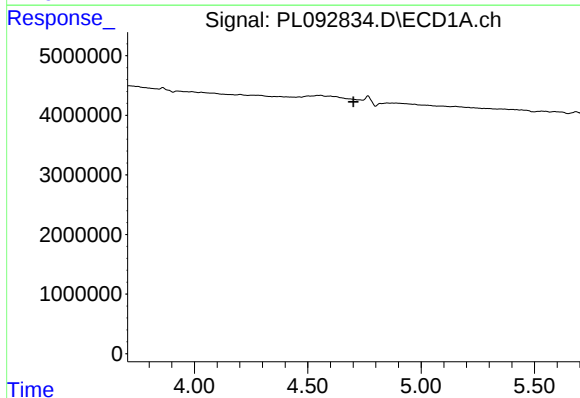


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.702 min
Response: 0
Conc: N.D.

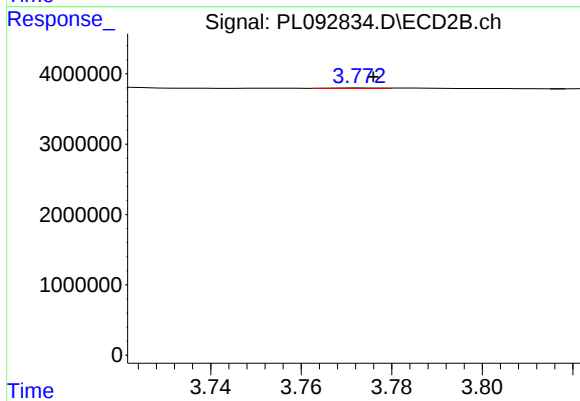

#23 Chlordane-1


R.T.: 3.774 min
Delta R.T.: -0.002 min
Response: 43131
Conc: 0.41 ng/ml

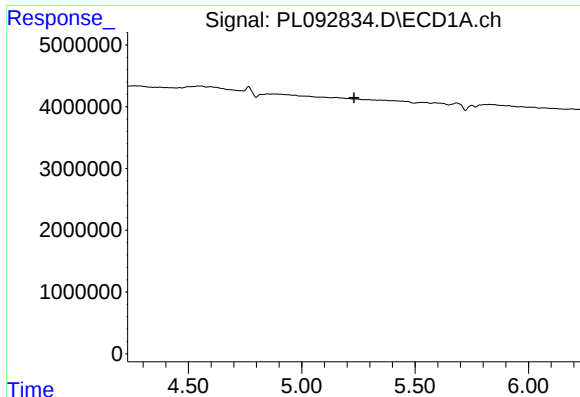

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-6

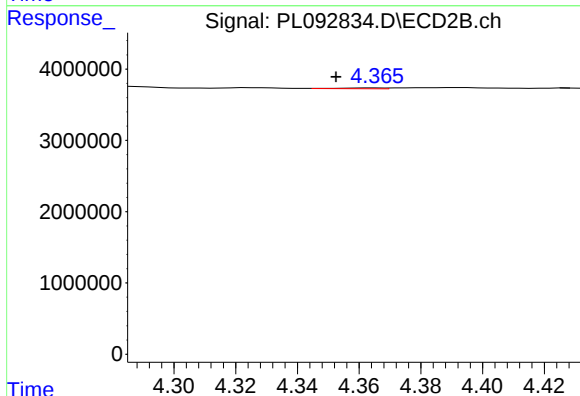


#24 Chlordane-2

R.T.: 4.365 min
Delta R.T.: 0.013 min
Response: 104888
Conc: 0.85 ng/ml

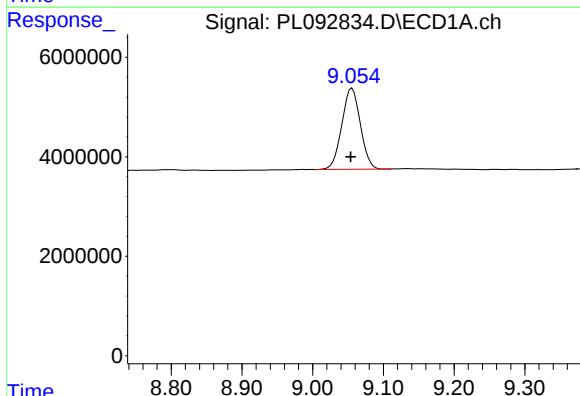

#28 Decachlorobiphenyl

R.T.: 9.056 min
Delta R.T.: 0.002 min
Response: 29717616
Conc: 15.44 ng/ml

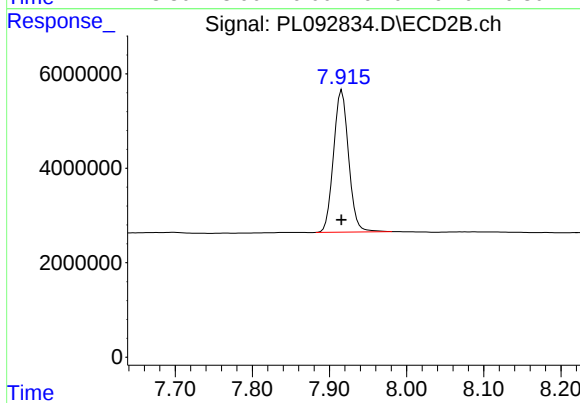

#28 Decachlorobiphenyl

R.T.: 7.916 min
Delta R.T.: 0.000 min
Response: 40974872
Conc: 15.01 ng/ml