

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110424\
 Data File : PL092826.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Nov 2024 15:11
 Operator : AR\AJ
 Sample : P4667-13
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BP-F-7

Manual Integrations
 APPROVED

Reviewed By :Abdul
 Mirza

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 03:13:23 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 28 18:58:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

11/05/2024
 Supervised By :Ankita
 Jodhani

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	11/05/2024

System Monitoring Compounds							
1) SA Tetrachlo...	3.540	2.779	56451321	62750097	23.039m	23.060	
28) SA Decachlor...	9.056	7.916	41672426	55594713	21.653	20.370	

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110424\
Data File : PL092826.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Nov 2024 15:11
Operator : AR\AJ
Sample : P4667-13
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
BP-F-7


Manual Integrations
APPROVED


Reviewed By : Abdul
Mirza

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 03:13:23 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 28 18:58:23 2024
Response via : Initial Calibration
Integrator: ChemStation

11/05/2024
Supervised By : Ankita
Jodhani

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

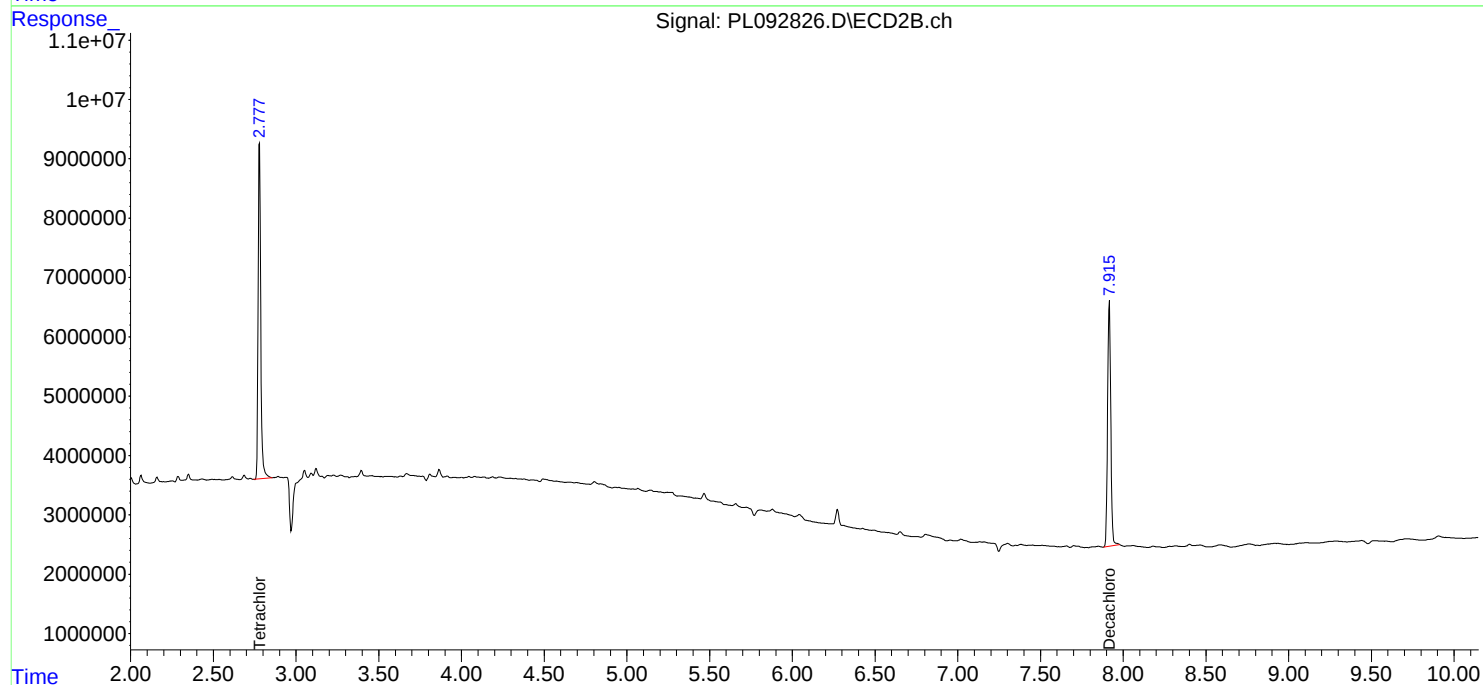

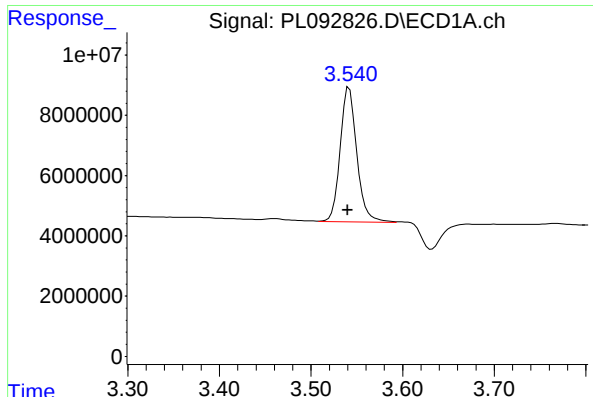


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: 0.000 min
Response: 56451321
Conc: 23.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
BP-F-7

Manual Integrations
APPROVED

Reviewed By :Abdul
Mirza

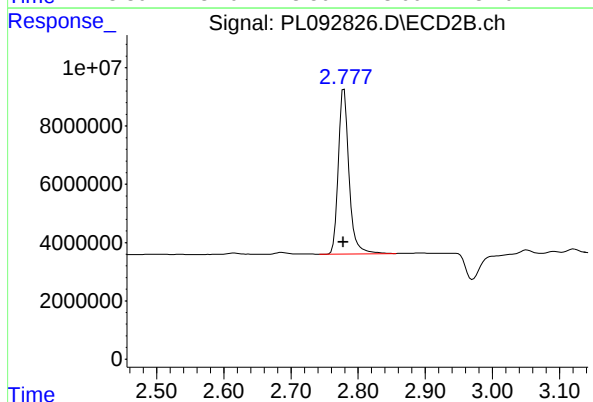


#1 Tetrachloro-m-xylene

R.T.: 2.779 min
Delta R.T.: 0.001 min
Response: 62750097
Conc: 23.06 ng/ml


11/05/2024
Supervised By :Ankita
Jodhani

11/05/2024

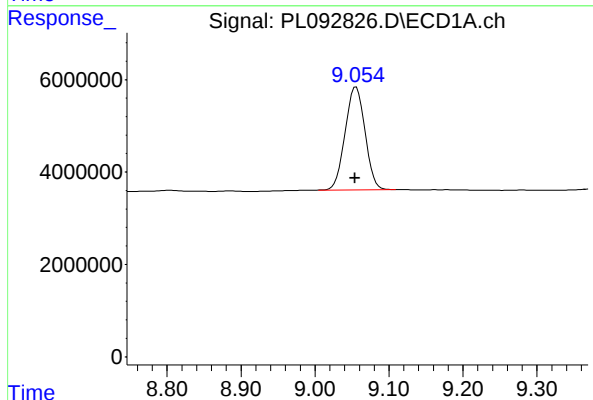

#28 Decachlorobiphenyl

R.T.: 9.056 min
Delta R.T.: 0.002 min
Response: 41672426
Conc: 21.65 ng/ml

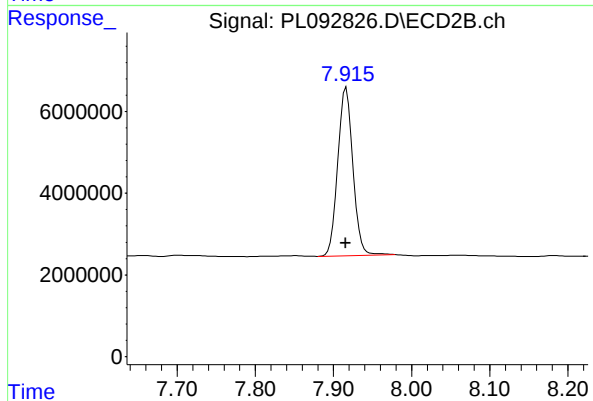

#28 Decachlorobiphenyl

R.T.: 7.916 min
Delta R.T.: 0.000 min
Response: 55594713
Conc: 20.37 ng/ml