

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110518\
 Data File : PL041780.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Nov 2018 16:13
 Operator : AJ\SJ
 Sample : J5816-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 23:47:13 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.472	4.104	69835167	37082384	10.963	12.039
28)	SA Decachlor...	8.213	9.233	62314692	25501681	9.407	9.953
Target Compounds							
6)	B beta-BHC	4.407f	0.000	5154077	0	1.367	N.D. #
7)	B delta-BHC	0.000	5.150f	0	1279574	N.D.	0.317 #
8)	B Heptachlo...	5.232f	0.000	119935	0	0.015	N.D. #
10)	B gamma-Chl...	5.406	0.000	610704	0	0.075	N.D. #
11)	B alpha-Chl...	5.406f	0.000	610704	0	0.075	N.D. #
12)	B 4,4'-DDE	5.629	0.000	2510397	0	0.351	N.D. #
17)	MA 4,4'-DDT	6.380	0.000	1814682	0	0.298	N.D. #
23)	Chlordane-1	4.407	5.150	5154077	1279574	18.178	9.213 #
24)	Chlordane-2	4.821	0.000	2086277	0	7.084	N.D. #
25)	Chlordane-3	5.406	0.000	610704	0	0.685	N.D. #
26)	Chlordane-4	5.406	0.000	610704	0	0.780	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110518\
Data File : PL041780.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Nov 2018 16:13
Operator : AJ\SJ
Sample : J5816-03
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 23:47:13 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

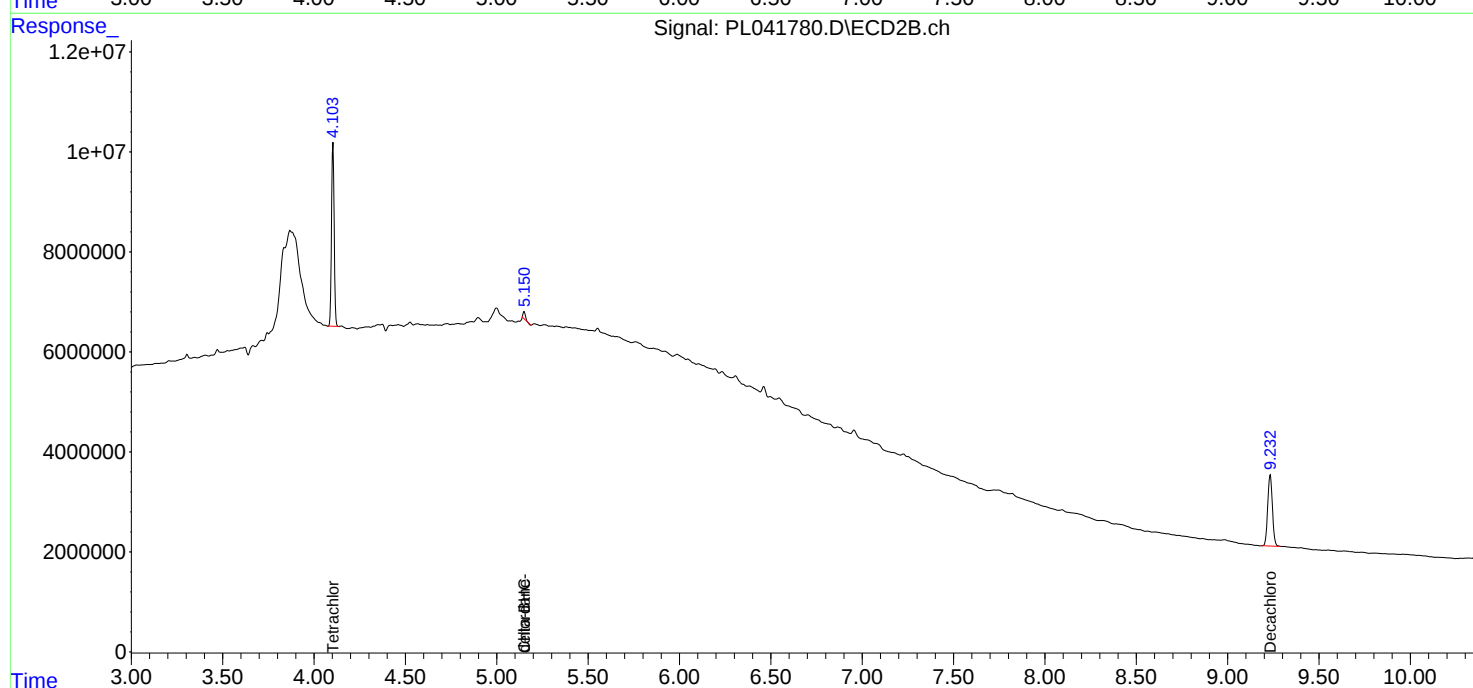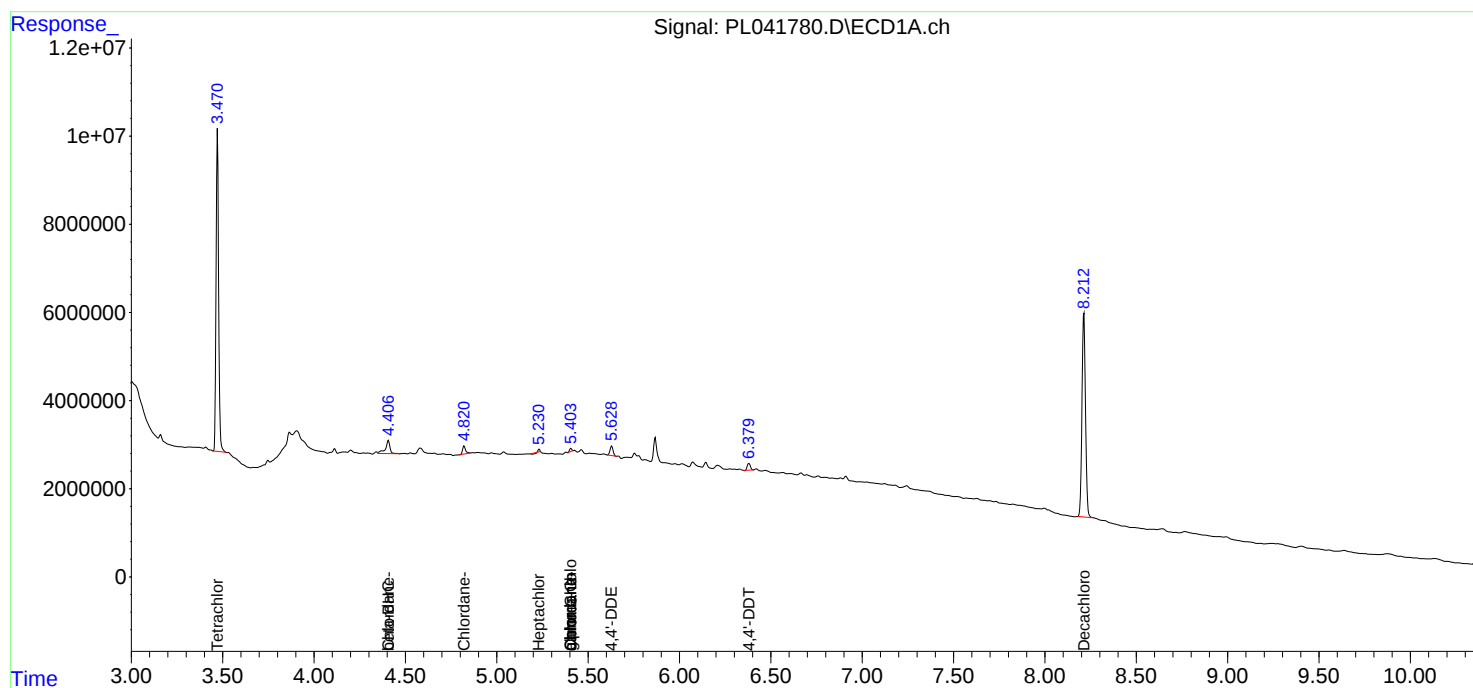


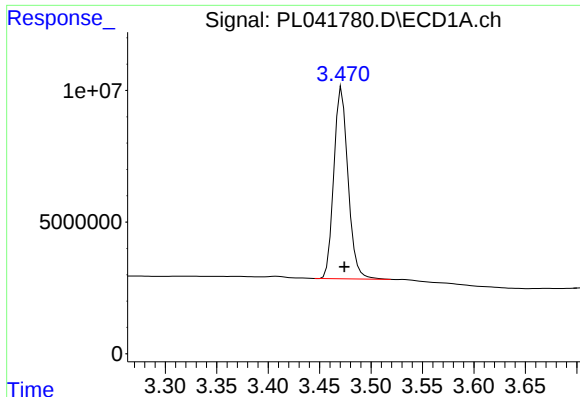

#1 Tetrachloro-m-xylene


R.T.: 3.472 min
Delta R.T.: -0.002 min
Response: 69835167
Conc: 10.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

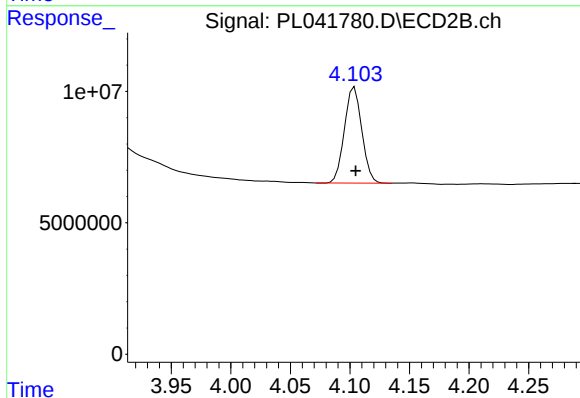


#1 Tetrachloro-m-xylene

R.T.: 4.104 min
Delta R.T.: 0.000 min
Response: 37082384
Conc: 12.04 ng/ml

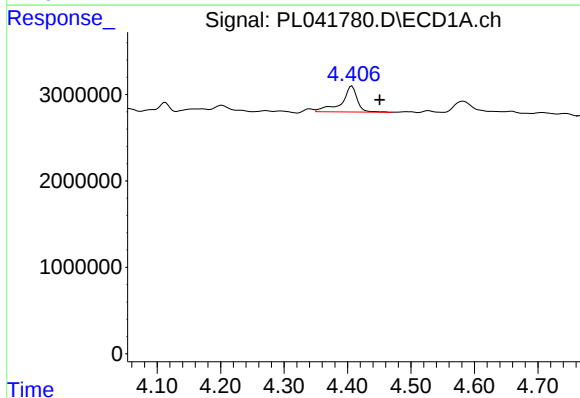


#6 beta-BHC

R.T.: 4.407 min
Delta R.T.: -0.044 min
Response: 5154077
Conc: 1.37 ng/ml

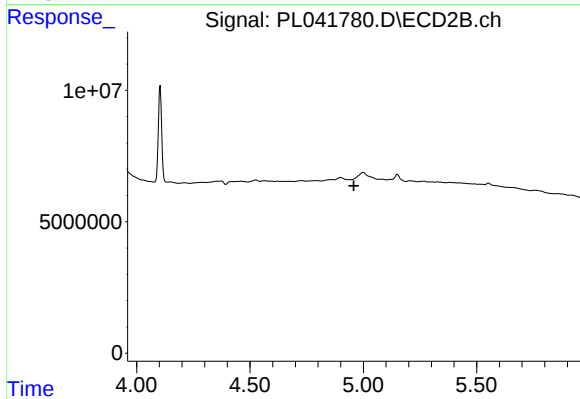

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.957 min
Response: 0
Conc: N.D.

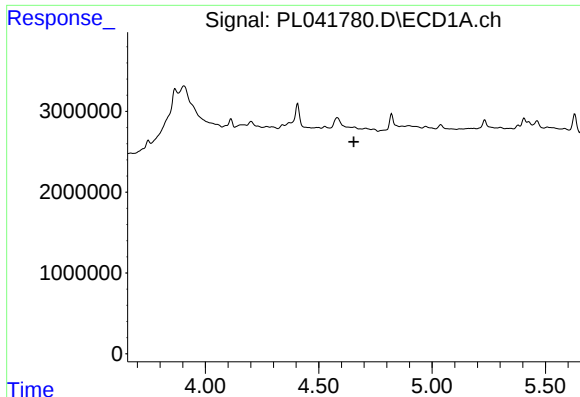

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.654 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

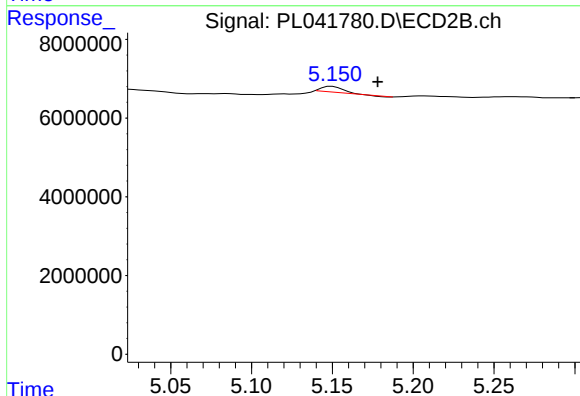


#7 delta-BHC

R.T.: 5.150 min
Delta R.T.: -0.028 min
Response: 1279574
Conc: 0.32 ng/ml

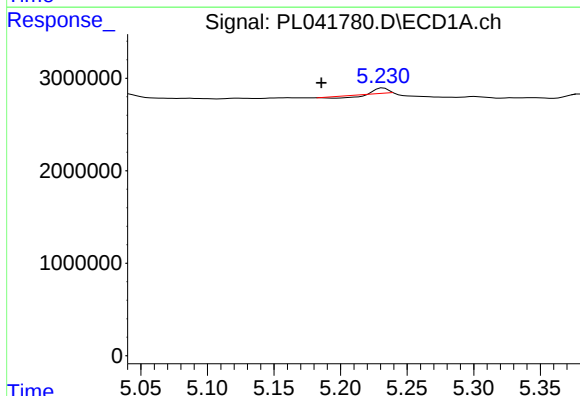


#8 Heptachlor epoxide

R.T.: 5.232 min
Delta R.T.: 0.046 min
Response: 119935
Conc: 0.01 ng/ml

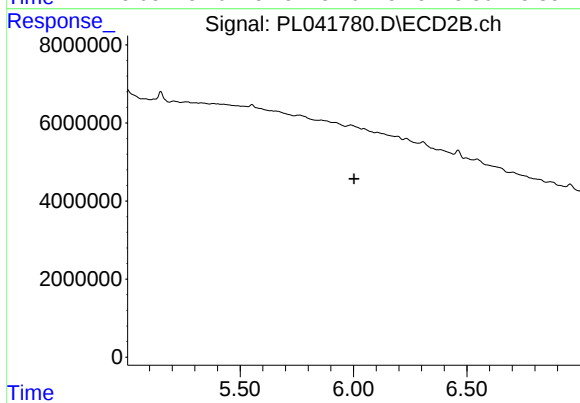

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 6.002 min
Response: 0
Conc: N.D.

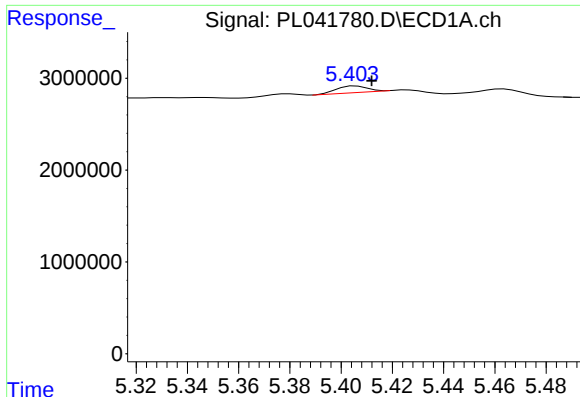

#10 gamma-Chlordane


R.T.: 5.406 min
Delta R.T.: -0.006 min
Response: 610704
Conc: 0.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

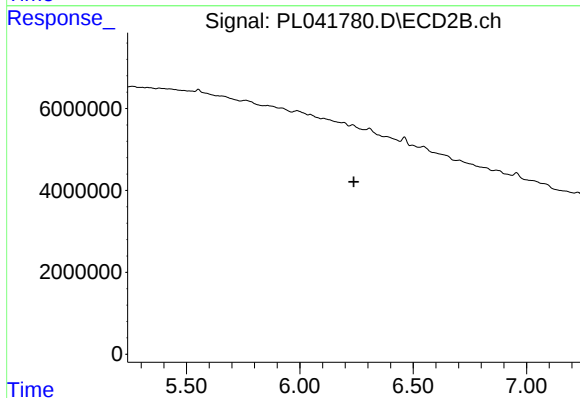


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.237 min
Response: 0
Conc: N.D.

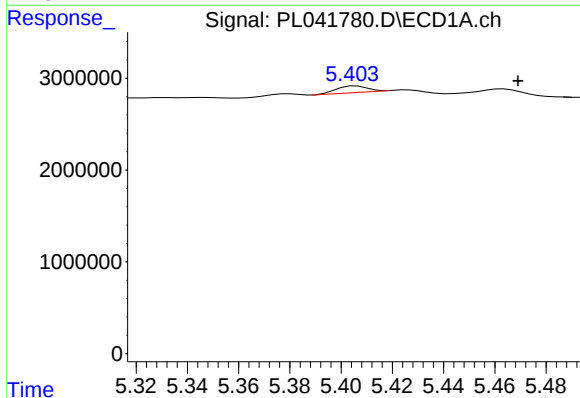


#11 alpha-Chlordane

R.T.: 5.406 min
Delta R.T.: -0.063 min
Response: 610704
Conc: 0.08 ng/ml

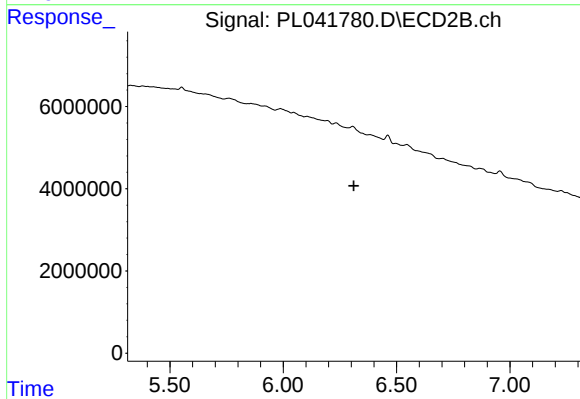

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.311 min
Response: 0
Conc: N.D.

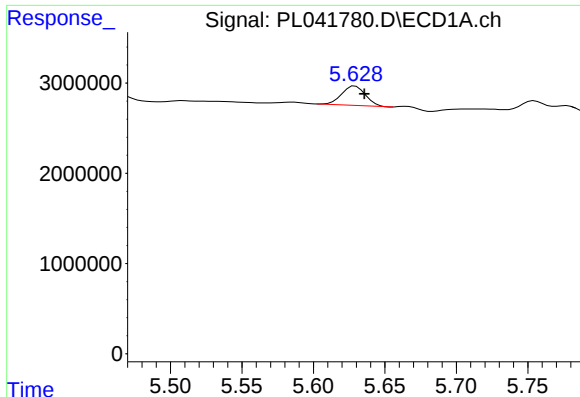

#12 4,4'-DDE


R.T.: 5.629 min
Delta R.T.: -0.006 min
Response: 2510397
Conc: 0.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

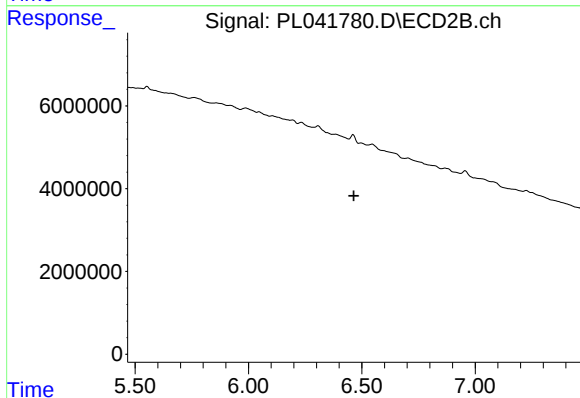


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.465 min
Response: 0
Conc: N.D.

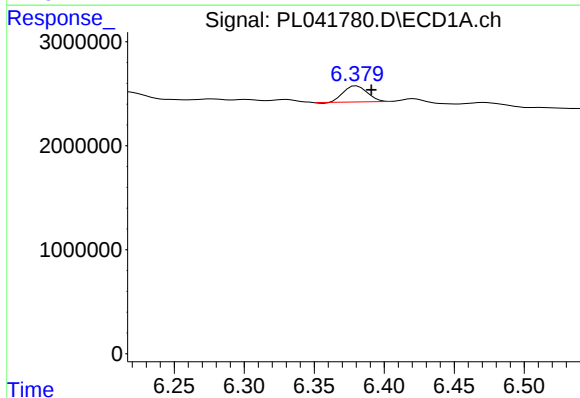


#17 4,4'-DDT

R.T.: 6.380 min
Delta R.T.: -0.011 min
Response: 1814682
Conc: 0.30 ng/ml

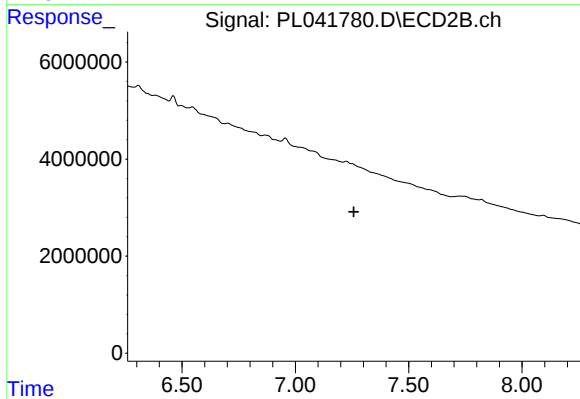

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.258 min
Response: 0
Conc: N.D.

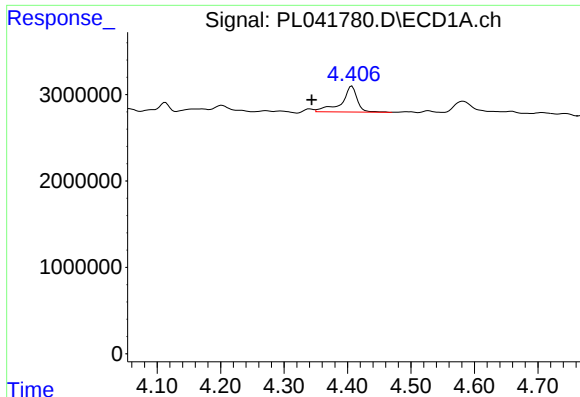

#23 Chlordane-1


R.T.: 4.407 min
Delta R.T.: 0.063 min
Response: 5154077
Conc: 18.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

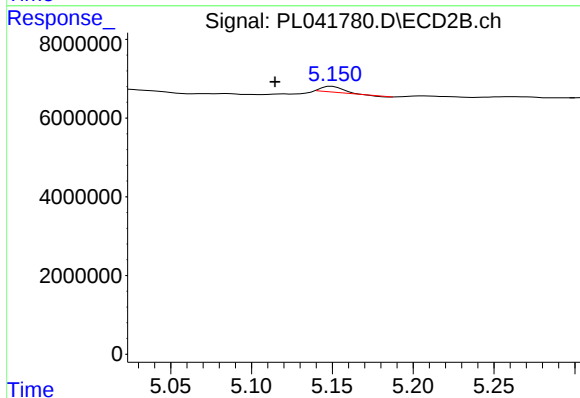


#23 Chlordane-1

R.T.: 5.150 min
Delta R.T.: 0.035 min
Response: 1279574
Conc: 9.21 ng/ml

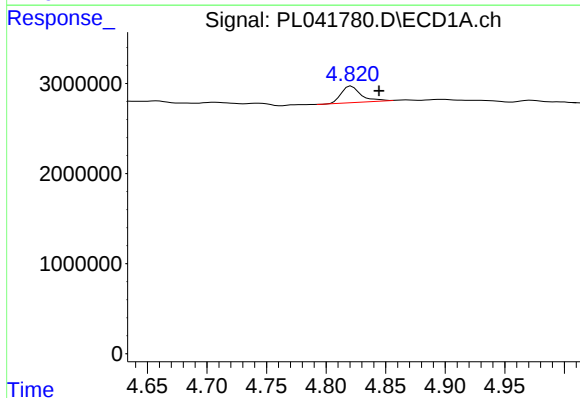


#24 Chlordane-2

R.T.: 4.821 min
Delta R.T.: -0.023 min
Response: 2086277
Conc: 7.08 ng/ml

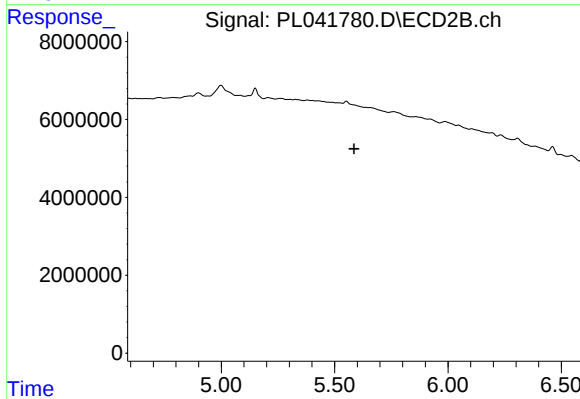

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.586 min
Response: 0
Conc: N.D.

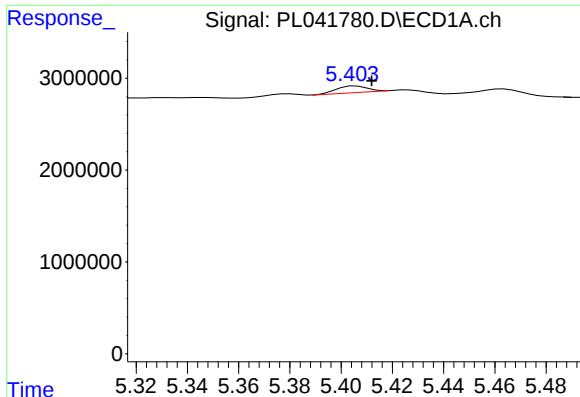

#25 Chlordane-3


R.T.: 5.406 min
Delta R.T.: -0.006 min
Response: 610704
Conc: 0.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

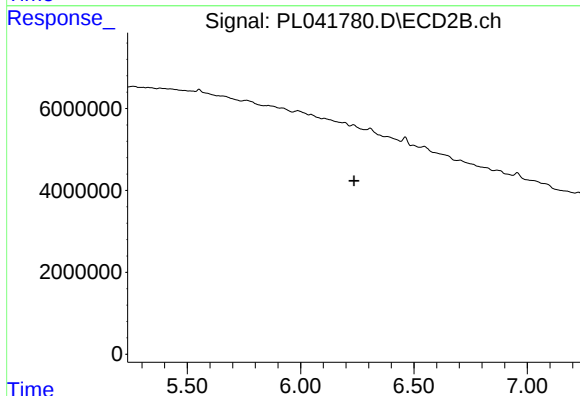


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.237 min
Response: 0
Conc: N.D.

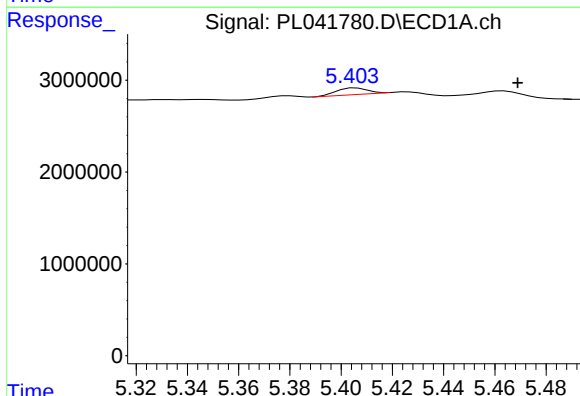


#26 Chlordane-4

R.T.: 5.406 min
Delta R.T.: -0.063 min
Response: 610704
Conc: 0.78 ng/ml

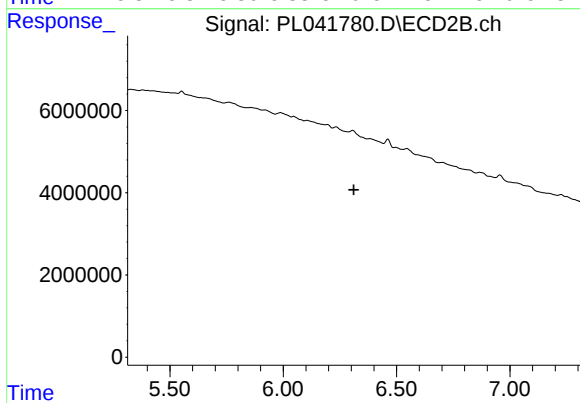

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.311 min
Response: 0
Conc: N.D.

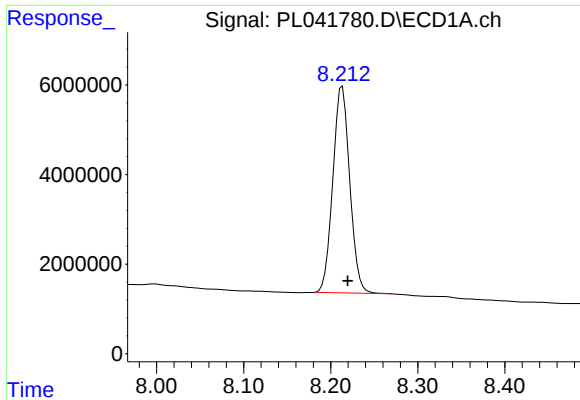

#28 Decachlorobiphenyl

R.T.: 8.213 min
Delta R.T.: -0.006 min
Response: 62314692
Conc: 9.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

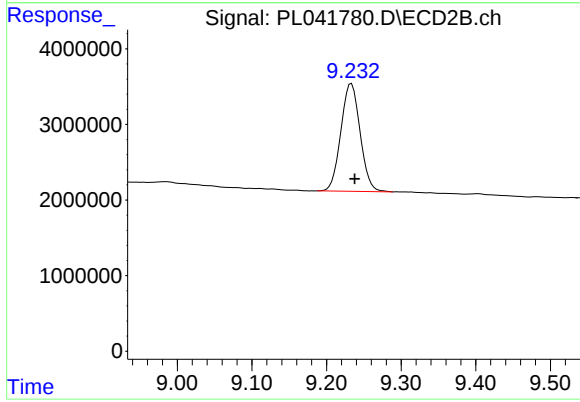

#28 Decachlorobiphenyl

R.T.: 9.233 min
Delta R.T.: -0.004 min
Response: 25501681
Conc: 9.95 ng/ml