

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110518\
 Data File : PL041804.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Nov 2018 22:03
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 23:49:28 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 30 01:26:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.472	4.104	134.1E6	71125398	21.053	23.091
28)	SA Decachlor...	8.213	9.235	127.2E6	50196770	19.202	19.592
Target Compounds							
6)	B beta-BHC	4.407f	0.000	3090162	0	0.820	N.D. #
23)	Chlordane-1	4.369	0.000	1734328	0	6.117	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110518\
Data File : PL041804.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Nov 2018 22:03
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 23:49:28 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102918.M
Quant Title : GC Extractables
QLast Update : Tue Oct 30 01:26:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

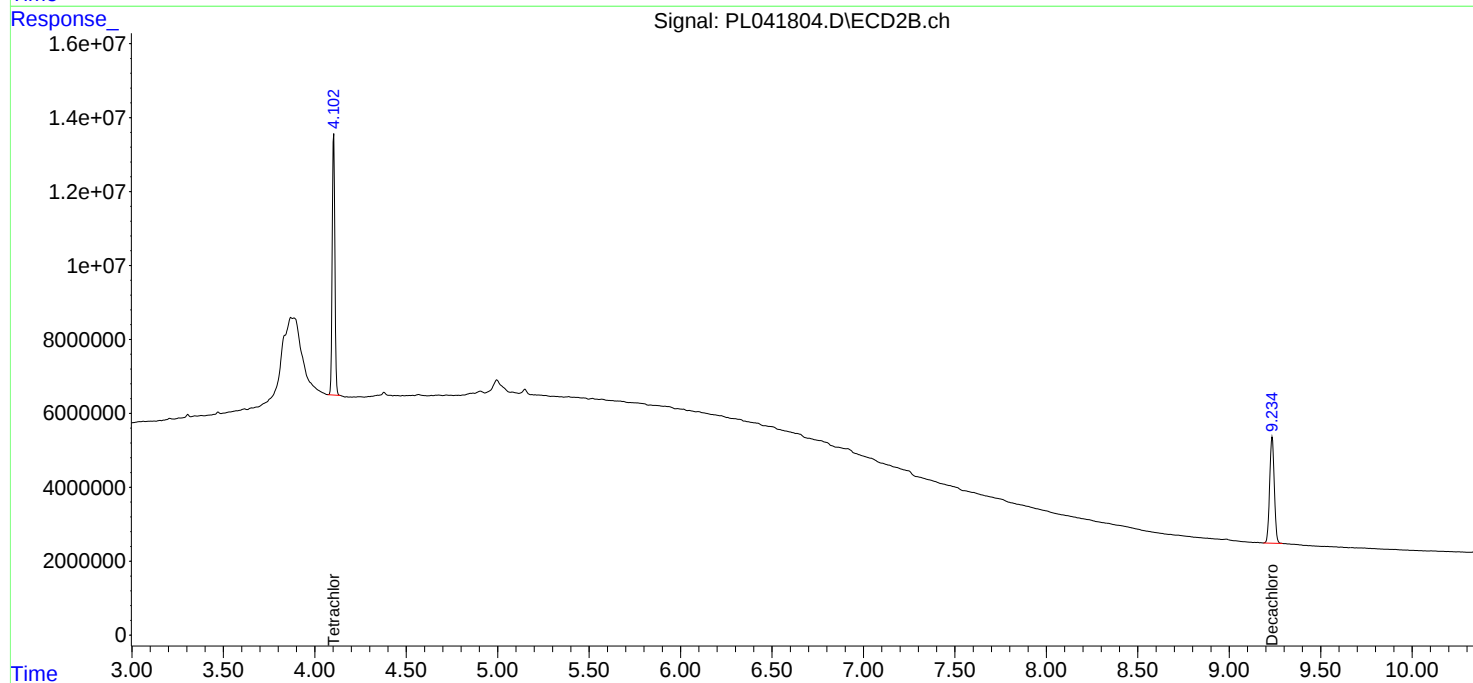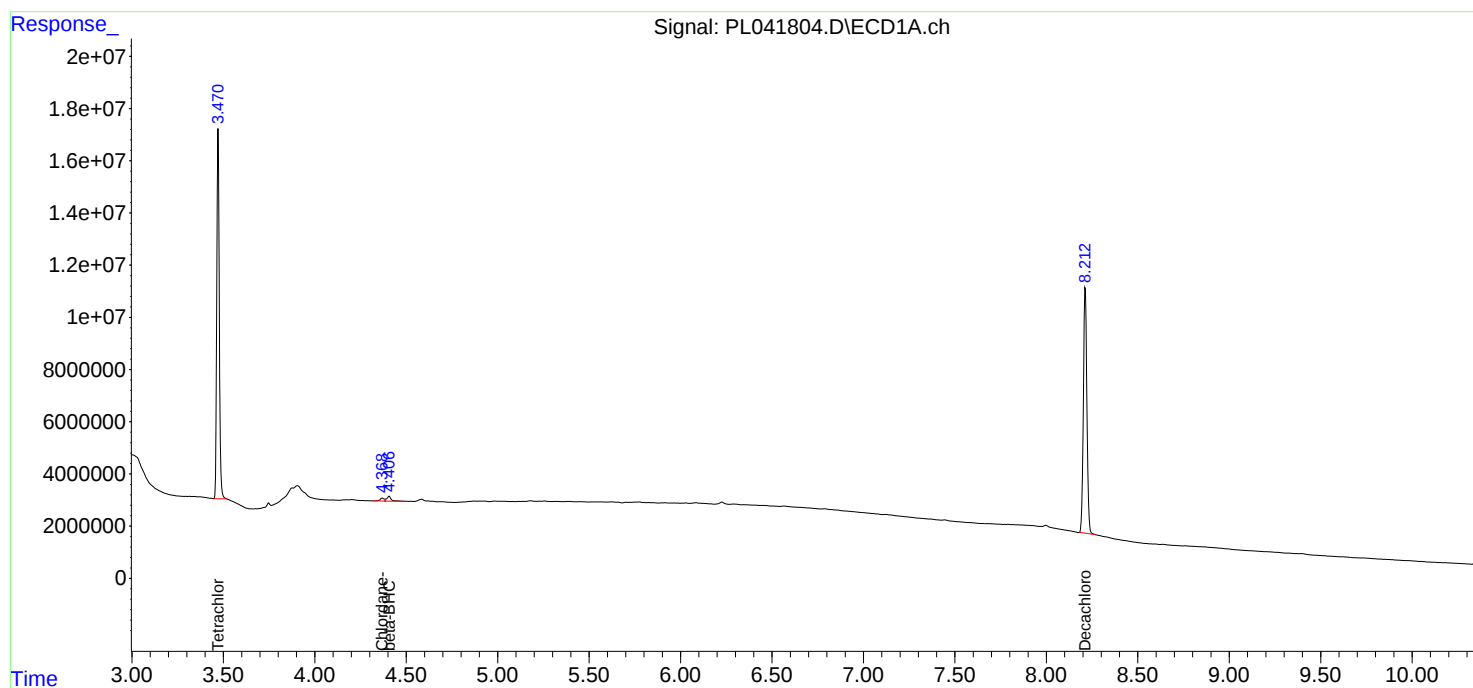


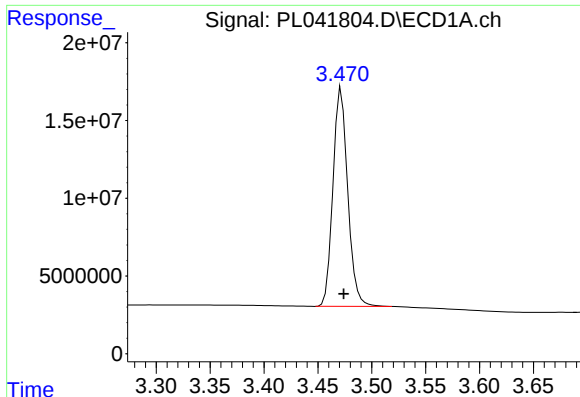

#1 Tetrachloro-m-xylene


R.T.: 3.472 min
Delta R.T.: -0.002 min
Response: 134109324
Conc: 21.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

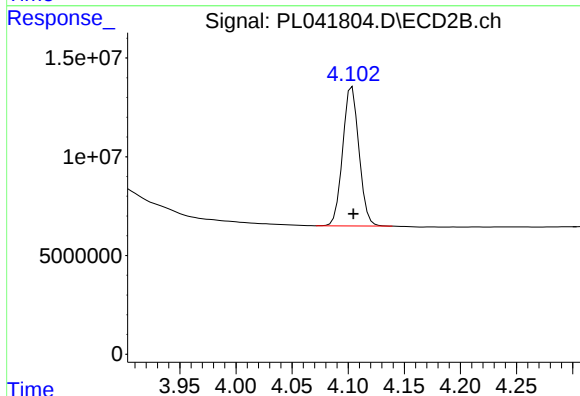


#1 Tetrachloro-m-xylene

R.T.: 4.104 min
Delta R.T.: -0.001 min
Response: 71125398
Conc: 23.09 ng/ml

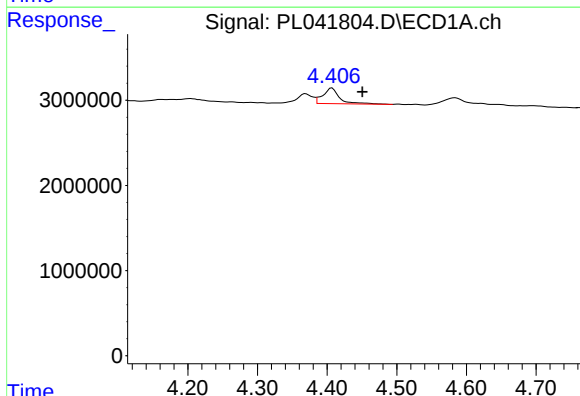


#6 beta-BHC

R.T.: 4.407 min
Delta R.T.: -0.044 min
Response: 3090162
Conc: 0.82 ng/ml

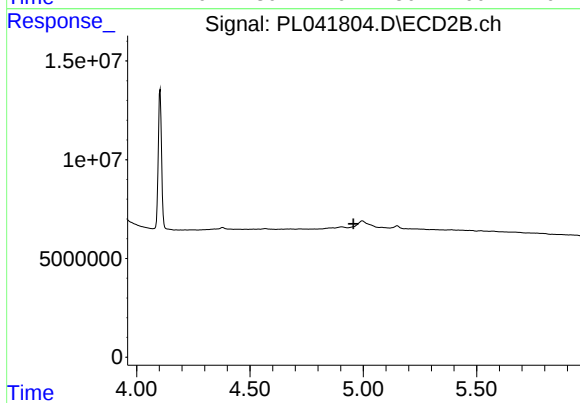

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.957 min
Response: 0
Conc: N.D.

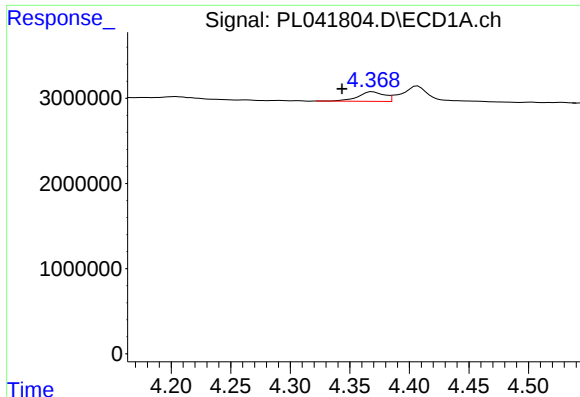

#23 Chlordane-1


R.T.: 4.369 min
Delta R.T.: 0.026 min
Response: 1734328
Conc: 6.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

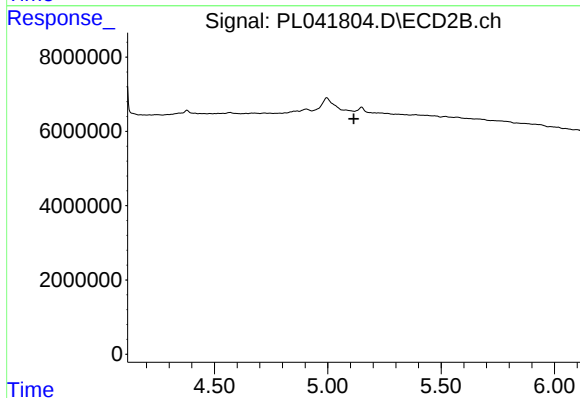


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.115 min
Response: 0
Conc: N.D.

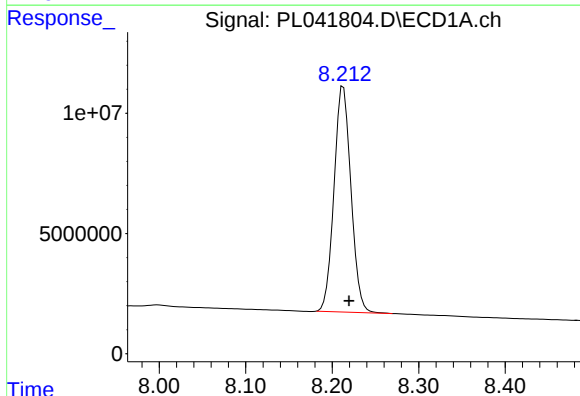

#28 Decachlorobiphenyl

R.T.: 8.213 min
Delta R.T.: -0.006 min
Response: 127191545
Conc: 19.20 ng/ml

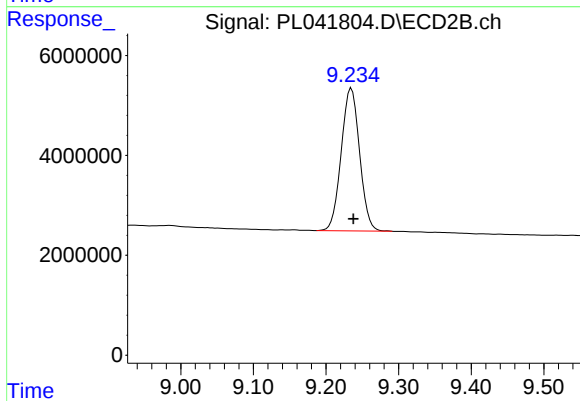

#28 Decachlorobiphenyl

R.T.: 9.235 min
Delta R.T.: -0.003 min
Response: 50196770
Conc: 19.59 ng/ml