

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110521\
 Data File : PL070798.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Nov 2021 10:38
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 08 03:18:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 04 19:28:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
2) A	alpha-BHC	0.000	6.060f	0	1001524	N.D. 0.544 #
8) B	Heptachlo...	0.000	7.969	0	4419860	N.D. 2.900 #
10) B	gamma-Chl...	0.000	8.201f	0	1208745	N.D. 0.781 #
13) MA	Dieldrin	7.701	0.000	947769	0	1.518 N.D. #
14) MA	Endrin	8.007f	0.000	2460124	0	4.339 N.D. #
25)	Chlordane-3	0.000	8.201f	0	1208745	N.D. 5.980 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL110521\
Data File : PL070798.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Nov 2021 10:38
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 08 03:18:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
Quant Title : GC Extractables
QLast Update : Thu Nov 04 19:28:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

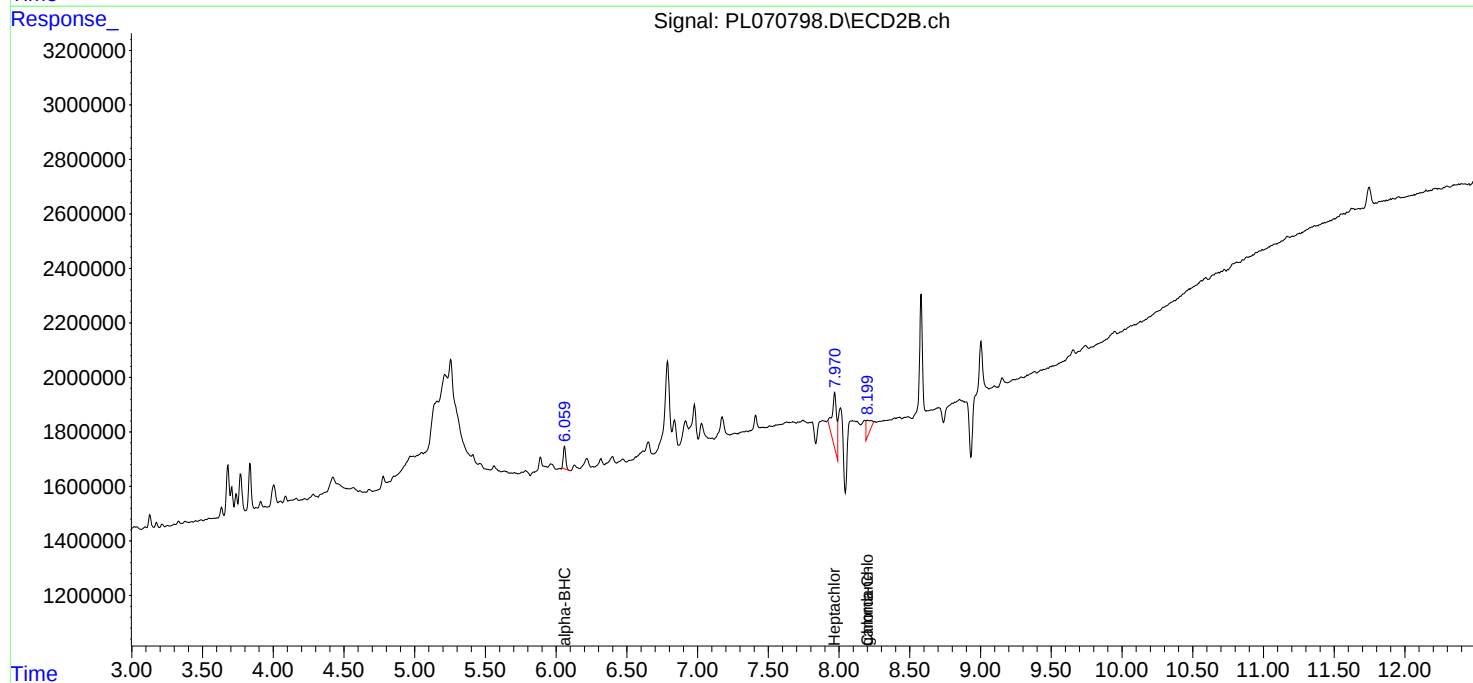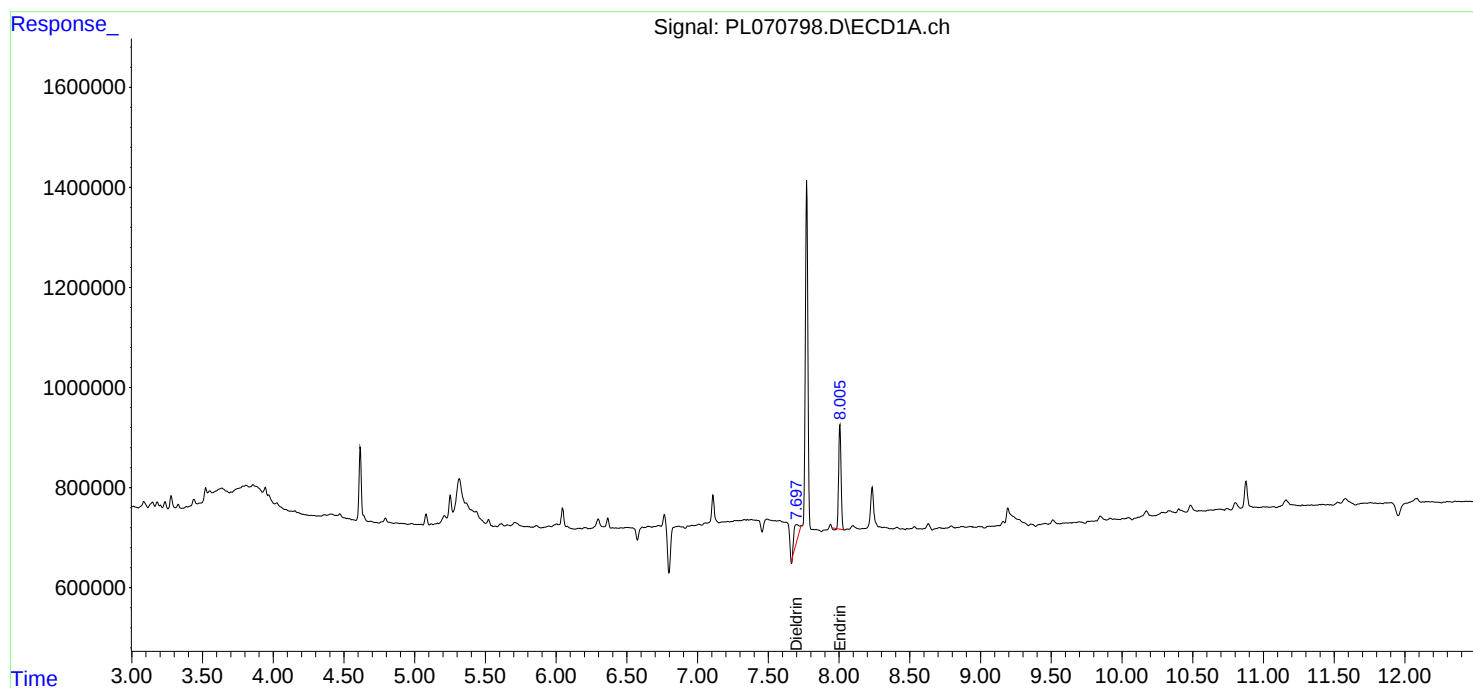


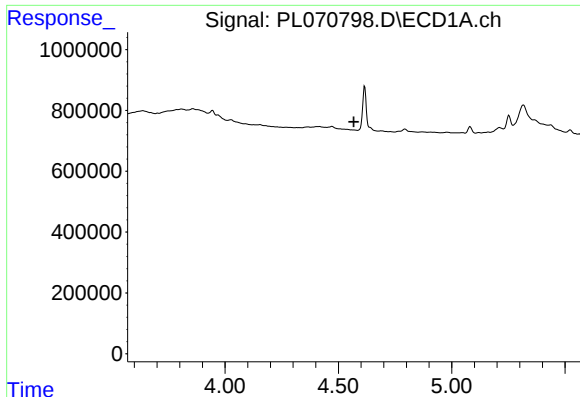

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.568 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

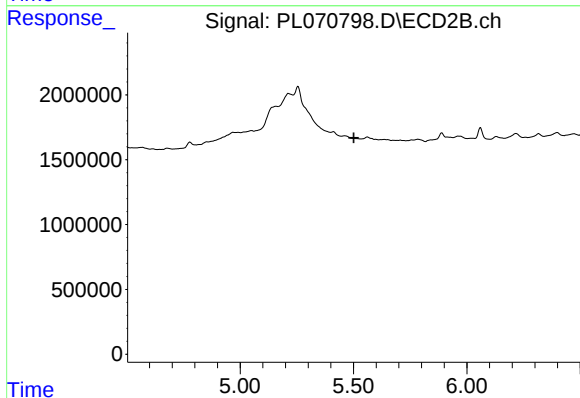


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

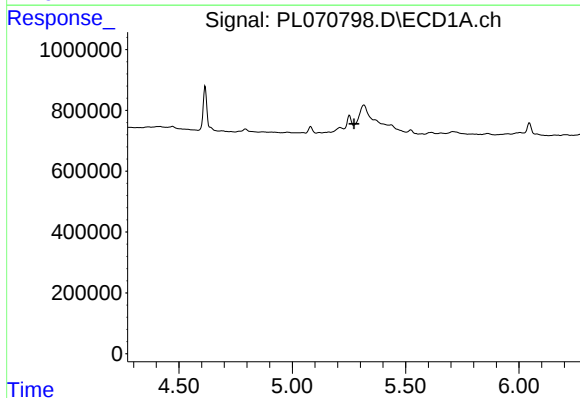


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.273 min
Response: 0
Conc: N.D.

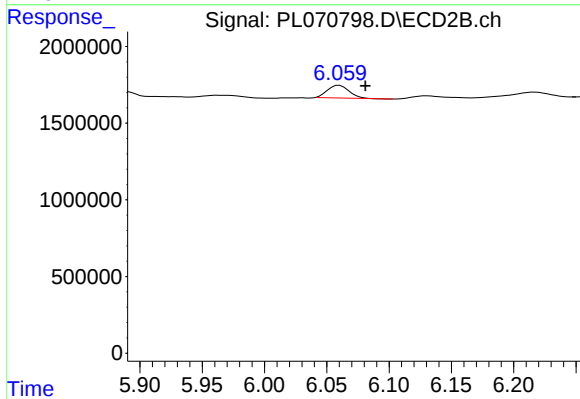

#2 alpha-BHC


R.T.: 6.060 min
Delta R.T.: -0.021 min
Response: 1001524
Conc: 0.54 ng/ml

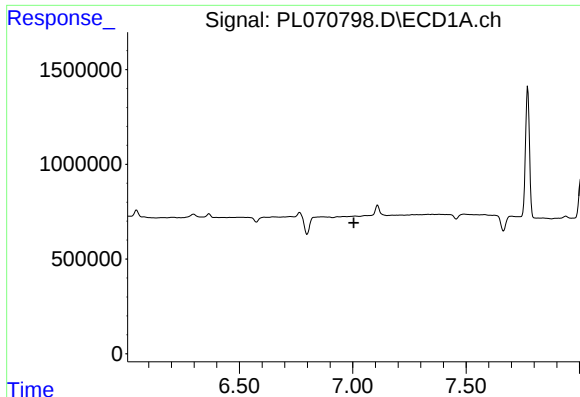

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 7.005 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

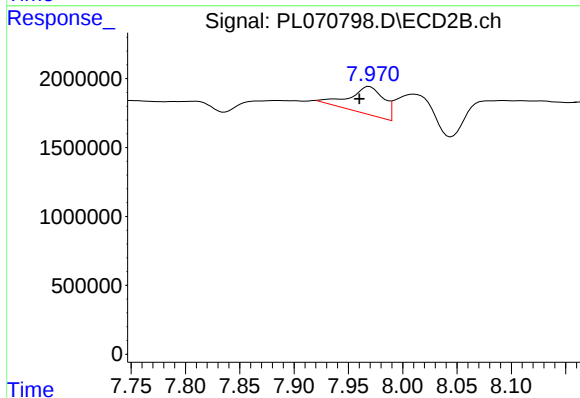


#8 Heptachlor epoxide

R.T.: 7.969 min
Delta R.T.: 0.009 min
Response: 4419860
Conc: 2.90 ng/ml

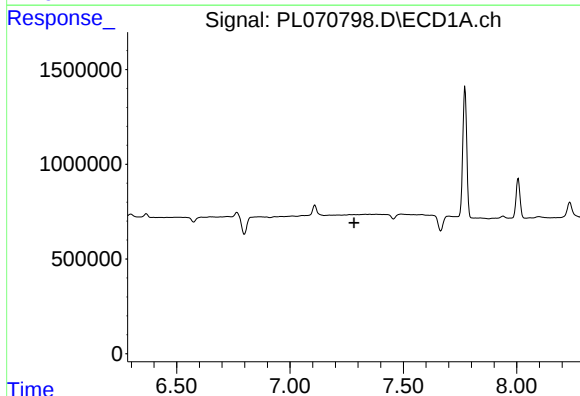


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.283 min
Response: 0
Conc: N.D.

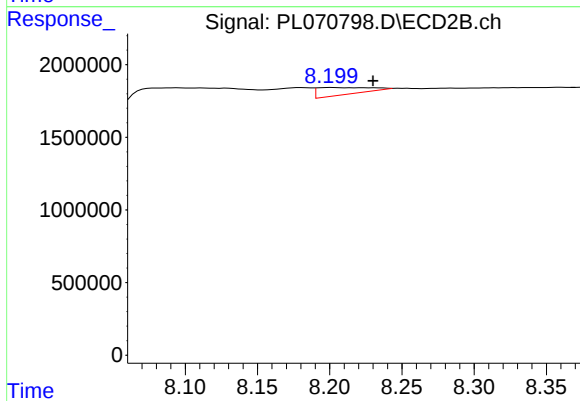

#10 gamma-Chlordane


R.T.: 8.201 min
Delta R.T.: -0.029 min
Response: 1208745
Conc: 0.78 ng/ml

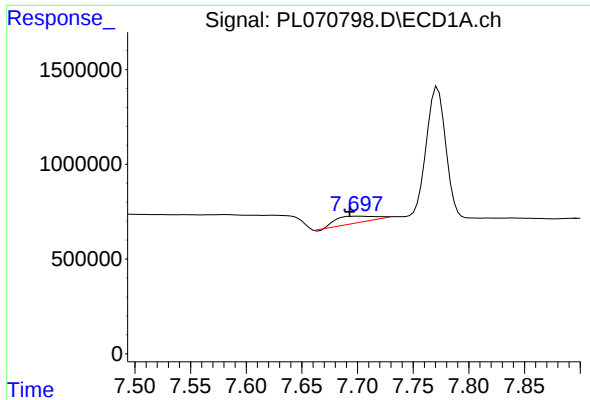

#13 Dieldrin


R.T.: 7.701 min
Delta R.T.: 0.008 min
Response: 947769
Conc: 1.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

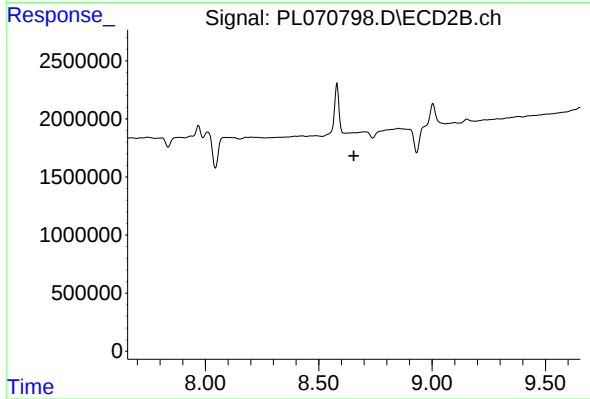


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.654 min
Response: 0
Conc: N.D.

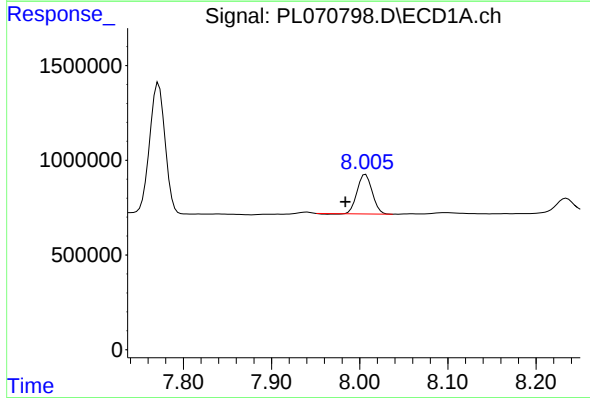


#14 Endrin

R.T.: 8.007 min
Delta R.T.: 0.023 min
Response: 2460124
Conc: 4.34 ng/ml

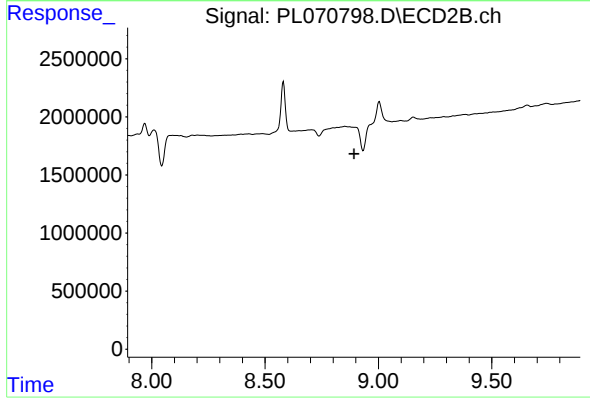

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 8.893 min
Response: 0
Conc: N.D.

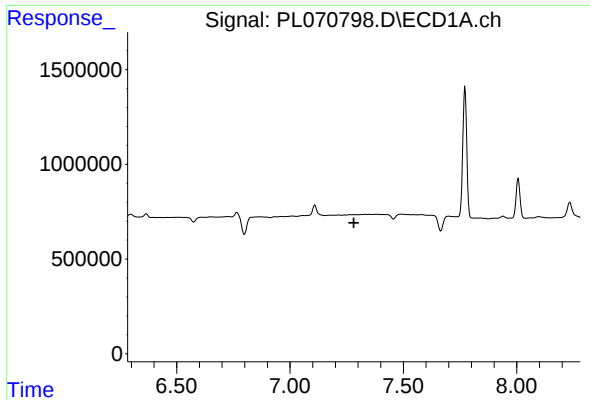

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 7.281 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

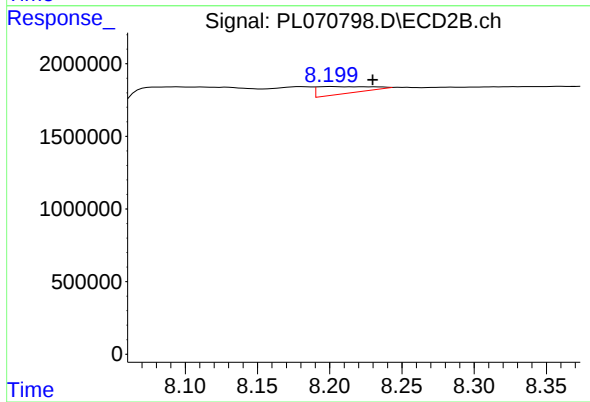


#25 Chlordane-3

R.T.: 8.201 min
Delta R.T.: -0.029 min
Response: 1208745
Conc: 5.98 ng/ml

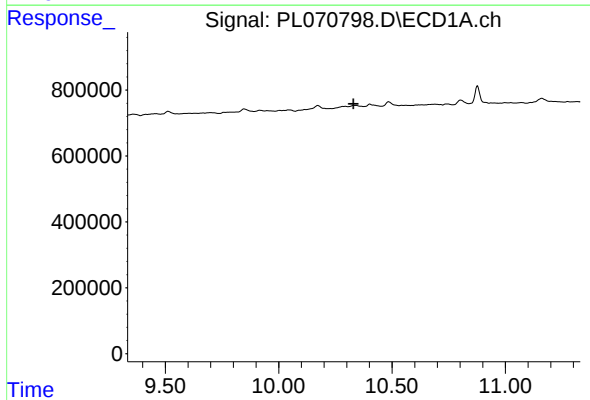

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.330 min
Response: 0
Conc: N.D.

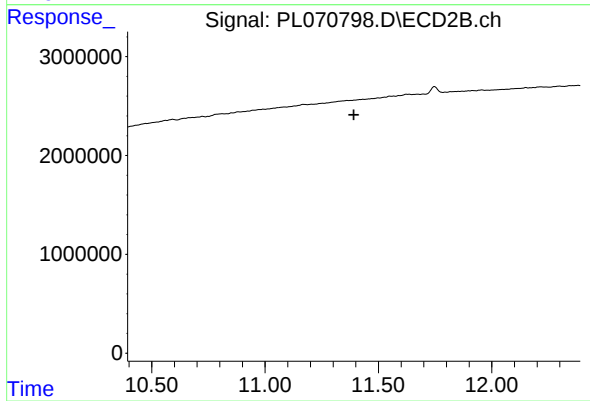

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 11.392 min
Response: 0
Conc: N.D.